

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032322\
 Data File : FB026807.D
 Signal(s) : FID2B.CH
 Acq On : 24 Mar 2022 00:31
 Operator : AJ/MA
 Sample : N1970-09 50X
 Misc : 5.01G/5.00 ML MEOH
 ALS Vial : 22 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 24 07:25:22 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	209066	19.924 ng/ml
Target Compounds			
4) t Benzene	7.887	38240	1.657 ng/ml
6) t Toluene	10.607	6932	0.317 ng/ml
7) t Ethylbenzene	13.053	26169	1.302 ng/ml
8) t m-Xylene	13.183	18028	0.895 ng/ml
9) t O-Xylene	13.918	3152	0.158 ng/ml
10) t 1,2,4-Trimethylbenzene	16.183	9439	0.474 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032322\
Data File : FB026807.D
Signal(s) : FID2B.CH
Acq On : 24 Mar 2022 00:31
Operator : AJ/MA
Sample : N1970-09 50X
Misc : 5.01G/5.00 ML MEOH
ALS Vial : 22 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 24 07:25:22 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

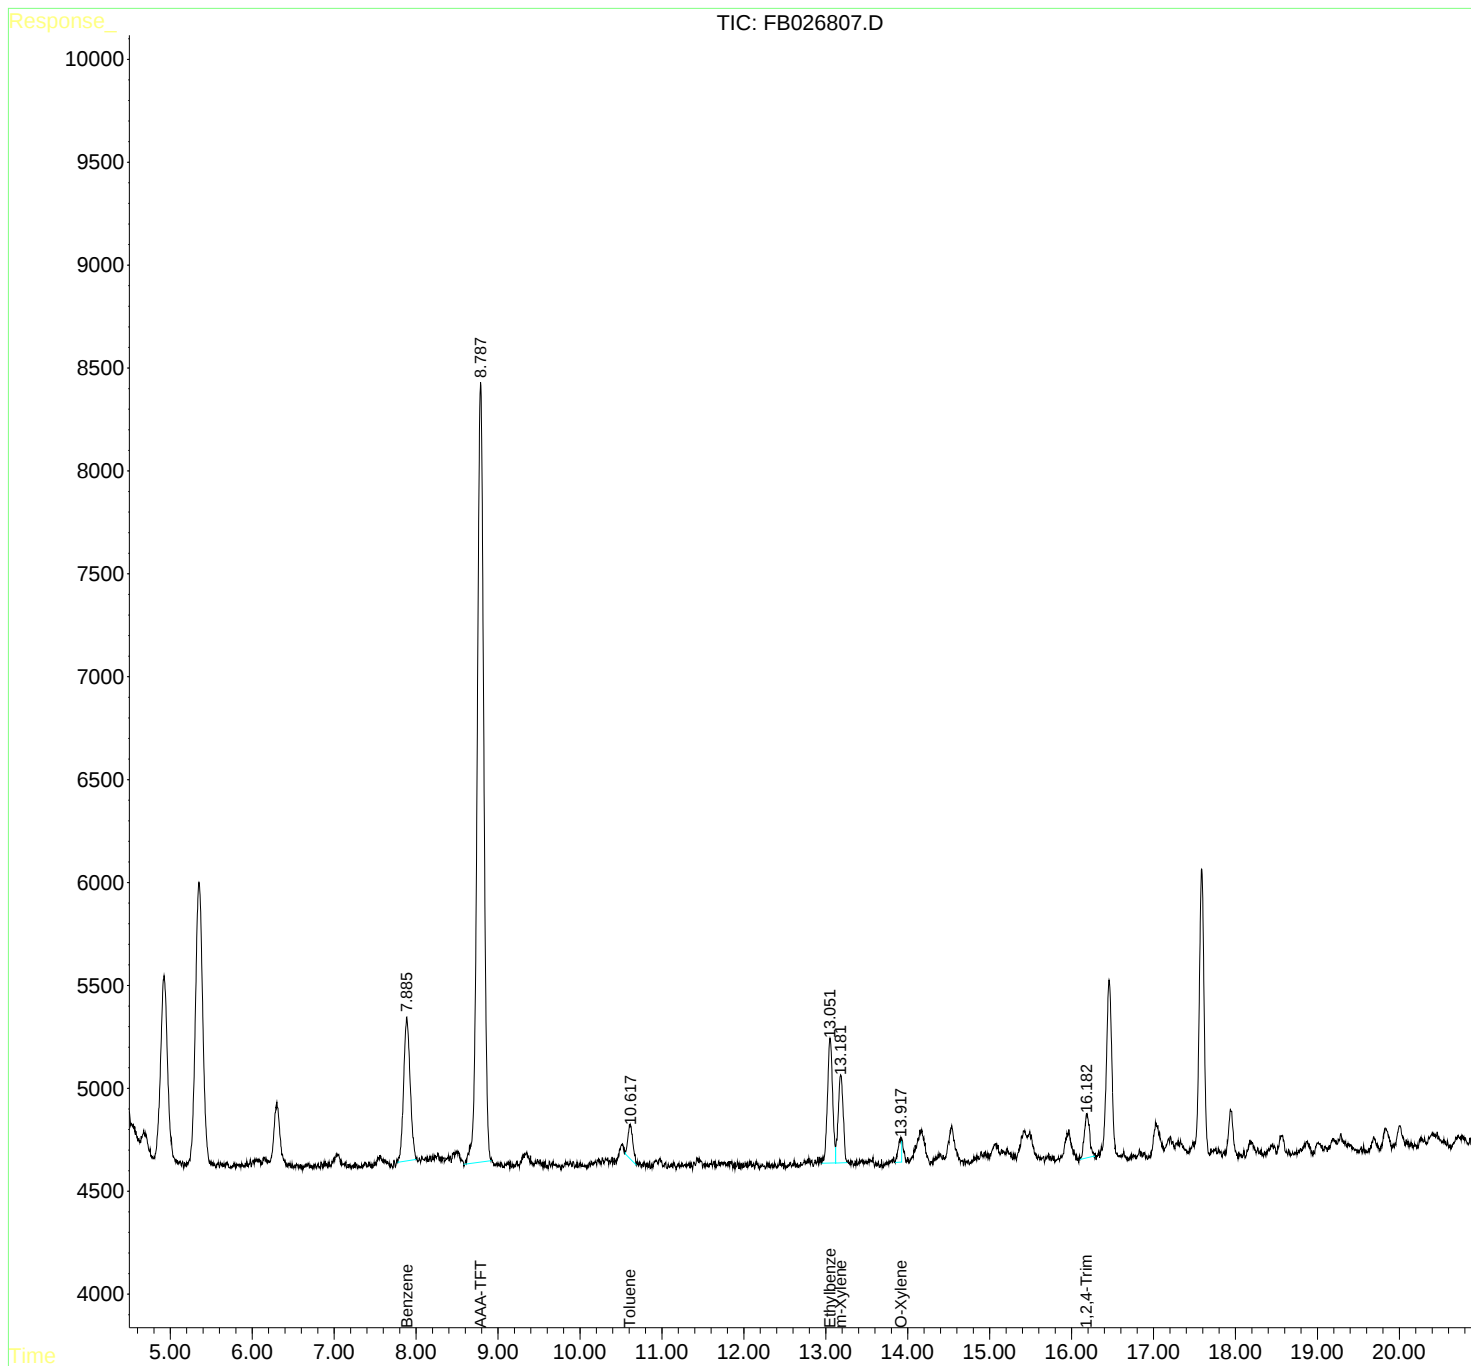


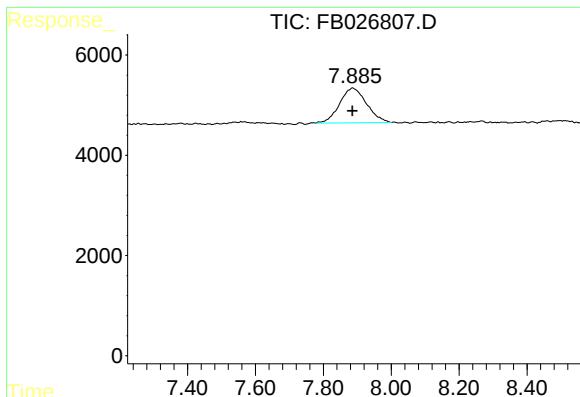

#4 Benzene


R.T.: 7.887 min
Delta R.T.: 0.001 min
Response: 38240
Conc: 1.66 ng/ml

Instrument :
FID_B
ClientSampleId :

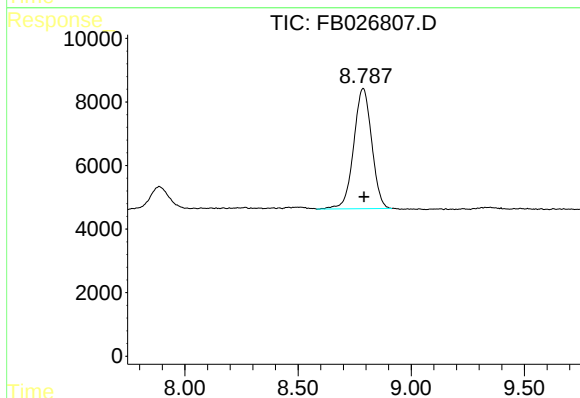


#5 AAA-TFT

R.T.: 8.789 min
Delta R.T.: -0.003 min
Response: 209066
Conc: 19.92 ng/ml

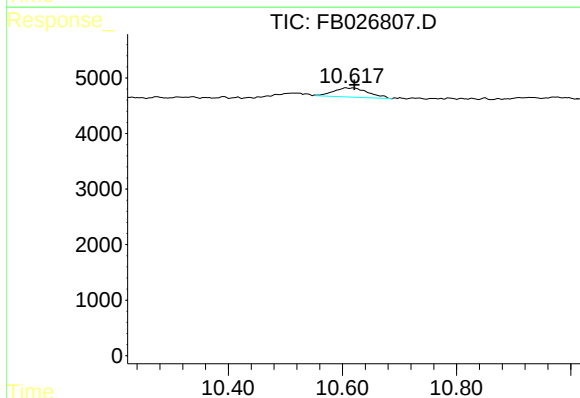


#6 Toluene

R.T.: 10.607 min
Delta R.T.: -0.014 min
Response: 6932
Conc: 0.32 ng/ml

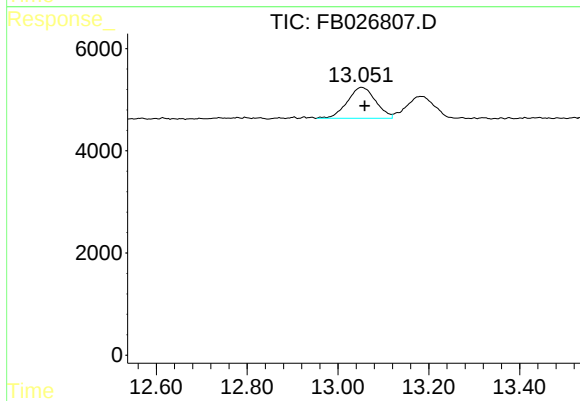

#7 Ethylbenzene


R.T.: 13.053 min
Delta R.T.: -0.006 min
Response: 26169
Conc: 1.30 ng/ml

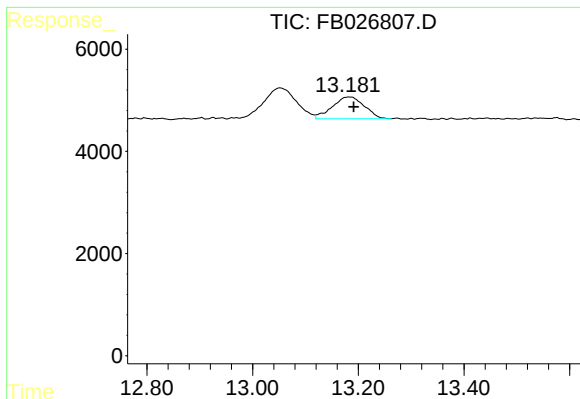

#8 m-Xylene


R.T.: 13.183 min
Delta R.T.: -0.009 min
Response: 18028
Conc: 0.89 ng/ml

Instrument :
FID_B
ClientSampleId :

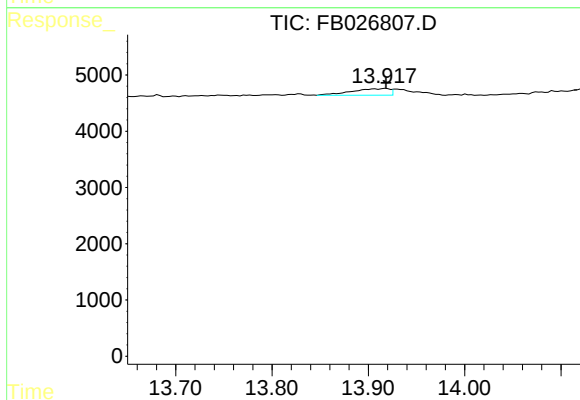

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.000 min
Response: 3152
Conc: 0.16 ng/ml

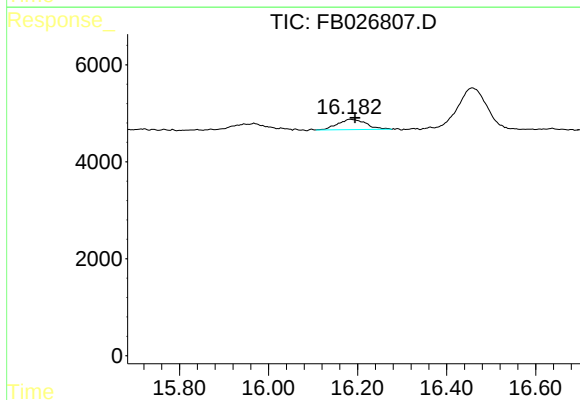

#10 1,2,4-Trimethylbenzene

R.T.: 16.183 min
Delta R.T.: -0.011 min
Response: 9439
Conc: 0.47 ng/ml