

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032322\
 Data File : FB026811.D
 Signal(s) : FID2B.CH
 Acq On : 24 Mar 2022 3:06
 Operator : AJ/MA
 Sample : 20 PPB GRO STD
 Misc :
 ALS Vial : 26 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 24 07:25:54 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	208531	19.873 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.705	443191	23.408 ng/ml
2) t 2,2,4-Trimethylpentane	7.430	509069	24.560 ng/ml
3) t n-Heptane	7.749	156388	7.901 ng/ml
4) t Benzene	7.885	224340	9.722 ng/ml
6) t Toluene	10.617	630002	28.777 ng/ml
7) t Ethylbenzene	13.054	192766	9.591 ng/ml
8) t m-Xylene	13.187	384008	19.055 ng/ml
9) t O-Xylene	13.914	379463	19.021 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	369275	18.534 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032322\
Data File : FB026811.D
Signal(s) : FID2B.CH
Acq On : 24 Mar 2022 3:06
Operator : AJ/MA
Sample : 20 PPB GRO STD
Misc :
ALS Vial : 26 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 24 07:25:54 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

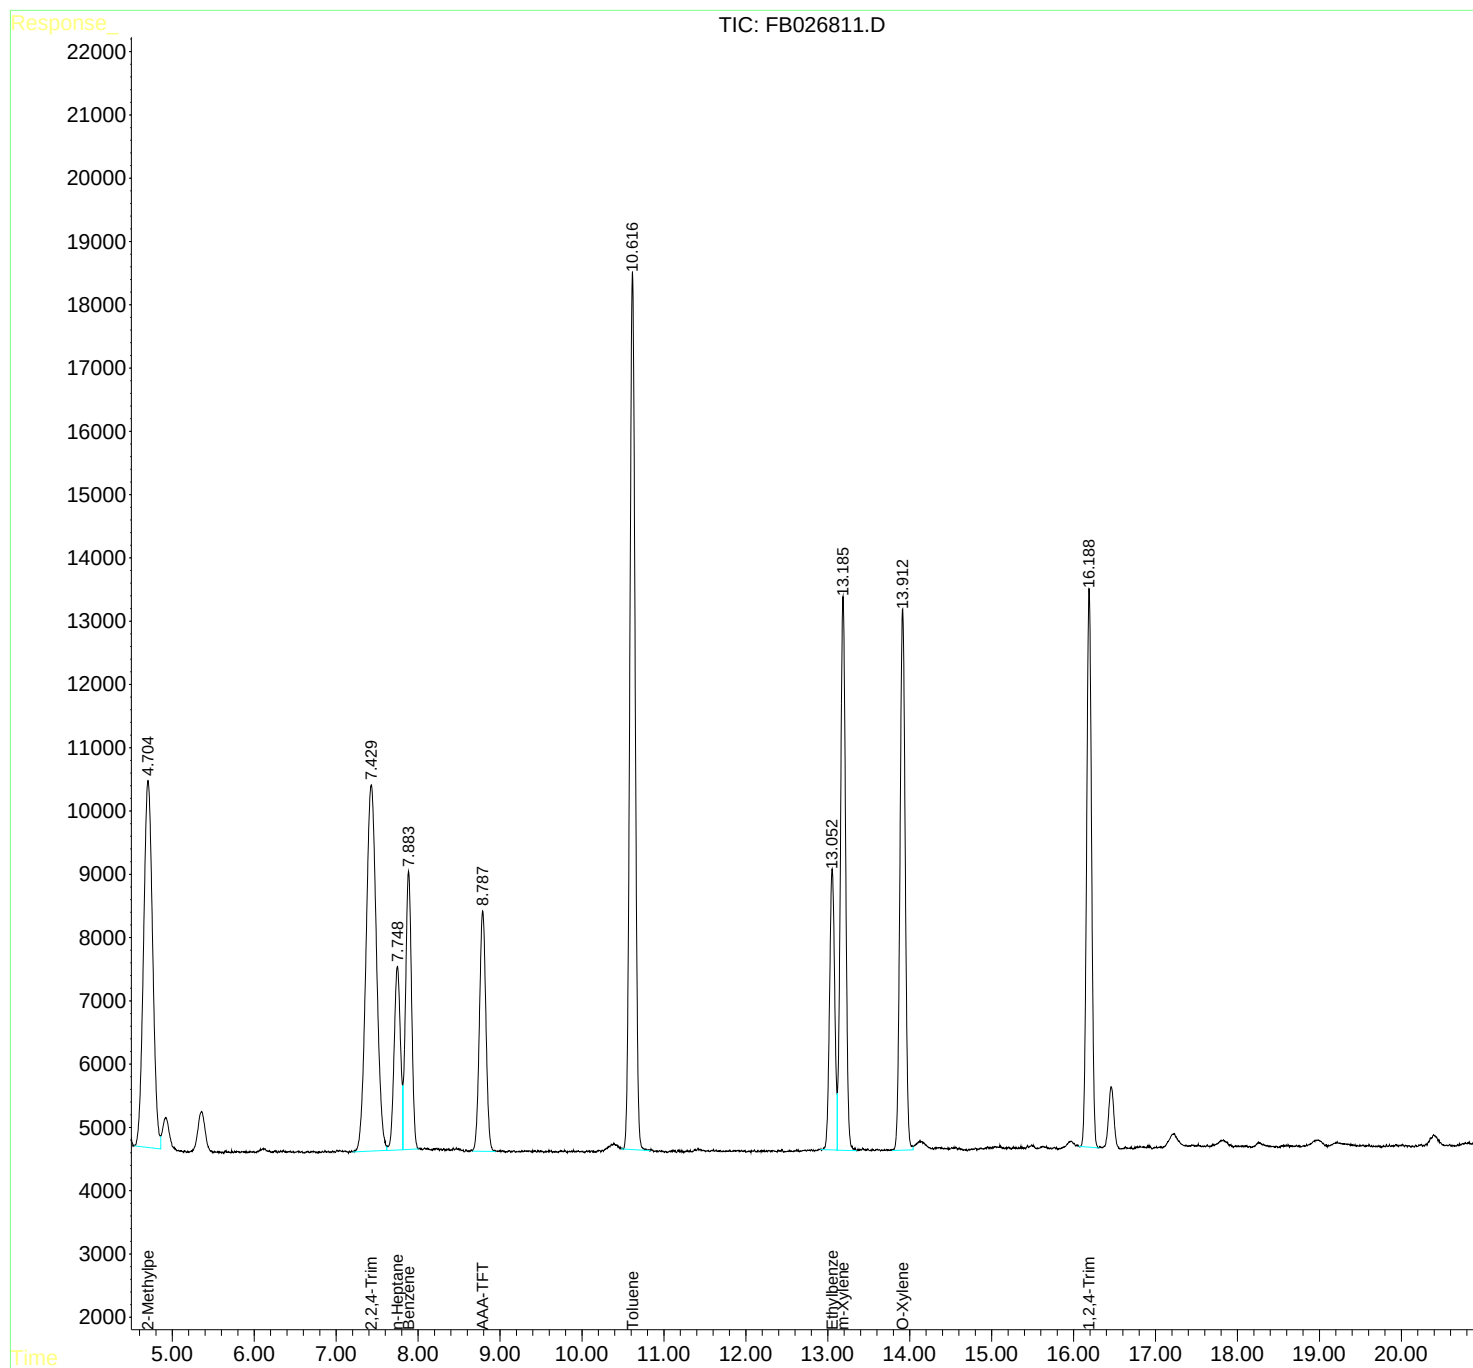


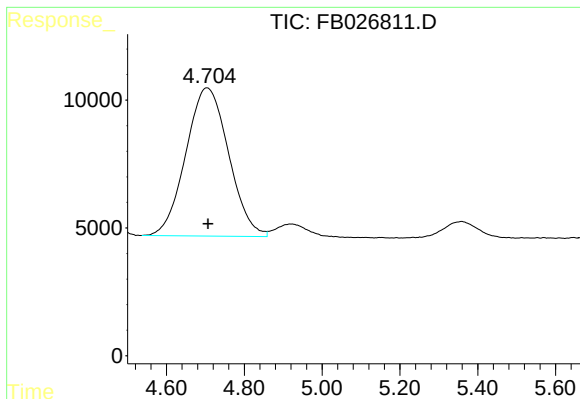

#1 2-Methylpentane


R.T.: 4.705 min
Delta R.T.: -0.002 min
Response: 443191
Conc: 23.41 ng/ml

Instrument :
FID_B
ClientSampleId :

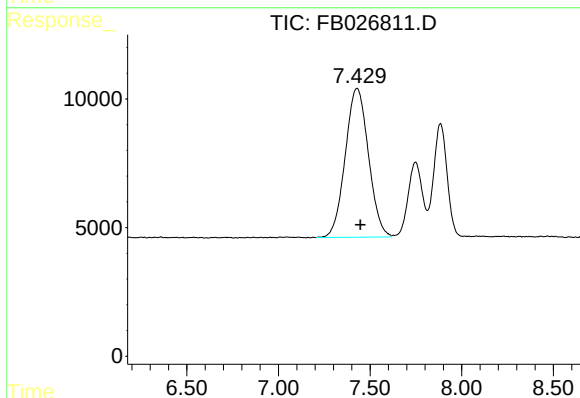


#2 2,2,4-Trimethylpentane

R.T.: 7.430 min
Delta R.T.: -0.017 min
Response: 509069
Conc: 24.56 ng/ml

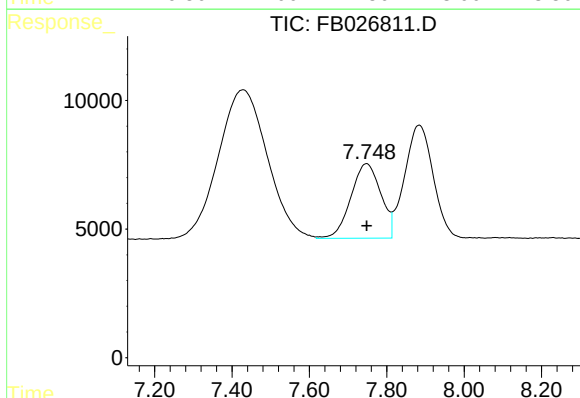


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: 0.000 min
Response: 156388
Conc: 7.90 ng/ml

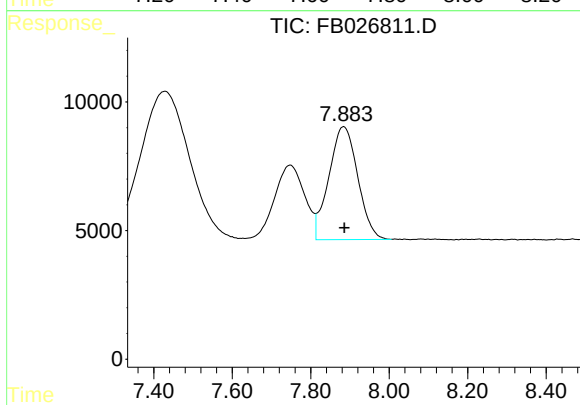

#4 Benzene


R.T.: 7.885 min
Delta R.T.: -0.001 min
Response: 224340
Conc: 9.72 ng/ml

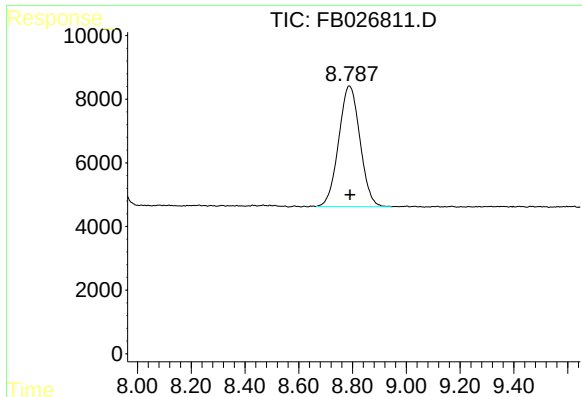

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: -0.003 min
Response: 208531
Conc: 19.87 ng/ml

Instrument :
FID_B
ClientSampleId :

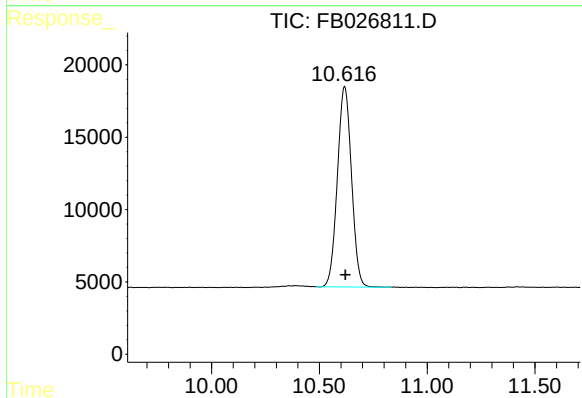


#6 Toluene

R.T.: 10.617 min
Delta R.T.: -0.004 min
Response: 630002
Conc: 28.78 ng/ml

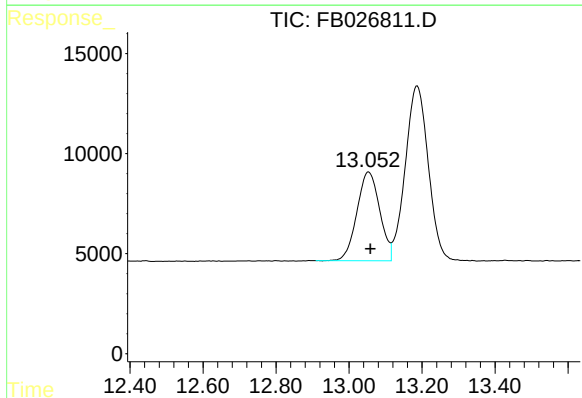


#7 Ethylbenzene

R.T.: 13.054 min
Delta R.T.: -0.005 min
Response: 192766
Conc: 9.59 ng/ml

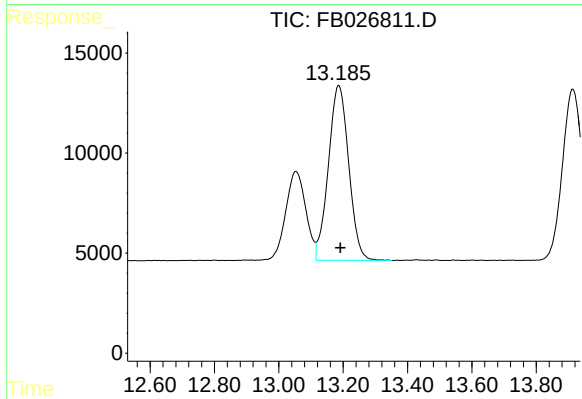

#8 m-Xylene

R.T.: 13.187 min
Delta R.T.: -0.005 min
Response: 384008
Conc: 19.05 ng/ml

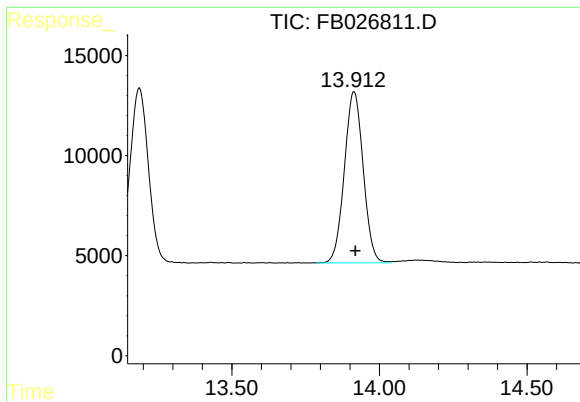


#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: -0.005 min
Response: 379463
Conc: 19.02 ng/ml

Instrument :

FID_B

ClientSampleId :

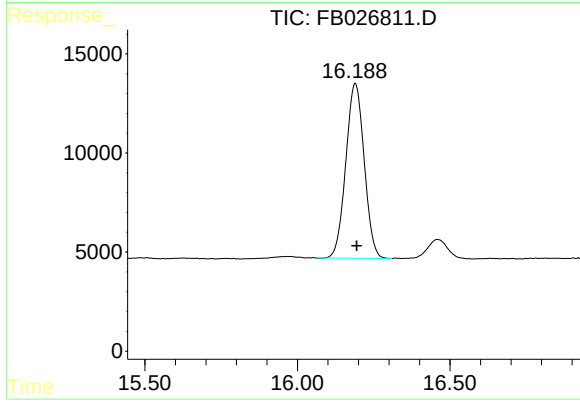

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: -0.004 min
Response: 369275
Conc: 18.53 ng/ml