

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032322\
 Data File : FB026788.D
 Signal(s) : FID2B.CH
 Acq On : 23 Mar 2022 11:47
 Operator : AJ/MA
 Sample : BSF0322S1
 Misc : 5.02G/5.00 ML DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0323S1

Integration File: Calibration.e
 Quant Time: Mar 23 16:08:16 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.787	249275	23.755 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.704	439233	23.199 ng/ml
2) t 2,2,4-Trimethylpentane	7.427	514677	24.831 ng/ml
3) t n-Heptane	7.747	158724	8.019 ng/ml
4) t Benzene	7.882	220198	9.543 ng/ml
6) t Toluene	10.615	629676	28.762 ng/ml
7) t Ethylbenzene	13.052	196850	9.795 ng/ml
8) t m-Xylene	13.185	392563	19.479 ng/ml
9) t O-Xylene	13.912	382646	19.180 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	387949	19.471 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032322\
Data File : FB026788.D
Signal(s) : FID2B.CH
Acq On : 23 Mar 2022 11:47
Operator : AJ/MA
Sample : BSF0322S1
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0323S1

Integration File: Calibration.e
Quant Time: Mar 23 16:08:16 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

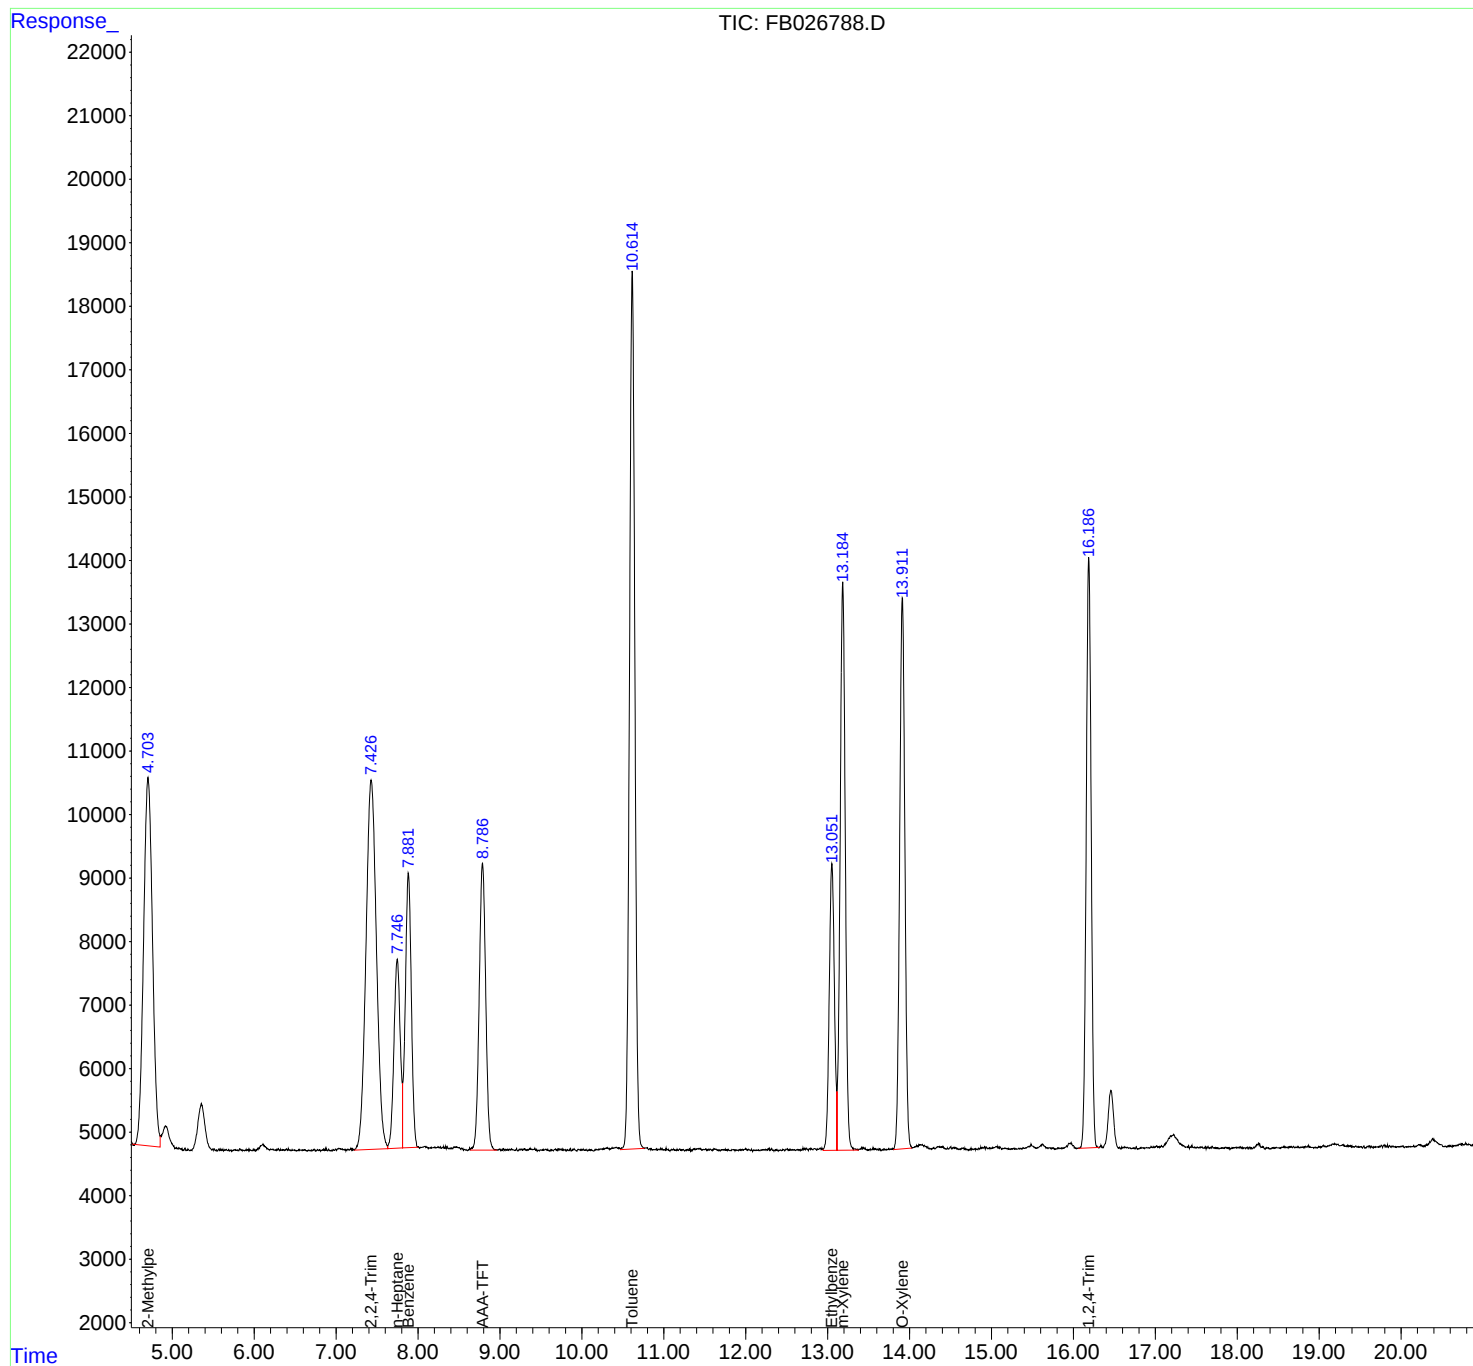


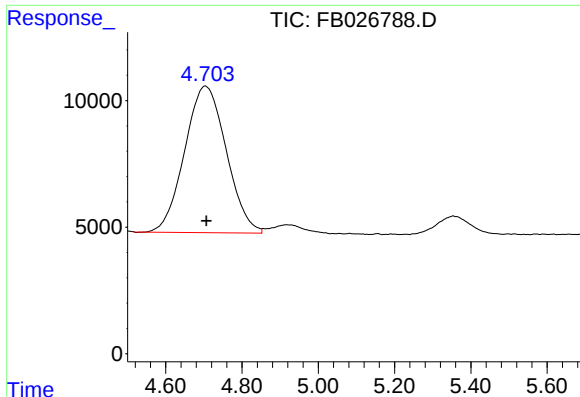

#1 2-Methylpentane


R.T.: 4.704 min
Delta R.T.: -0.003 min
Response: 439233
Conc: 23.20 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0323S1

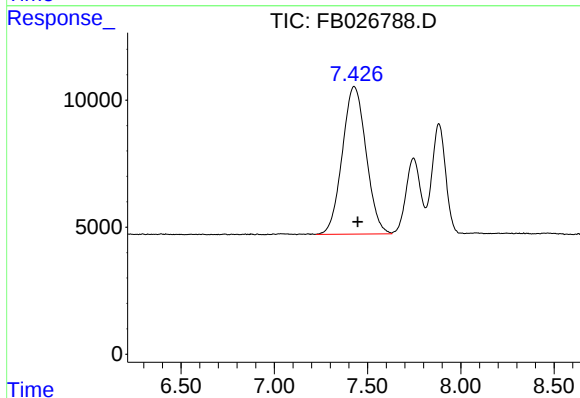


#2 2,2,4-Trimethylpentane

R.T.: 7.427 min
Delta R.T.: -0.020 min
Response: 514677
Conc: 24.83 ng/ml

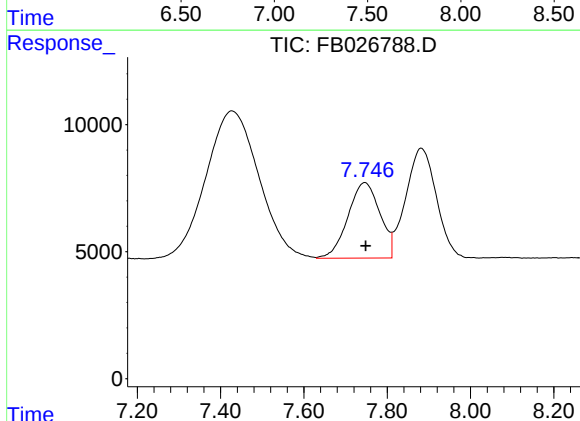


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: -0.002 min
Response: 158724
Conc: 8.02 ng/ml

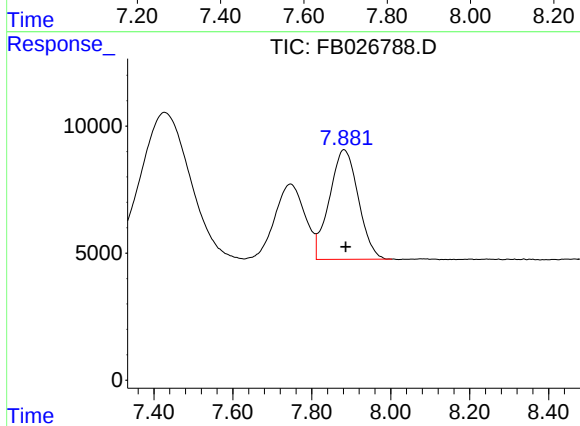

#4 Benzene


R.T.: 7.882 min
Delta R.T.: -0.004 min
Response: 220198
Conc: 9.54 ng/ml

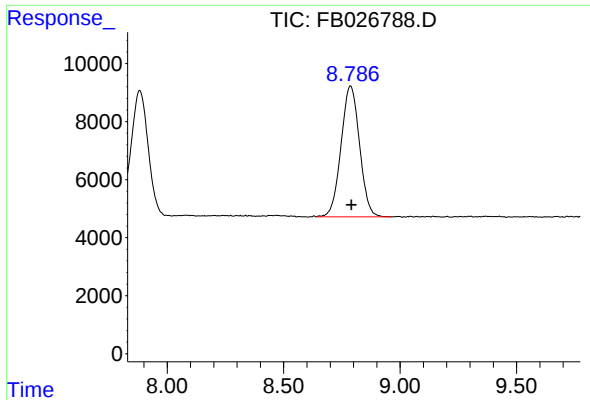

#5 AAA-TFT


R.T.: 8.787 min
Delta R.T.: -0.004 min
Response: 249275
Conc: 23.76 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0323S1

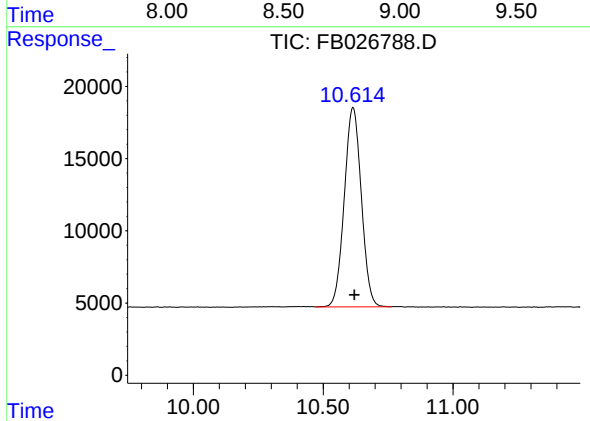


#6 Toluene

R.T.: 10.615 min
Delta R.T.: -0.006 min
Response: 629676
Conc: 28.76 ng/ml

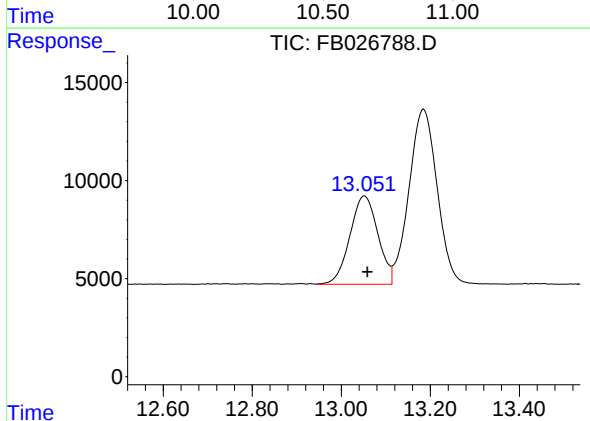


#7 Ethylbenzene

R.T.: 13.052 min
Delta R.T.: -0.007 min
Response: 196850
Conc: 9.79 ng/ml

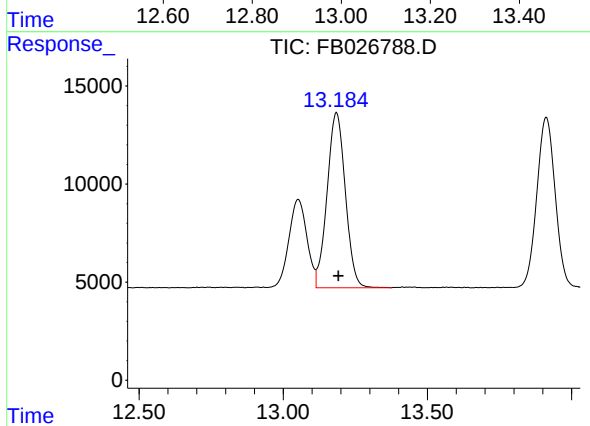

#8 m-Xylene


R.T.: 13.185 min
Delta R.T.: -0.007 min
Response: 392563
Conc: 19.48 ng/ml

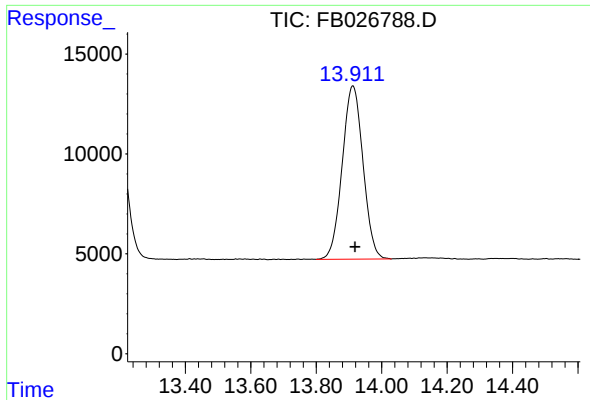

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: -0.006 min
Response: 382646
Conc: 19.18 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0323S1

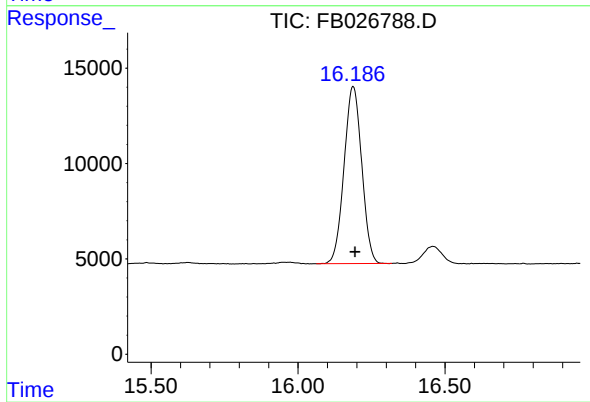

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: -0.006 min
Response: 387949
Conc: 19.47 ng/ml