

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032322\
 Data File : FB026791.D
 Signal(s) : FID2B.CH
 Acq On : 23 Mar 2022 13:41
 Operator : AJ/MA
 Sample : N1974-01
 Misc : 5.06G/5.00 ML DI WATER
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 G-5-11-25-26

Integration File: Calibration.e
 Quant Time: Mar 23 16:08:35 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	11185	1.066 ng/ml
Target Compounds			
4) t Benzene	7.890	17456	0.757 ng/ml
7) t Ethylbenzene	13.051	12611	0.627 ng/ml
8) t m-Xylene	13.173	222	0.011 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032322\
Data File : FB026791.D
Signal(s) : FID2B.CH
Acq On : 23 Mar 2022 13:41
Operator : AJ/MA
Sample : N1974-01
Misc : 5.06G/5.00 ML DI WATER
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
G-5-11-25-26

Integration File: Calibration.e
Quant Time: Mar 23 16:08:35 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

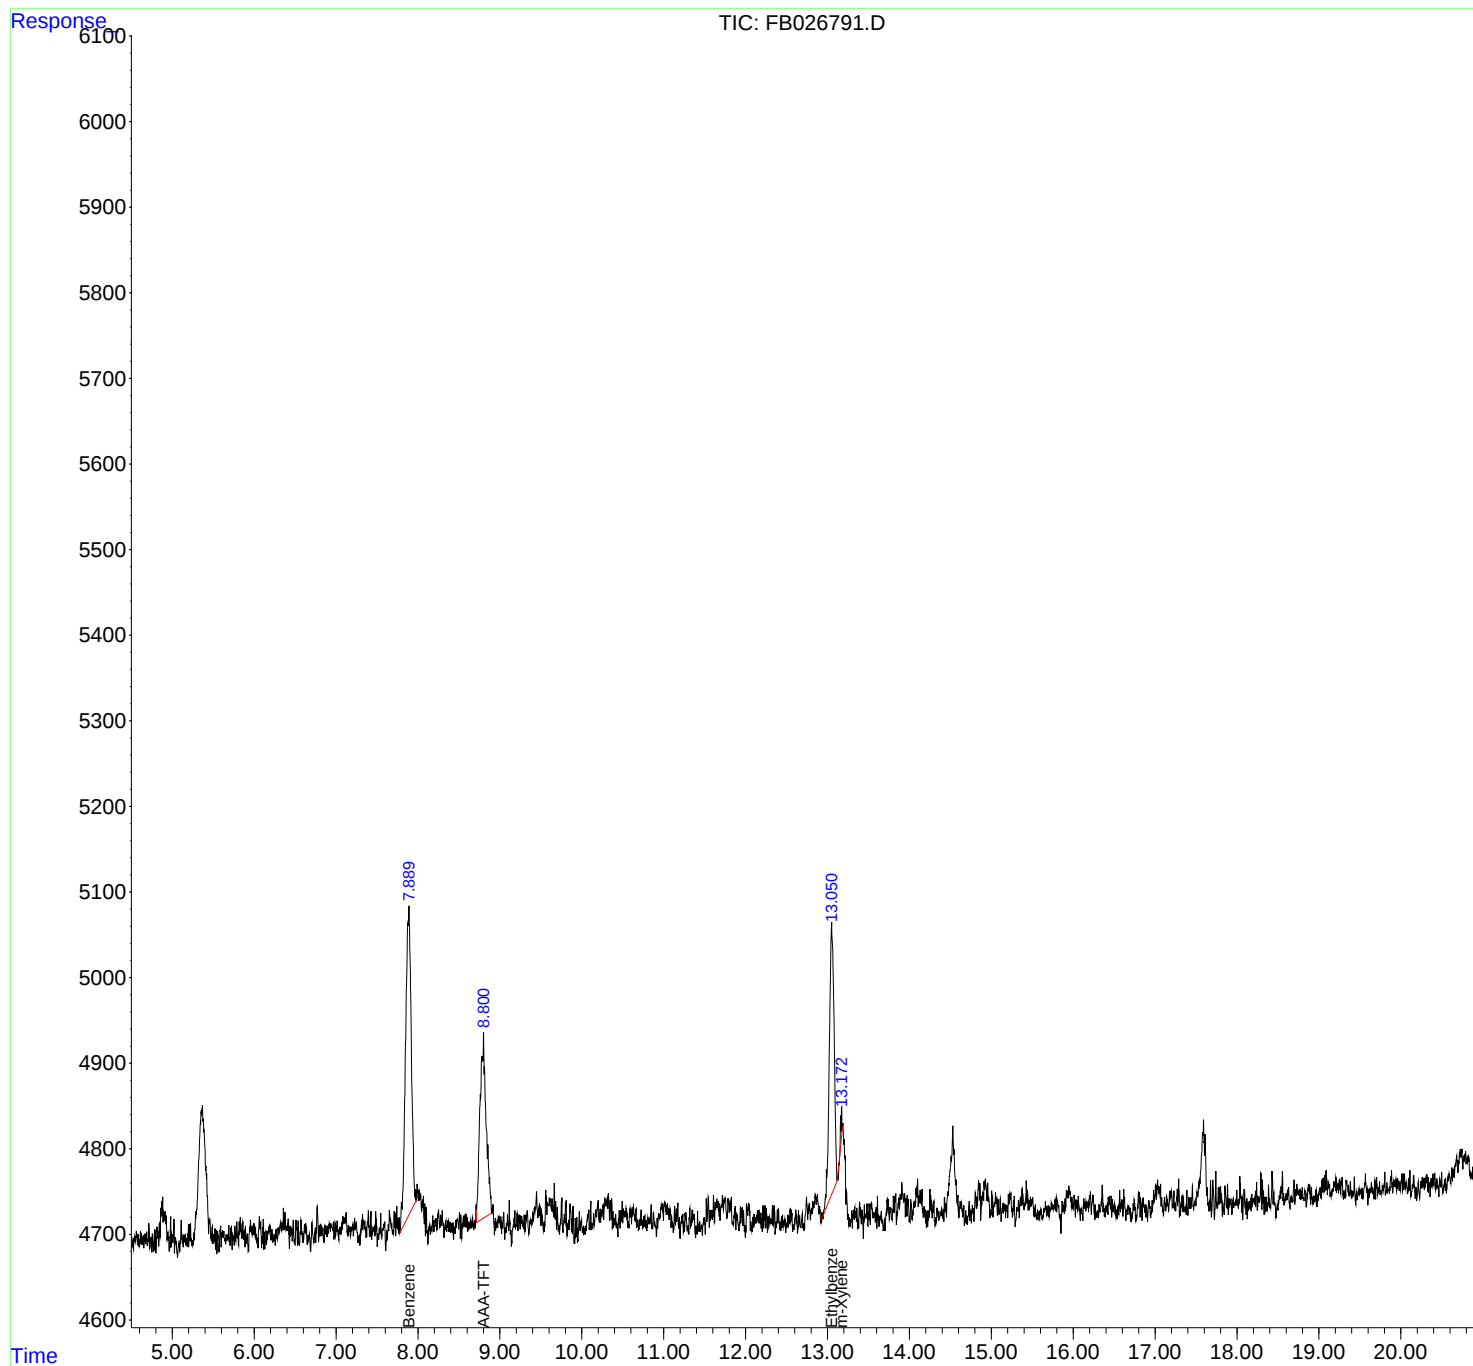


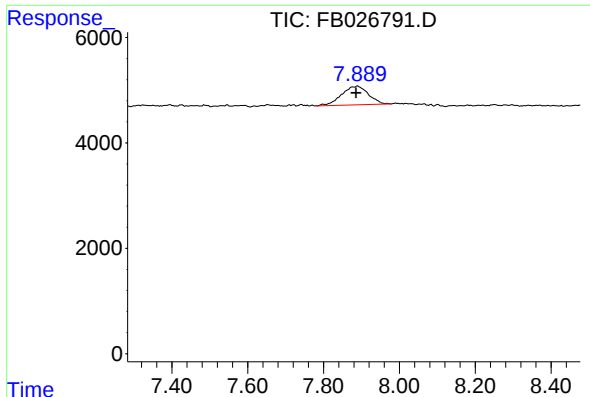

#4 Benzene


R.T.: 7.890 min
Delta R.T.: 0.005 min
Response: 17456
Conc: 0.76 ng/ml

Instrument :
FID_B
ClientSampleId :
G-5-11-25-26

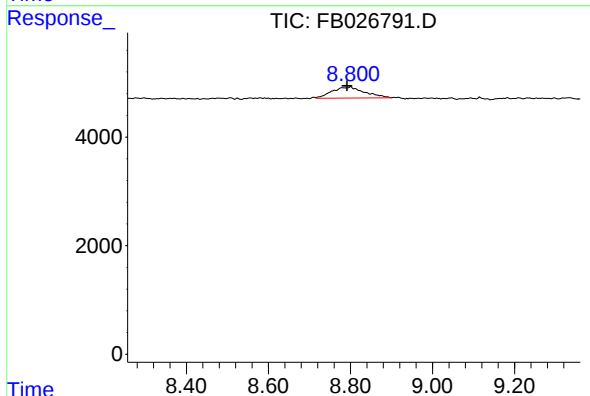


#5 AAA-TFT

R.T.: 8.801 min
Delta R.T.: 0.010 min
Response: 11185
Conc: 1.07 ng/ml

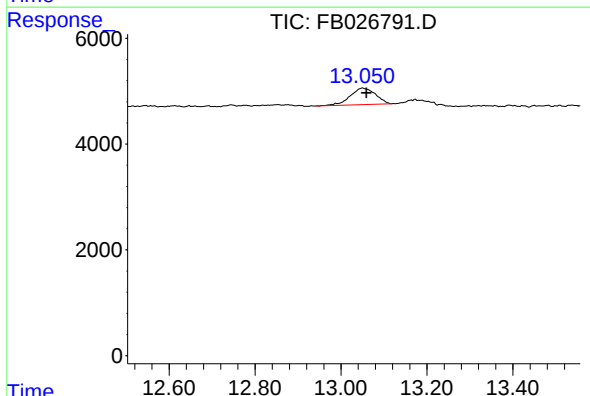

#7 Ethylbenzene

R.T.: 13.051 min
Delta R.T.: -0.008 min
Response: 12611
Conc: 0.63 ng/ml

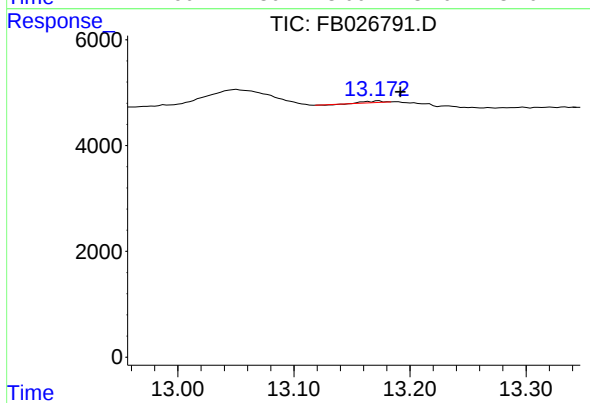

#8 m-Xylene

R.T.: 13.173 min
Delta R.T.: -0.018 min
Response: 222
Conc: 0.01 ng/ml