

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032322\
 Data File : FB026804.D
 Signal(s) : FID2B.CH
 Acq On : 23 Mar 2022 21:57
 Operator : AJ/MA
 Sample : N1995-08MS
 Misc : 5.02G/5.00 ML DI WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB-08-COMPMS

Integration File: Calibration.e
 Quant Time: Mar 24 07:24:55 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	229732	21.893 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.705	419851	22.175 ng/ml
2) t 2,2,4-Trimethylpentane	7.429	487870	23.537 ng/ml
3) t n-Heptane	7.748	149129	7.534 ng/ml
4) t Benzene	7.884	216120	9.366 ng/ml
6) t Toluene	10.618	606349	27.696 ng/ml
7) t Ethylbenzene	13.053	190605	9.484 ng/ml
8) t m-Xylene	13.187	373112	18.514 ng/ml
9) t O-Xylene	13.913	364420	18.267 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	362677	18.203 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032322\
Data File : FB026804.D
Signal(s) : FID2B.CH
Acq On : 23 Mar 2022 21:57
Operator : AJ/MA
Sample : N1995-08MS
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-08-COMPMS

Integration File: Calibration.e
Quant Time: Mar 24 07:24:55 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

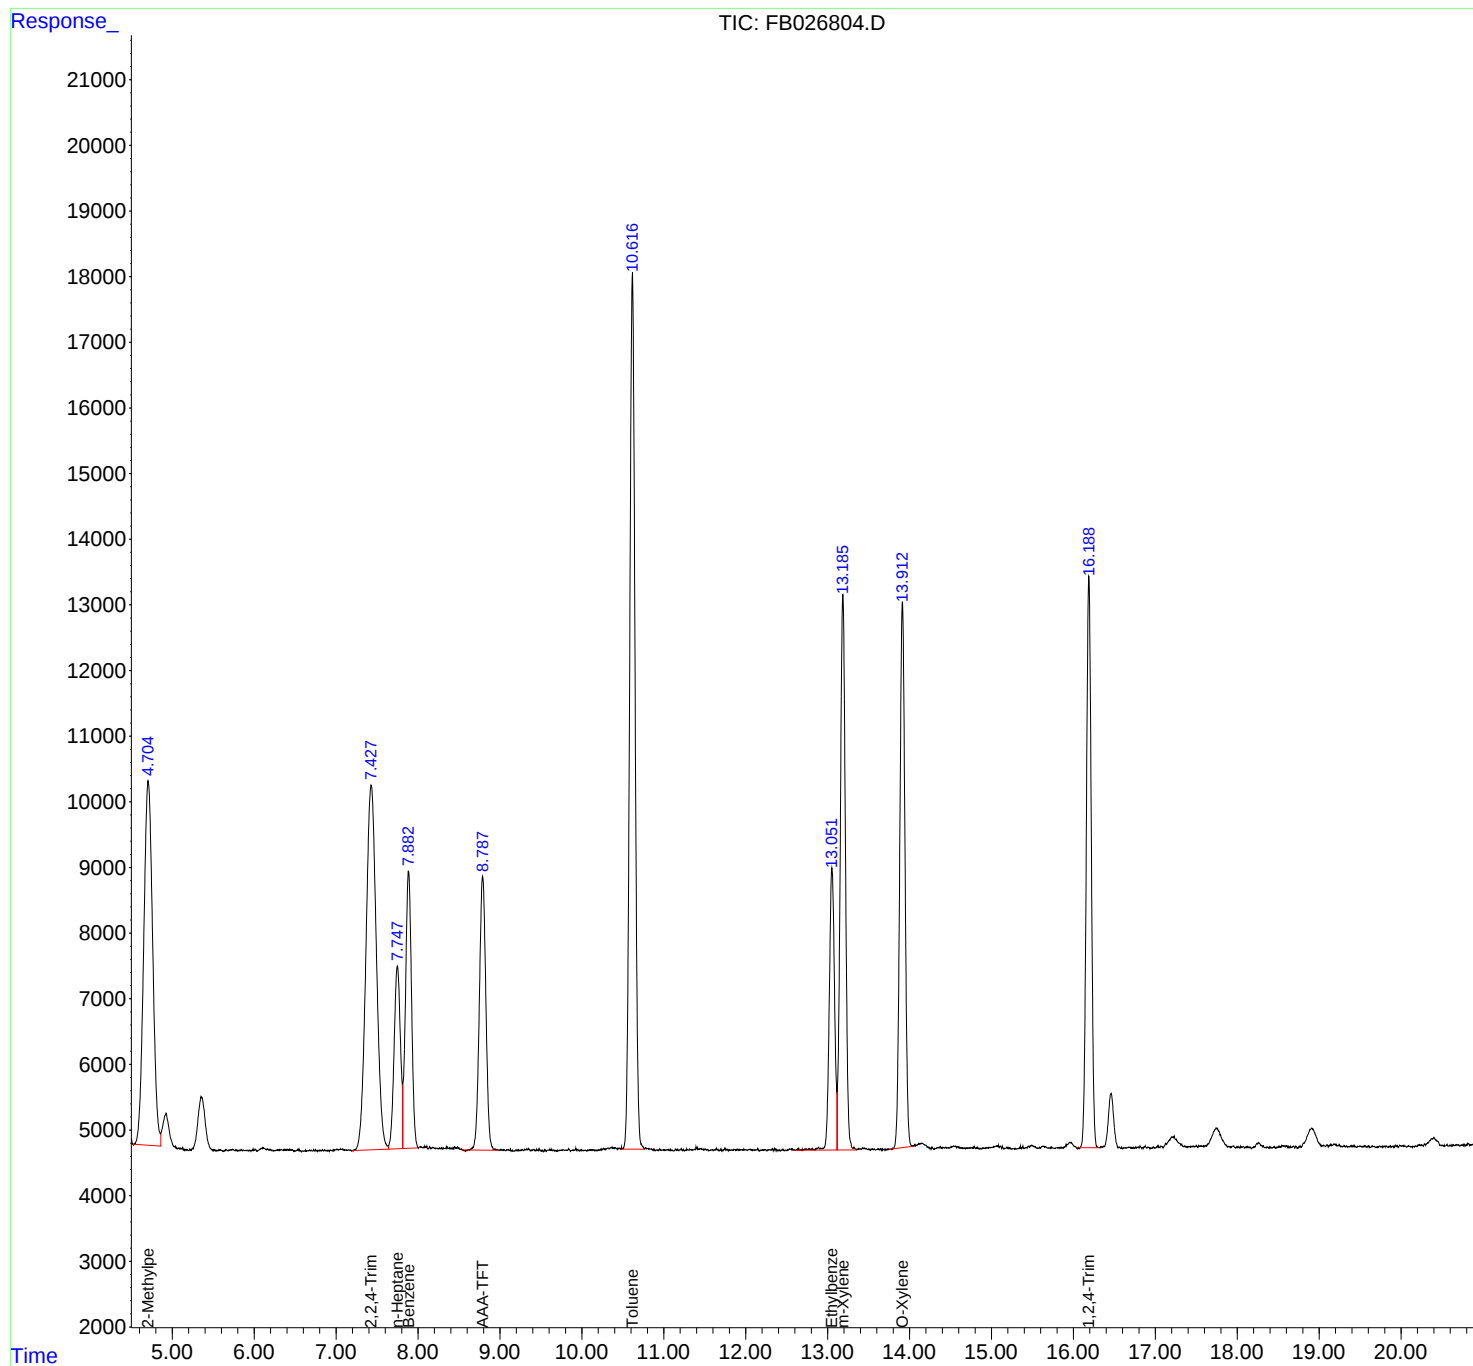


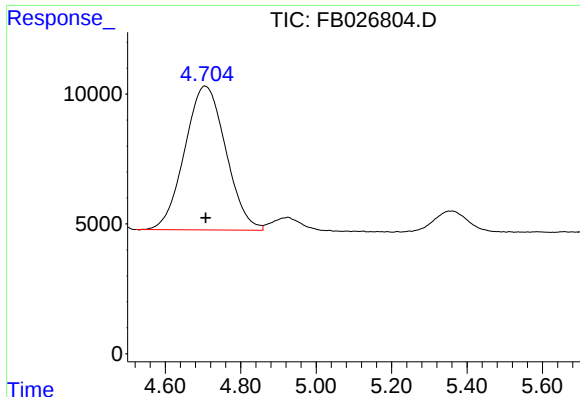

#1 2-Methylpentane


R.T.: 4.705 min
Delta R.T.: -0.002 min
Response: 419851
Conc: 22.18 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-08-COMPMS

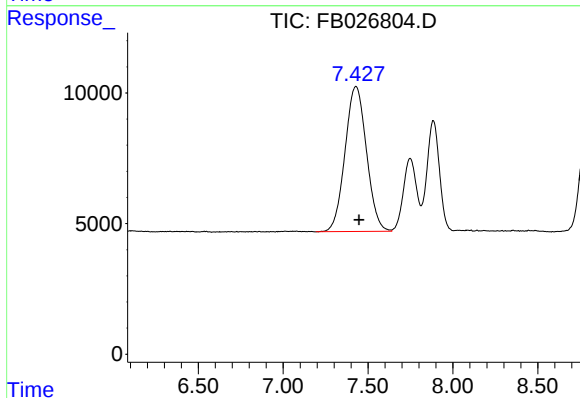


#2 2,2,4-Trimethylpentane

R.T.: 7.429 min
Delta R.T.: -0.018 min
Response: 487870
Conc: 23.54 ng/ml

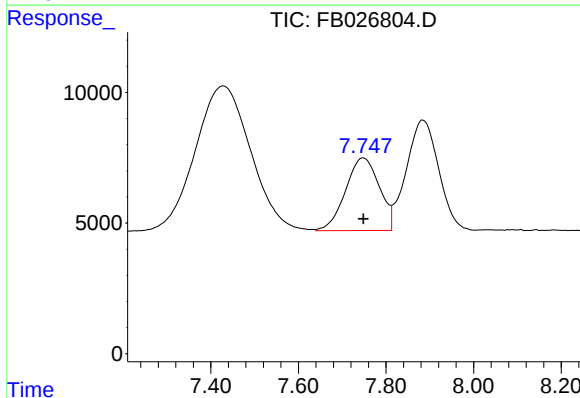


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: 0.000 min
Response: 149129
Conc: 7.53 ng/ml

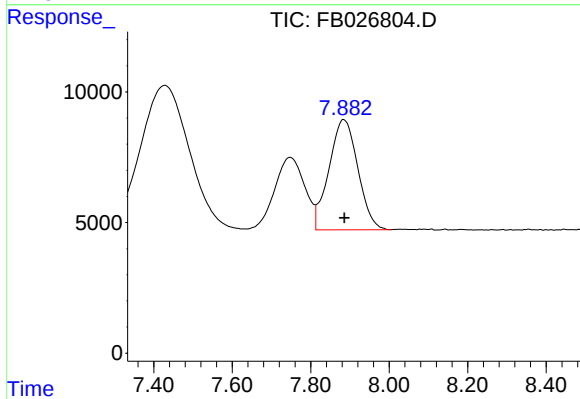

#4 Benzene


R.T.: 7.884 min
Delta R.T.: -0.002 min
Response: 216120
Conc: 9.37 ng/ml

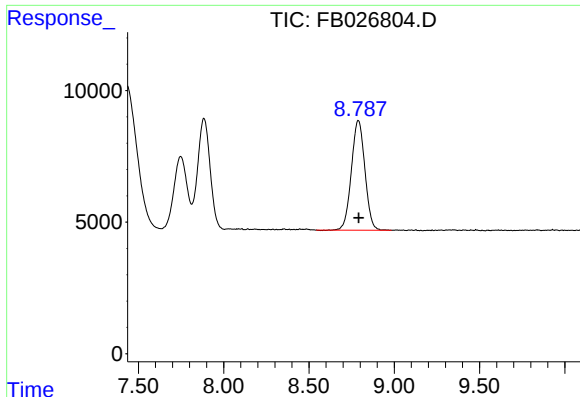

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: -0.003 min
Response: 229732
Conc: 21.89 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-08-COMPMS

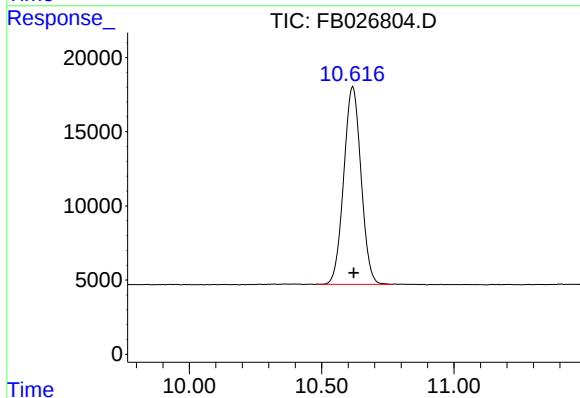


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.003 min
Response: 606349
Conc: 27.70 ng/ml

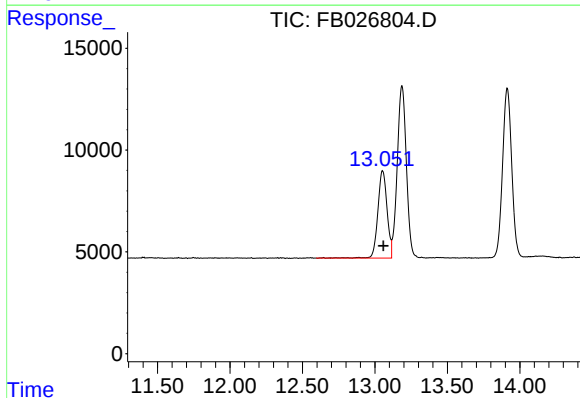


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: -0.006 min
Response: 190605
Conc: 9.48 ng/ml

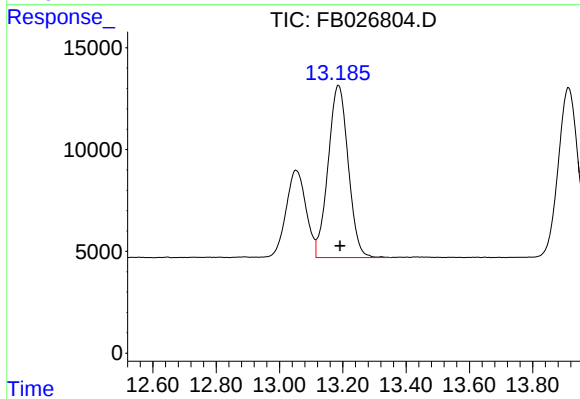

#8 m-Xylene


R.T.: 13.187 min
Delta R.T.: -0.005 min
Response: 373112
Conc: 18.51 ng/ml

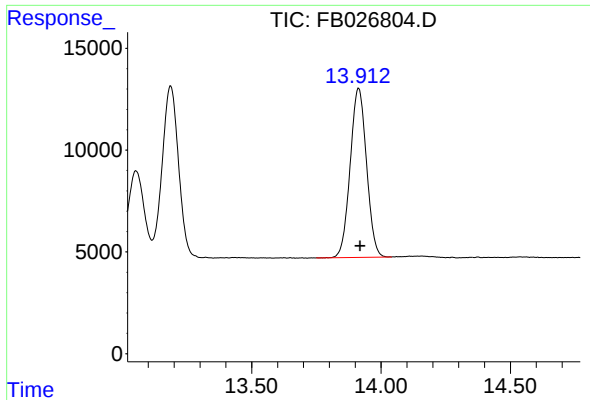

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: -0.005 min
Response: 364420
Conc: 18.27 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-08-COMPMS

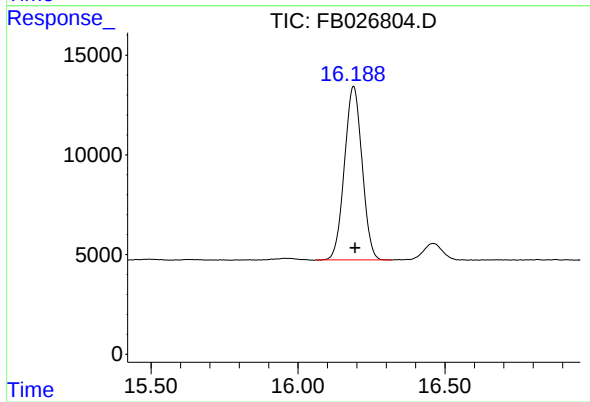

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: -0.005 min
Response: 362677
Conc: 18.20 ng/ml