

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032322\
 Data File : FB026805.D
 Signal(s) : FID2B.CH
 Acq On : 23 Mar 2022 22:36
 Operator : AJ/MA
 Sample : N1995-08MSD
 Misc : 5.05G/5.00 ML DI WATER
 ALS Vial : 20 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 SB-08-COMPMSD

Integration File: Calibration.e
 Quant Time: Mar 24 07:25:04 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	217995	20.774 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.707	422251	22.302 ng/ml
2) t 2,2,4-Trimethylpentane	7.430	496201	23.939 ng/ml
3) t n-Heptane	7.746	146152	7.384 ng/ml
4) t Benzene	7.883	210470	9.121 ng/ml
6) t Toluene	10.616	593043	27.089 ng/ml
7) t Ethylbenzene	13.053	183545	9.133 ng/ml
8) t m-Xylene	13.186	368293	18.275 ng/ml
9) t O-Xylene	13.913	365102	18.301 ng/ml
10) t 1,2,4-Trimethylbenzene	16.189	373766	18.759 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032322\
Data File : FB026805.D
Signal(s) : FID2B.CH
Acq On : 23 Mar 2022 22:36
Operator : AJ/MA
Sample : N1995-08MSD
Misc : 5.05G/5.00 ML DI WATER
ALS Vial : 20 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
SB-08-COMPMSD

Integration File: Calibration.e
Quant Time: Mar 24 07:25:04 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

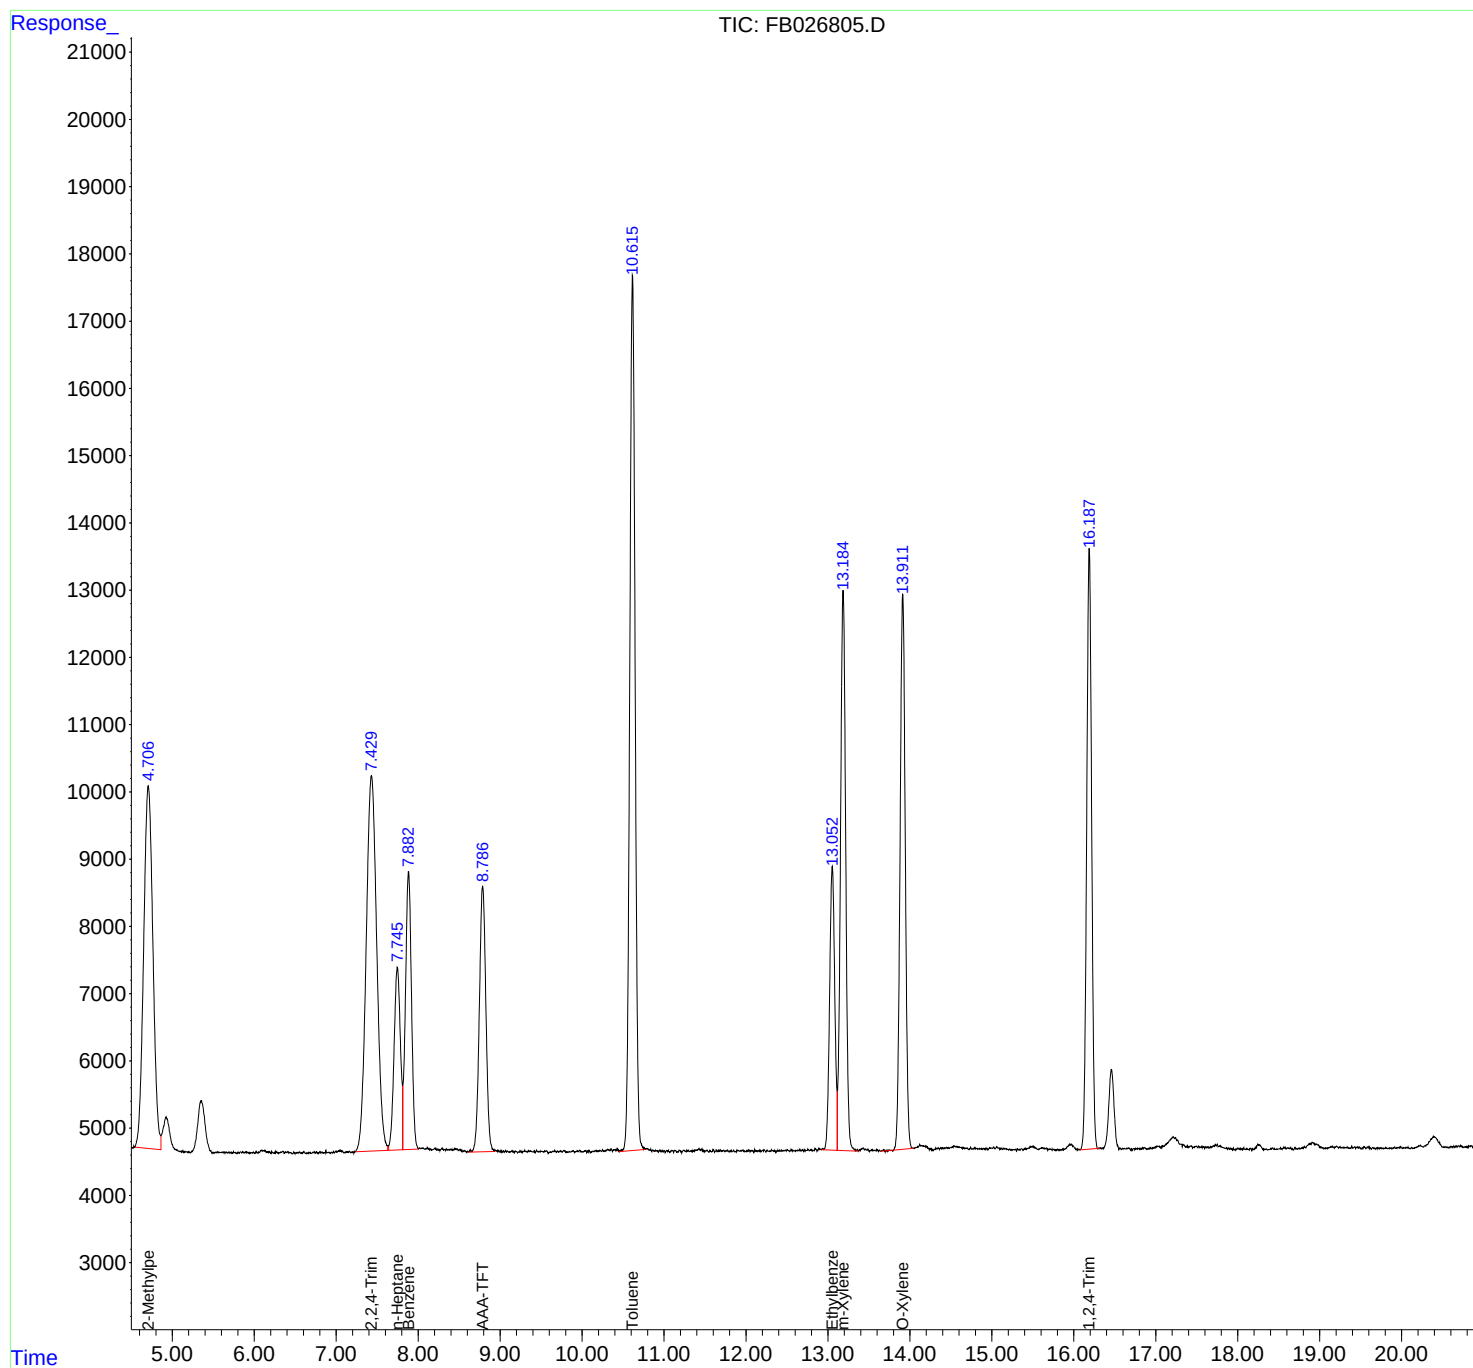


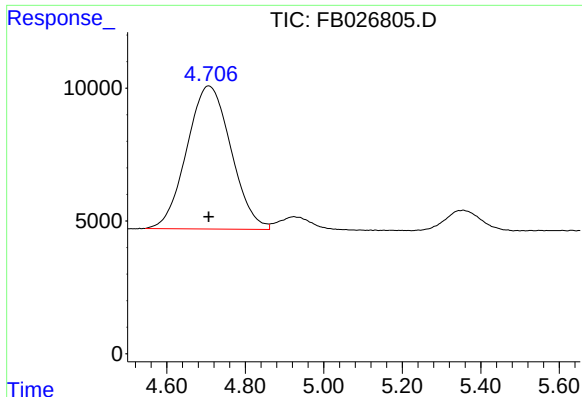

#1 2-Methylpentane


R.T.: 4.707 min
Delta R.T.: 0.000 min
Response: 422251
Conc: 22.30 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-08-COMPMSD

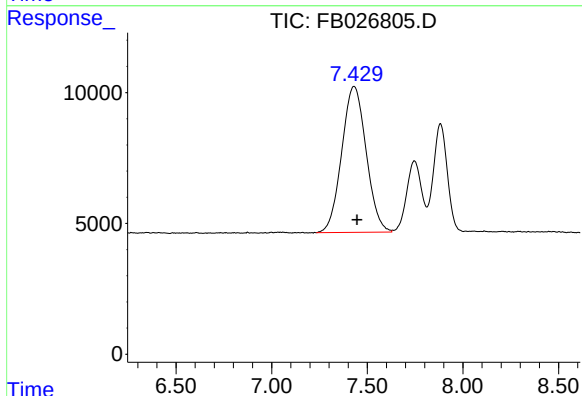


#2 2,2,4-Trimethylpentane

R.T.: 7.430 min
Delta R.T.: -0.017 min
Response: 496201
Conc: 23.94 ng/ml

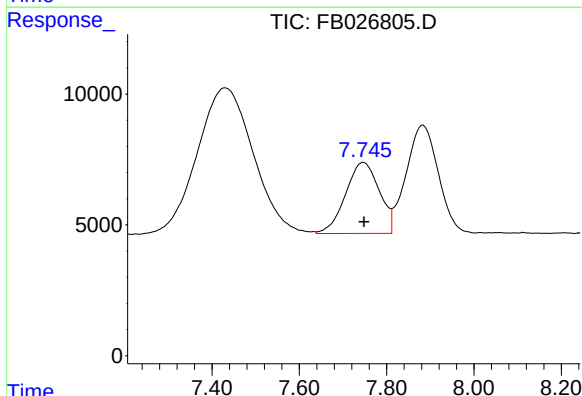


#3 n-Heptane

R.T.: 7.746 min
Delta R.T.: -0.002 min
Response: 146152
Conc: 7.38 ng/ml

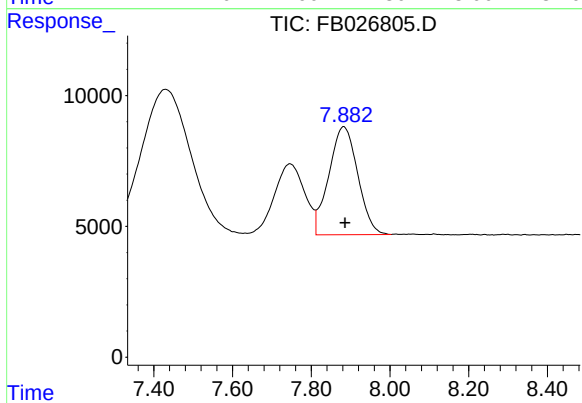

#4 Benzene


R.T.: 7.883 min
Delta R.T.: -0.003 min
Response: 210470
Conc: 9.12 ng/ml

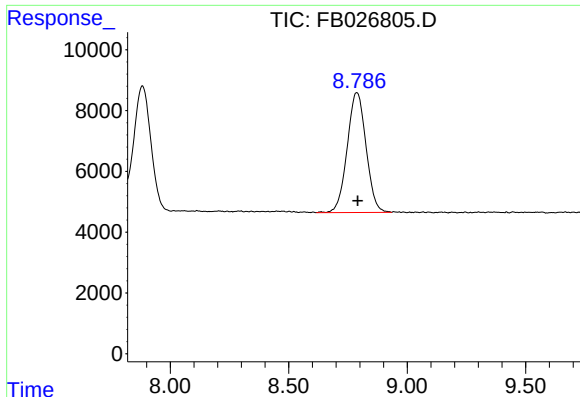

#5 AAA-TFT


R.T.: 8.788 min
Delta R.T.: -0.004 min
Response: 217995
Conc: 20.77 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-08-COMPMSD

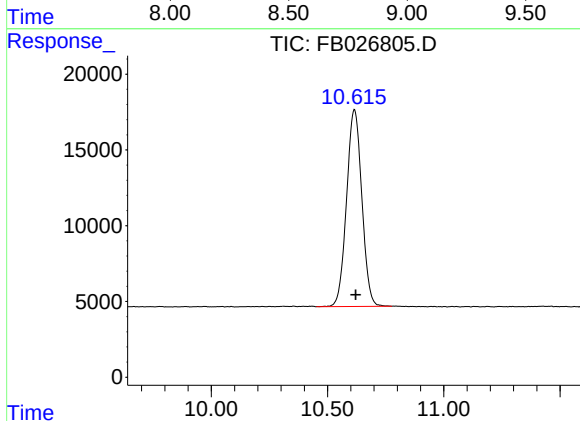


#6 Toluene

R.T.: 10.616 min
Delta R.T.: -0.005 min
Response: 593043
Conc: 27.09 ng/ml

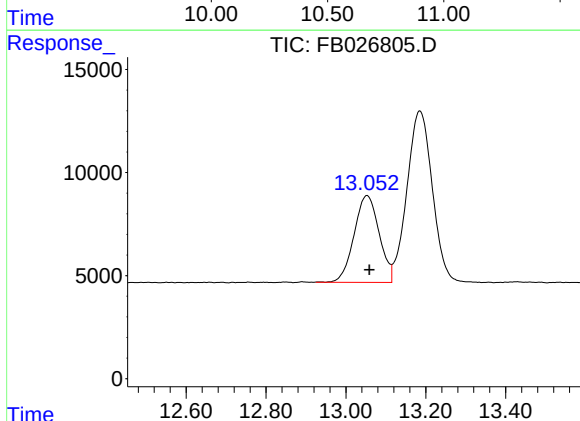


#7 Ethylbenzene

R.T.: 13.053 min
Delta R.T.: -0.005 min
Response: 183545
Conc: 9.13 ng/ml

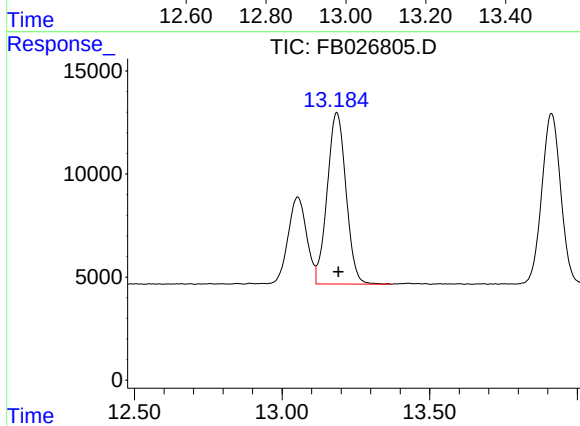

#8 m-Xylene


R.T.: 13.186 min
Delta R.T.: -0.006 min
Response: 368293
Conc: 18.28 ng/ml

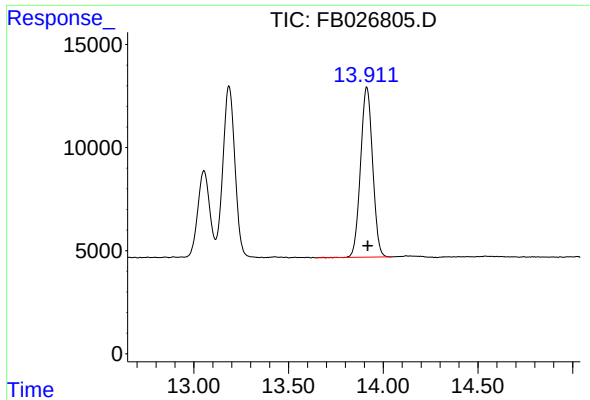

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: -0.005 min
Response: 365102
Conc: 18.30 ng/ml

Instrument :
FID_B
ClientSampleId :
SB-08-COMPMSD

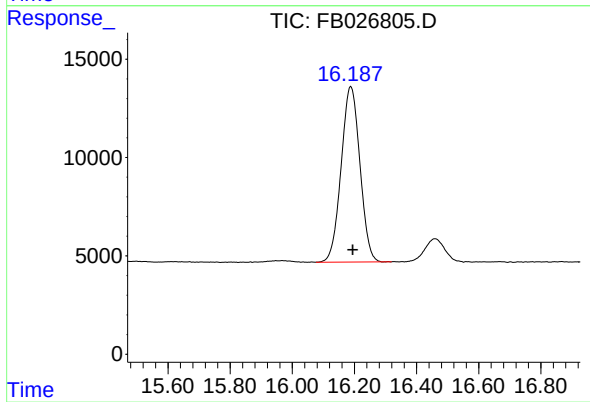

#10 1,2,4-Trimethylbenzene

R.T.: 16.189 min
Delta R.T.: -0.005 min
Response: 373766
Conc: 18.76 ng/ml