

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032323\
 Data File : FB029554.D
 Signal(s) : FID2B.CH
 Acq On : 23 Mar 2023 9:58
 Operator : YP/AJ
 Sample : 50 GRO STD
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 23 11:06:25 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
 Quant Title :
 QLast Update : Thu Mar 23 10:30:22 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	725959	51.687 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.710	1357339	84.094 ng/ml
2) t 2,2,4-Trimethylpentane	7.423	1502788	86.480 ng/ml
3) t n-Heptane	7.751	538944	29.605 ng/ml
4) t Benzene	7.888	623696	29.906 ng/ml
6) t Toluene	10.621	1839315	89.718 ng/ml
7) t Ethylbenzene	13.057	563147	28.760 ng/ml
8) t m-Xylene	13.190	1111019	57.247 ng/ml
9) t O-Xylene	13.917	1055175	55.547 ng/ml
10) t 1,2,4-Trimethylbenzene	16.192	964933	50.578 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032323\
Data File : FB029554.D
Signal(s) : FID2B.CH
Acq On : 23 Mar 2023 9:58
Operator : YP/AJ
Sample : 50 GRO STD
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 23 11:06:25 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
Quant Title :
QLast Update : Thu Mar 23 10:30:22 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

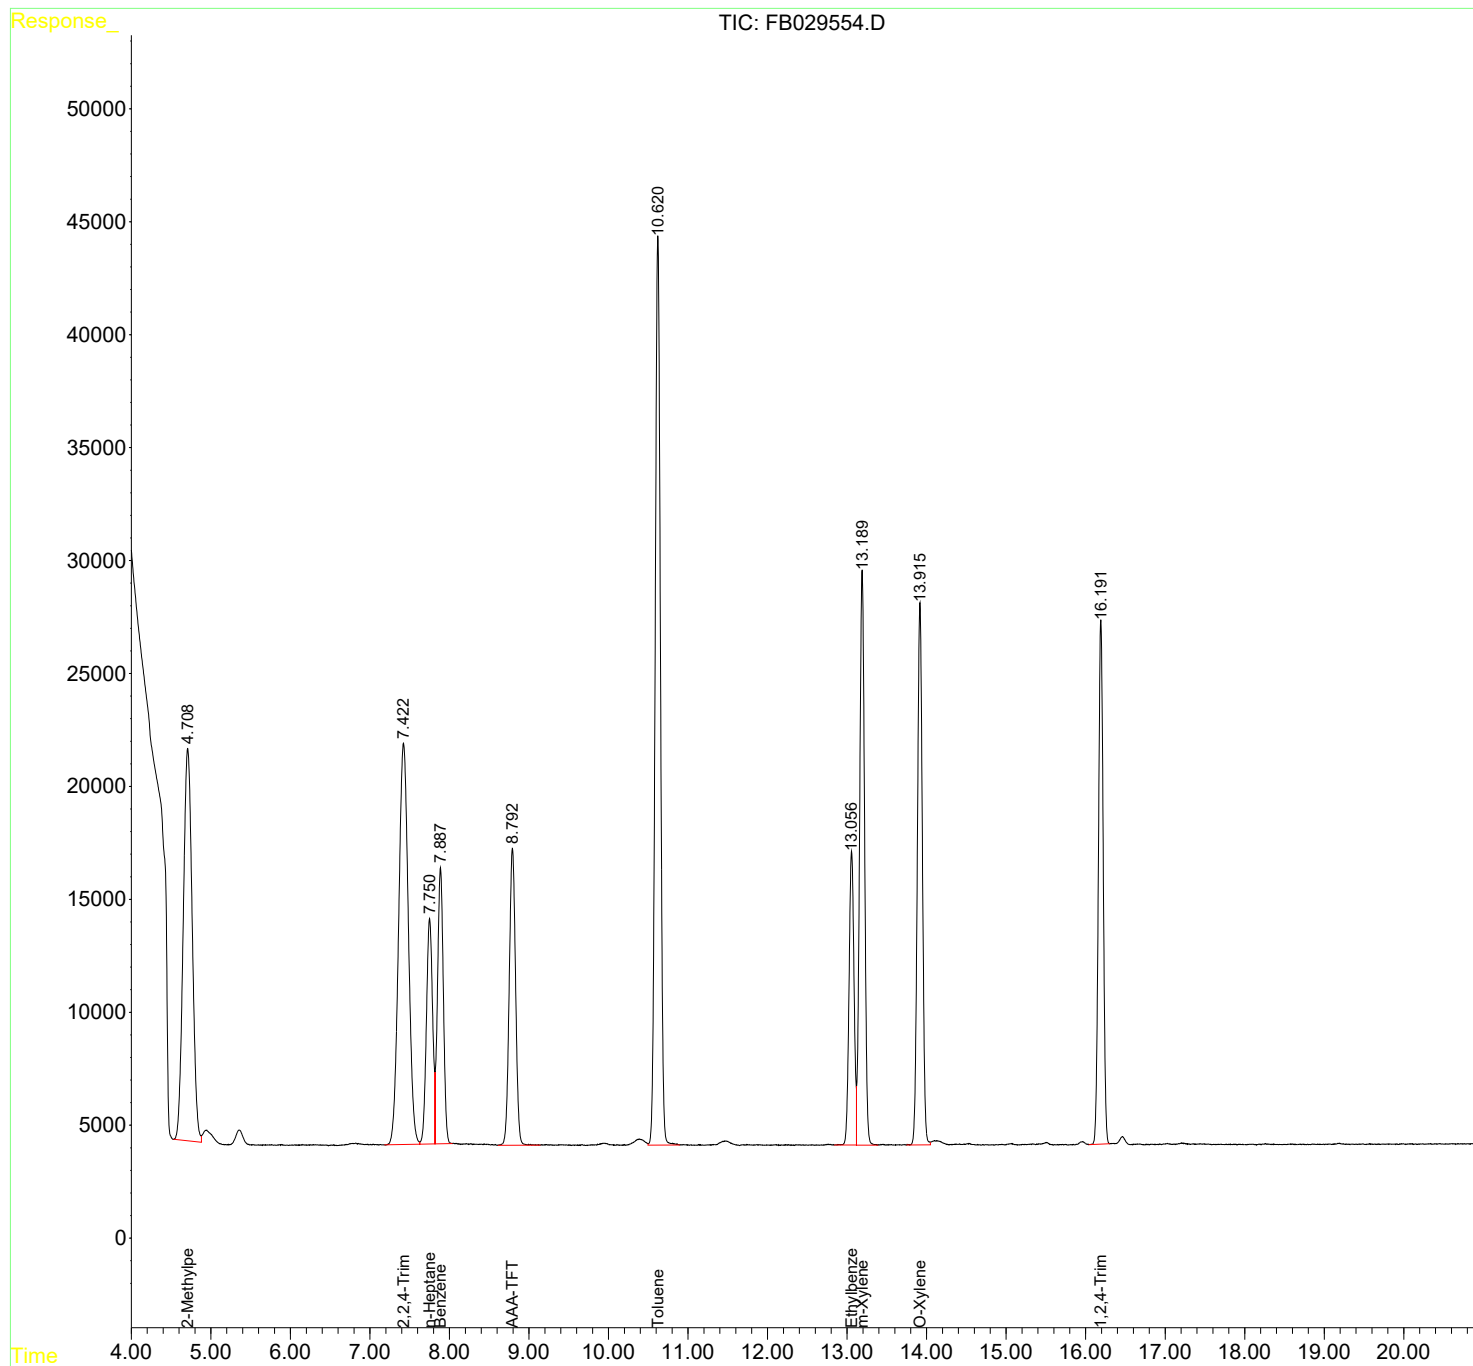


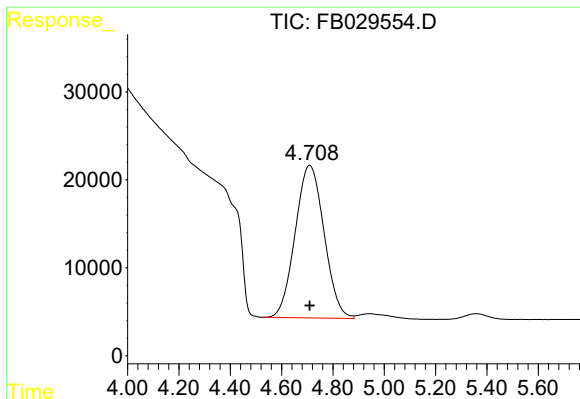

#1 2-Methylpentane


R.T.: 4.710 min
Delta R.T.: 0.000 min
Response: 1357339
Conc: 84.09 ng/ml

Instrument :
FID_B
ClientSampleId :

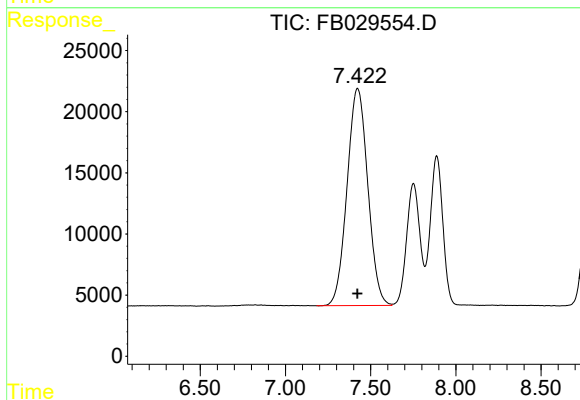


#2 2,2,4-Trimethylpentane

R.T.: 7.423 min
Delta R.T.: 0.000 min
Response: 1502788
Conc: 86.48 ng/ml

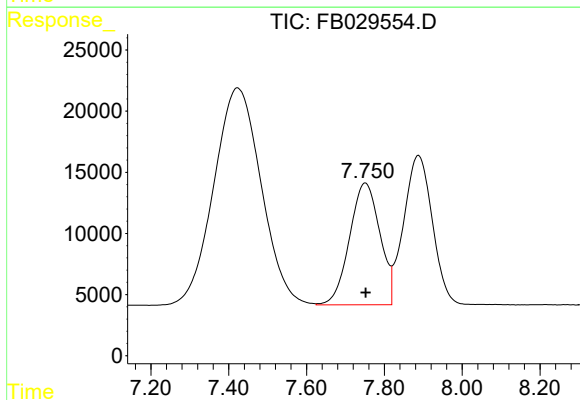


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: -0.001 min
Response: 538944
Conc: 29.60 ng/ml

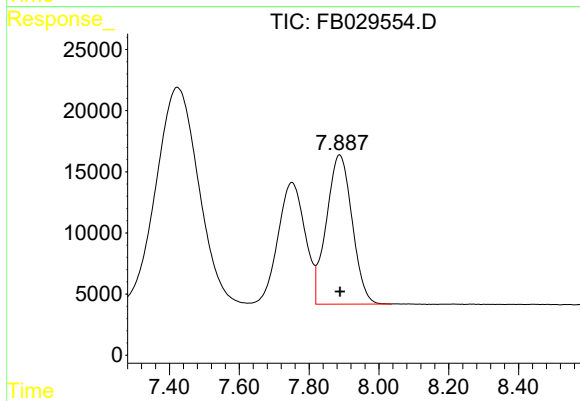

#4 Benzene


R.T.: 7.888 min
Delta R.T.: -0.001 min
Response: 623696
Conc: 29.91 ng/ml

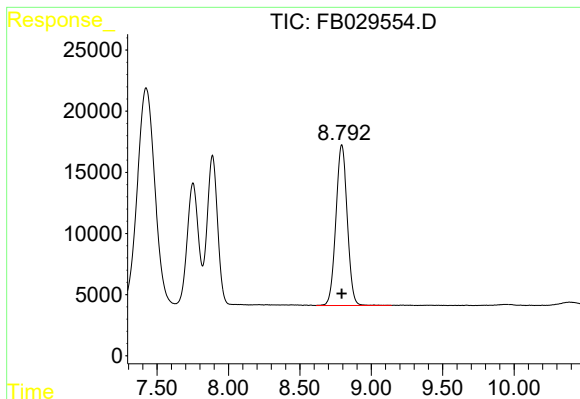

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.000 min
Response: 725959
Conc: 51.69 ng/ml

Instrument :
FID_B
ClientSampleId :

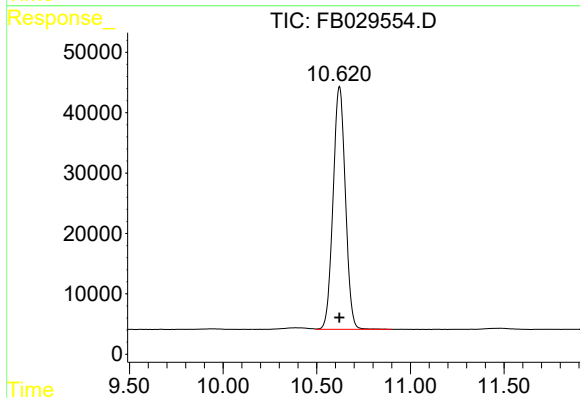


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.000 min
Response: 1839315
Conc: 89.72 ng/ml

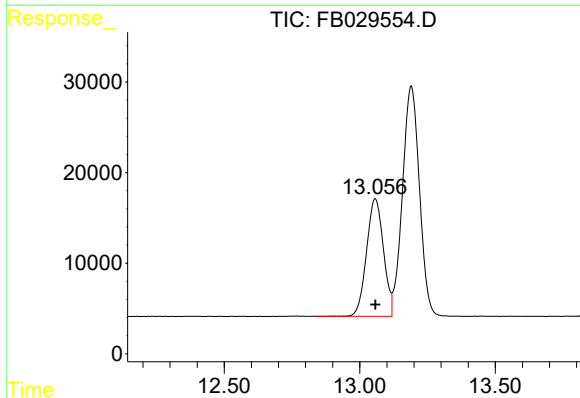


#7 Ethylbenzene

R.T.: 13.057 min
Delta R.T.: 0.000 min
Response: 563147
Conc: 28.76 ng/ml

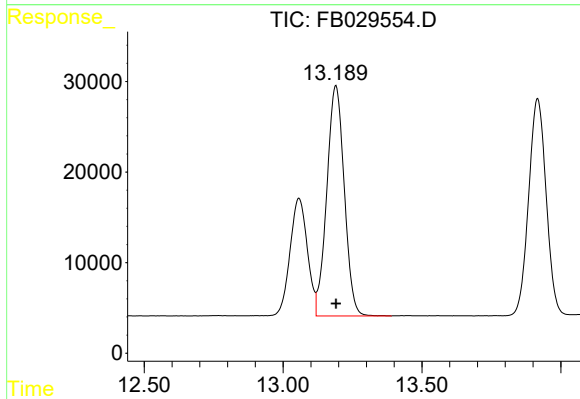

#8 m-Xylene


R.T.: 13.190 min
Delta R.T.: 0.000 min
Response: 1111019
Conc: 57.25 ng/ml

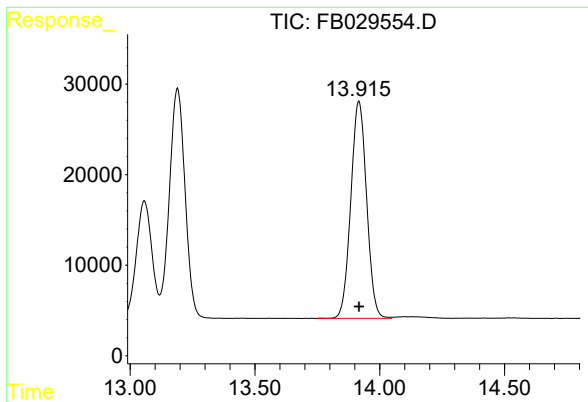

#9 O-Xylene

R.T.: 13.917 min
Delta R.T.: 0.000 min
Response: 1055175
Conc: 55.55 ng/ml

Instrument :
FID_B
ClientSampleId :

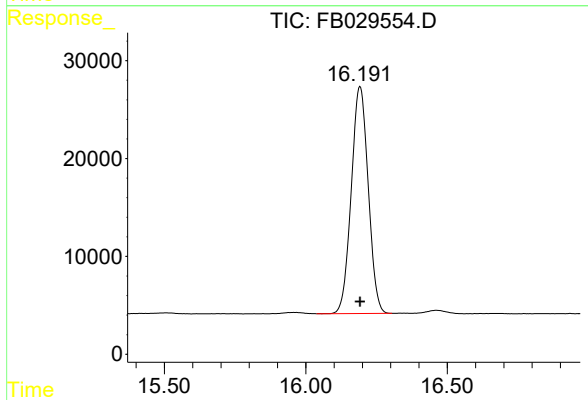

#10 1,2,4-Trimethylbenzene

R.T.: 16.192 min
Delta R.T.: 0.000 min
Response: 964933
Conc: 50.58 ng/ml