

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032323\
 Data File : FB029551.D
 Signal(s) : FID2B.CH
 Acq On : 23 Mar 2023 8:00
 Operator : YP/AJ
 Sample : 5 GRO STD
 Misc :
 ALS Vial : 1 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 5 GRO STD

Integration File: Calibration.e
 Quant Time: Mar 23 10:27:34 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
 Quant Title :
 QLast Update : Thu Mar 23 10:23:42 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	76071	5.678 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.704	131950	8.082 ng/ml
2) t 2,2,4-Trimethylpentane	7.414	136078	7.657 ng/ml
3) t n-Heptane	7.748	48101	2.543 ng/ml
4) t Benzene	7.886	54786	2.538 ng/ml
6) t Toluene	10.617	165682	7.805 ng/ml
7) t Ethylbenzene	13.056	52363	2.624 ng/ml
8) t m-Xylene	13.185	104362	5.246 ng/ml
9) t O-Xylene	13.913	103938	5.421 ng/ml
10) t 1,2,4-Trimethylbenzene	16.188	104453	5.536 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032323\
Data File : FB029551.D
Signal(s) : FID2B.CH
Acq On : 23 Mar 2023 8:00
Operator : YP/AJ
Sample : 5 GRO STD
Misc :
ALS Vial : 1 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
5 GRO STD

Integration File: Calibration.e
Quant Time: Mar 23 10:27:34 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
Quant Title :
QLast Update : Thu Mar 23 10:23:42 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

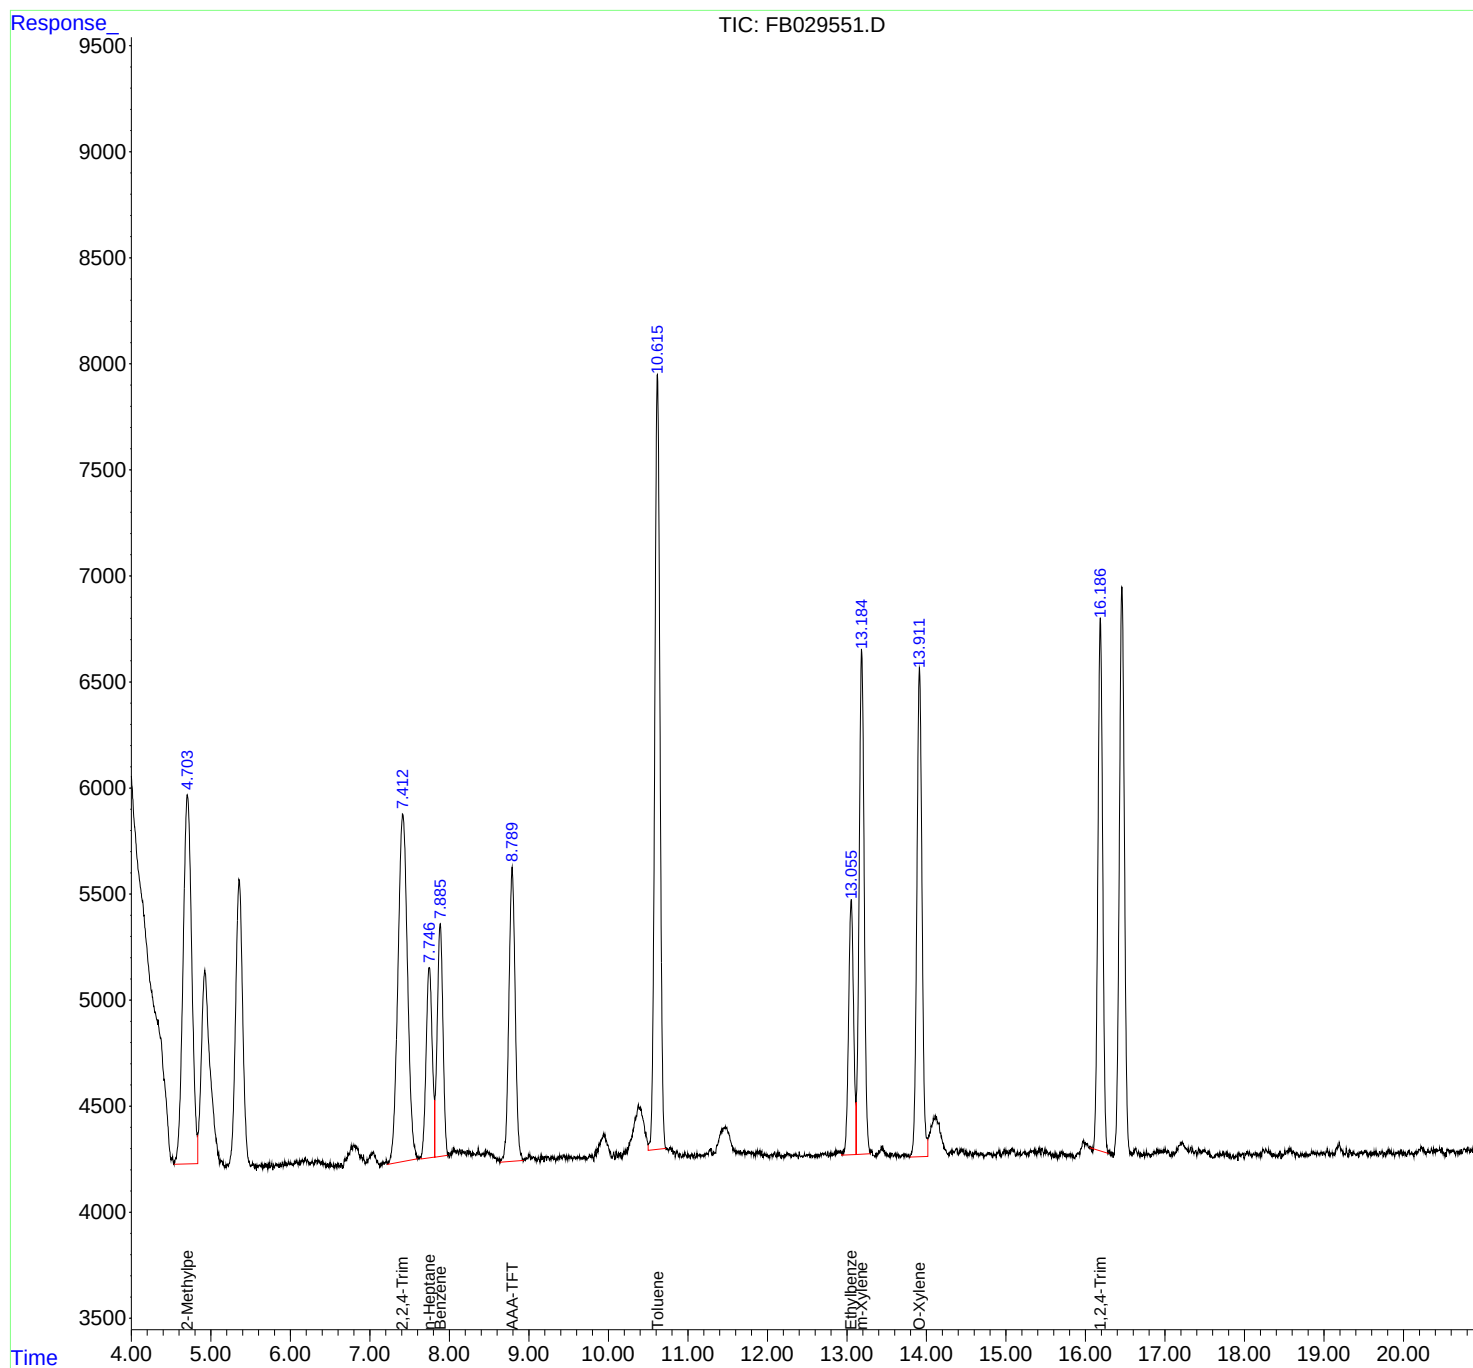


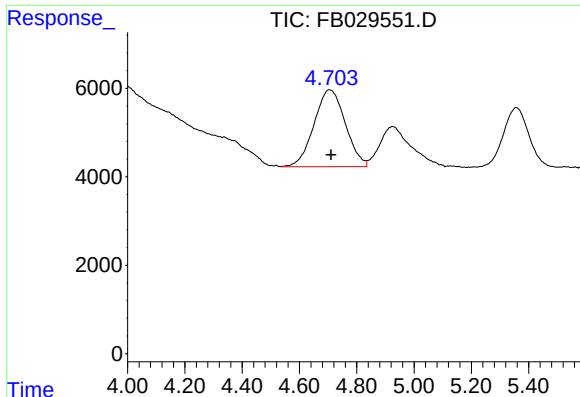

#1 2-Methylpentane


R.T.: 4.704 min
Delta R.T.: -0.006 min
Response: 131950
Conc: 8.08 ng/ml

Instrument :
FID_B
ClientSampleId :
5 GRO STD

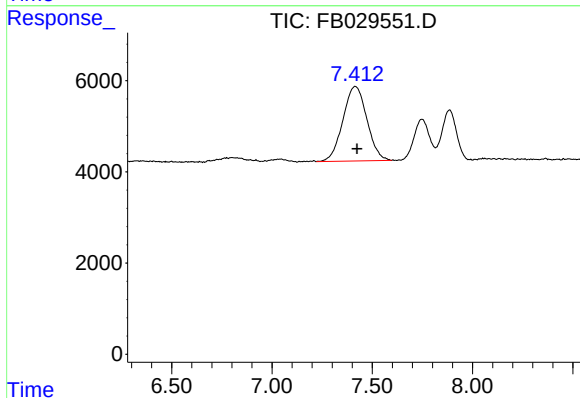


#2 2,2,4-Trimethylpentane

R.T.: 7.414 min
Delta R.T.: -0.010 min
Response: 136078
Conc: 7.66 ng/ml

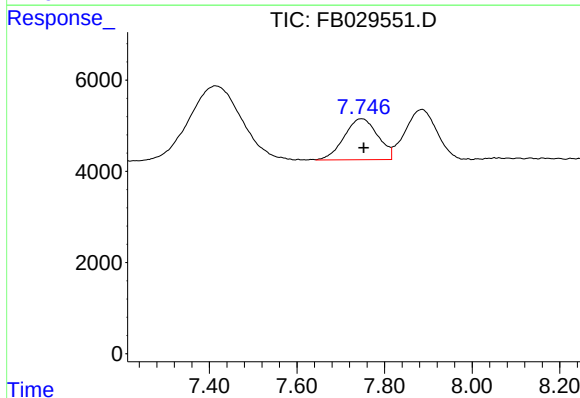


#3 n-Heptane

R.T.: 7.748 min
Delta R.T.: -0.004 min
Response: 48101
Conc: 2.54 ng/ml

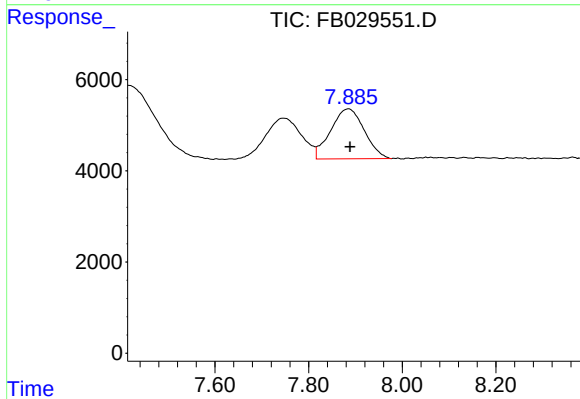

#4 Benzene


R.T.: 7.886 min
Delta R.T.: -0.003 min
Response: 54786
Conc: 2.54 ng/ml

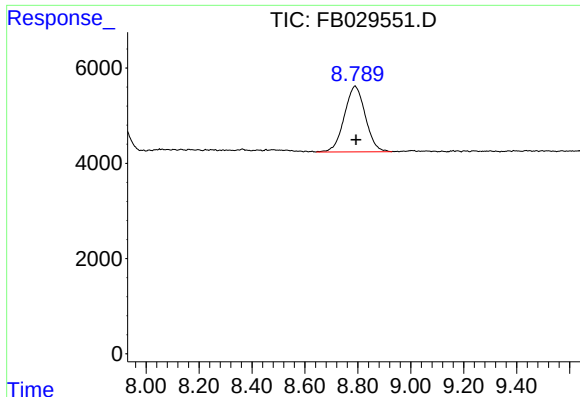

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: -0.004 min
Response: 76071
Conc: 5.68 ng/ml

Instrument :
FID_B
ClientSampleId :
5 GRO STD

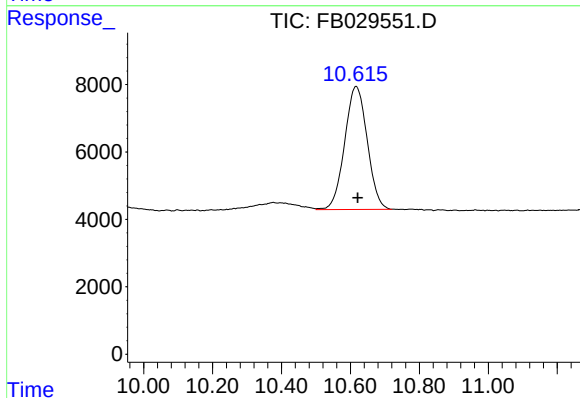


#6 Toluene

R.T.: 10.617 min
Delta R.T.: -0.005 min
Response: 165682
Conc: 7.81 ng/ml

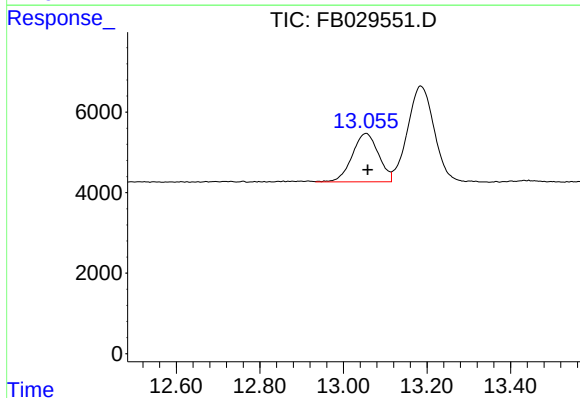


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: -0.002 min
Response: 52363
Conc: 2.62 ng/ml

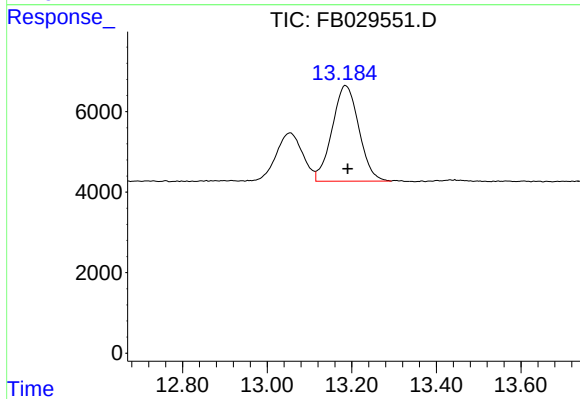

#8 m-Xylene


R.T.: 13.185 min
Delta R.T.: -0.005 min
Response: 104362
Conc: 5.25 ng/ml

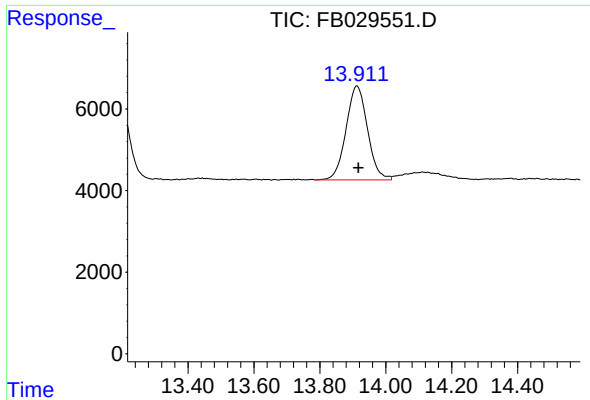

#9 O-Xylene

R.T.: 13.913 min
Delta R.T.: -0.004 min
Response: 103938
Conc: 5.42 ng/ml

Instrument :
FID_B
ClientSampleId :
5 GRO STD

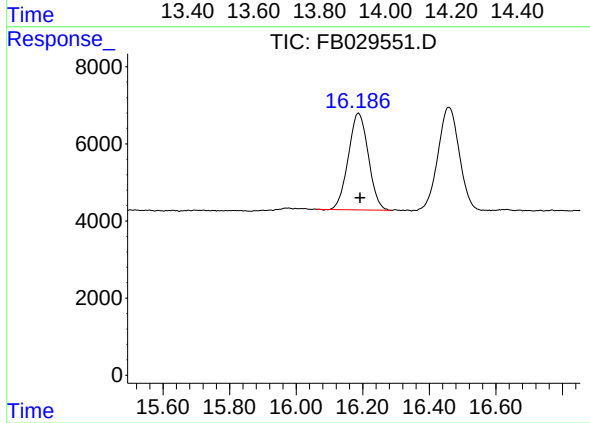

#10 1,2,4-Trimethylbenzene

R.T.: 16.188 min
Delta R.T.: -0.004 min
Response: 104453
Conc: 5.54 ng/ml