

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032323\
 Data File : FB029552.D
 Signal(s) : FID2B.CH
 Acq On : 23 Mar 2023 8:38
 Operator : YP/AJ
 Sample : 10 GRO STD
 Misc :
 ALS Vial : 2 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 10 GRO STD

Integration File: Calibration.e
 Quant Time: Mar 23 10:29:01 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
 Quant Title :
 QLast Update : Thu Mar 23 10:23:42 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	135248	9.454 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	217541	12.827 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	243262	13.547 ng/ml
3) t n-Heptane	7.752	82285	4.313 ng/ml
4) t Benzene	7.887	95319	4.382 ng/ml
6) t Toluene	10.620	272786	12.595 ng/ml
7) t Ethylbenzene	13.056	89191	4.361 ng/ml
8) t m-Xylene	13.189	174584	8.566 ng/ml
9) t O-Xylene	13.916	170271	8.522 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	174758	8.791 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032323\
Data File : FB029552.D
Signal(s) : FID2B.CH
Acq On : 23 Mar 2023 8:38
Operator : YP/AJ
Sample : 10 GRO STD
Misc :
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
10 GRO STD

Integration File: Calibration.e
Quant Time: Mar 23 10:29:01 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
Quant Title :
QLast Update : Thu Mar 23 10:23:42 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

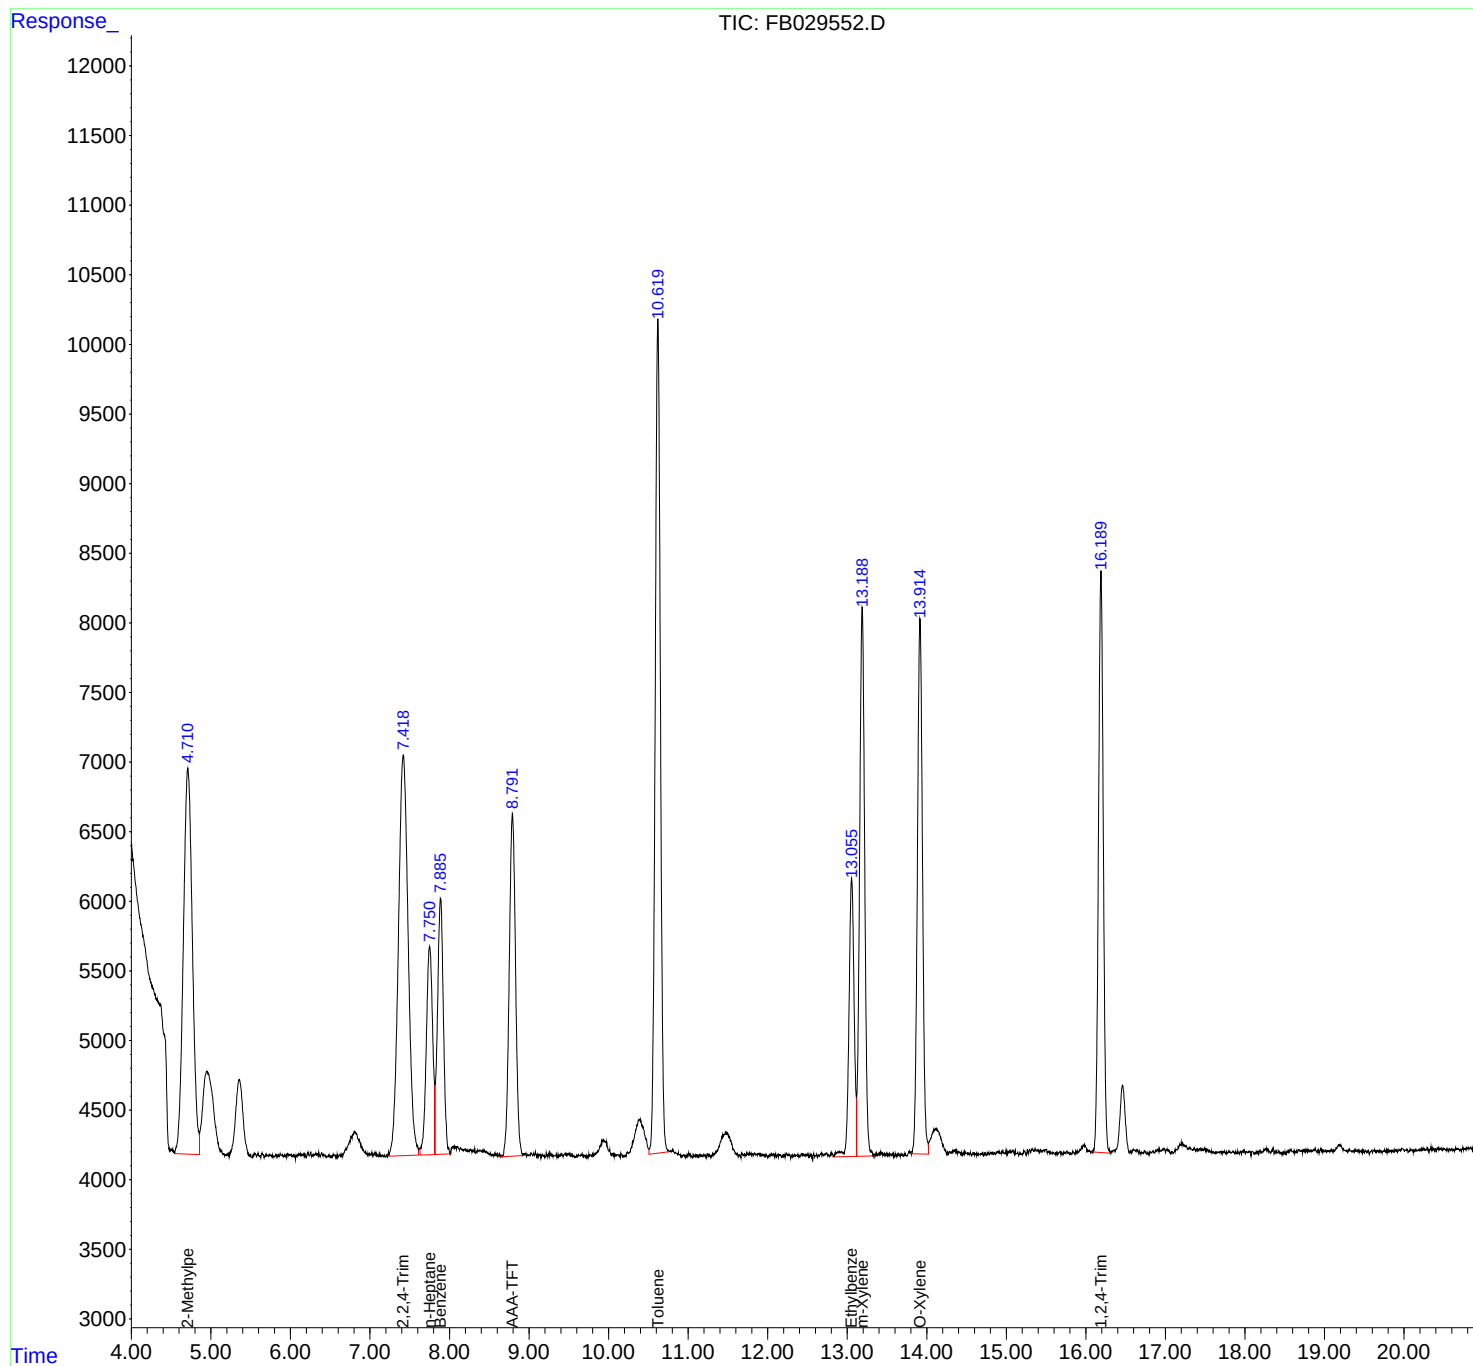


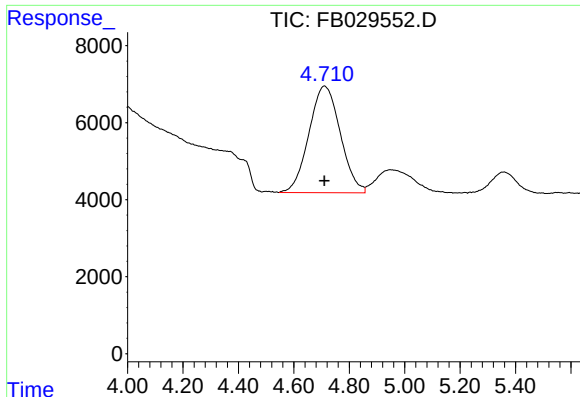

#1 2-Methylpentane


R.T.: 4.711 min
Delta R.T.: 0.001 min
Response: 217541
Conc: 12.83 ng/ml

Instrument :
FID_B
ClientSampleId :
10 GRO STD

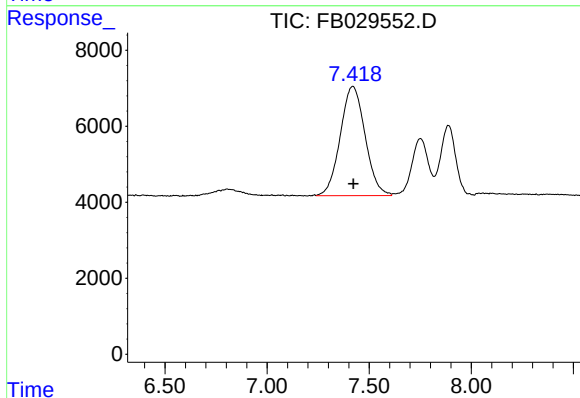


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: -0.003 min
Response: 243262
Conc: 13.55 ng/ml

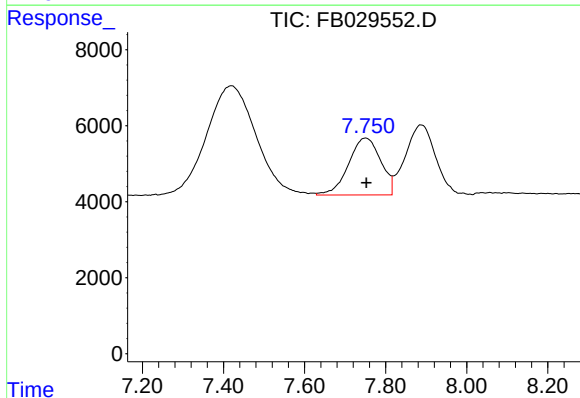


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.000 min
Response: 82285
Conc: 4.31 ng/ml

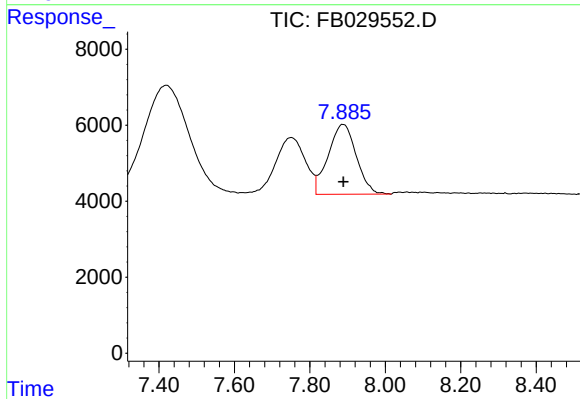

#4 Benzene


R.T.: 7.887 min
Delta R.T.: -0.002 min
Response: 95319
Conc: 4.38 ng/ml

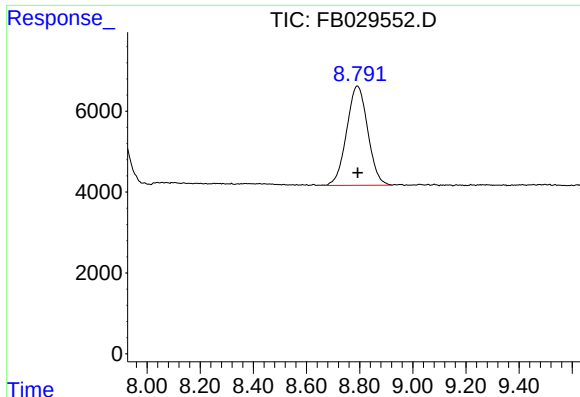

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: -0.002 min
Response: 135248
Conc: 9.45 ng/ml

Instrument :
FID_B
ClientSampleId :
10 GRO STD

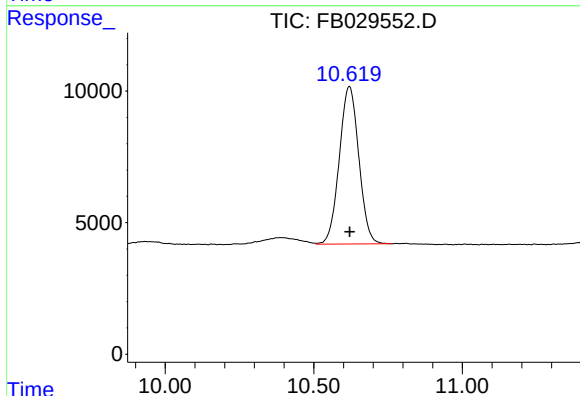


#6 Toluene

R.T.: 10.620 min
Delta R.T.: -0.001 min
Response: 272786
Conc: 12.59 ng/ml

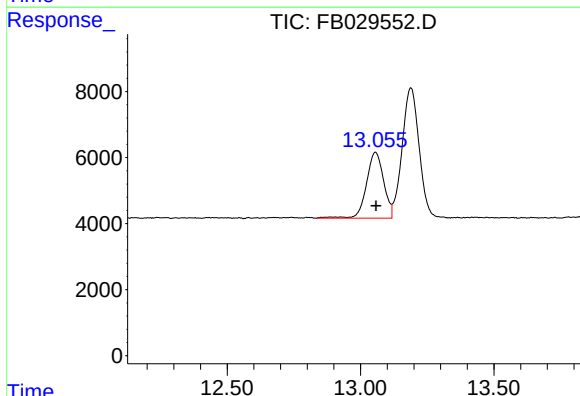


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: -0.002 min
Response: 89191
Conc: 4.36 ng/ml

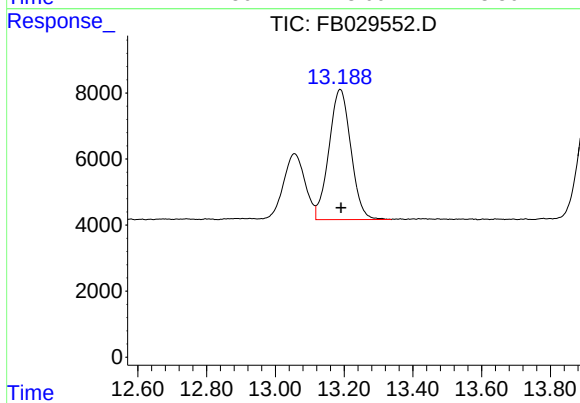

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: -0.001 min
Response: 174584
Conc: 8.57 ng/ml

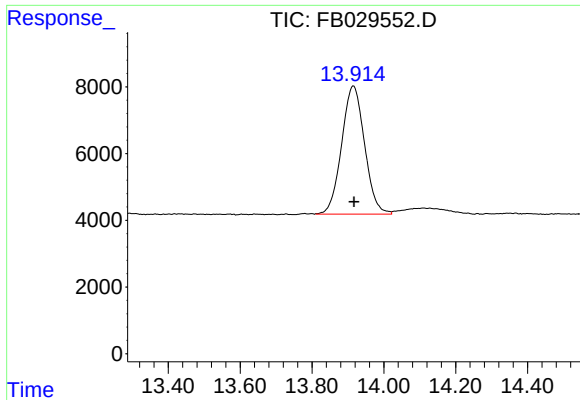

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: -0.002 min
Response: 170271
Conc: 8.52 ng/ml

Instrument :
FID_B
ClientSampleId :
10 GRO STD

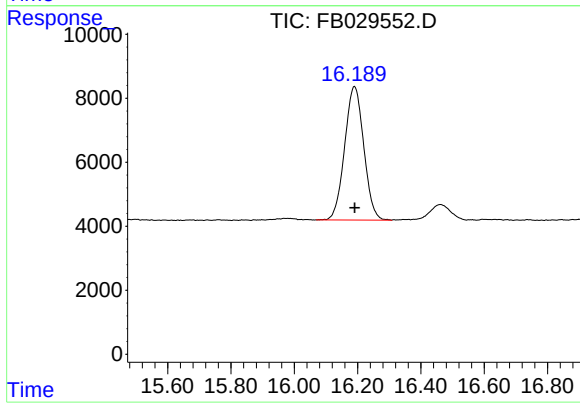

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: 0.000 min
Response: 174758
Conc: 8.79 ng/ml