

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032323\
 Data File : FB029556.D
 Signal(s) : FID2B.CH
 Acq On : 23 Mar 2023 12:08
 Operator : YP/AJ
 Sample : FB032323GROICV
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 FB032323GROICV

Integration File: Calibration.e
 Quant Time: Mar 23 13:16:37 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
 Quant Title :
 QLast Update : Thu Mar 23 11:44:29 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	260686	18.289 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.715	497528	29.634 ng/ml
2) t 2,2,4-Trimethylpentane	7.423	581979	31.613 ng/ml
3) t n-Heptane	7.752	180402	9.261 ng/ml
4) t Benzene	7.889	211515	9.362 ng/ml
6) t Toluene	10.622	616859	27.982 ng/ml
7) t Ethylbenzene	13.059	199402	9.646 ng/ml
8) t m-Xylene	13.191	402227	19.658 ng/ml
9) t O-Xylene	13.918	398286	20.104 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	424321	22.226 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032323\
Data File : FB029556.D
Signal(s) : FID2B.CH
Acq On : 23 Mar 2023 12:08
Operator : YP/AJ
Sample : FB032323GROICV
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
FB032323GROICV

Integration File: Calibration.e
Quant Time: Mar 23 13:16:37 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
Quant Title :
QLast Update : Thu Mar 23 11:44:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

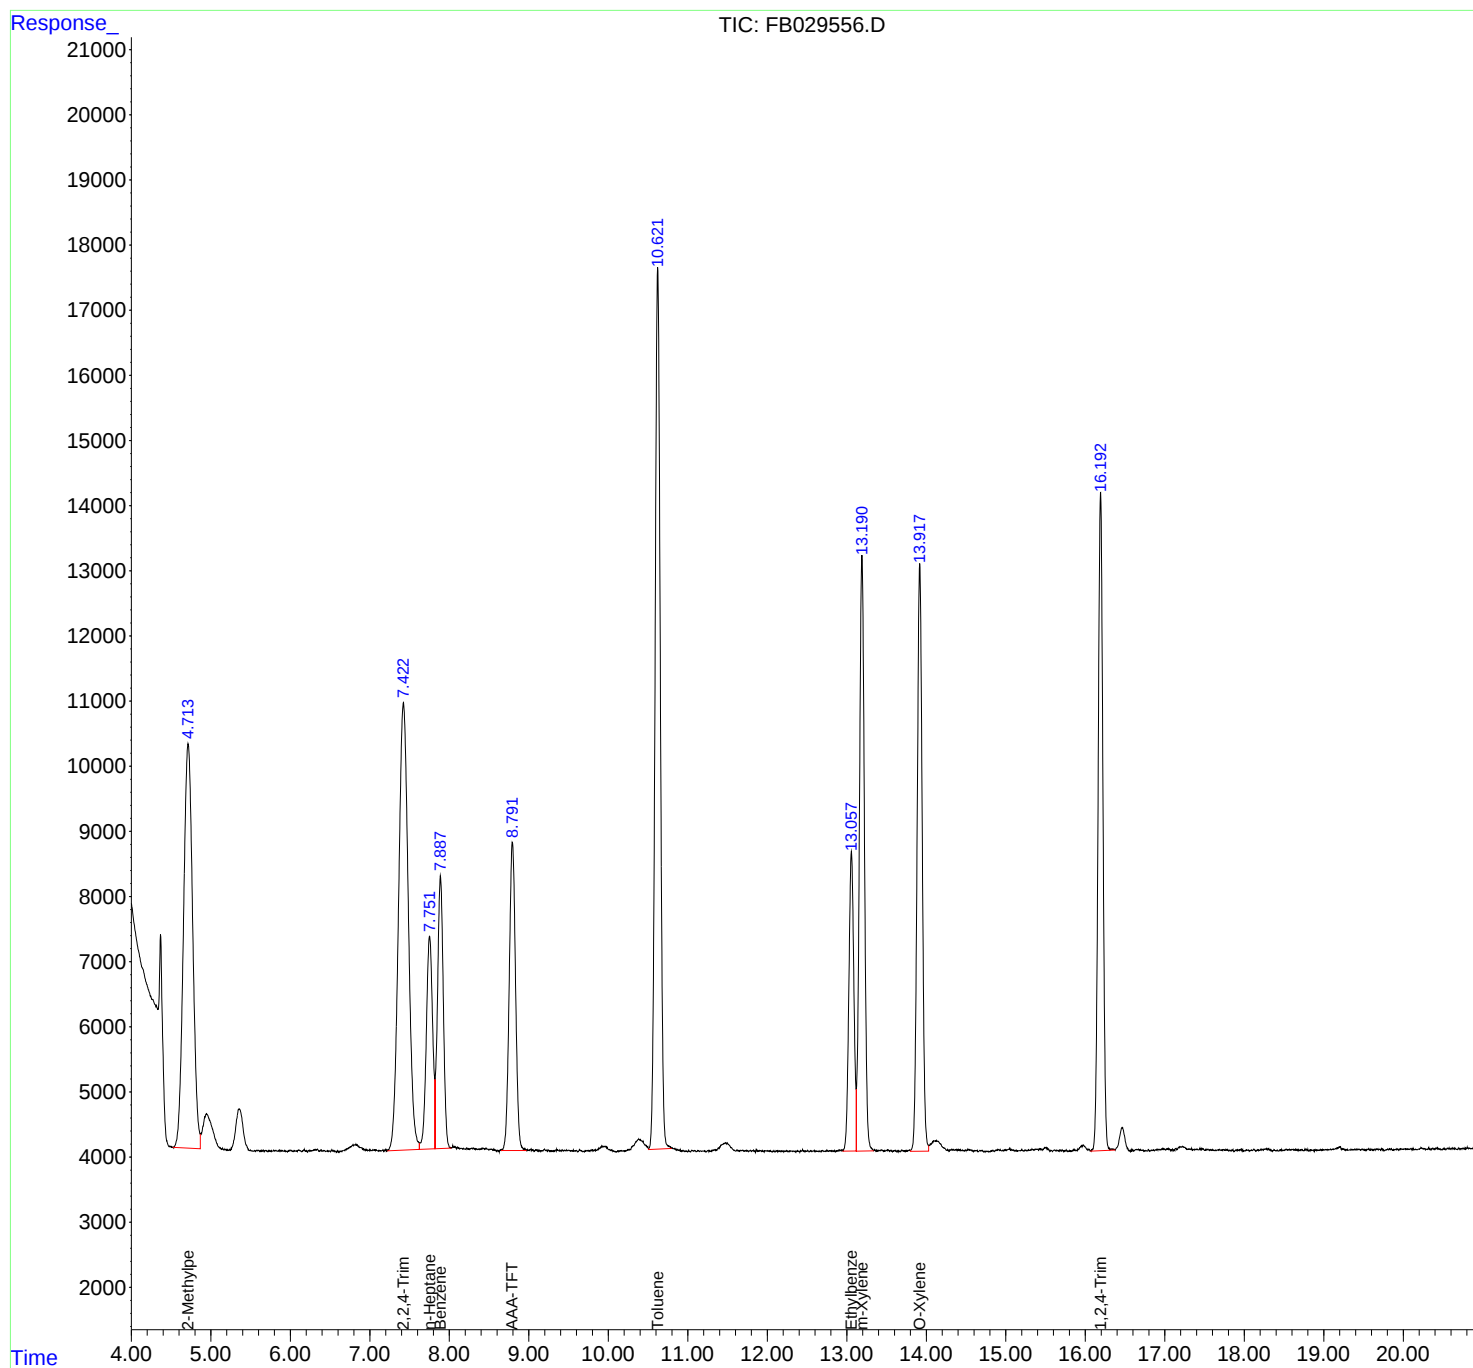


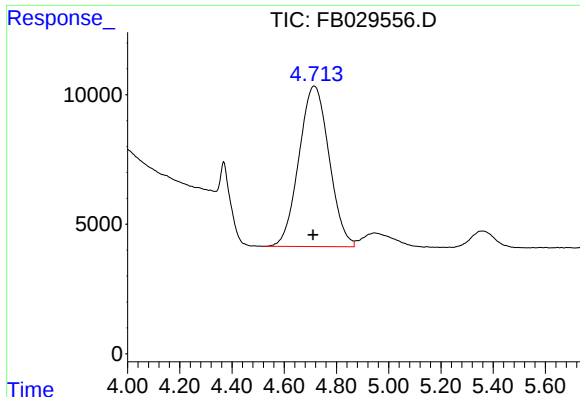

#1 2-Methylpentane


R.T.: 4.715 min
Delta R.T.: 0.005 min
Response: 497528
Conc: 29.63 ng/ml

Instrument :
FID_B
ClientSampleId :
FB032323GROICV

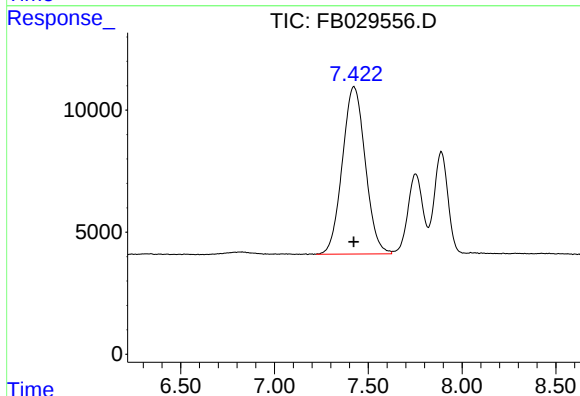


#2 2,2,4-Trimethylpentane

R.T.: 7.423 min
Delta R.T.: 0.000 min
Response: 581979
Conc: 31.61 ng/ml

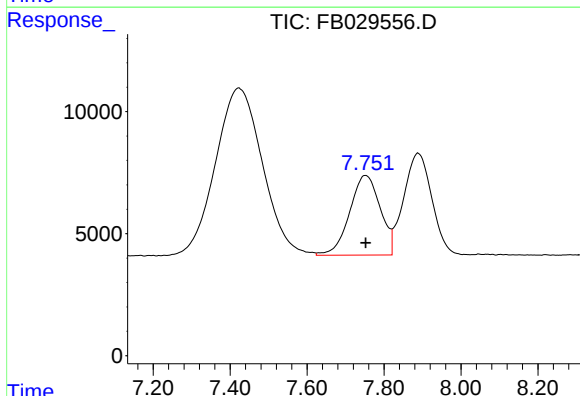


#3 n-Heptane

R.T.: 7.752 min
Delta R.T.: 0.000 min
Response: 180402
Conc: 9.26 ng/ml

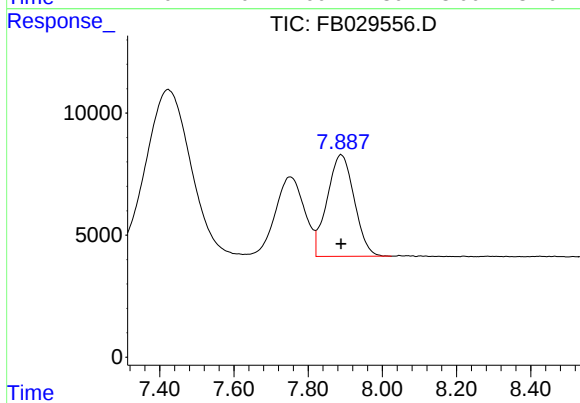

#4 Benzene


R.T.: 7.889 min
Delta R.T.: 0.000 min
Response: 211515
Conc: 9.36 ng/ml

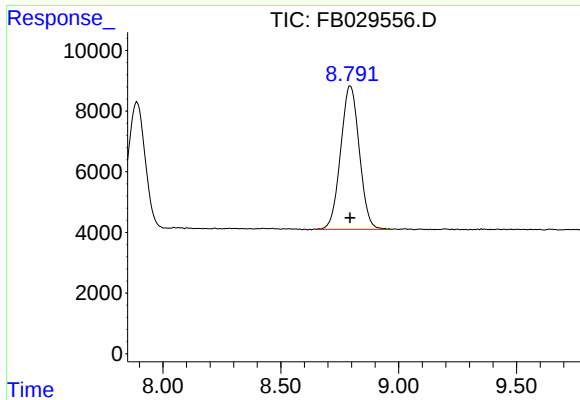

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.000 min
Response: 260686
Conc: 18.29 ng/ml

Instrument : FID_B
ClientSampleId : FB032323GROICV

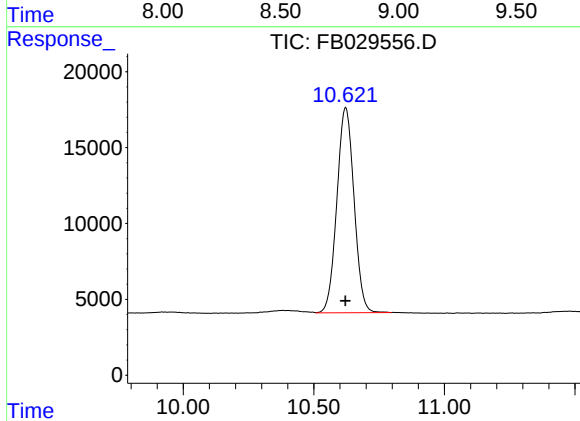


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.000 min
Response: 616859
Conc: 27.98 ng/ml

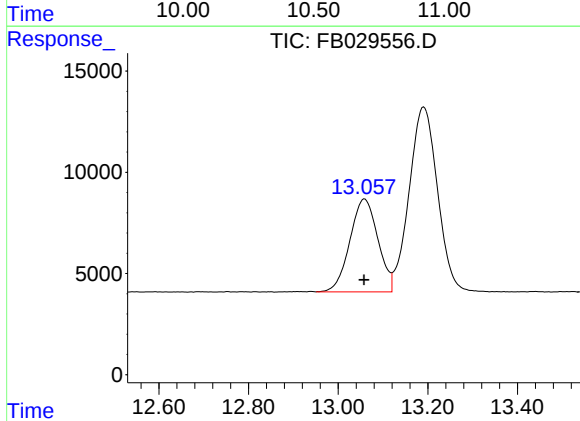


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: 0.000 min
Response: 199402
Conc: 9.65 ng/ml

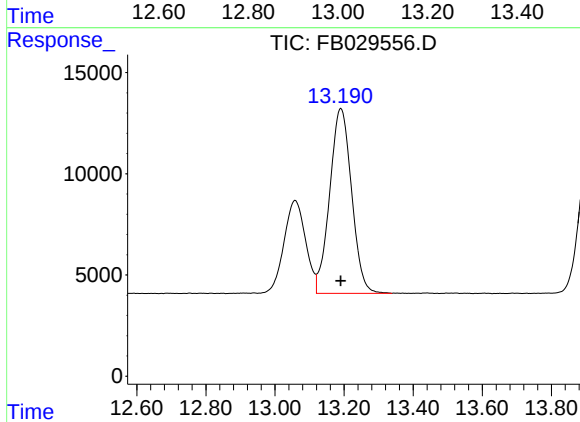

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.000 min
Response: 402227
Conc: 19.66 ng/ml

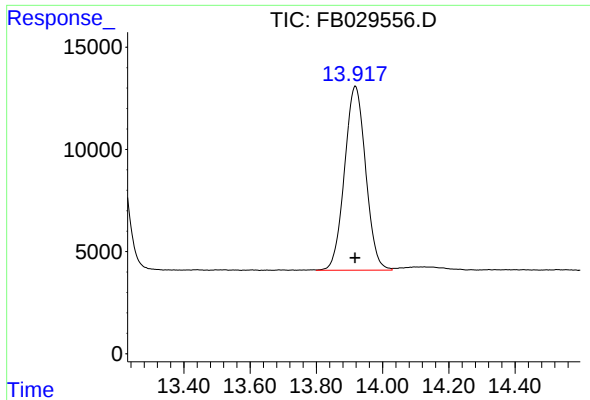

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.001 min
Response: 398286
Conc: 20.10 ng/ml

Instrument :
FID_B
ClientSampleId :
FB032323GROICV

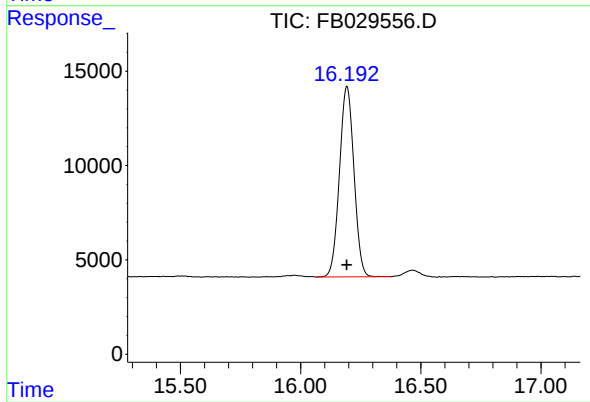

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.001 min
Response: 424321
Conc: 22.23 ng/ml