

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032423\
 Data File : FB029565.D
 Signal(s) : FID2B.CH
 Acq On : 24 Mar 2023 16:23
 Operator : YP/AJ
 Sample : 02064-01MSD 50X
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 24 23:56:52 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
 Quant Title :
 QLast Update : Thu Mar 23 11:44:29 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	258612	18.144 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	493722	29.408 ng/ml
2) t 2,2,4-Trimethylpentane	7.428	582151	31.622 ng/ml
3) t n-Heptane	7.750	196799	10.103 ng/ml
4) t Benzene	7.888	249698	11.052 ng/ml
6) t Toluene	10.622	726739	32.967 ng/ml
7) t Ethylbenzene	13.059	221618	10.721 ng/ml
8) t m-Xylene	13.192	442581	21.630 ng/ml
9) t O-Xylene	13.919	430775	21.744 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	393259	20.599 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032423\
Data File : FB029565.D
Signal(s) : FID2B.CH
Acq On : 24 Mar 2023 16:23
Operator : YP/AJ
Sample : 02064-01MSD 50X
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 24 23:56:52 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
Quant Title :
QLast Update : Thu Mar 23 11:44:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

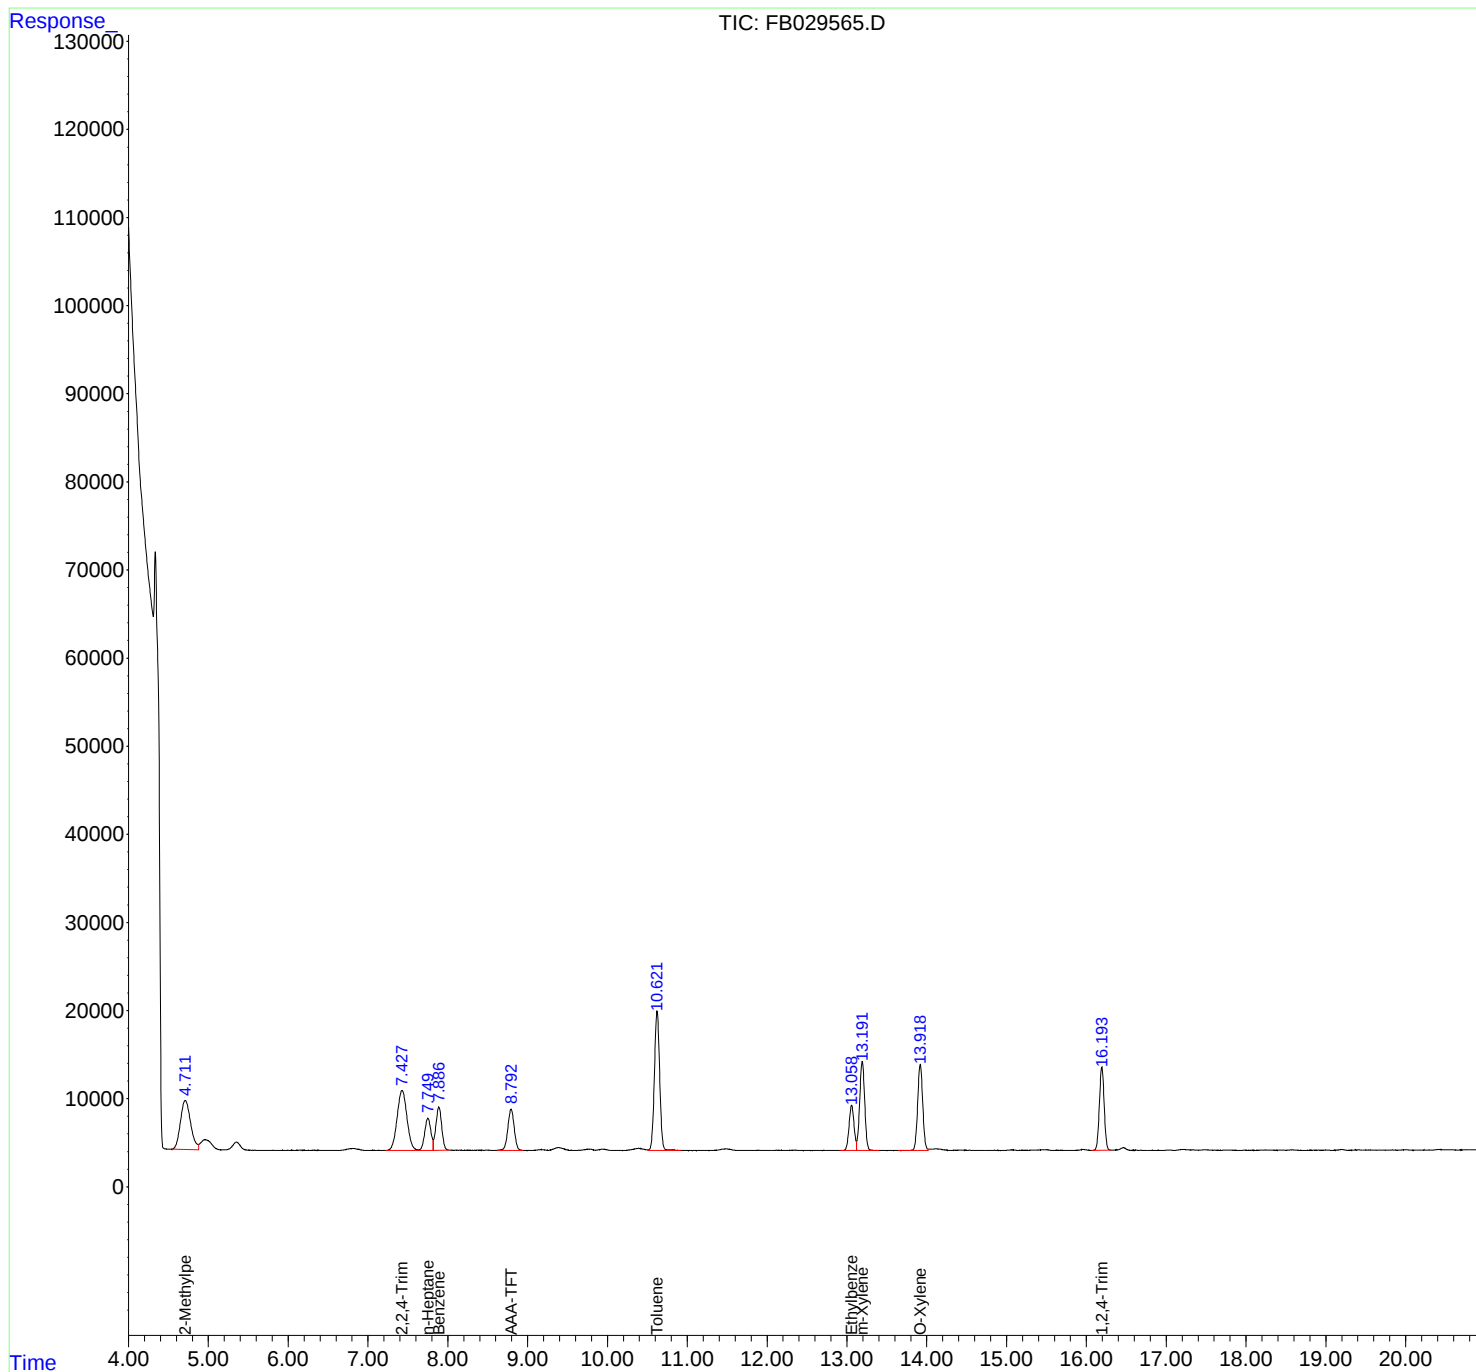

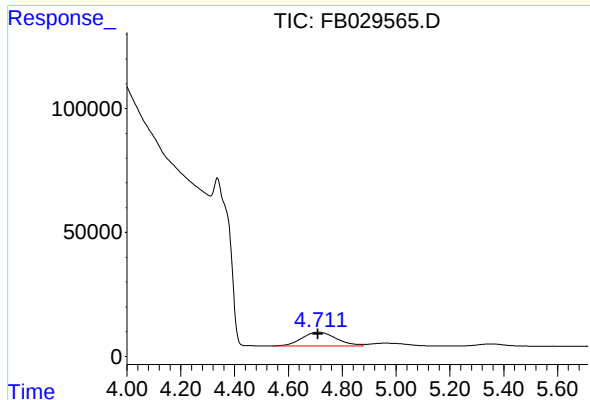


#1 2-Methylpentane

R.T.: 4.712 min
Delta R.T.: 0.002 min
Response: 493722
Conc: 29.41 ng/ml


Instrument : FID_B

ClientSampleId :

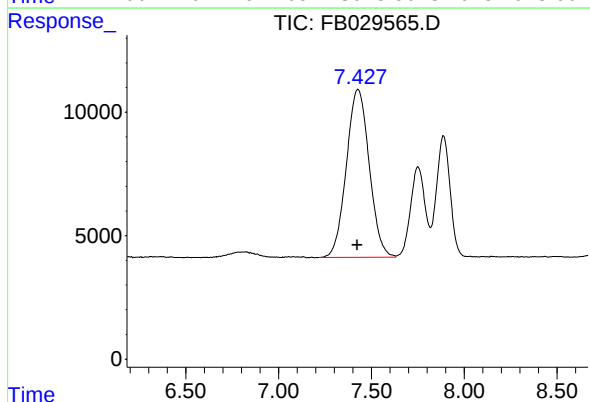


#2 2,2,4-Trimethylpentane

R.T.: 7.428 min
Delta R.T.: 0.005 min
Response: 582151
Conc: 31.62 ng/ml

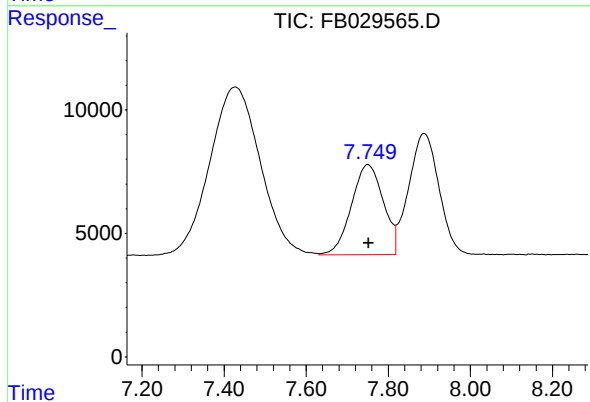


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: -0.002 min
Response: 196799
Conc: 10.10 ng/ml

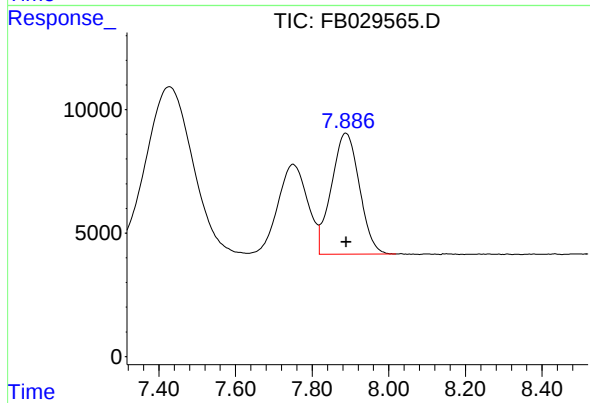

#4 Benzene


R.T.: 7.888 min
Delta R.T.: -0.001 min
Response: 249698
Conc: 11.05 ng/ml

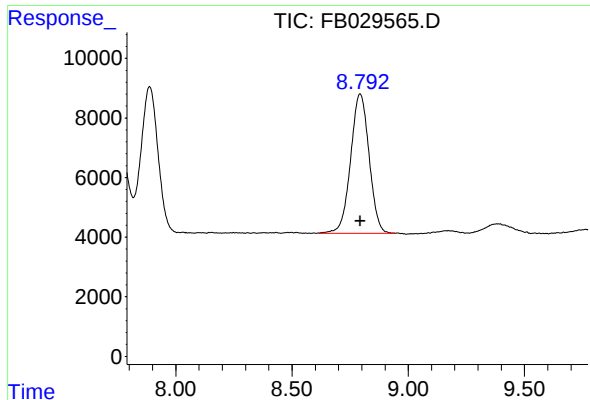

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.000 min
Response: 258612
Conc: 18.14 ng/ml

Instrument :
FID_B
ClientSampleId :

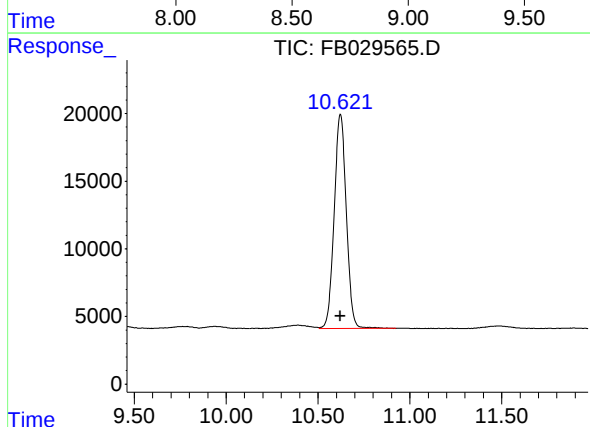


#6 Toluene

R.T.: 10.622 min
Delta R.T.: 0.000 min
Response: 726739
Conc: 32.97 ng/ml

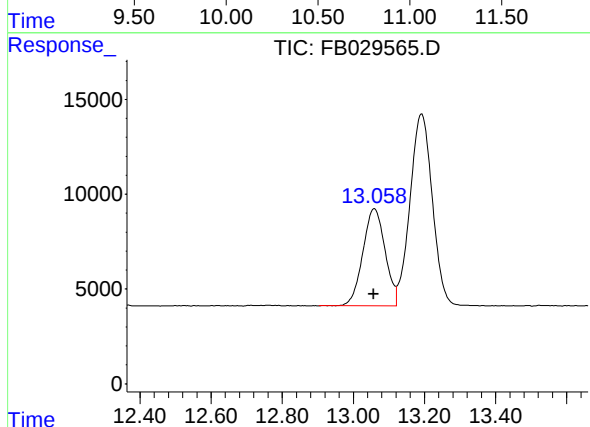


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: 0.002 min
Response: 221618
Conc: 10.72 ng/ml

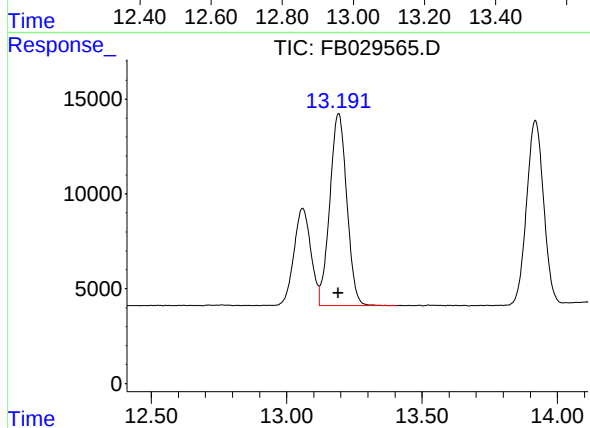

#8 m-Xylene


R.T.: 13.192 min
Delta R.T.: 0.002 min
Response: 442581
Conc: 21.63 ng/ml

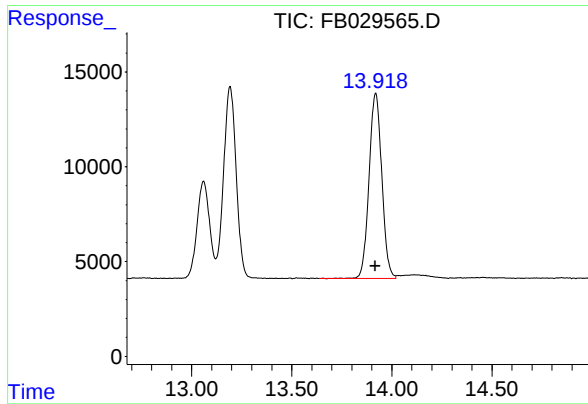

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: 0.002 min
Response: 430775
Conc: 21.74 ng/ml

Instrument :
FID_B
ClientSampleId :

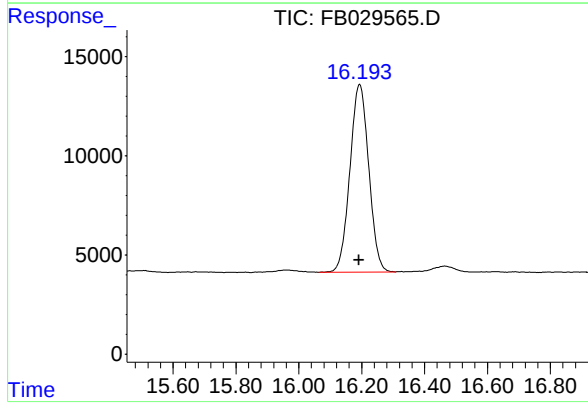

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.002 min
Response: 393259
Conc: 20.60 ng/ml