

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032423\
Data File : FB029559.D
Signal(s) : FID2B.CH
Acq On : 24 Mar 2023 12:32
Operator : YP/AJ
Sample : VBF0324S2 50X
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF0324S2

Integration File: Calibration.e
Quant Time: Mar 24 23:56:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
Quant Title :
QLast Update : Thu Mar 23 11:44:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	308506	21.644 ng/ml
Target Compounds			

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032423\
Data File : FB029559.D
Signal(s) : FID2B.CH
Acq On : 24 Mar 2023 12:32
Operator : YP/AJ
Sample : VBF0324S2 50X
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF0324S2

Integration File: Calibration.e
Quant Time: Mar 24 23:56:17 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
Quant Title :
QLast Update : Thu Mar 23 11:44:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

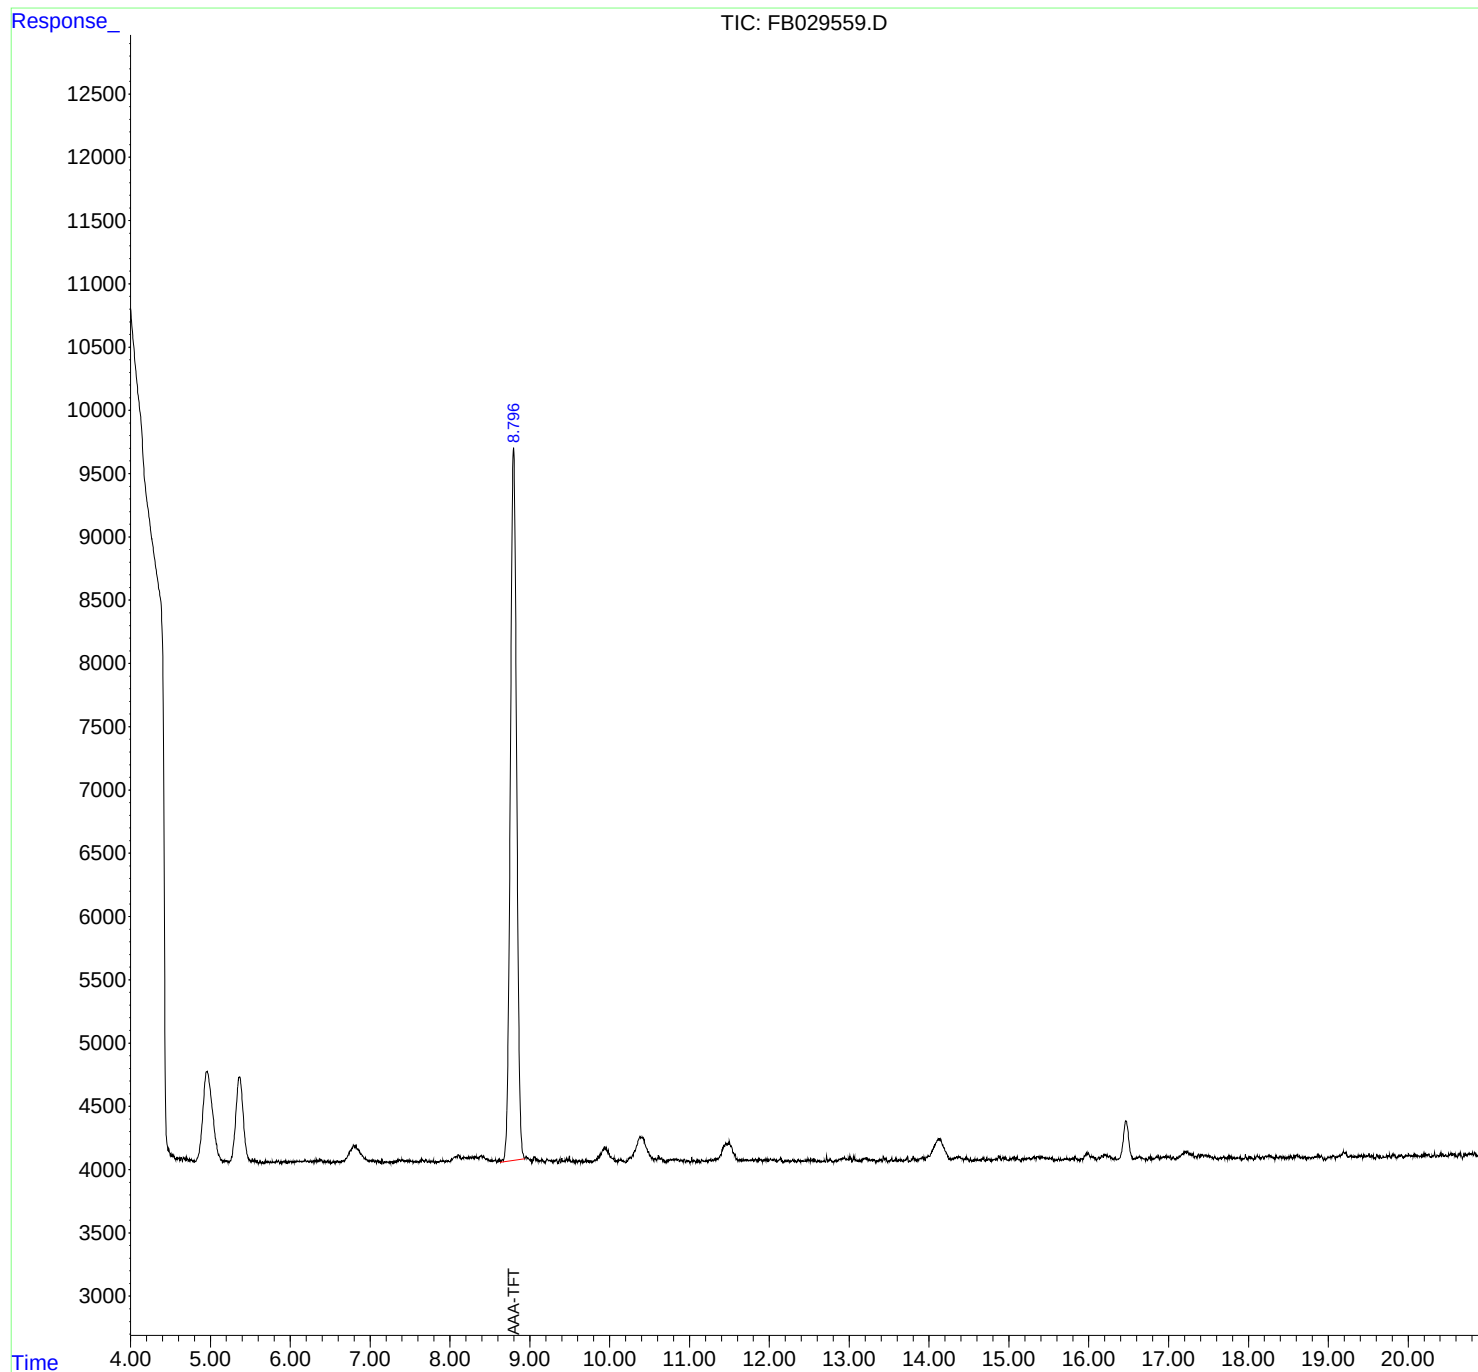

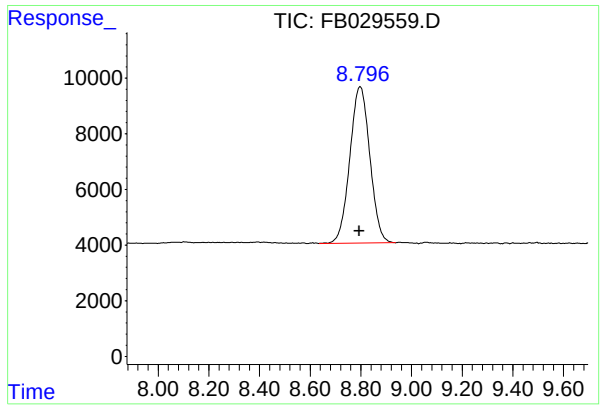

#5 AAA-TFT

R.T.: 8.798 min
Delta R.T.: 0.004 min
Response: 308506
Conc: 21.64 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF0324S2