

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032423\
 Data File : FB029564.D
 Signal(s) : FID2B.CH
 Acq On : 24 Mar 2023 15:44
 Operator : YP/AJ
 Sample : 02064-01MS 50X
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BU-03-032323MS

Integration File: Calibration.e
 Quant Time: Mar 24 23:56:46 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
 Quant Title :
 QLast Update : Thu Mar 23 11:44:29 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.794	285097	20.002 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	478629	28.509 ng/ml
2) t 2,2,4-Trimethylpentane	7.425	572235	31.084 ng/ml
3) t n-Heptane	7.751	205083	10.528 ng/ml
4) t Benzene	7.888	245445	10.864 ng/ml
6) t Toluene	10.623	741166	33.621 ng/ml
7) t Ethylbenzene	13.059	225417	10.905 ng/ml
8) t m-Xylene	13.192	443522	21.676 ng/ml
9) t O-Xylene	13.919	421217	21.262 ng/ml
10) t 1,2,4-Trimethylbenzene	16.194	369130	19.335 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032423\
Data File : FB029564.D
Signal(s) : FID2B.CH
Acq On : 24 Mar 2023 15:44
Operator : YP/AJ
Sample : 02064-01MS 50X
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BU-03-032323MS

Integration File: Calibration.e
Quant Time: Mar 24 23:56:46 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
Quant Title :
QLast Update : Thu Mar 23 11:44:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

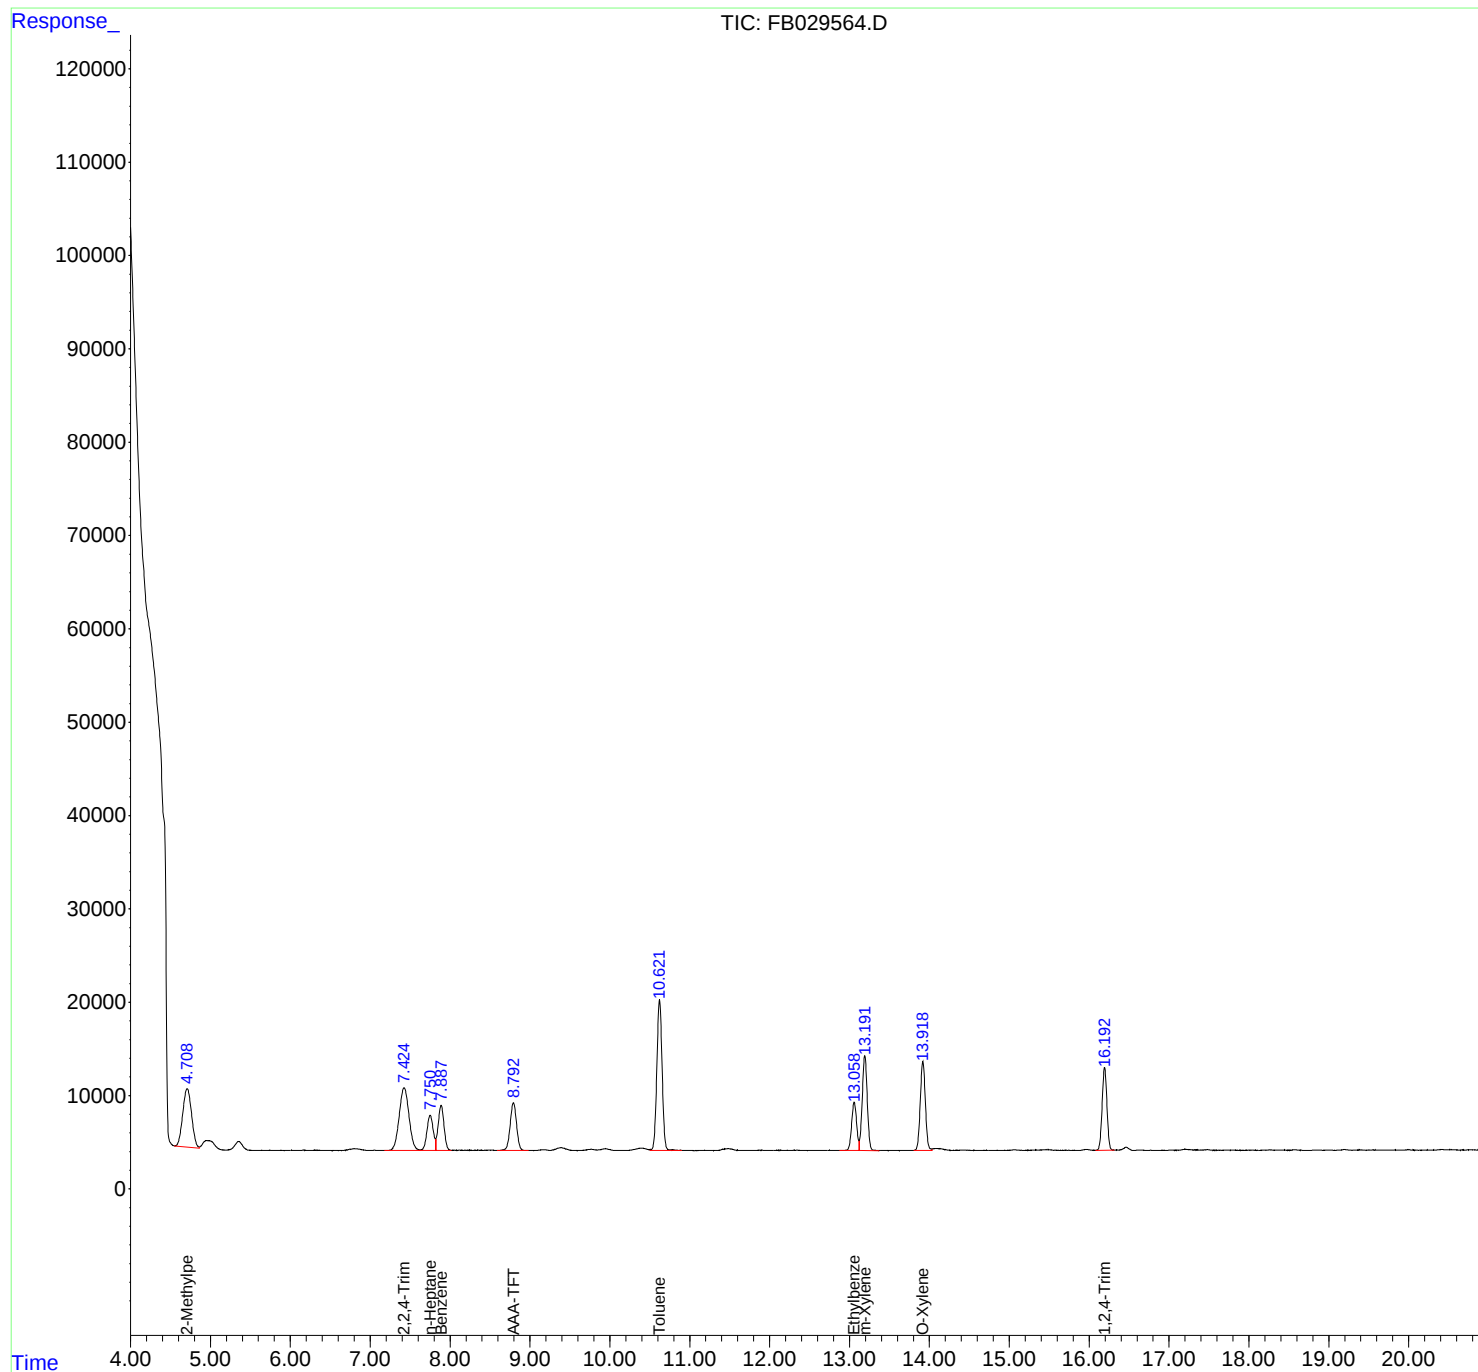


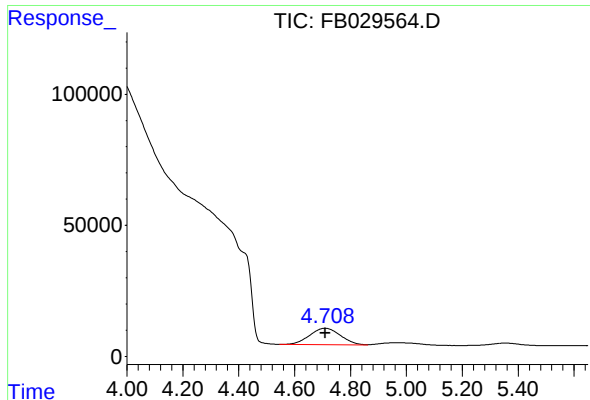

#1 2-Methylpentane


R.T.: 4.709 min
Delta R.T.: 0.000 min
Response: 478629
Conc: 28.51 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-03-032323MS

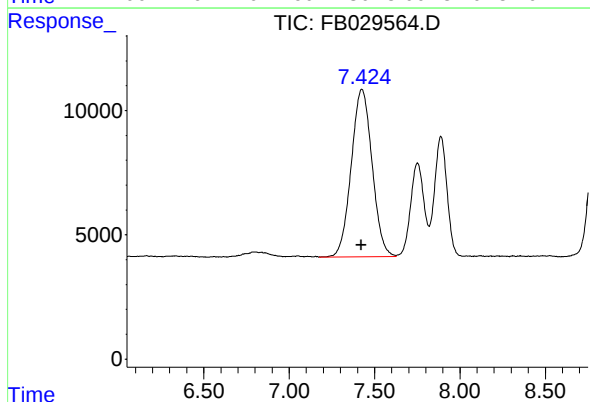


#2 2,2,4-Trimethylpentane

R.T.: 7.425 min
Delta R.T.: 0.002 min
Response: 572235
Conc: 31.08 ng/ml

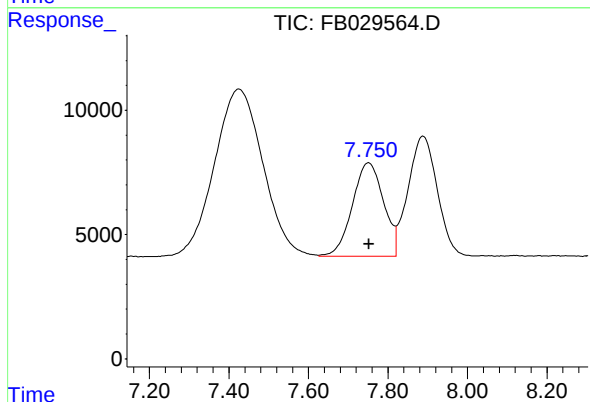


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: -0.001 min
Response: 205083
Conc: 10.53 ng/ml

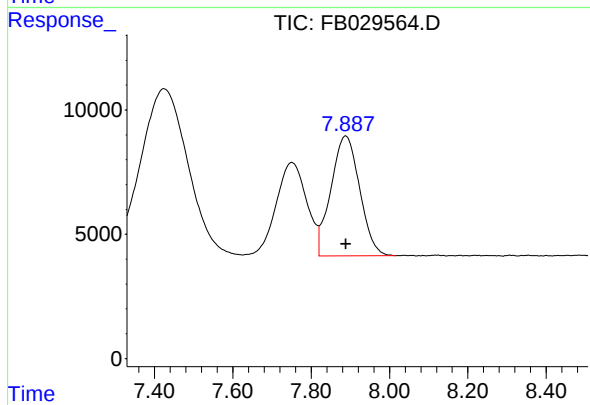

#4 Benzene


R.T.: 7.888 min
Delta R.T.: 0.000 min
Response: 245445
Conc: 10.86 ng/ml

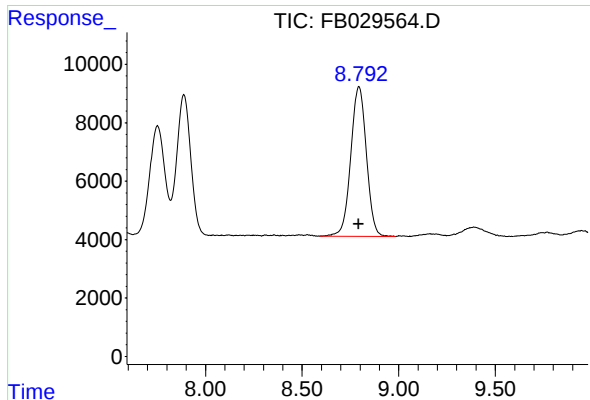

#5 AAA-TFT


R.T.: 8.794 min
Delta R.T.: 0.000 min
Response: 285097
Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-03-032323MS

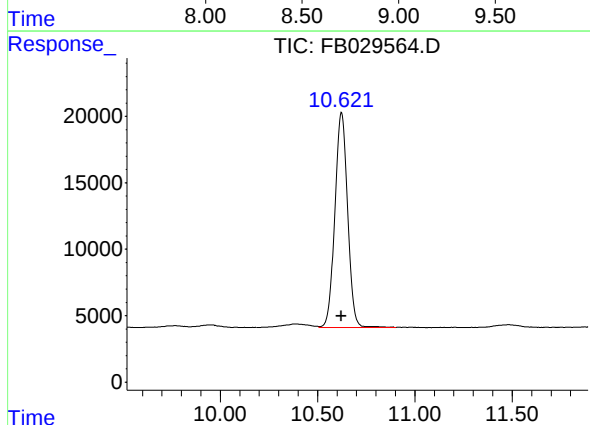


#6 Toluene

R.T.: 10.623 min
Delta R.T.: 0.000 min
Response: 741166
Conc: 33.62 ng/ml

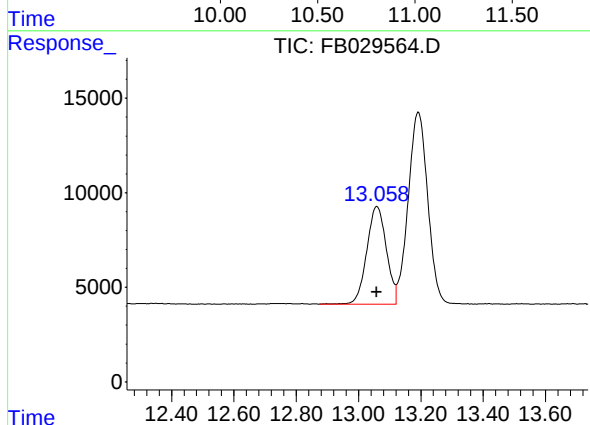


#7 Ethylbenzene

R.T.: 13.059 min
Delta R.T.: 0.001 min
Response: 225417
Conc: 10.90 ng/ml

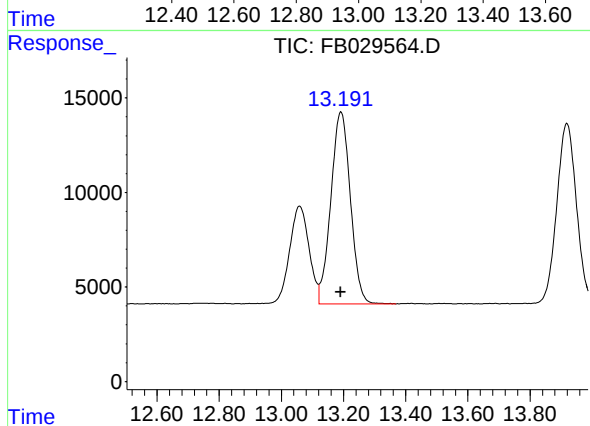

#8 m-Xylene


R.T.: 13.192 min
Delta R.T.: 0.002 min
Response: 443522
Conc: 21.68 ng/ml

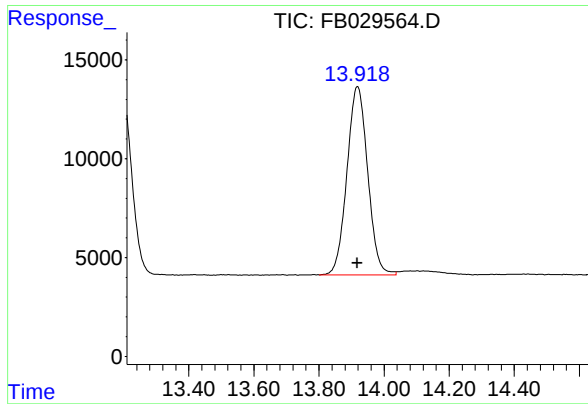

#9 O-Xylene

R.T.: 13.919 min
Delta R.T.: 0.002 min
Response: 421217
Conc: 21.26 ng/ml

Instrument :
FID_B
ClientSampleId :
BU-03-032323MS

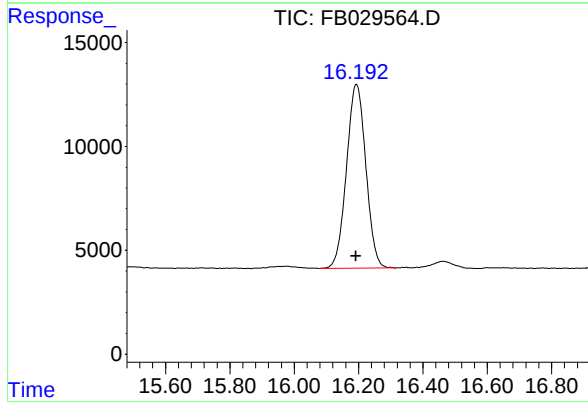

#10 1,2,4-Trimethylbenzene

R.T.: 16.194 min
Delta R.T.: 0.002 min
Response: 369130
Conc: 19.34 ng/ml