

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032425\
Data File : FB031612.D
Signal(s) : FID2B.CH
Acq On : 24 Mar 2025 17:08
Operator : YP/AJ
Sample : Q1626-01
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 25 07:57:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030625.M
Quant Title :
QLast Update : Mon Mar 17 08:39:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	311099	13.738 ng/ml
Target Compounds			
6) t Toluene	10.624	7759	0.196 ng/ml
8) t m-Xylene	13.191	7793	0.202 ng/ml
9) t O-Xylene	13.925	11481	0.311 ng/ml
10) t 1,2,4-Trimethylbenzene	16.200	17976	0.636 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032425\
Data File : FB031612.D
Signal(s) : FID2B.CH
Acq On : 24 Mar 2025 17:08
Operator : YP/AJ
Sample : Q1626-01
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 25 07:57:37 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030625.M
Quant Title :
QLast Update : Mon Mar 17 08:39:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

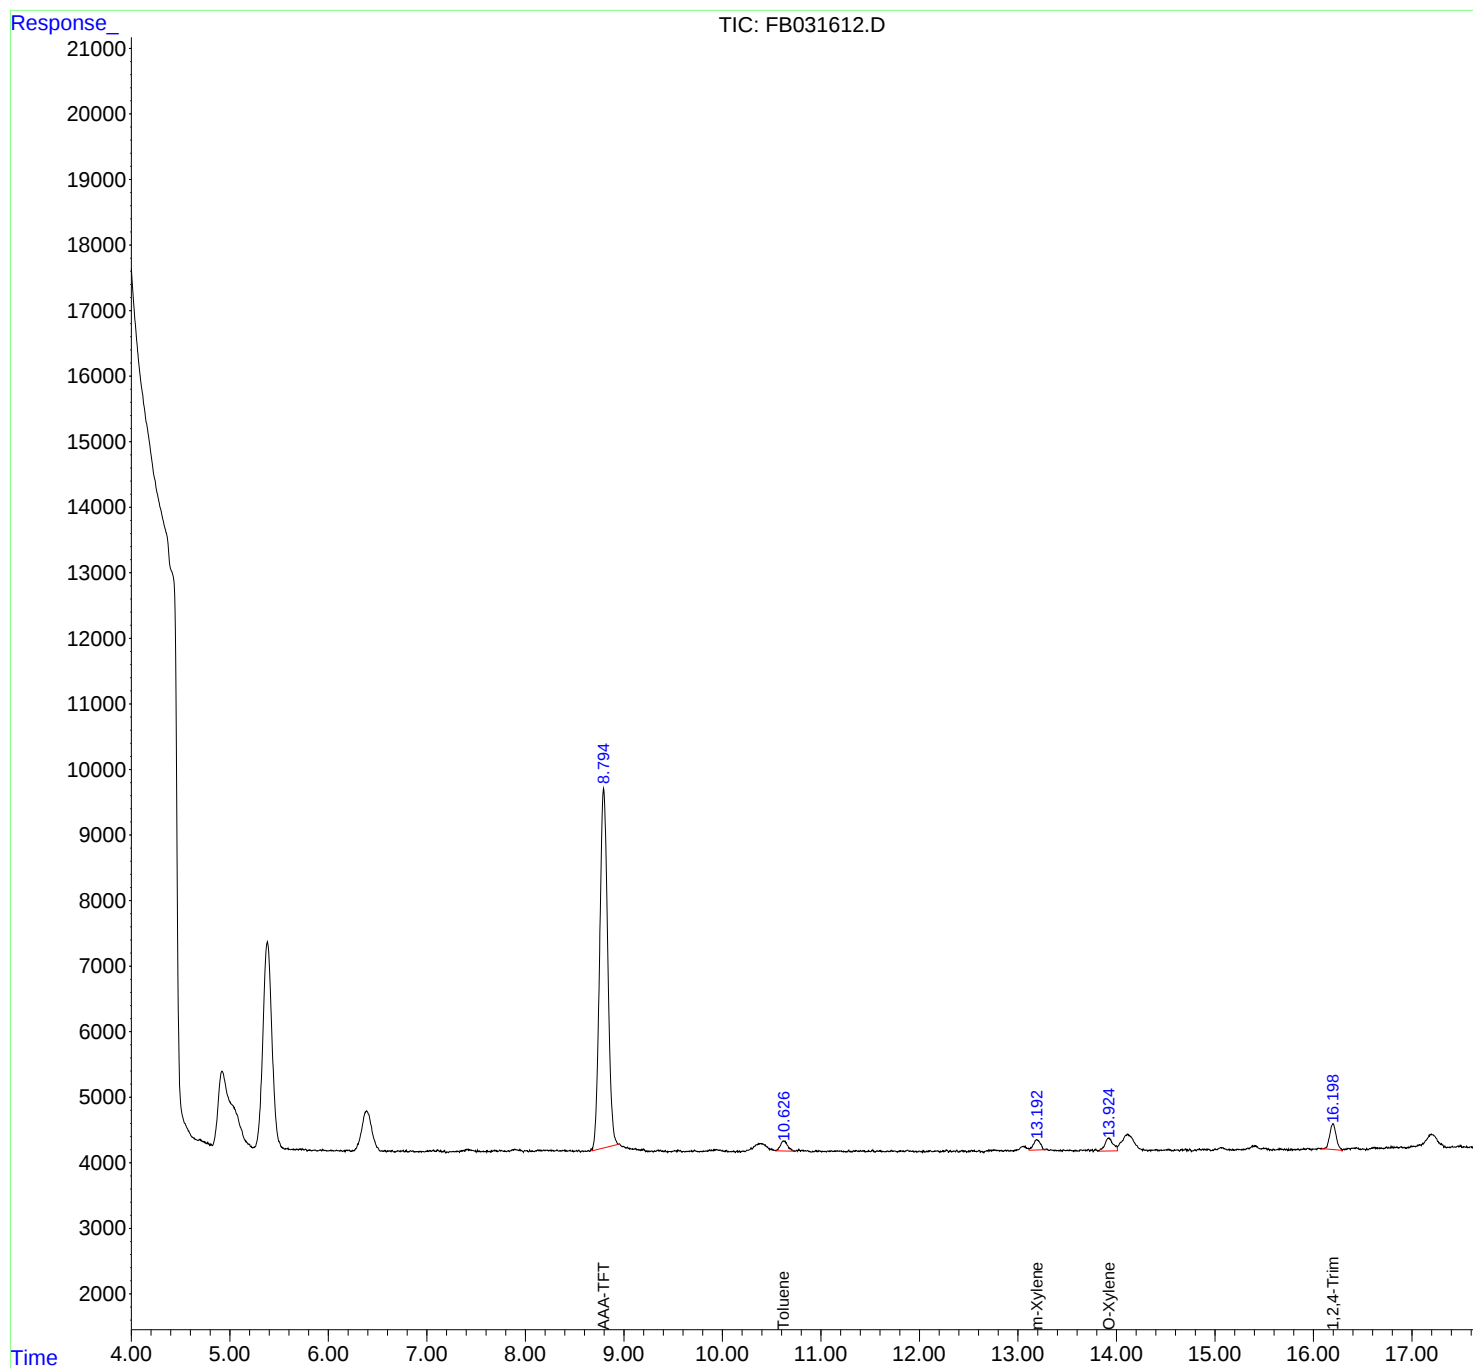


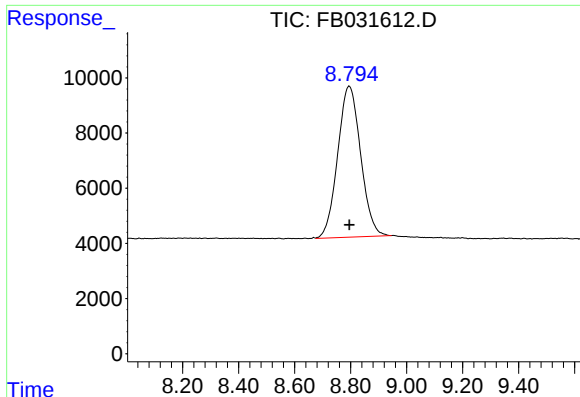

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.001 min
Response: 311099
Conc: 13.74 ng/ml

Instrument :
FID_B
ClientSampleId :

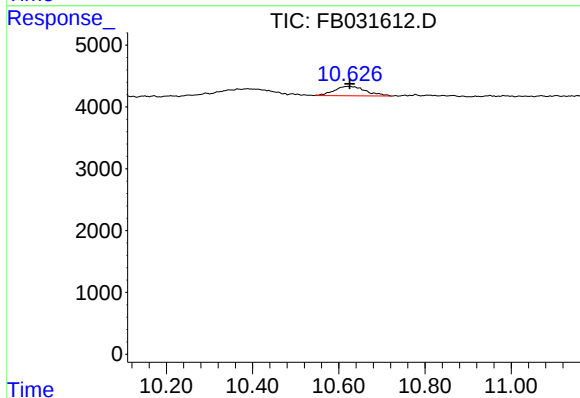


#6 Toluene

R.T.: 10.624 min
Delta R.T.: -0.002 min
Response: 7759
Conc: 0.20 ng/ml

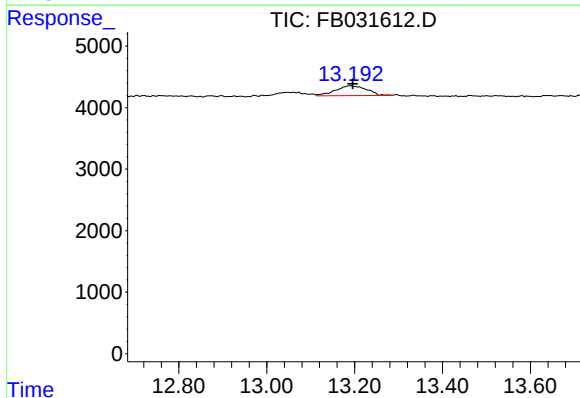


#8 m-Xylene

R.T.: 13.191 min
Delta R.T.: -0.004 min
Response: 7793
Conc: 0.20 ng/ml

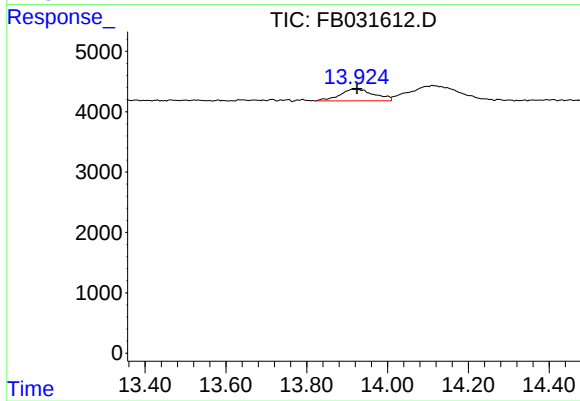

#9 O-Xylene

R.T.: 13.925 min
Delta R.T.: 0.000 min
Response: 11481
Conc: 0.31 ng/ml

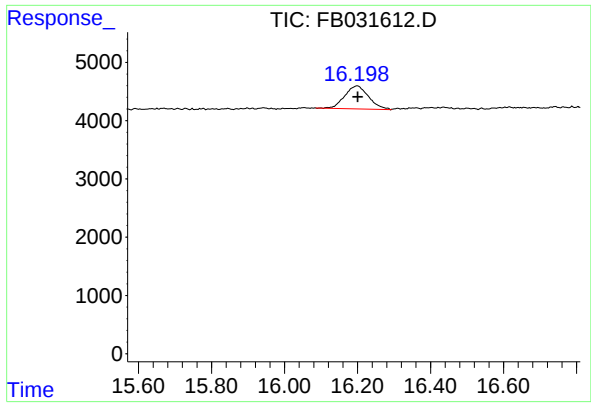

#10 1,2,4-Trimethylbenzene

R.T.: 16.200 min
Delta R.T.: 0.000 min
Response: 17976
Conc: 0.64 ng/ml

Instrument :
FID_B
ClientSampleId :