

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032425\
 Data File : FB031611.D
 Signal(s) : FID2B.CH
 Acq On : 24 Mar 2025 16:40
 Operator : YP/AJ
 Sample : BSF0324S1
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0324S1

Integration File: Calibration.e
 Quant Time: Mar 25 07:57:24 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030625.M
 Quant Title :
 QLast Update : Mon Mar 17 08:39:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	442676	19.549 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.725	1027192	40.388 ng/ml
2) t 2,2,4-Trimethylpentane	7.424	1210454	34.913 ng/ml
3) t n-Heptane	7.757	358378	11.577 ng/ml
4) t Benzene	7.896	449105	10.626 ng/ml
6) t Toluene	10.624	1278892	32.331 ng/ml
7) t Ethylbenzene	13.060	373865	10.600 ng/ml
8) t m-Xylene	13.194	818182	21.225 ng/ml
9) t O-Xylene	13.922	767354	20.793 ng/ml
10) t 1,2,4-Trimethylbenzene	16.198	567850	20.098 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032425\
Data File : FB031611.D
Signal(s) : FID2B.CH
Acq On : 24 Mar 2025 16:40
Operator : YP/AJ
Sample : BSF0324S1
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0324S1

Integration File: Calibration.e
Quant Time: Mar 25 07:57:24 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030625.M
Quant Title :
QLast Update : Mon Mar 17 08:39:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

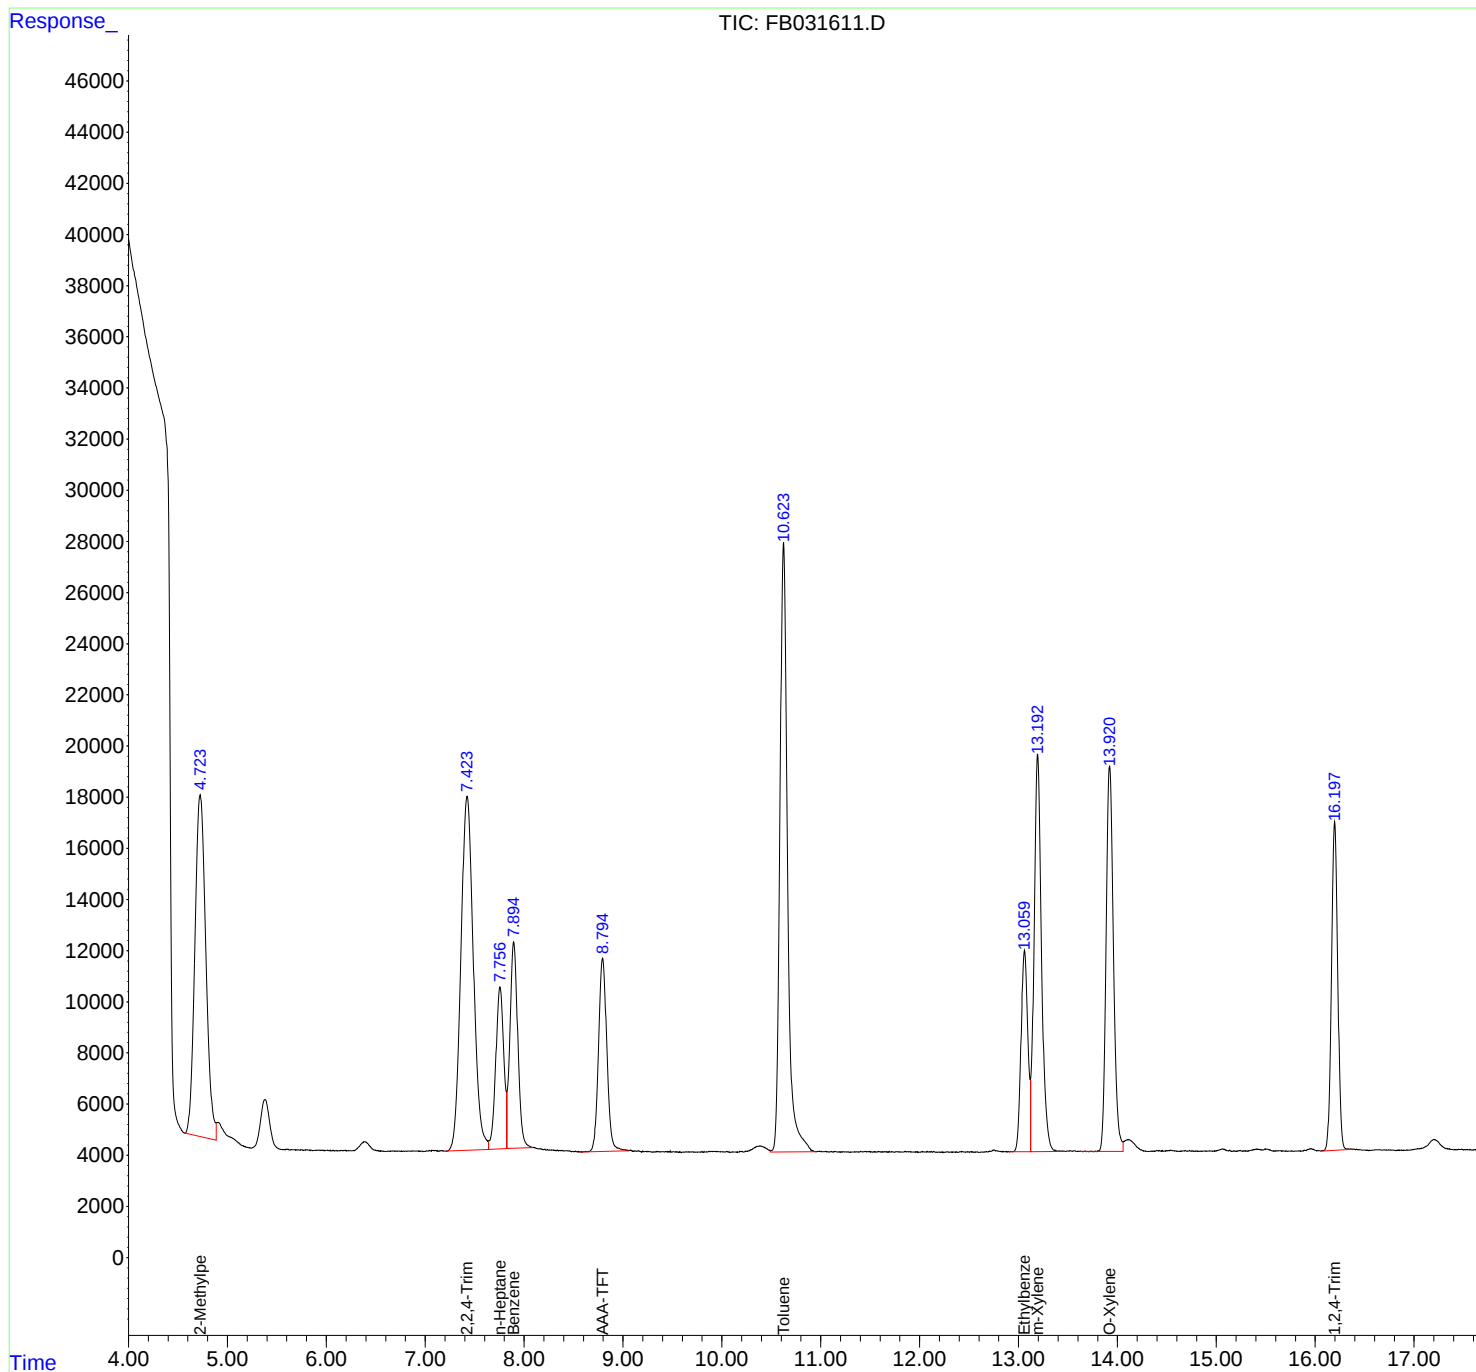


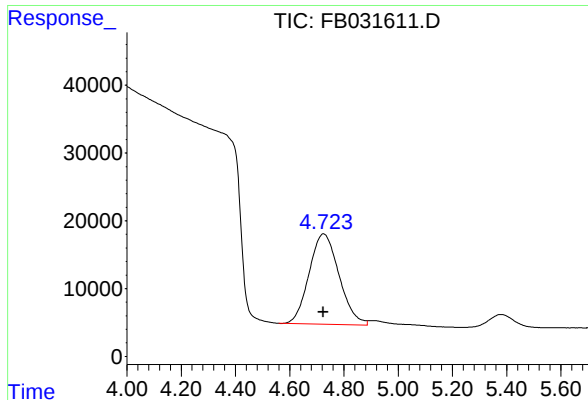

#1 2-Methylpentane


R.T.: 4.725 min
Delta R.T.: 0.000 min
Response: 1027192
Conc: 40.39 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0324S1

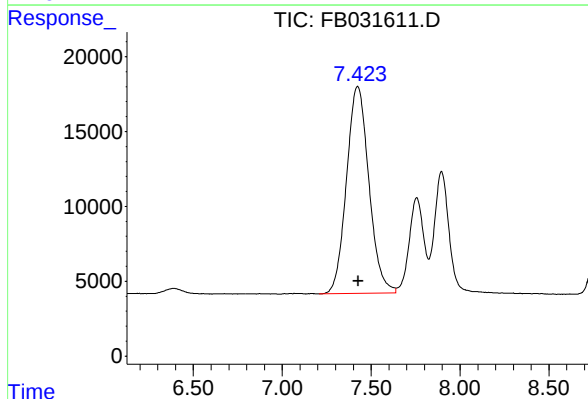


#2 2,2,4-Trimethylpentane

R.T.: 7.424 min
Delta R.T.: -0.004 min
Response: 1210454
Conc: 34.91 ng/ml

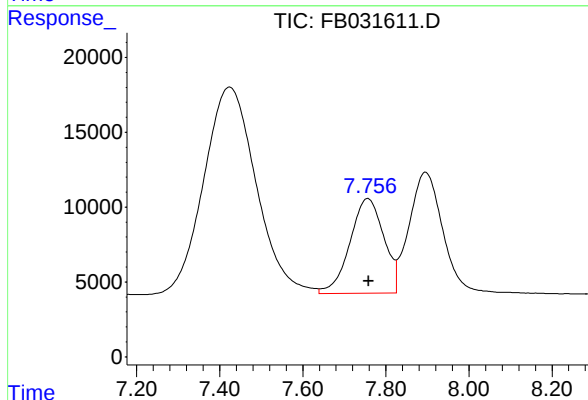


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: -0.002 min
Response: 358378
Conc: 11.58 ng/ml

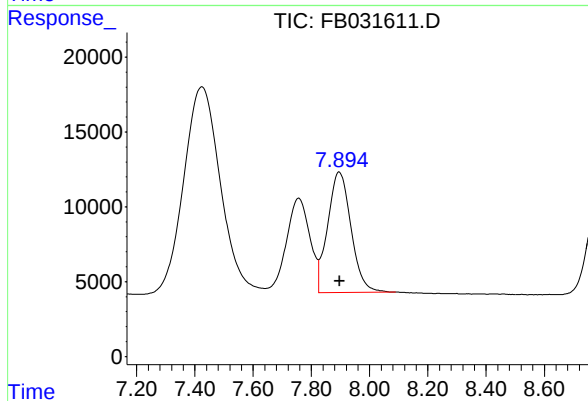

#4 Benzene


R.T.: 7.896 min
Delta R.T.: -0.001 min
Response: 449105
Conc: 10.63 ng/ml

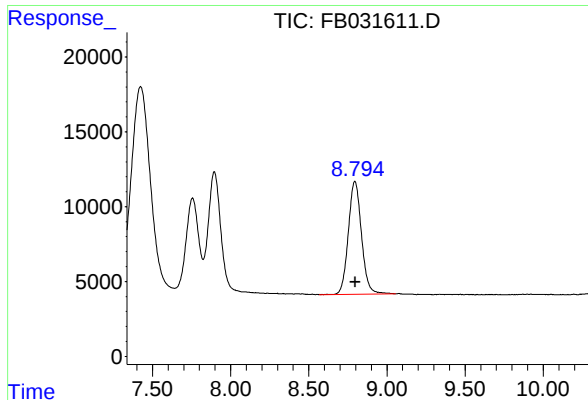

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: 0.000 min
Response: 442676
Conc: 19.55 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0324S1

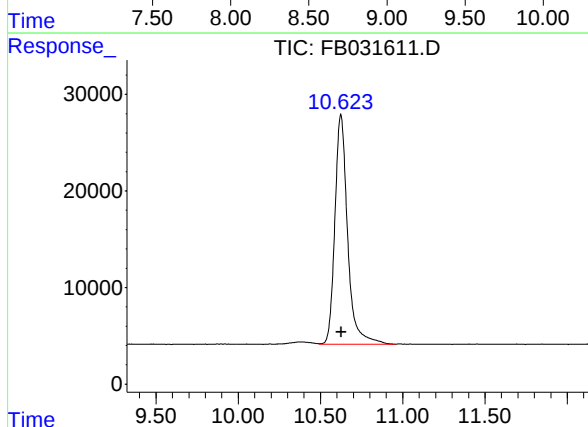


#6 Toluene

R.T.: 10.624 min
Delta R.T.: -0.001 min
Response: 1278892
Conc: 32.33 ng/ml

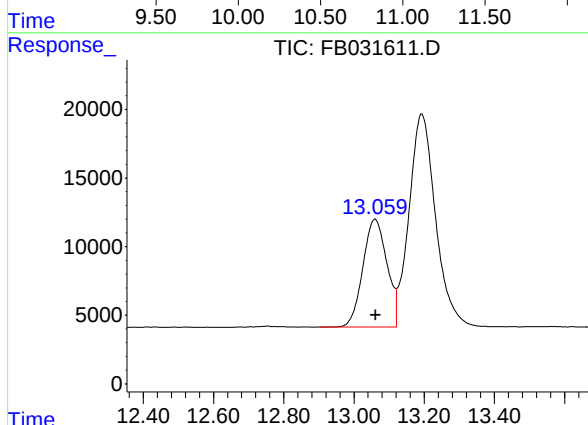


#7 Ethylbenzene

R.T.: 13.060 min
Delta R.T.: -0.002 min
Response: 373865
Conc: 10.60 ng/ml

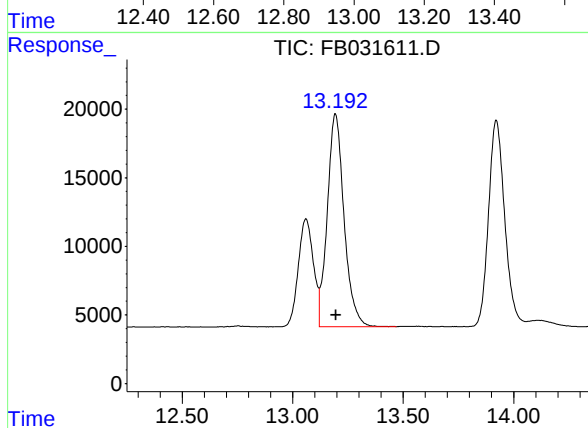

#8 m-Xylene


R.T.: 13.194 min
Delta R.T.: -0.002 min
Response: 818182
Conc: 21.23 ng/ml

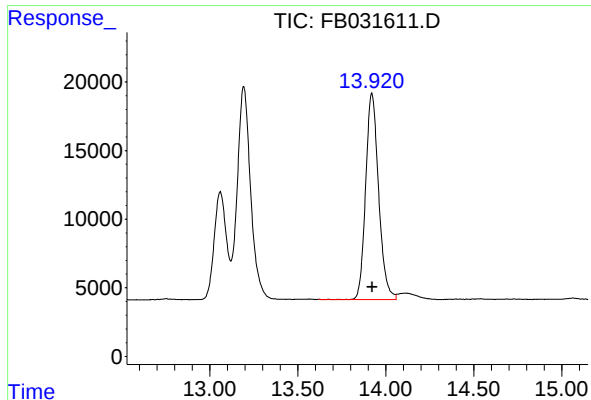

#9 O-Xylene

R.T.: 13.922 min
Delta R.T.: -0.003 min
Response: 767354
Conc: 20.79 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0324S1

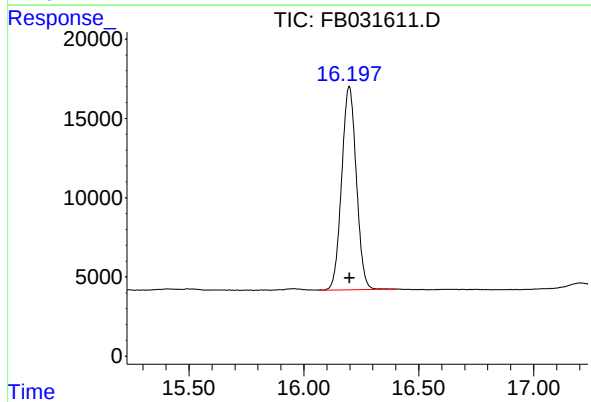

#10 1,2,4-Trimethylbenzene

R.T.: 16.198 min
Delta R.T.: -0.003 min
Response: 567850
Conc: 20.10 ng/ml