

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032425\
 Data File : FB031613.D
 Signal(s) : FID2B.CH
 Acq On : 24 Mar 2025 18:29
 Operator : YP/AJ
 Sample : BSF0324S2
 Misc : 5.00G/5.00 ML DI WATER
 ALS Vial : 8 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0324S2

Integration File: Calibration.e
 Quant Time: Mar 25 07:57:49 2025
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030625.M
 Quant Title :
 QLast Update : Mon Mar 17 08:39:01 2025
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.795	509120	22.483 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.726	1046783	41.158 ng/ml
2) t 2,2,4-Trimethylpentane	7.423	1247304	35.976 ng/ml
3) t n-Heptane	7.757	372958	12.048 ng/ml
4) t Benzene	7.896	472518	11.180 ng/ml
6) t Toluene	10.625	1291586	32.652 ng/ml
7) t Ethylbenzene	13.061	374647	10.622 ng/ml
8) t m-Xylene	13.195	818894	21.244 ng/ml
9) t O-Xylene	13.923	769704	20.857 ng/ml
10) t 1,2,4-Trimethylbenzene	16.199	547998	19.395 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032425\
Data File : FB031613.D
Signal(s) : FID2B.CH
Acq On : 24 Mar 2025 18:29
Operator : YP/AJ
Sample : BSF0324S2
Misc : 5.00G/5.00 ML DI WATER
ALS Vial : 8 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0324S2

Integration File: Calibration.e
Quant Time: Mar 25 07:57:49 2025
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030625.M
Quant Title :
QLast Update : Mon Mar 17 08:39:01 2025
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

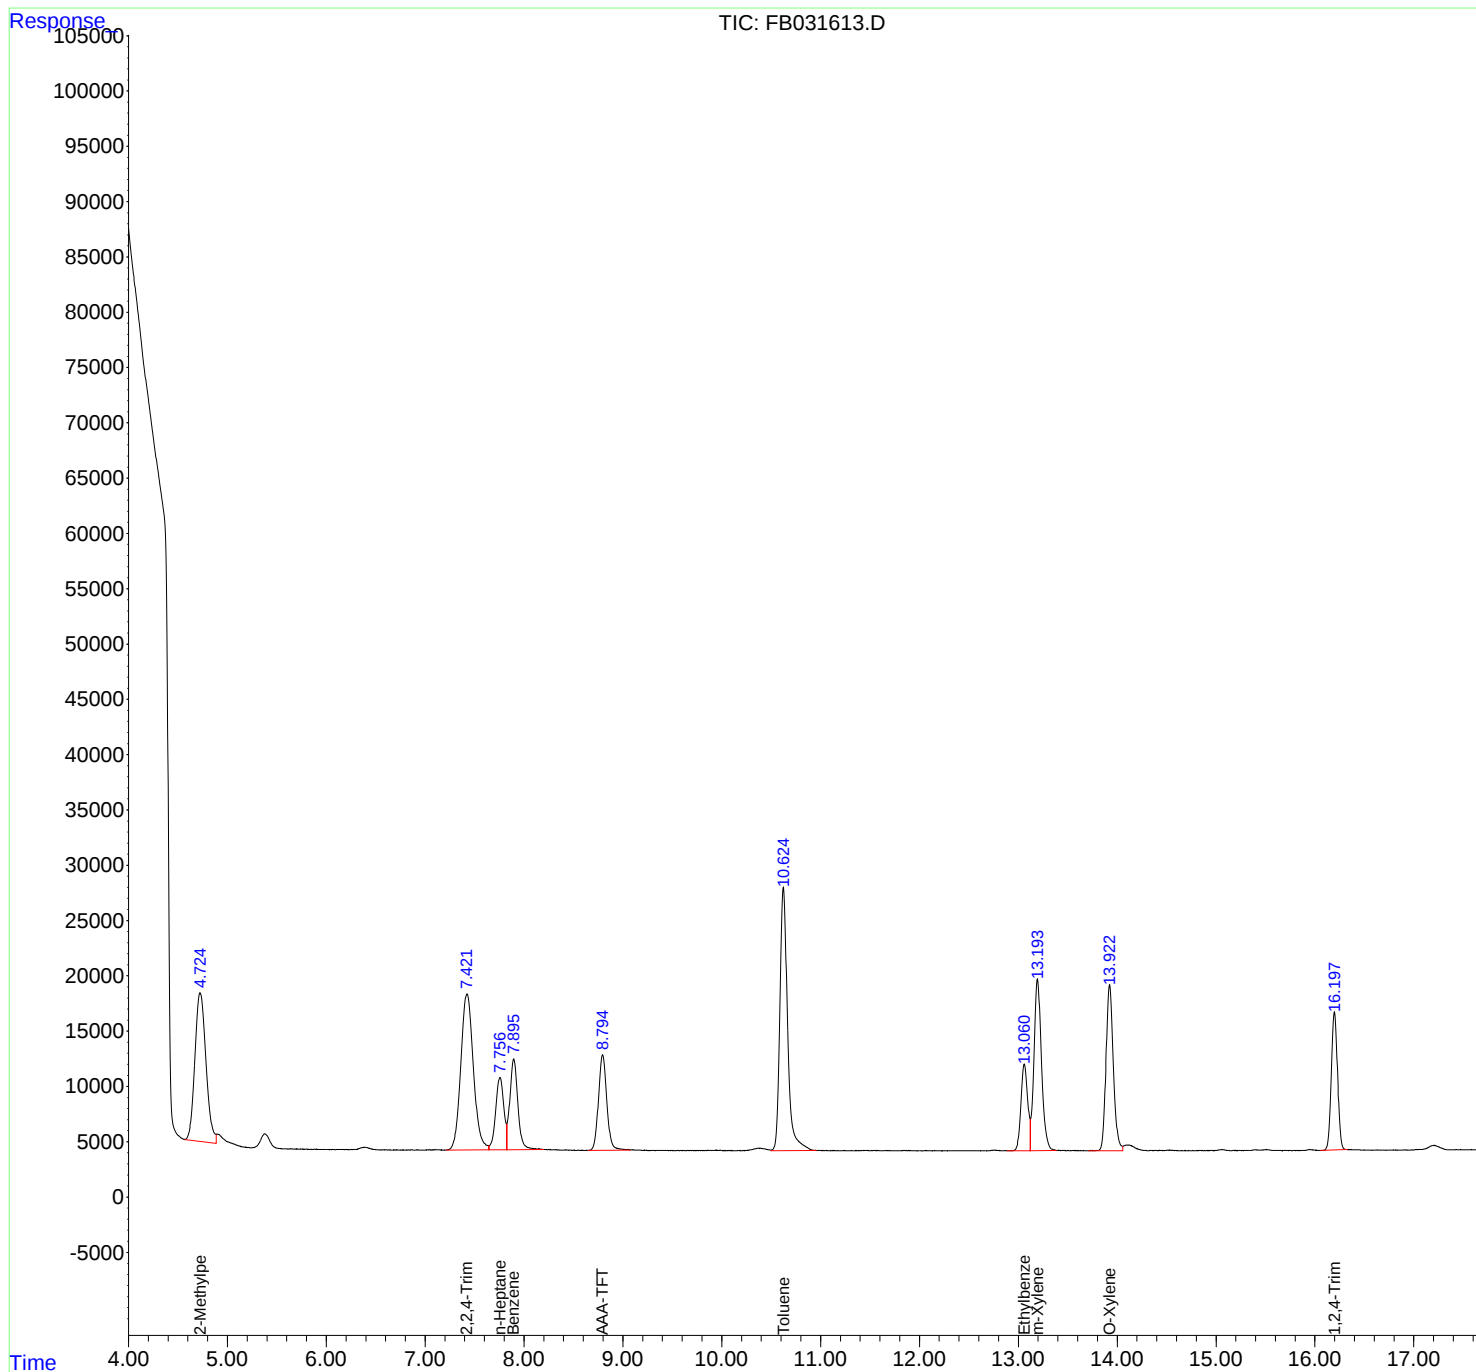


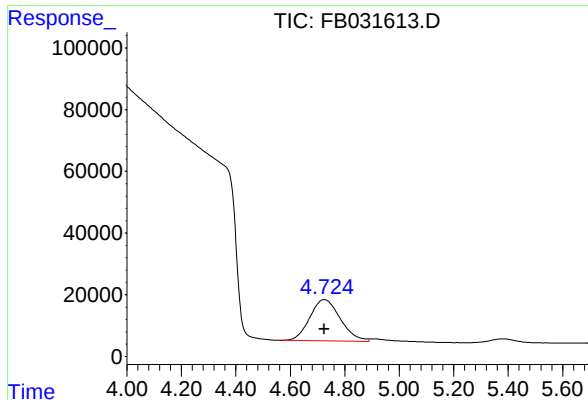

#1 2-Methylpentane


R.T.: 4.726 min
Delta R.T.: 0.002 min
Response: 1046783
Conc: 41.16 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0324S2

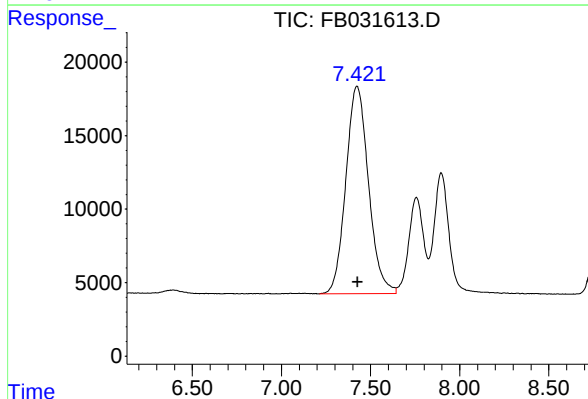


#2 2,2,4-Trimethylpentane

R.T.: 7.423 min
Delta R.T.: -0.005 min
Response: 1247304
Conc: 35.98 ng/ml

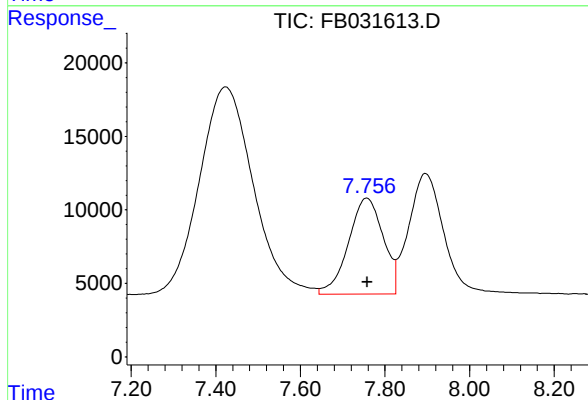


#3 n-Heptane

R.T.: 7.757 min
Delta R.T.: -0.001 min
Response: 372958
Conc: 12.05 ng/ml

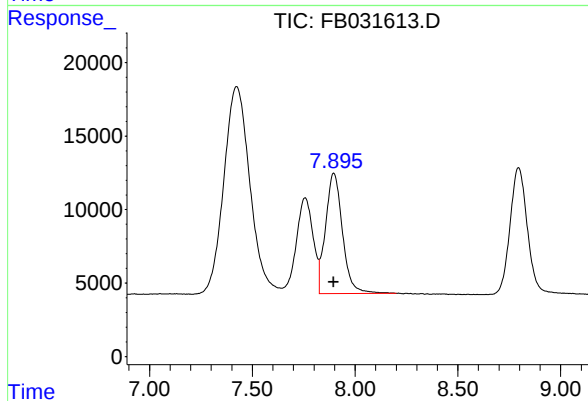

#4 Benzene


R.T.: 7.896 min
Delta R.T.: 0.000 min
Response: 472518
Conc: 11.18 ng/ml

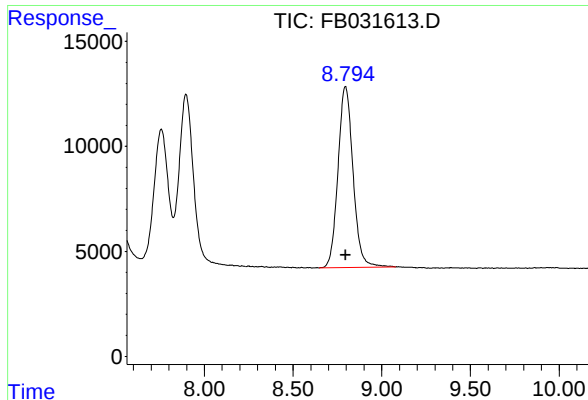

#5 AAA-TFT


R.T.: 8.795 min
Delta R.T.: -0.001 min
Response: 509120
Conc: 22.48 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0324S2

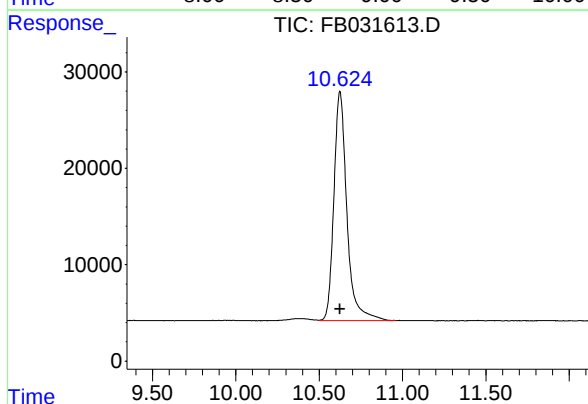


#6 Toluene

R.T.: 10.625 min
Delta R.T.: 0.000 min
Response: 1291586
Conc: 32.65 ng/ml

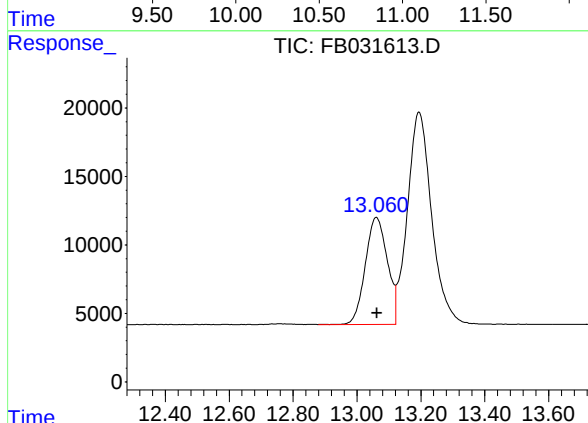


#7 Ethylbenzene

R.T.: 13.061 min
Delta R.T.: -0.001 min
Response: 374647
Conc: 10.62 ng/ml

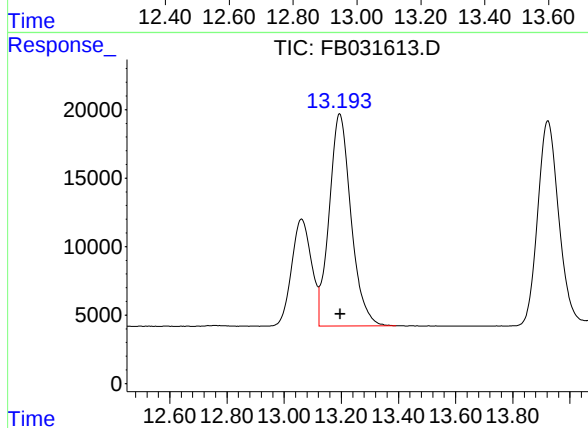

#8 m-Xylene


R.T.: 13.195 min
Delta R.T.: -0.001 min
Response: 818894
Conc: 21.24 ng/ml

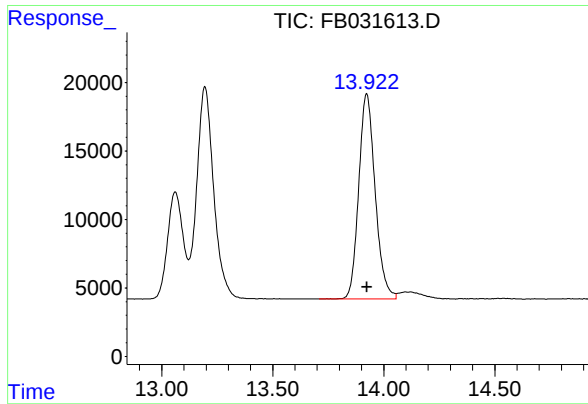

#9 O-Xylene

R.T.: 13.923 min
Delta R.T.: -0.001 min
Response: 769704
Conc: 20.86 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0324S2

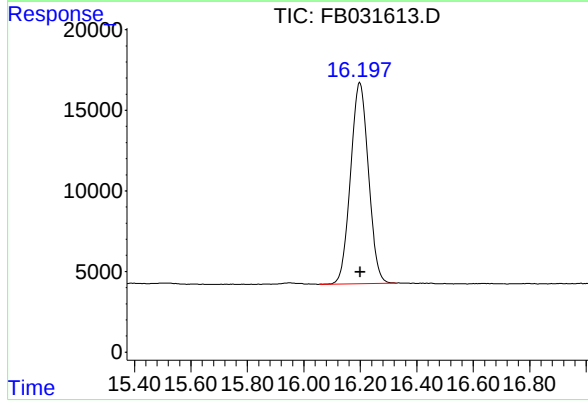

#10 1,2,4-Trimethylbenzene

R.T.: 16.199 min
Delta R.T.: -0.002 min
Response: 547998
Conc: 19.40 ng/ml