

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032619\
 Data File : FB020353.D
 Signal(s) : FID2B.CH
 Acq On : 26 Mar 2019 11:24
 Operator : MJ/SJ
 Sample : 20 GRO STD
 Misc :
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 20 GRO STD

Integration File: Calibration.e
 Quant Time: Mar 26 12:02:18 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
 Quant Title :
 QLast Update : Tue Mar 26 12:00:57 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.040	393202	20.000 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.899	837983	30.000 ng/ml
2) t 2,2,4-Trimethylpentane	7.666	718379	30.000 ng/ml
3) t n-Heptane	7.995	325648	10.000 ng/ml
4) t Benzene	8.133	351601	10.000 ng/ml
6) t Toluene	10.888	772900	30.000 ng/ml
7) t Ethylbenzene	13.340	191051	10.000 ng/ml
8) t m-Xylene	13.473	389201	20.000 ng/ml
9) t O-Xylene	14.205	388323	20.000 ng/ml
10) t 1,2,4-Trimethylbenzene	16.491	397964	20.000 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032619\
Data File : FB020353.D
Signal(s) : FID2B.CH
Acq On : 26 Mar 2019 11:24
Operator : MJ/SJ
Sample : 20 GRO STD
Misc :
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
20 GRO STD

Integration File: Calibration.e
Quant Time: Mar 26 12:02:18 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
Quant Title :
QLast Update : Tue Mar 26 12:00:57 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

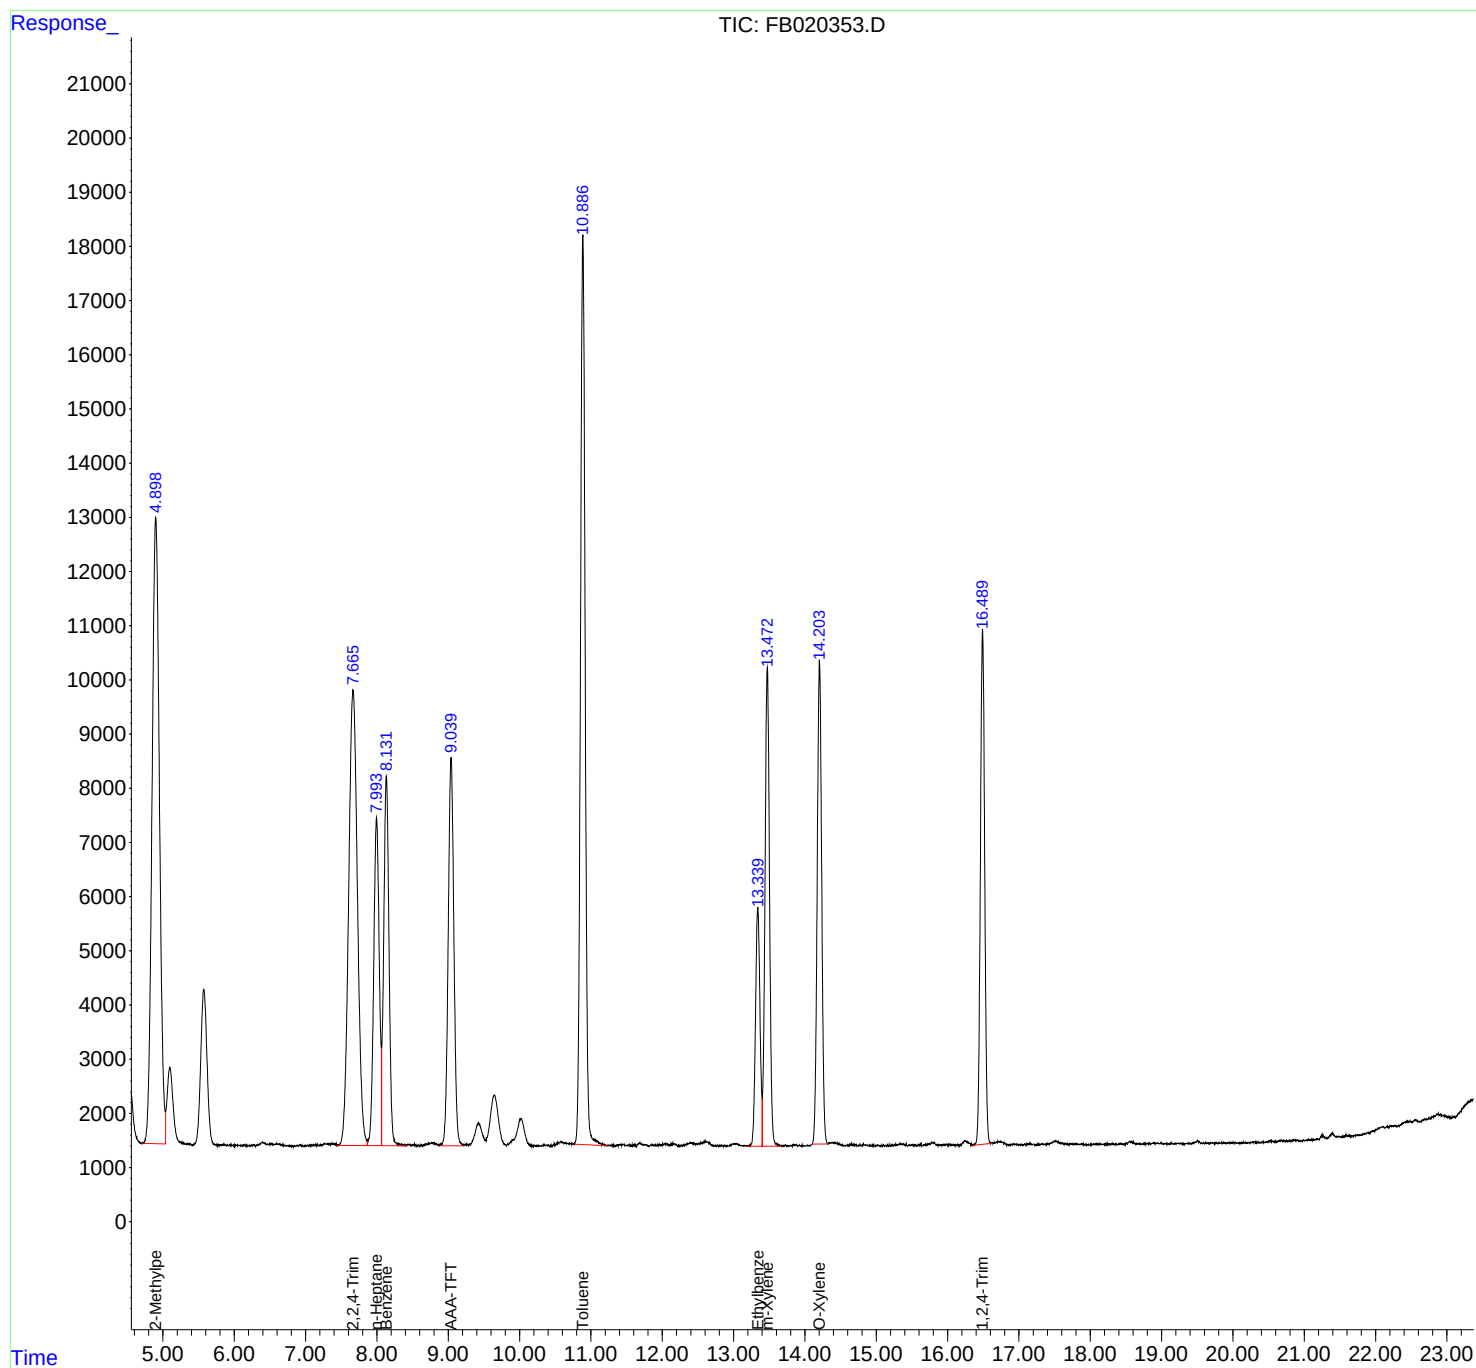


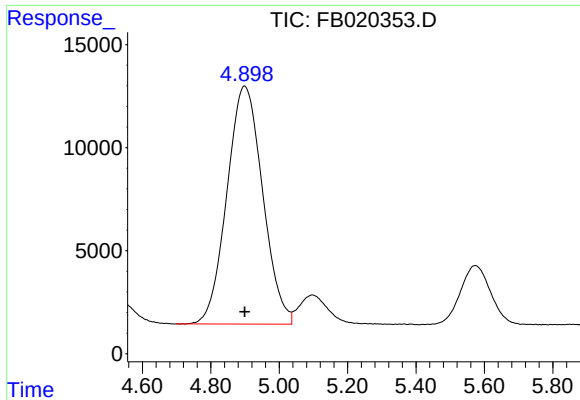

#1 2-Methylpentane


R.T.: 4.899 min
Delta R.T.: 0.000 min
Response: 837983
Conc: 30.00 ng/ml

Instrument :
FID_B
ClientSampleId :
20 GRO STD

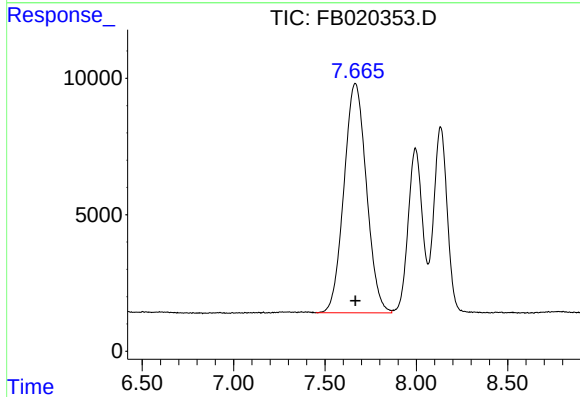


#2 2,2,4-Trimethylpentane

R.T.: 7.666 min
Delta R.T.: 0.000 min
Response: 718379
Conc: 30.00 ng/ml

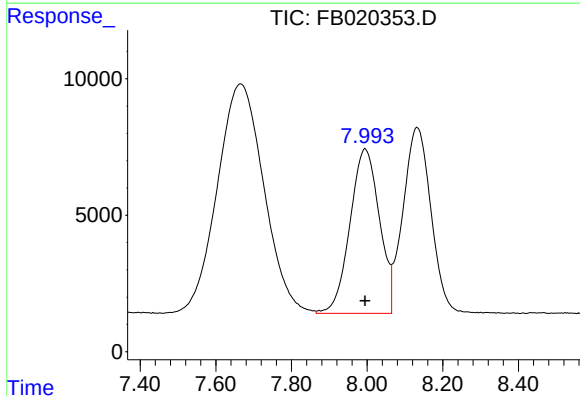


#3 n-Heptane

R.T.: 7.995 min
Delta R.T.: 0.000 min
Response: 325648
Conc: 10.00 ng/ml

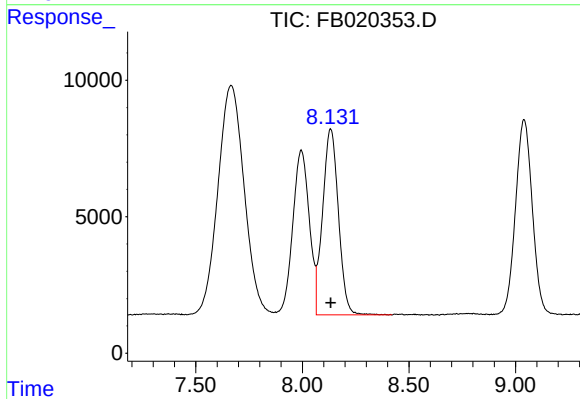

#4 Benzene


R.T.: 8.133 min
Delta R.T.: 0.000 min
Response: 351601
Conc: 10.00 ng/ml

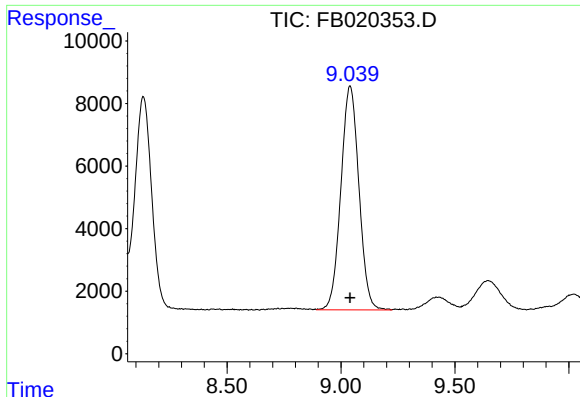

#5 AAA-TFT


R.T.: 9.040 min
Delta R.T.: 0.000 min
Response: 393202
Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :
20 GRO STD

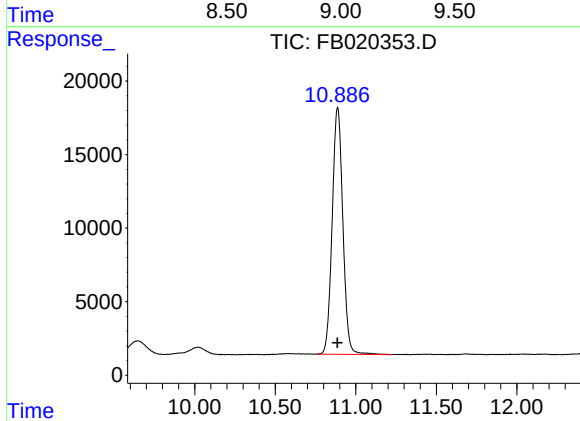


#6 Toluene

R.T.: 10.888 min
Delta R.T.: 0.000 min
Response: 772900
Conc: 30.00 ng/ml

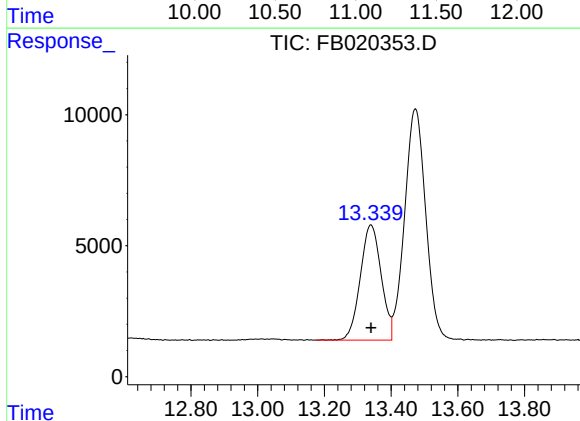


#7 Ethylbenzene

R.T.: 13.340 min
Delta R.T.: 0.000 min
Response: 191051
Conc: 10.00 ng/ml

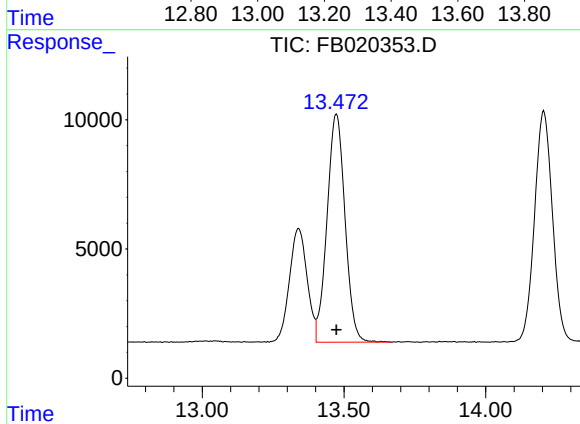

#8 m-Xylene


R.T.: 13.473 min
Delta R.T.: 0.000 min
Response: 389201
Conc: 20.00 ng/ml

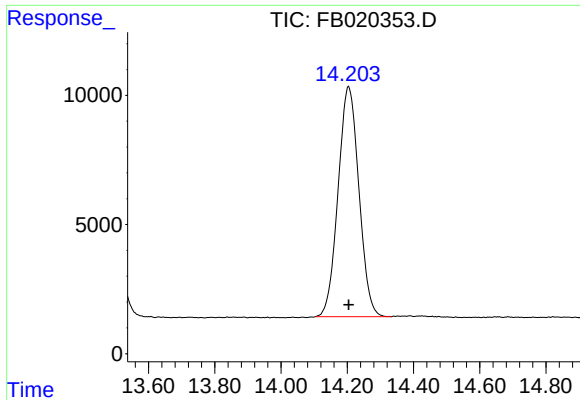

#9 O-Xylene

R.T.: 14.205 min
Delta R.T.: 0.000 min
Response: 388323
Conc: 20.00 ng/ml

Instrument :
FID_B
ClientSampleId :
20 GRO STD

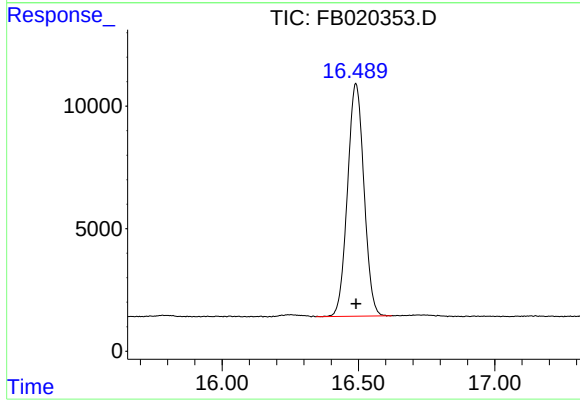

#10 1,2,4-Trimethylbenzene

R.T.: 16.491 min
Delta R.T.: 0.000 min
Response: 397964
Conc: 20.00 ng/ml