

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032619\
 Data File : FB020356.D
 Signal(s) : FID2B.CH
 Acq On : 26 Mar 2019 13:44
 Operator : MJ/SJ
 Sample : FB032619GROICV
 Misc :
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 FB032619GROICV

Integration File: Calibration.e
 Quant Time: Mar 26 14:39:17 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
 Quant Title :
 QLast Update : Tue Mar 26 12:48:09 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.040	380816	19.766 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.899	823004	29.692 ng/ml
2) t 2,2,4-Trimethylpentane	7.666	701450	29.252 ng/ml
3) t n-Heptane	7.995	317535	9.713 ng/ml
4) t Benzene	8.133	339575	9.805 ng/ml
6) t Toluene	10.887	757461	29.204 ng/ml
7) t Ethylbenzene	13.340	193987	9.854 ng/ml
8) t m-Xylene	13.473	396425	19.526 ng/ml
9) t O-Xylene	14.205	396871	19.595 ng/ml
10) t 1,2,4-Trimethylbenzene	16.492	406064	19.517 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032619\
Data File : FB020356.D
Signal(s) : FID2B.CH
Acq On : 26 Mar 2019 13:44
Operator : MJ/SJ
Sample : FB032619GROICV
Misc :
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
FB032619GROICV

Integration File: Calibration.e
Quant Time: Mar 26 14:39:17 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
Quant Title :
QLast Update : Tue Mar 26 12:48:09 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

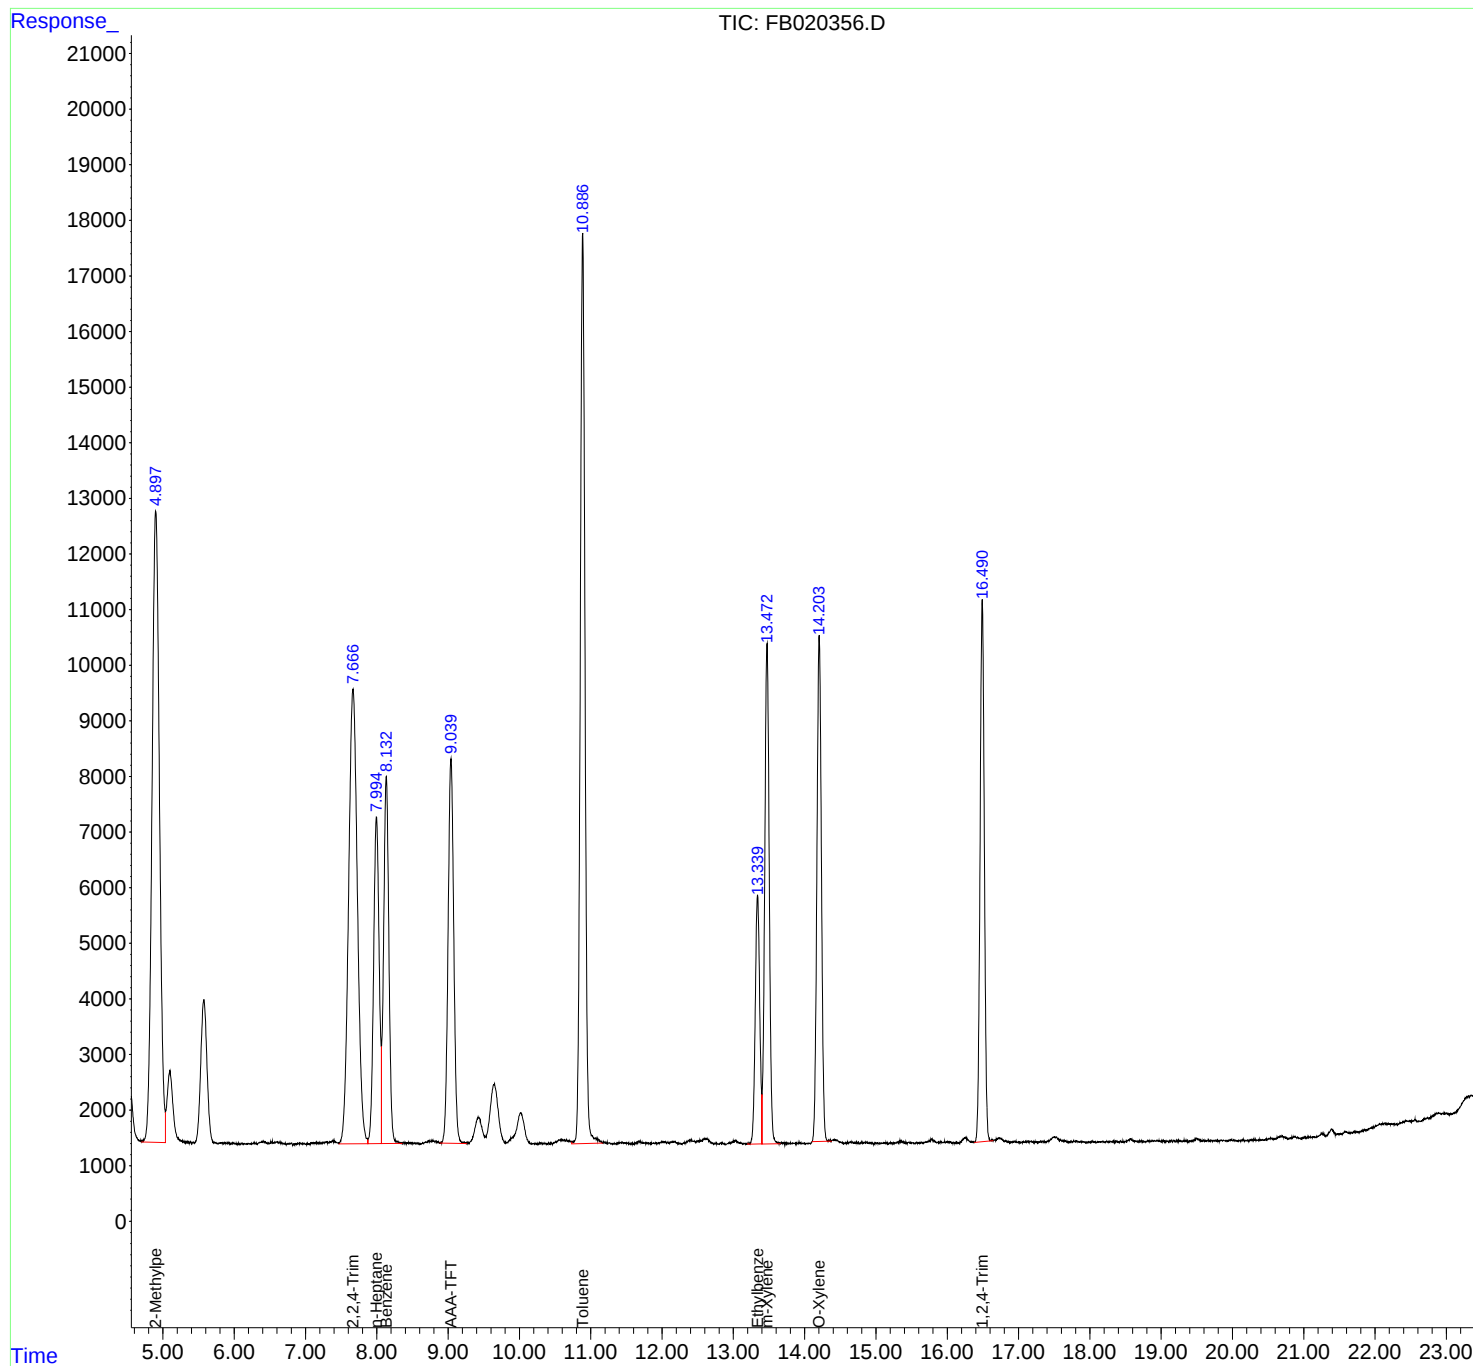


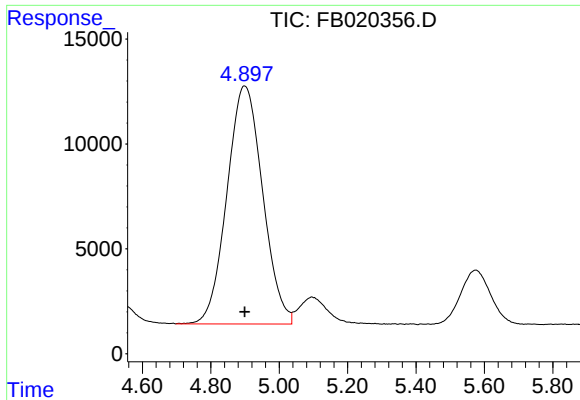

#1 2-Methylpentane


R.T.: 4.899 min
Delta R.T.: 0.000 min
Response: 823004
Conc: 29.69 ng/ml

Instrument :
FID_B
ClientSampleId :
FB032619GROICV

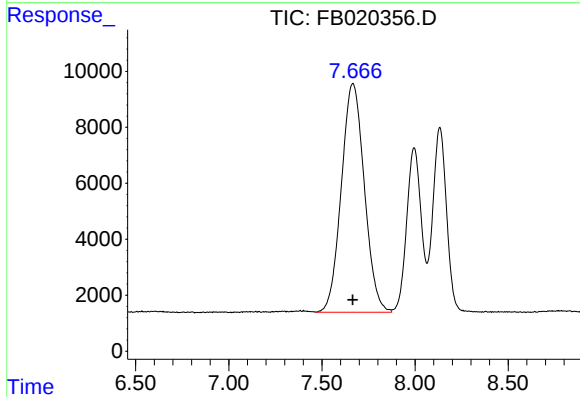


#2 2,2,4-Trimethylpentane

R.T.: 7.666 min
Delta R.T.: 0.000 min
Response: 701450
Conc: 29.25 ng/ml

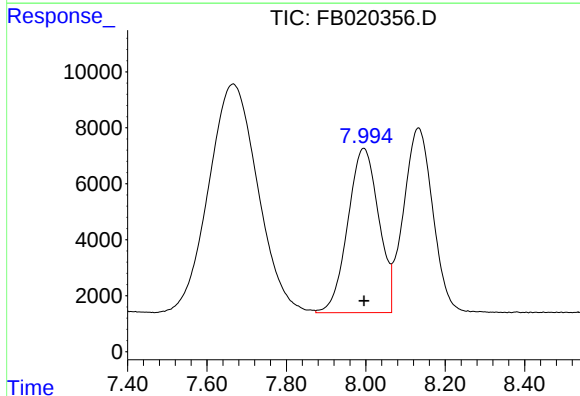


#3 n-Heptane

R.T.: 7.995 min
Delta R.T.: 0.000 min
Response: 317535
Conc: 9.71 ng/ml

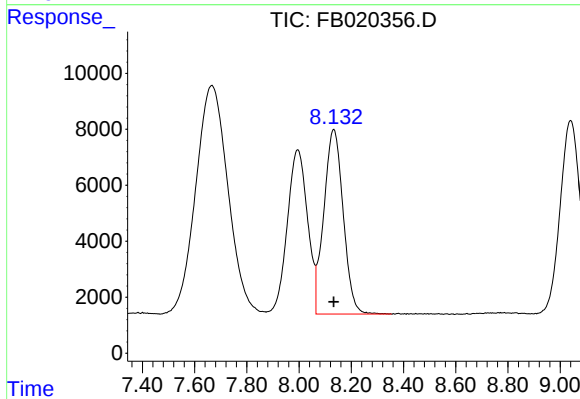


#4 Benzene

R.T.: 8.133 min
Delta R.T.: 0.000 min
Response: 339575
Conc: 9.81 ng/ml

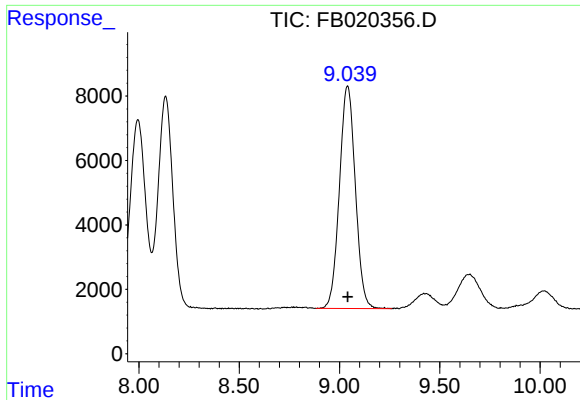


#5 AAA-TFT
 R.T.: 9.040 min
 Delta R.T.: 0.000 min
 Response: 380816
 Conc: 19.77 ng/ml


Instrument :
 FID_B
 ClientSampleId :
 FB032619GROICV

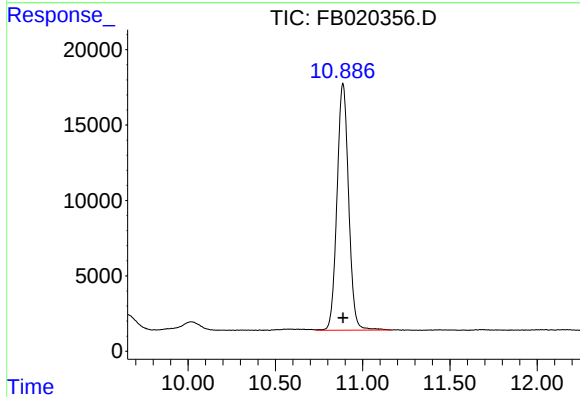


#6 Toluene
 R.T.: 10.887 min
 Delta R.T.: 0.000 min
 Response: 757461
 Conc: 29.20 ng/ml

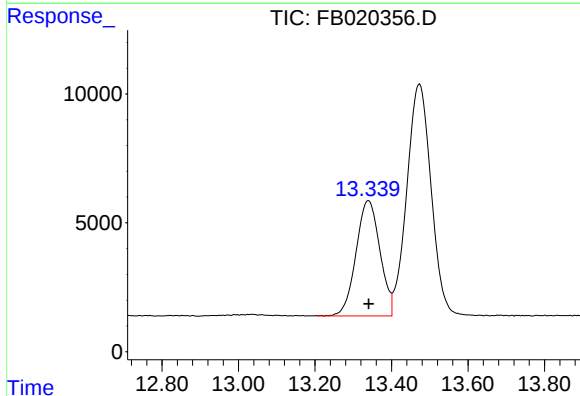

#7 Ethylbenzene
 R.T.: 13.340 min
 Delta R.T.: 0.000 min
 Response: 193987
 Conc: 9.85 ng/ml

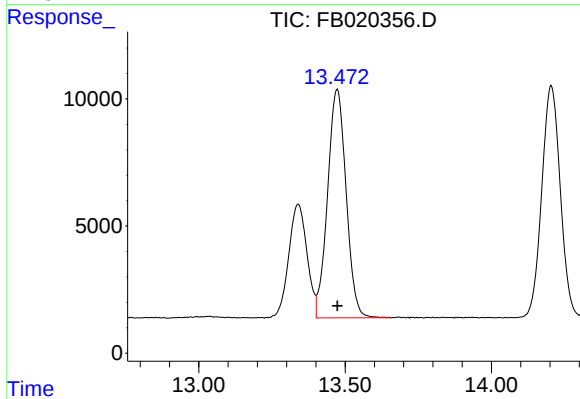


#8 m-Xylene
 R.T.: 13.473 min
 Delta R.T.: 0.000 min
 Response: 396425
 Conc: 19.53 ng/ml

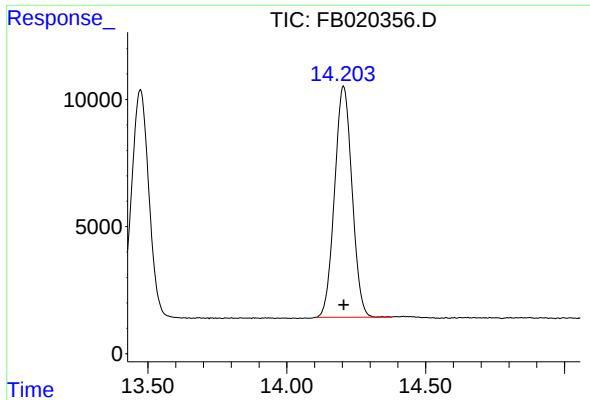

#9 O-Xylene

R.T.: 14.205 min
Delta R.T.: 0.000 min
Response: 396871
Conc: 19.60 ng/ml

Instrument :
FID_B
ClientSampleId :
FB032619GROICV

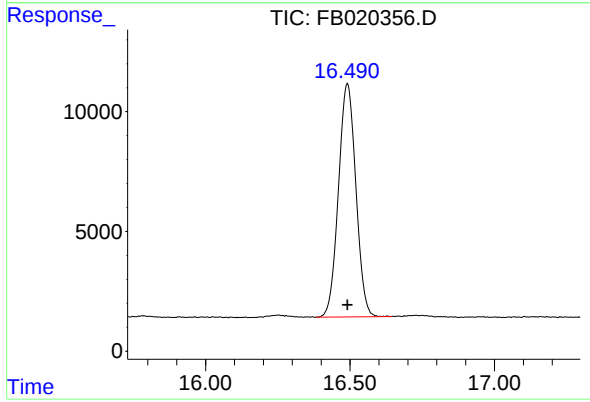

#10 1,2,4-Trimethylbenzene

R.T.: 16.492 min
Delta R.T.: 0.000 min
Response: 406064
Conc: 19.52 ng/ml