

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032619\
 Data File : FB020359.D
 Signal(s) : FID2B.CH
 Acq On : 26 Mar 2019 17:11
 Operator : MJ/SJ
 Sample : BSF0326S1
 Misc : 5.01gm/5.00ml DI WATER
 ALS Vial : 9 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0326S1

Integration File: Calibration.e
 Quant Time: Mar 27 02:16:49 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
 Quant Title :
 QLast Update : Tue Mar 26 12:48:09 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.041	453369	23.532 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.902	898423	32.413 ng/ml
2) t	2,2,4-Trimethylpentane	7.669	792525	33.050 ng/ml
3) t	n-Heptane	7.997	359805	11.005 ng/ml
4) t	Benzene	8.135	381343	11.011 ng/ml
6) t	Toluene	10.888	829856	31.995 ng/ml
7) t	Ethylbenzene	13.341	200006	10.159 ng/ml
8) t	m-Xylene	13.474	406690	20.031 ng/ml
9) t	O-Xylene	14.205	403339	19.915 ng/ml
10) t	1,2,4-Trimethylbenzene	16.491	417213	20.053 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032619\
Data File : FB020359.D
Signal(s) : FID2B.CH
Acq On : 26 Mar 2019 17:11
Operator : MJ/SJ
Sample : BSF0326S1
Misc : 5.01gm/5.00ml DI WATER
ALS Vial : 9 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0326S1

Integration File: Calibration.e
Quant Time: Mar 27 02:16:49 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
Quant Title :
QLast Update : Tue Mar 26 12:48:09 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

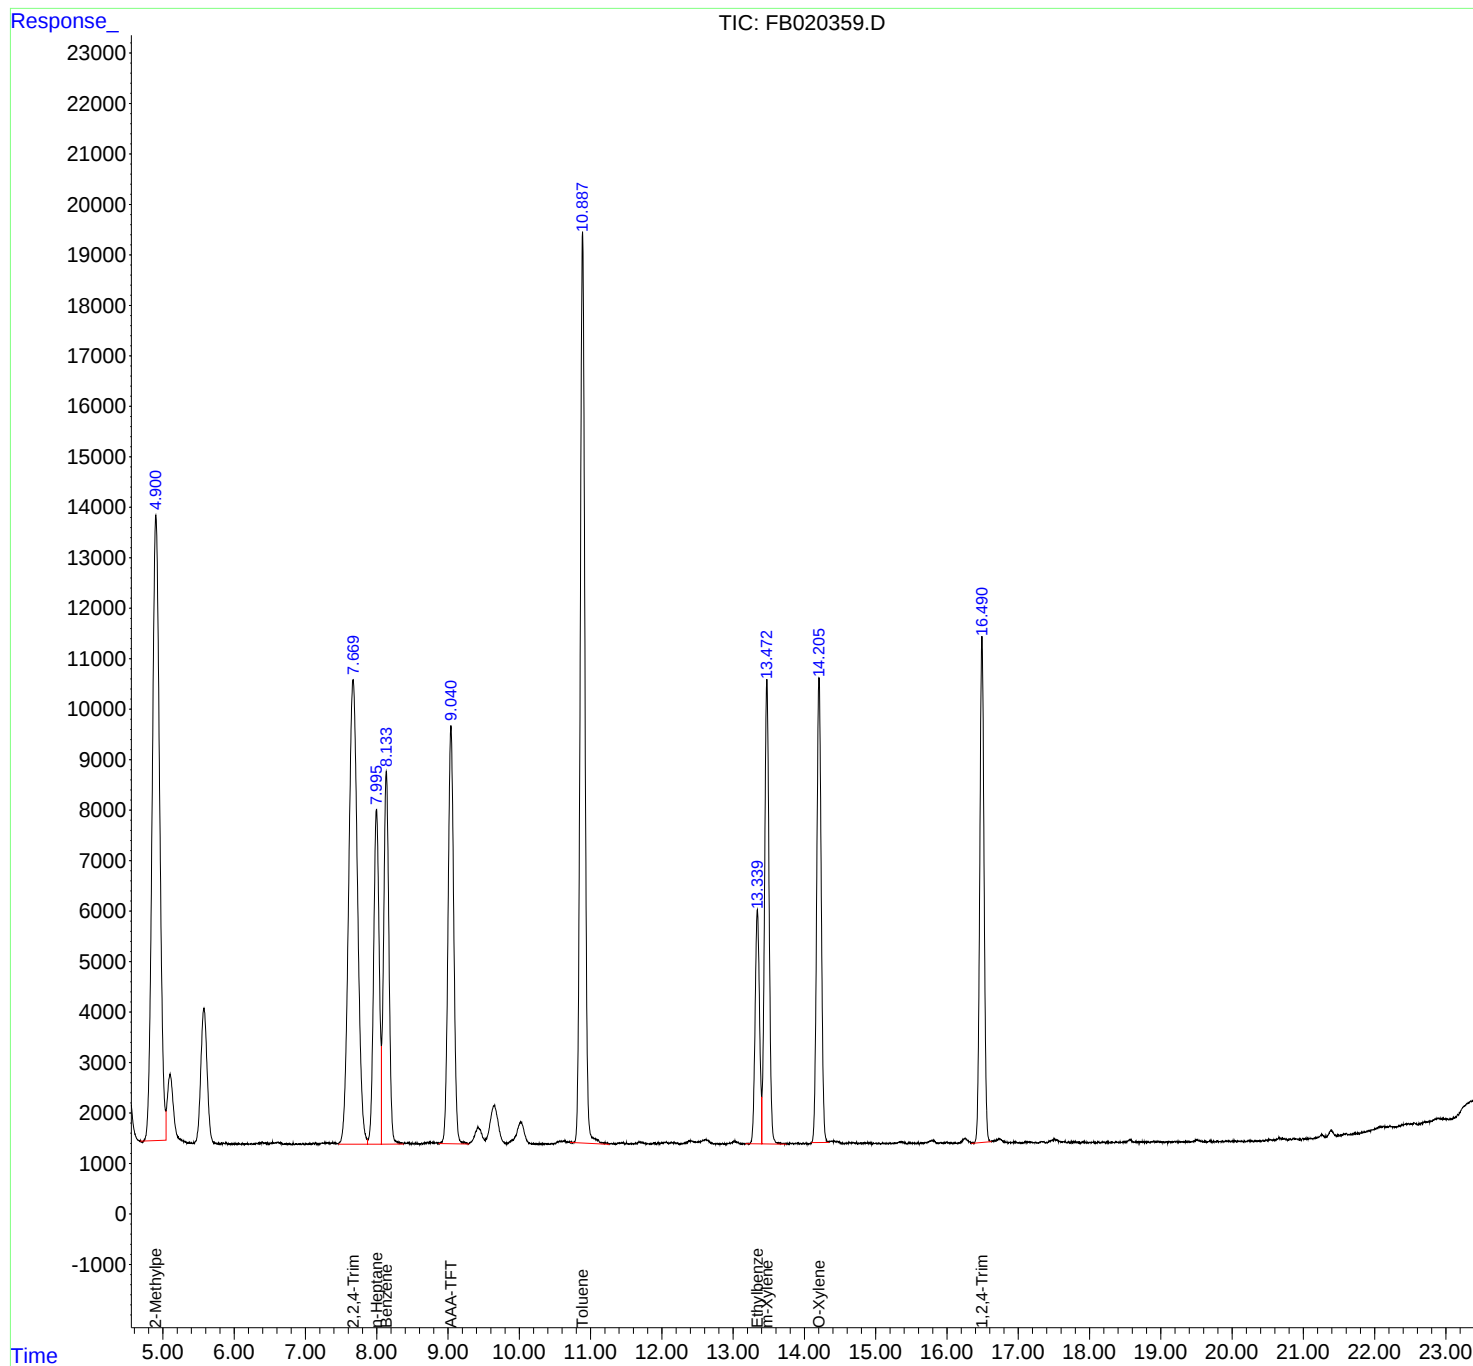


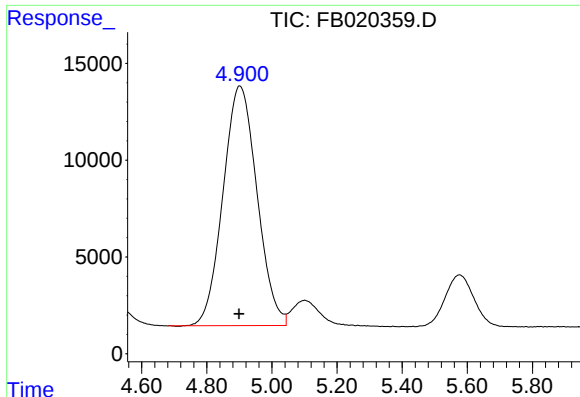

#1 2-Methylpentane


R.T.: 4.902 min
Delta R.T.: 0.003 min
Response: 898423
Conc: 32.41 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0326S1

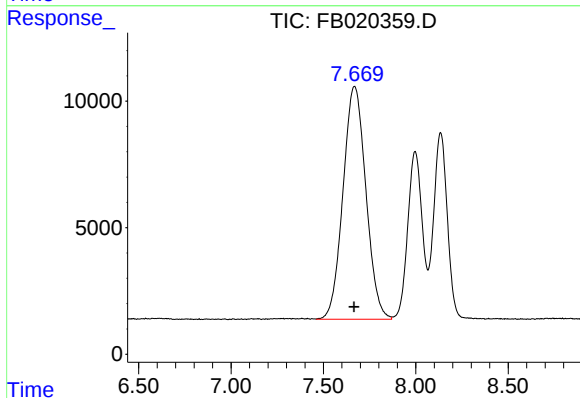


#2 2,2,4-Trimethylpentane

R.T.: 7.669 min
Delta R.T.: 0.002 min
Response: 792525
Conc: 33.05 ng/ml

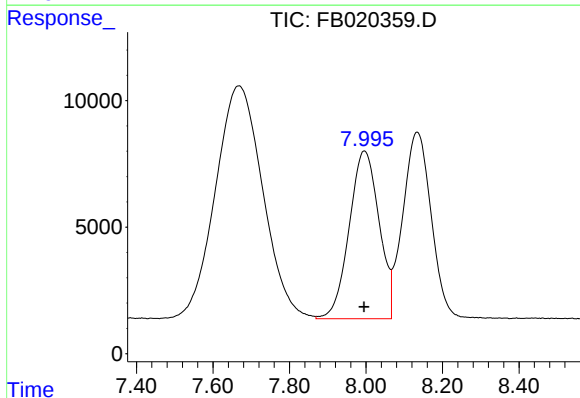


#3 n-Heptane

R.T.: 7.997 min
Delta R.T.: 0.001 min
Response: 359805
Conc: 11.01 ng/ml

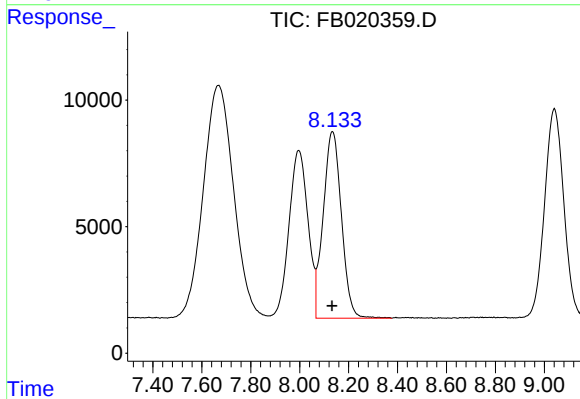

#4 Benzene


R.T.: 8.135 min
Delta R.T.: 0.002 min
Response: 381343
Conc: 11.01 ng/ml

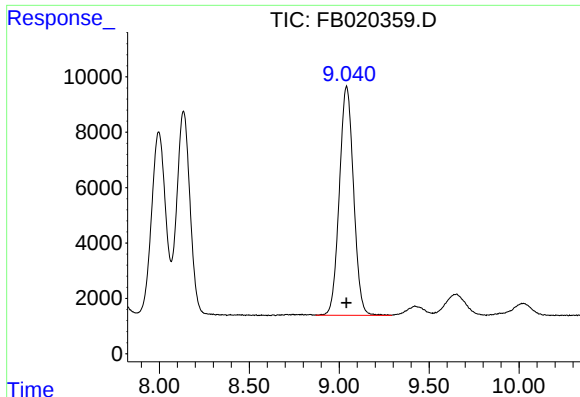

#5 AAA-TFT


R.T.: 9.041 min
Delta R.T.: 0.000 min
Response: 453369
Conc: 23.53 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0326S1

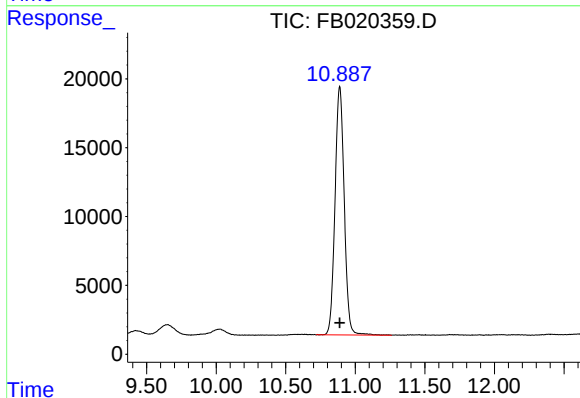


#6 Toluene

R.T.: 10.888 min
Delta R.T.: 0.000 min
Response: 829856
Conc: 32.00 ng/ml

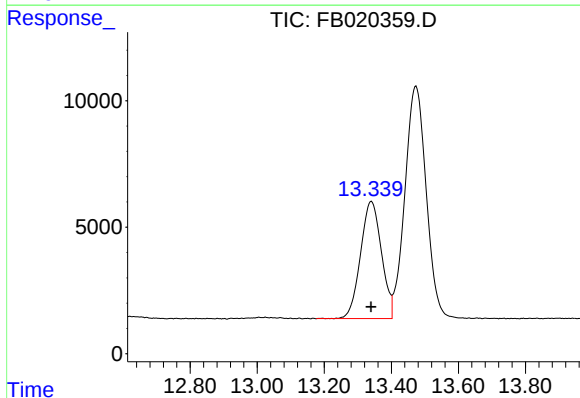


#7 Ethylbenzene

R.T.: 13.341 min
Delta R.T.: 0.000 min
Response: 200006
Conc: 10.16 ng/ml

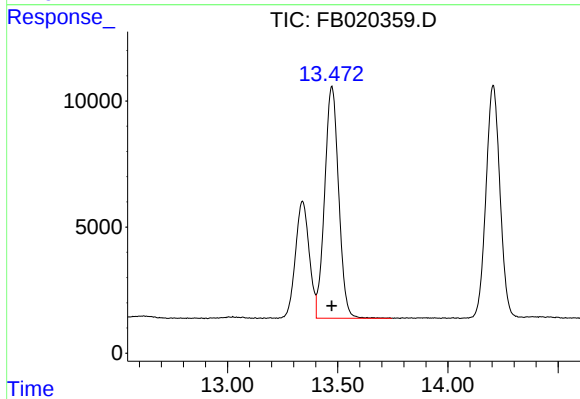

#8 m-Xylene


R.T.: 13.474 min
Delta R.T.: 0.000 min
Response: 406690
Conc: 20.03 ng/ml

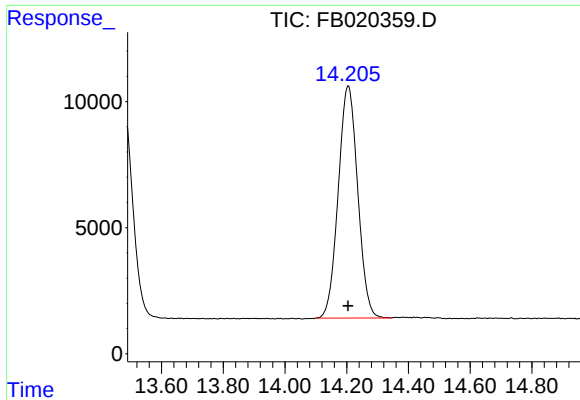

#9 O-Xylene

R.T.: 14.205 min
Delta R.T.: 0.000 min
Response: 403339
Conc: 19.91 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0326S1

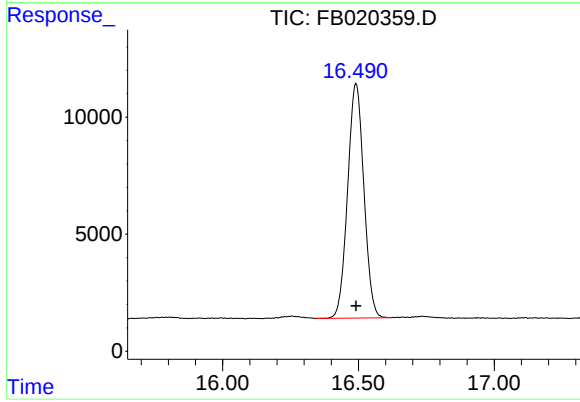

#10 1,2,4-Trimethylbenzene

R.T.: 16.491 min
Delta R.T.: 0.000 min
Response: 417213
Conc: 20.05 ng/ml