

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032619\
 Data File : FB020362.D
 Signal(s) : FID2B.CH
 Acq On : 26 Mar 2019 18:41
 Operator : MJ/SJ
 Sample : BSF0326W2
 Misc :
 ALS Vial : 12 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0326W2

Integration File: Calibration.e
 Quant Time: Mar 27 02:17:22 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
 Quant Title :
 QLast Update : Tue Mar 26 12:48:09 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.041	430996	22.370 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.901	893754	32.245 ng/ml
2) t 2,2,4-Trimethylpentane	7.666	778361	32.459 ng/ml
3) t n-Heptane	7.996	354114	10.831 ng/ml
4) t Benzene	8.134	376128	10.861 ng/ml
6) t Toluene	10.888	822198	31.700 ng/ml
7) t Ethylbenzene	13.341	202670	10.295 ng/ml
8) t m-Xylene	13.473	409685	20.179 ng/ml
9) t O-Xylene	14.205	406982	20.095 ng/ml
10) t 1,2,4-Trimethylbenzene	16.491	414967	19.945 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032619\
Data File : FB020362.D
Signal(s) : FID2B.CH
Acq On : 26 Mar 2019 18:41
Operator : MJ/SJ
Sample : BSF0326W2
Misc :
ALS Vial : 12 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0326W2

Integration File: Calibration.e
Quant Time: Mar 27 02:17:22 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
Quant Title :
QLast Update : Tue Mar 26 12:48:09 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

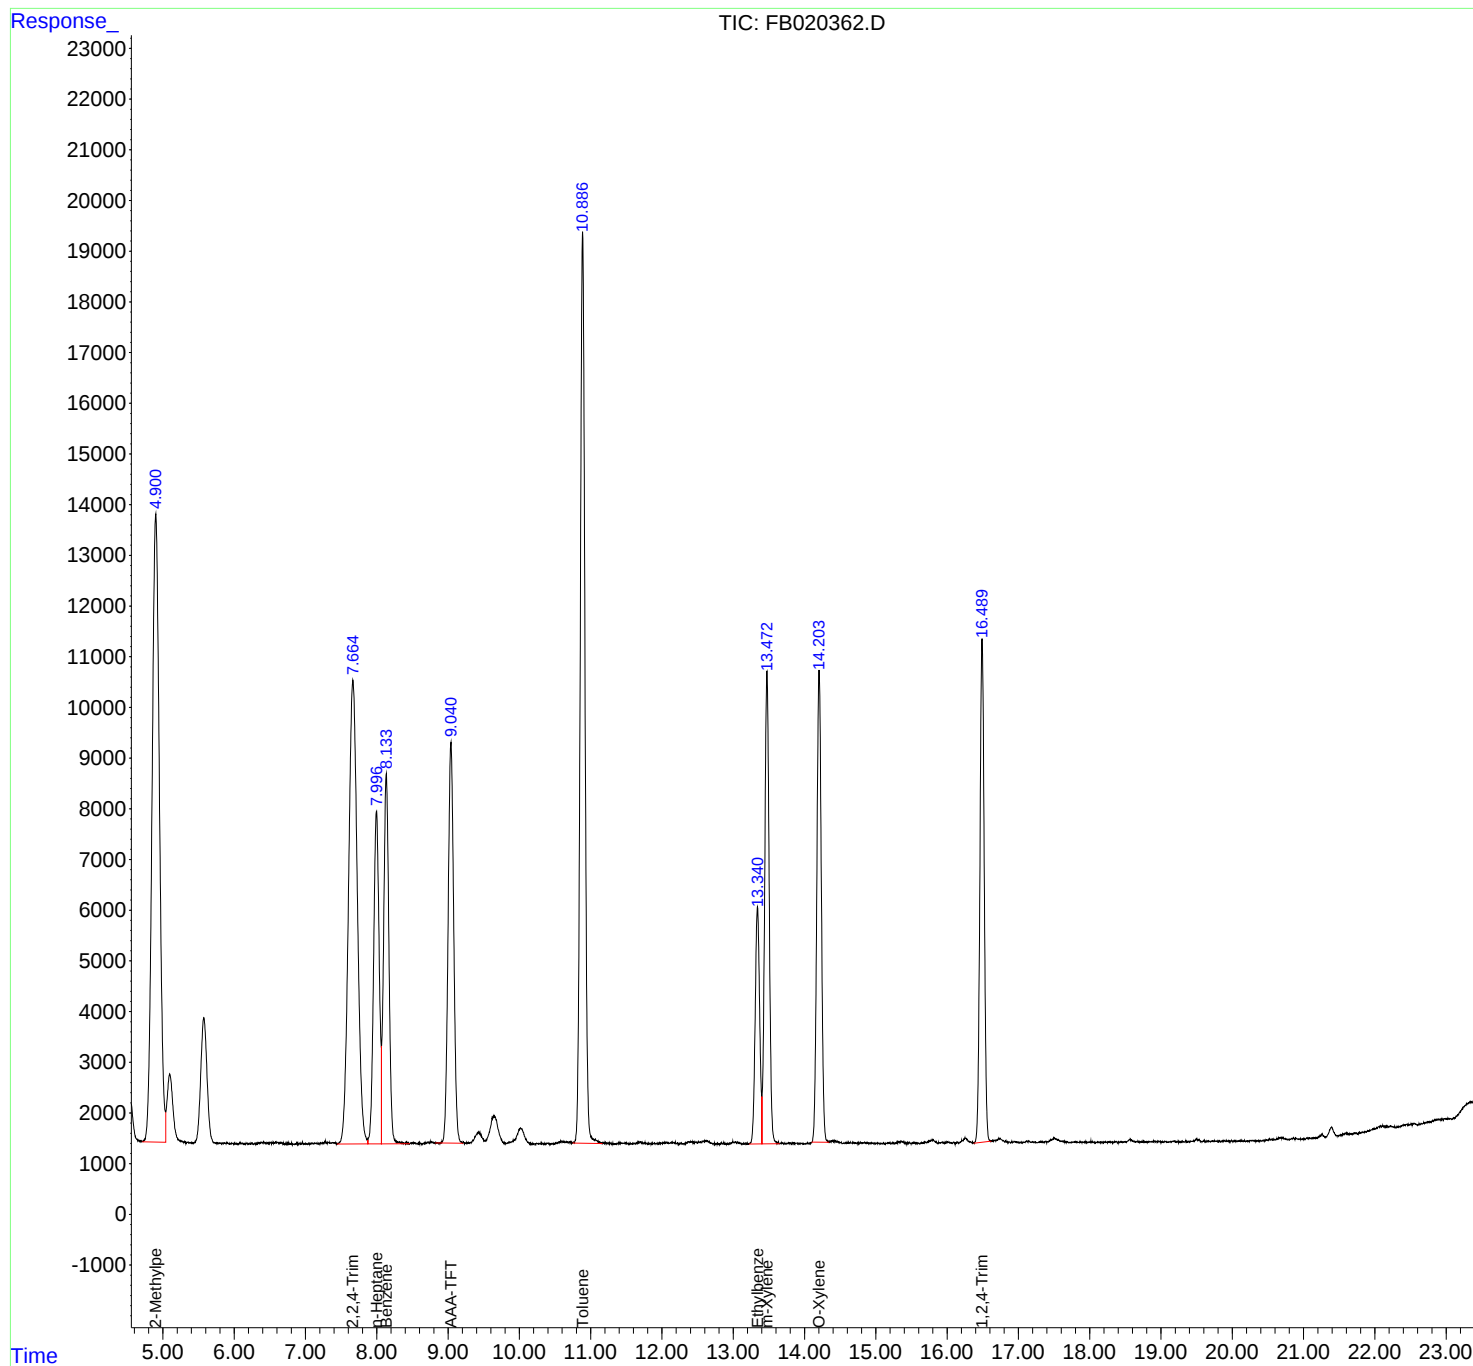


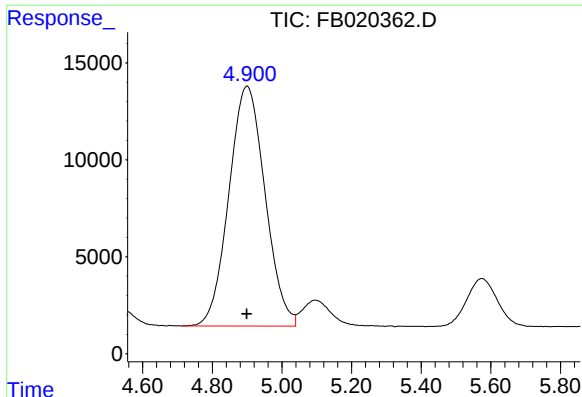

#1 2-Methylpentane


R.T.: 4.901 min
Delta R.T.: 0.002 min
Response: 893754
Conc: 32.24 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0326W2

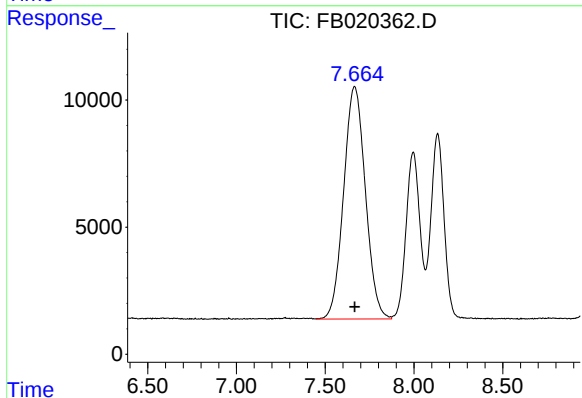


#2 2,2,4-Trimethylpentane

R.T.: 7.666 min
Delta R.T.: 0.000 min
Response: 778361
Conc: 32.46 ng/ml

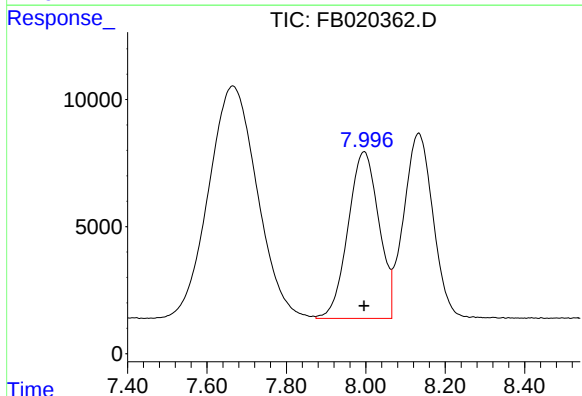


#3 n-Heptane

R.T.: 7.996 min
Delta R.T.: 0.000 min
Response: 354114
Conc: 10.83 ng/ml

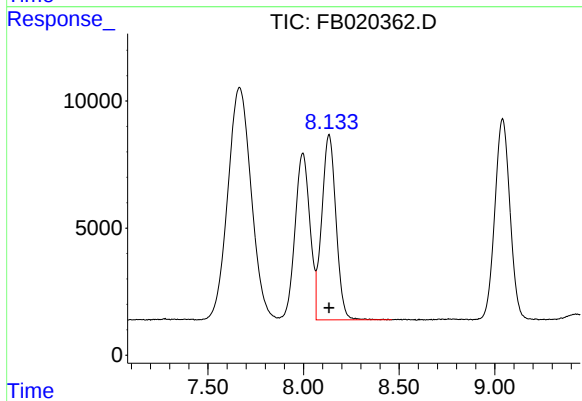

#4 Benzene


R.T.: 8.134 min
Delta R.T.: 0.000 min
Response: 376128
Conc: 10.86 ng/ml

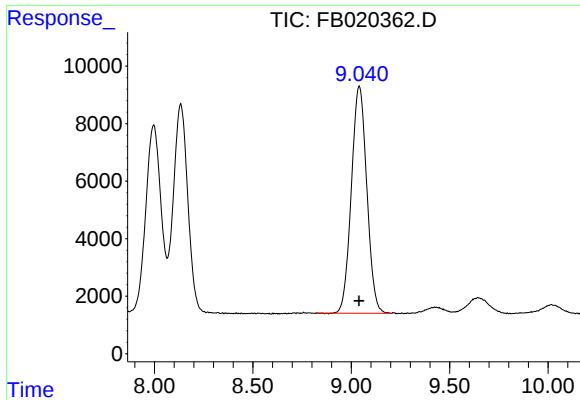

#5 AAA-TFT


R.T.: 9.041 min
Delta R.T.: 0.000 min
Response: 430996
Conc: 22.37 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0326W2

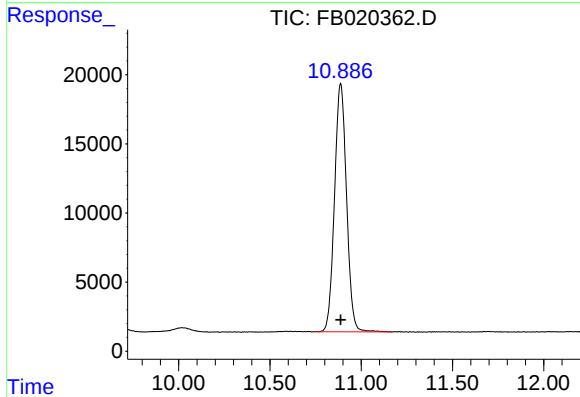


#6 Toluene

R.T.: 10.888 min
Delta R.T.: 0.000 min
Response: 822198
Conc: 31.70 ng/ml

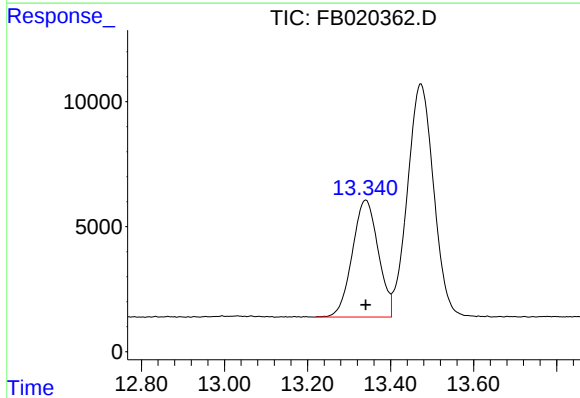


#7 Ethylbenzene

R.T.: 13.341 min
Delta R.T.: 0.000 min
Response: 202670
Conc: 10.29 ng/ml

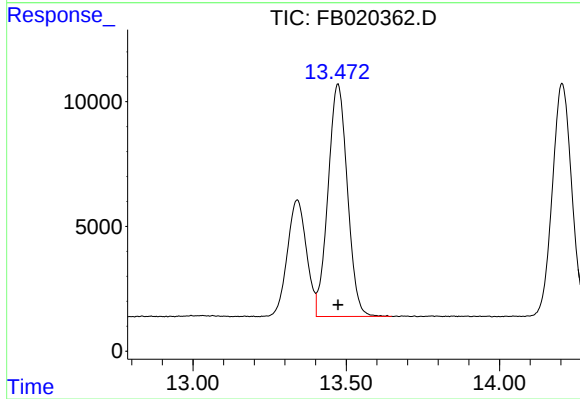

#8 m-Xylene


R.T.: 13.473 min
Delta R.T.: 0.000 min
Response: 409685
Conc: 20.18 ng/ml

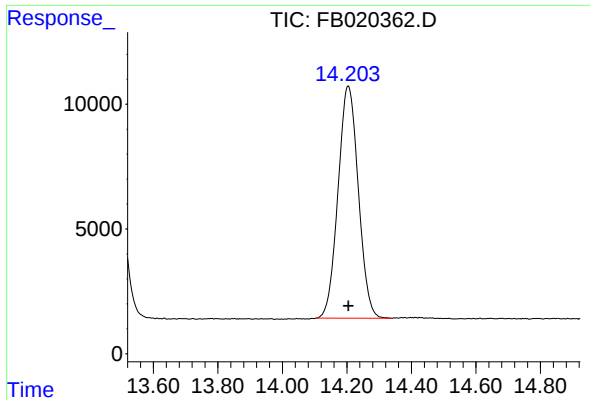

#9 O-Xylene

R.T.: 14.205 min
Delta R.T.: 0.000 min
Response: 406982
Conc: 20.09 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0326W2

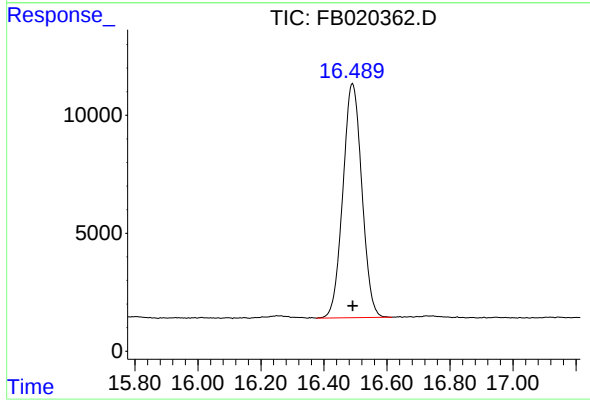

#10 1,2,4-Trimethylbenzene

R.T.: 16.491 min
Delta R.T.: 0.000 min
Response: 414967
Conc: 19.94 ng/ml