

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032619\
 Data File : FB020369.D
 Signal(s) : FID2B.CH
 Acq On : 26 Mar 2019 22:13
 Operator : MJ/SJ
 Sample : K2091-01MSD
 Misc : 5.02gm/5.00ml DI WATER
 ALS Vial : 19 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 DRUM-COMPMSD

Integration File: Calibration.e
 Quant Time: Mar 27 02:18:40 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
 Quant Title :
 QLast Update : Tue Mar 26 12:48:09 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.040	304449	15.802 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.899	438027	15.803 ng/ml
2) t 2,2,4-Trimethylpentane	7.663	245331	10.231 ng/ml
3) t n-Heptane	7.996	99782	3.052 ng/ml
4) t Benzene	8.133	291993	8.431 ng/ml
6) t Toluene	10.887	593896	22.898 ng/ml
7) t Ethylbenzene	13.339	143136	7.271 ng/ml
8) t m-Xylene	13.472	293860	14.474 ng/ml
9) t O-Xylene	14.204	289418	14.290 ng/ml
10) t 1,2,4-Trimethylbenzene	16.491	260091	12.501 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032619\
Data File : FB020369.D
Signal(s) : FID2B.CH
Acq On : 26 Mar 2019 22:13
Operator : MJ/SJ
Sample : K2091-01MSD
Misc : 5.02gm/5.00ml DI WATER
ALS Vial : 19 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
DRUM-COMPMSD

Integration File: Calibration.e
Quant Time: Mar 27 02:18:40 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
Quant Title :
QLast Update : Tue Mar 26 12:48:09 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

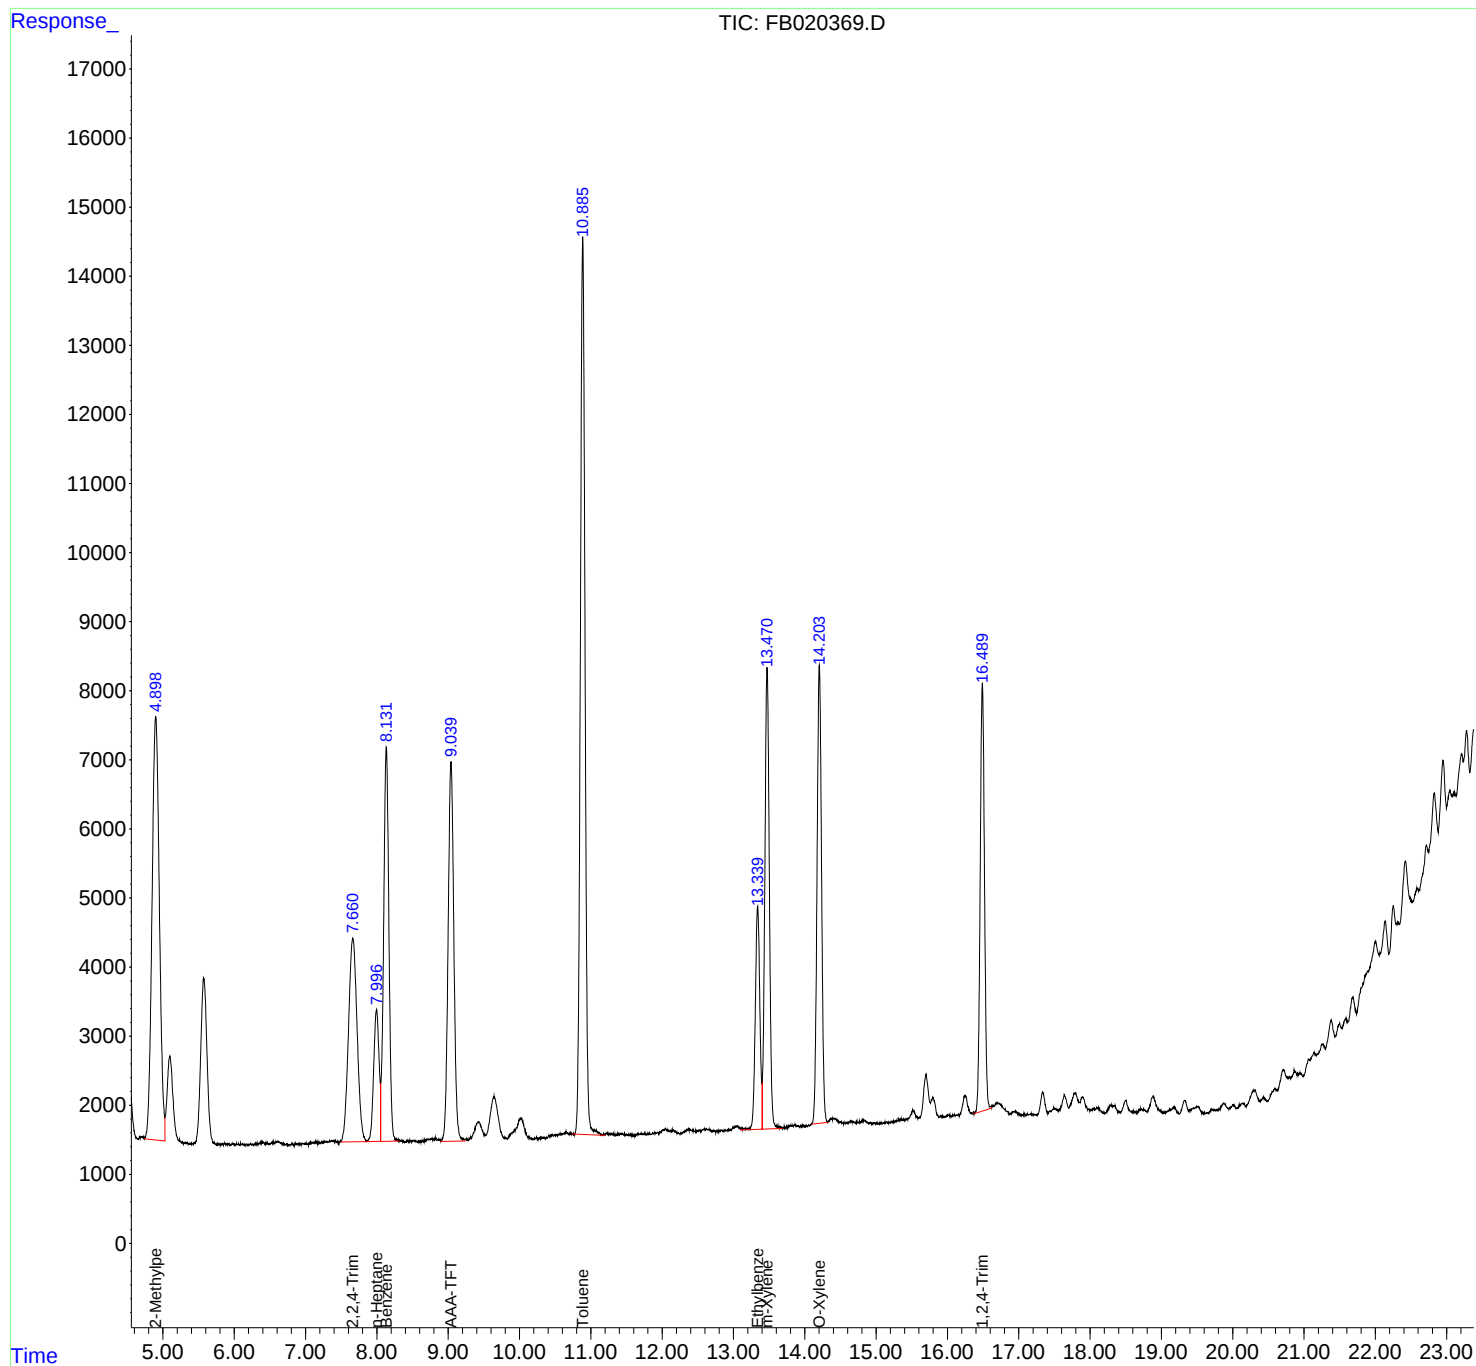


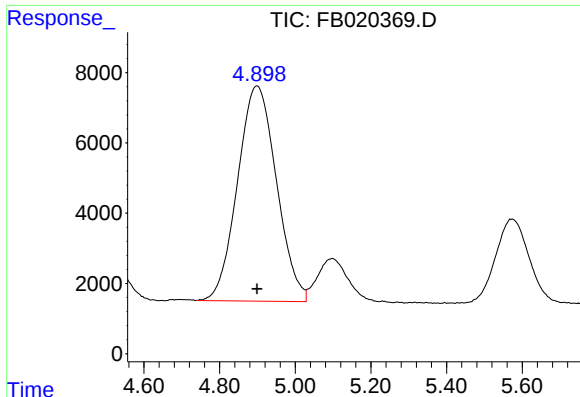

#1 2-Methylpentane


R.T.: 4.899 min
Delta R.T.: 0.000 min
Response: 438027
Conc: 15.80 ng/ml

Instrument :
FID_B
ClientSampleId :
DRUM-COMPMSD

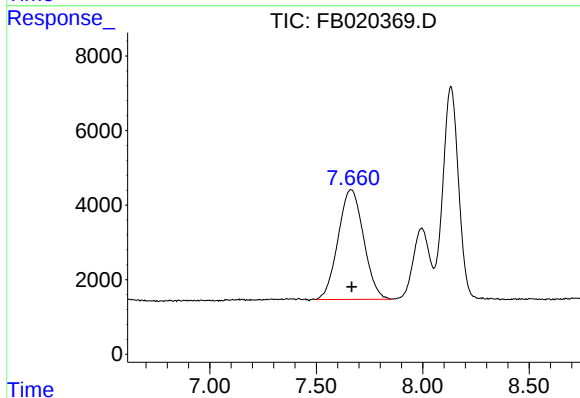


#2 2,2,4-Trimethylpentane

R.T.: 7.663 min
Delta R.T.: -0.003 min
Response: 245331
Conc: 10.23 ng/ml

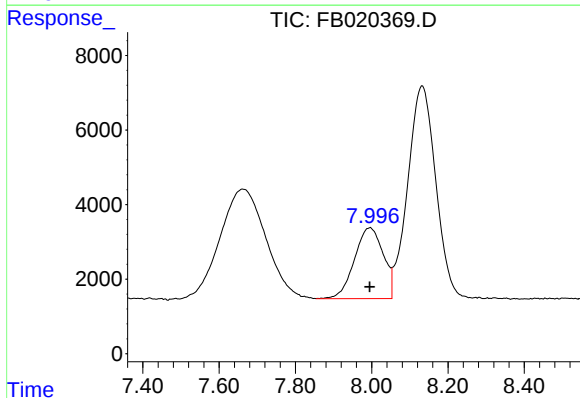


#3 n-Heptane

R.T.: 7.996 min
Delta R.T.: 0.001 min
Response: 99782
Conc: 3.05 ng/ml

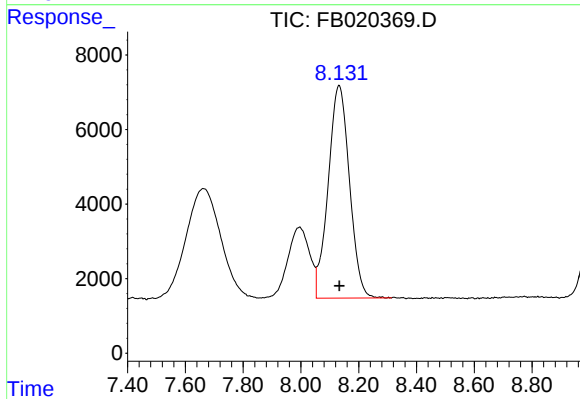

#4 Benzene


R.T.: 8.133 min
Delta R.T.: 0.000 min
Response: 291993
Conc: 8.43 ng/ml

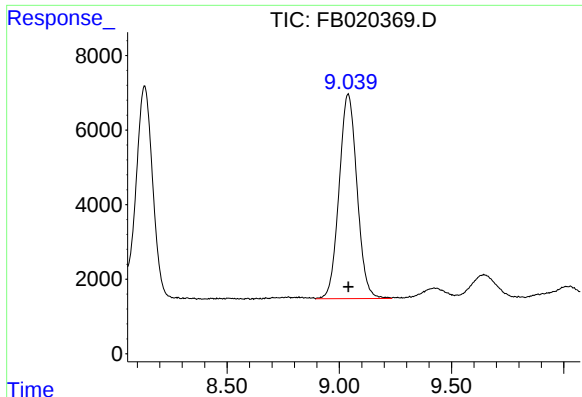

#5 AAA-TFT


R.T.: 9.040 min
Delta R.T.: 0.000 min
Response: 304449
Conc: 15.80 ng/ml

Instrument :
FID_B
ClientSampleId :
DRUM-COMPMSD

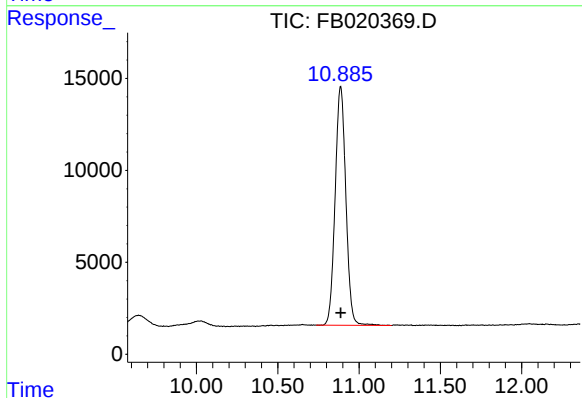


#6 Toluene

R.T.: 10.887 min
Delta R.T.: 0.000 min
Response: 593896
Conc: 22.90 ng/ml

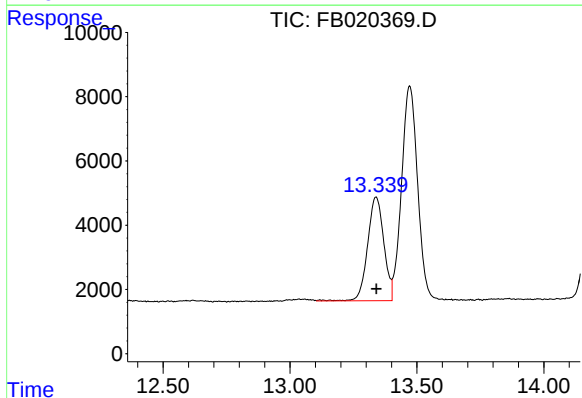


#7 Ethylbenzene

R.T.: 13.339 min
Delta R.T.: -0.001 min
Response: 143136
Conc: 7.27 ng/ml

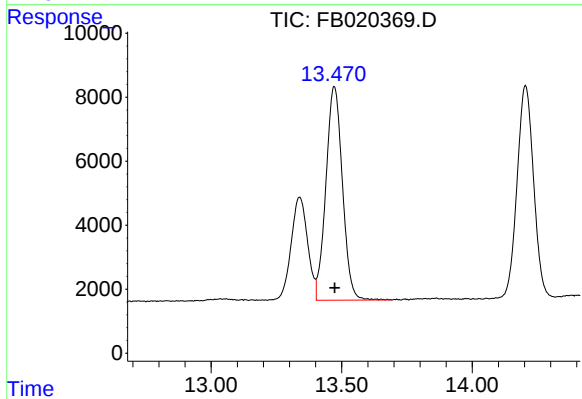

#8 m-Xylene


R.T.: 13.472 min
Delta R.T.: -0.001 min
Response: 293860
Conc: 14.47 ng/ml

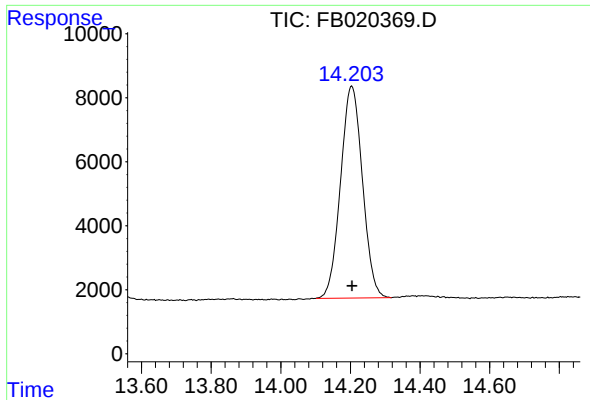

#9 O-Xylene

R.T.: 14.204 min
Delta R.T.: 0.000 min
Response: 289418
Conc: 14.29 ng/ml

Instrument :
FID_B
ClientSampleId :
DRUM-COMPMSD

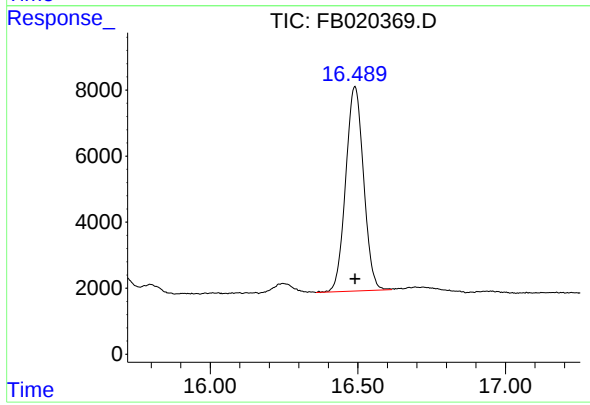

#10 1,2,4-Trimethylbenzene

R.T.: 16.491 min
Delta R.T.: 0.000 min
Response: 260091
Conc: 12.50 ng/ml