

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032620\
 Data File : FB024018.D
 Signal(s) : FID2B.CH
 Acq On : 26 Mar 2020 19:26
 Operator : DD/AJ
 Sample : 50 GRO STD
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 50 GRO STD

Integration File: Calibration.e
 Quant Time: Mar 27 11:14:53 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032620.M
 Quant Title :
 QLast Update : Fri Mar 27 11:13:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	1132755	49.354 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	2607748	75.892 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	2879729	82.778 ng/ml
3) t n-Heptane	7.759	941152	27.342 ng/ml
4) t Benzene	7.893	1139200	26.318 ng/ml
6) t Toluene	10.632	3312723	75.038 ng/ml
7) t Ethylbenzene	13.072	988791	25.038 ng/ml
8) t m-Xylene	13.206	1879546	48.942 ng/ml
9) t O-Xylene	13.933	1803876	48.506 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	1605508	51.063 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032620\
Data File : FB024018.D
Signal(s) : FID2B.CH
Acq On : 26 Mar 2020 19:26
Operator : DD/AJ
Sample : 50 GRO STD
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
50 GRO STD

Integration File: Calibration.e
Quant Time: Mar 27 11:14:53 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032620.M
Quant Title :
QLast Update : Fri Mar 27 11:13:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

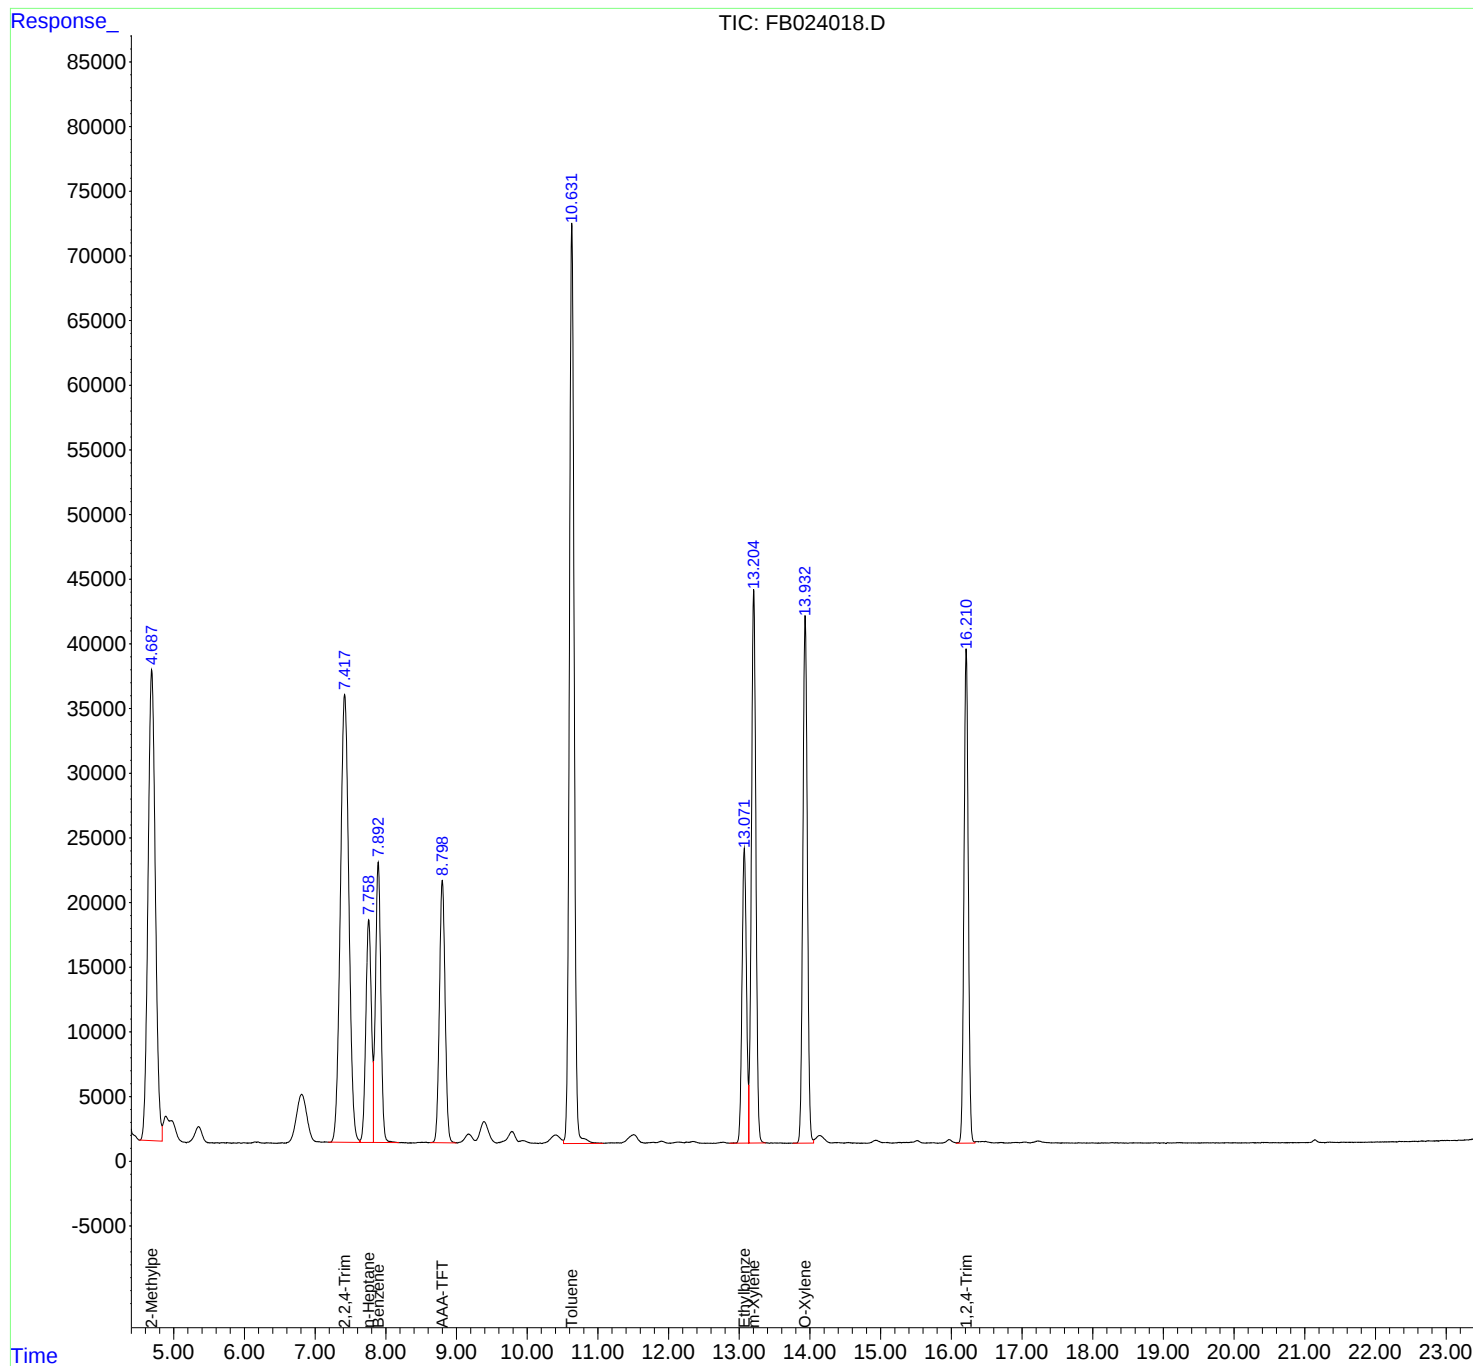


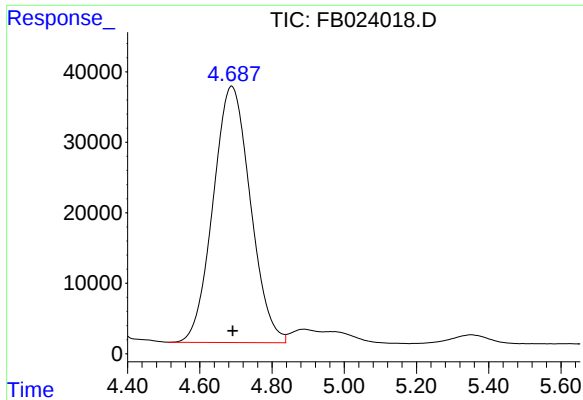

#1 2-Methylpentane


R.T.: 4.689 min
Delta R.T.: -0.002 min
Response: 2607748
Conc: 75.89 ng/ml

Instrument :
FID_B
ClientSampleId :
50 GRO STD

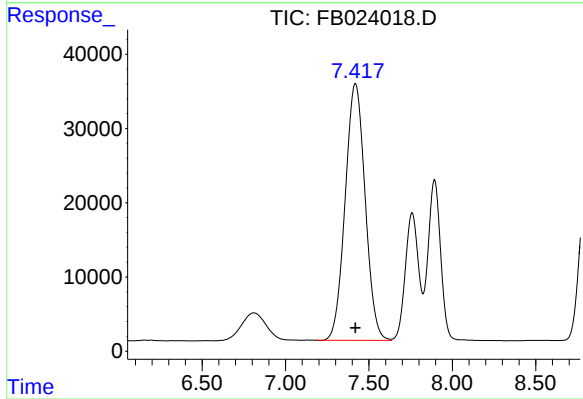


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: -0.001 min
Response: 2879729
Conc: 82.78 ng/ml

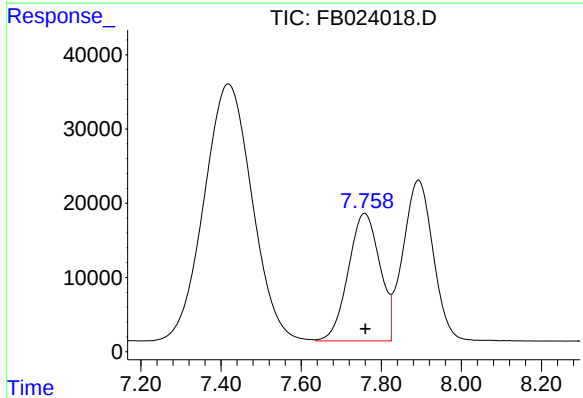


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: -0.001 min
Response: 941152
Conc: 27.34 ng/ml

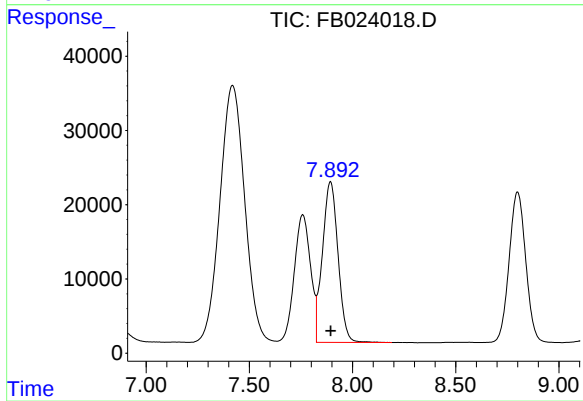

#4 Benzene


R.T.: 7.893 min
Delta R.T.: -0.001 min
Response: 1139200
Conc: 26.32 ng/ml

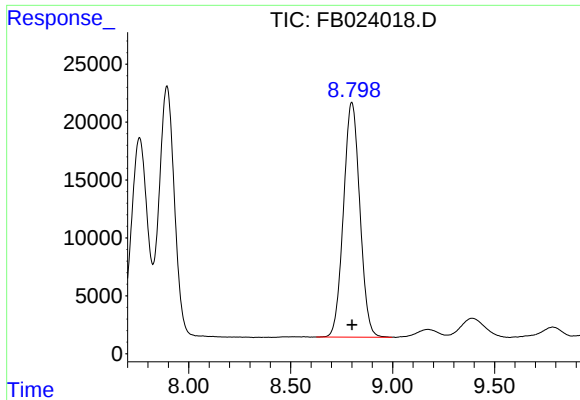

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: -0.001 min
Response: 1132755
Conc: 49.35 ng/ml

Instrument :
FID_B
ClientSampleId :
50 GRO STD

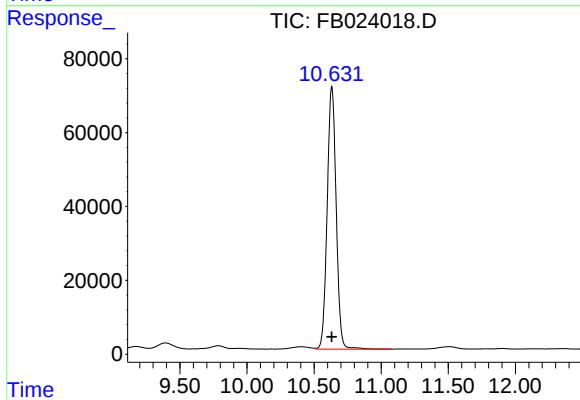


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.000 min
Response: 3312723
Conc: 75.04 ng/ml

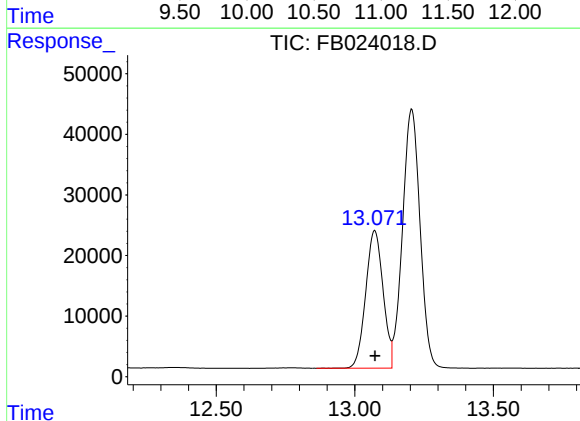


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.000 min
Response: 988791
Conc: 25.04 ng/ml

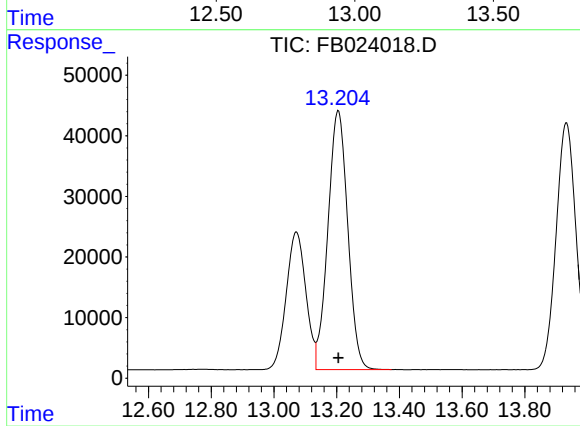

#8 m-Xylene


R.T.: 13.206 min
Delta R.T.: 0.000 min
Response: 1879546
Conc: 48.94 ng/ml

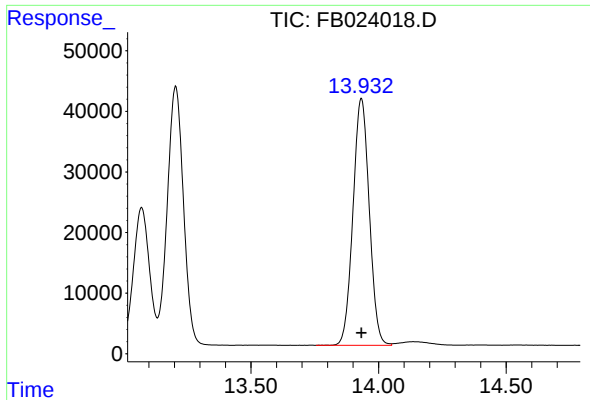

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.000 min
Response: 1803876
Conc: 48.51 ng/ml

Instrument :
FID_B
ClientSampleId :
50 GRO STD

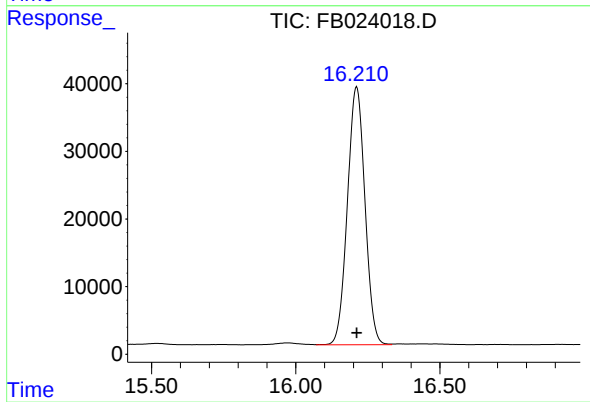

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.000 min
Response: 1605508
Conc: 51.06 ng/ml