

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032620\
 Data File : FB024020.D
 Signal(s) : FID2B.CH
 Acq On : 26 Mar 2020 20:27
 Operator : DD/AJ
 Sample : FB032620GROICV
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 FB032620GROICV

Integration File: Calibration.e
 Quant Time: Mar 27 11:15:01 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032620.M
 Quant Title :
 QLast Update : Fri Mar 27 11:13:36 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	457289	19.924 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.691	998120	29.048 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	1030865	29.632 ng/ml
3) t n-Heptane	7.760	338996	9.848 ng/ml
4) t Benzene	7.894	435168	10.053 ng/ml
6) t Toluene	10.632	1299760	29.442 ng/ml
7) t Ethylbenzene	13.072	372984	9.445 ng/ml
8) t m-Xylene	13.204	741812	19.316 ng/ml
9) t O-Xylene	13.932	719146	19.338 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	629145	20.010 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032620\
Data File : FB024020.D
Signal(s) : FID2B.CH
Acq On : 26 Mar 2020 20:27
Operator : DD/AJ
Sample : FB032620GROICV
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
FB032620GROICV

Integration File: Calibration.e
Quant Time: Mar 27 11:15:01 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032620.M
Quant Title :
QLast Update : Fri Mar 27 11:13:36 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

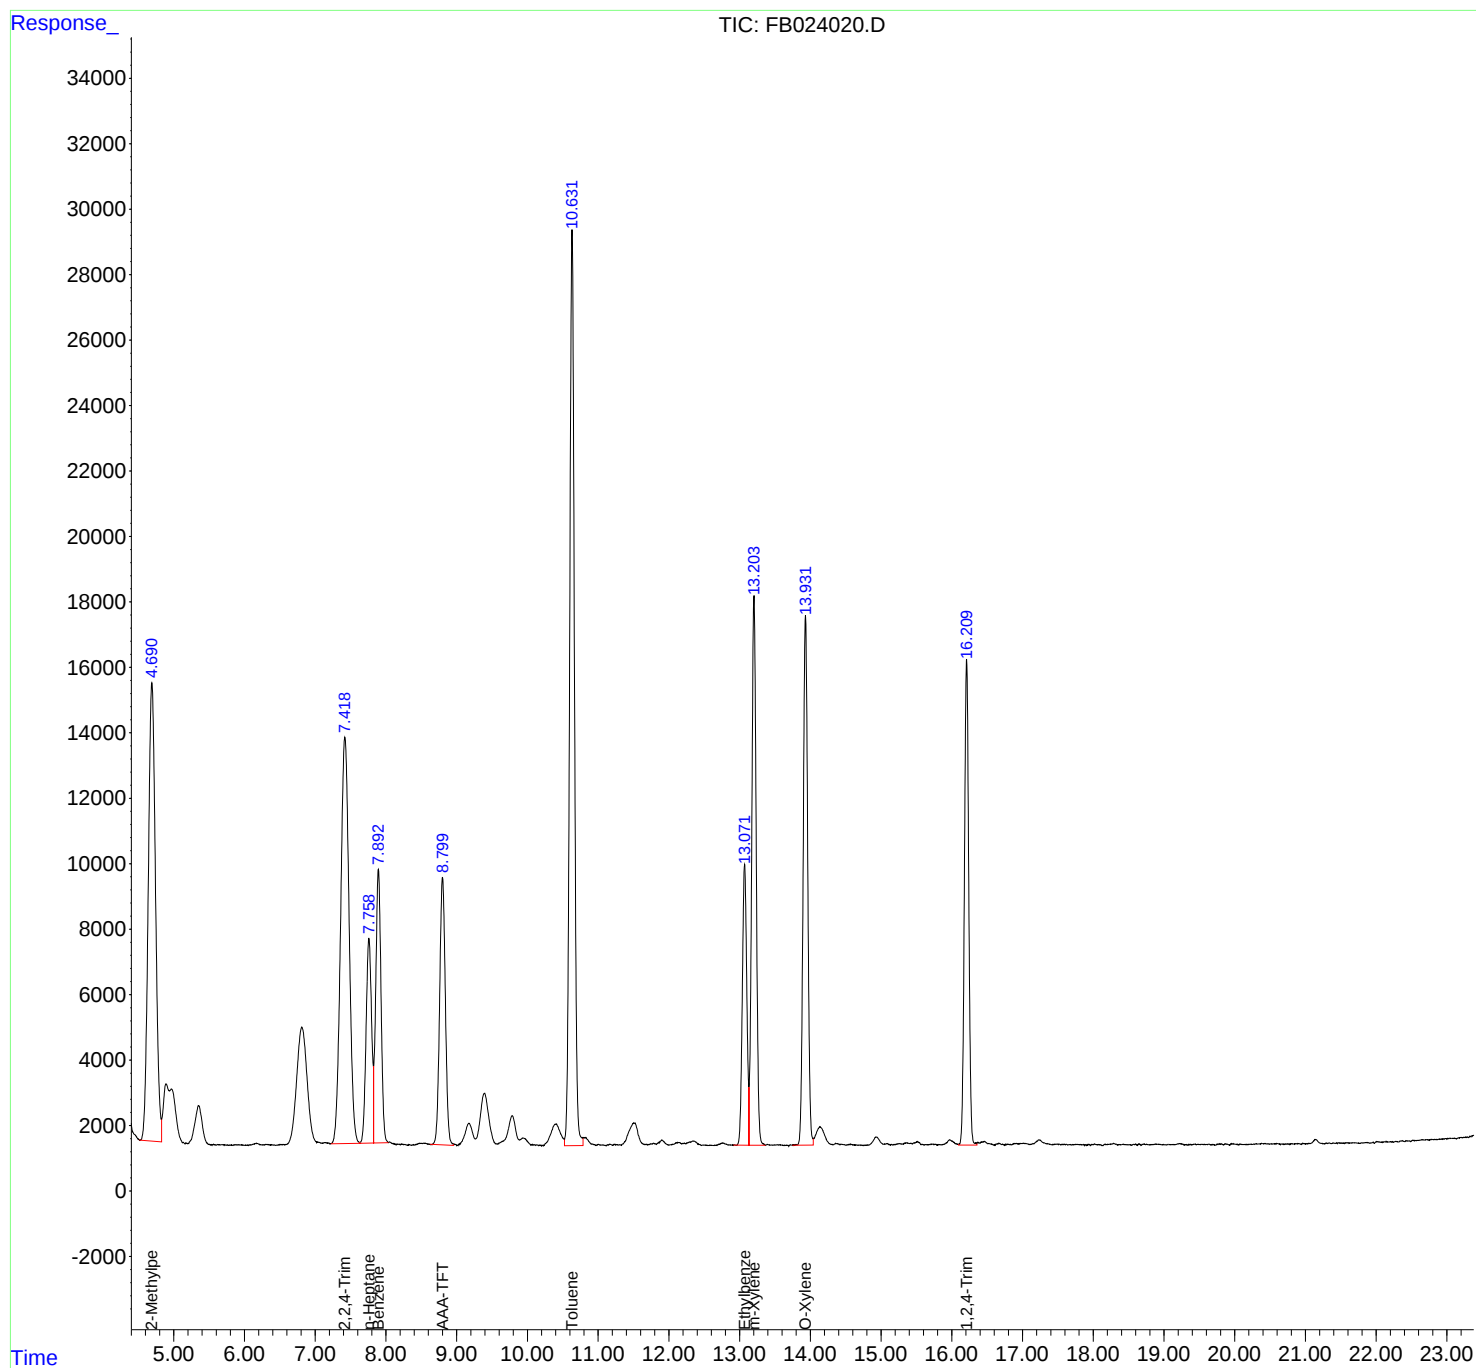


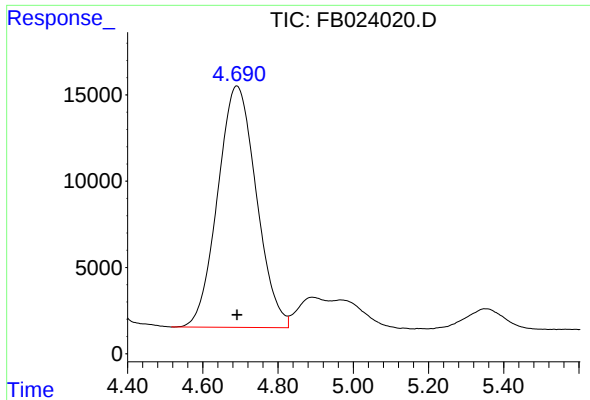

#1 2-Methylpentane


R.T.: 4.691 min
Delta R.T.: 0.000 min
Response: 998120
Conc: 29.05 ng/ml

Instrument :
FID_B
ClientSampleId :
FB032620GROICV

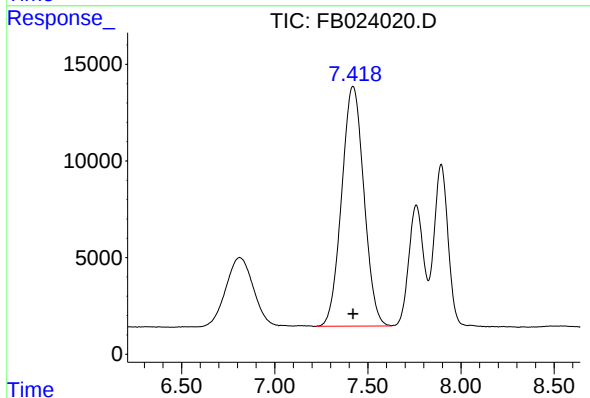


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.000 min
Response: 1030865
Conc: 29.63 ng/ml

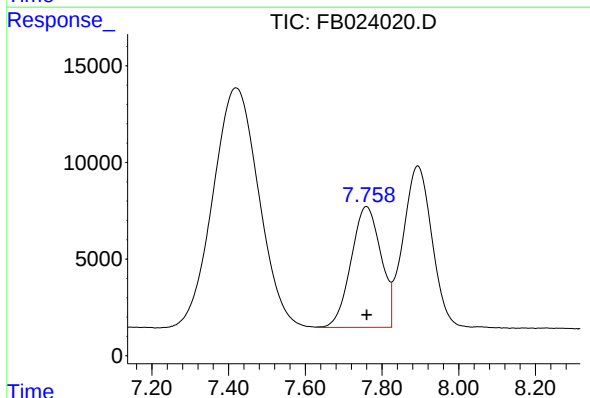


#3 n-Heptane

R.T.: 7.760 min
Delta R.T.: 0.000 min
Response: 338996
Conc: 9.85 ng/ml

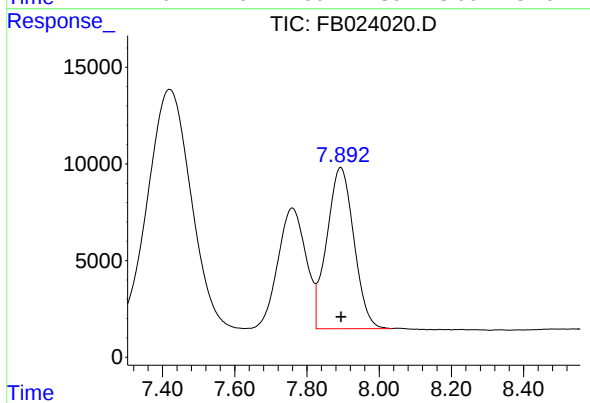

#4 Benzene


R.T.: 7.894 min
Delta R.T.: 0.000 min
Response: 435168
Conc: 10.05 ng/ml

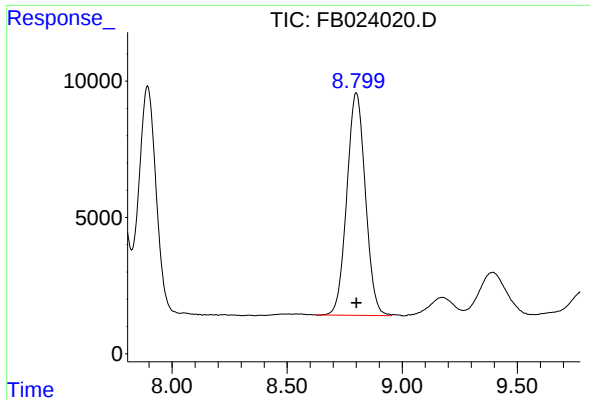

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: 0.000 min
Response: 457289
Conc: 19.92 ng/ml

Instrument :
FID_B
ClientSampleId :
FB032620GROICV

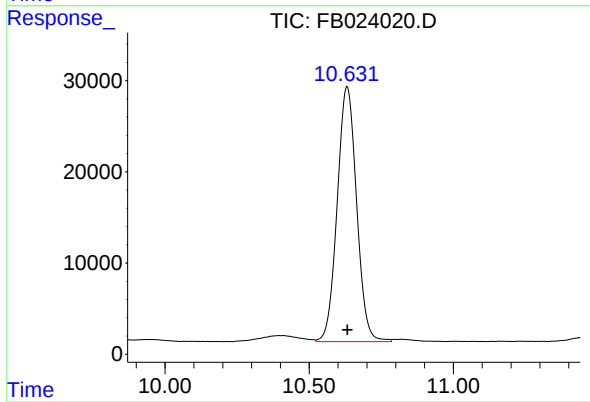


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.000 min
Response: 1299760
Conc: 29.44 ng/ml

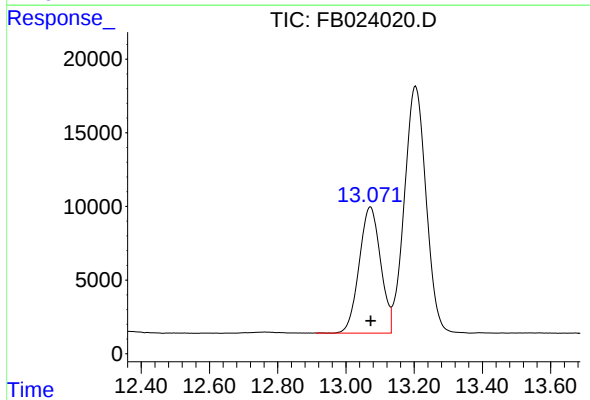


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.000 min
Response: 372984
Conc: 9.44 ng/ml

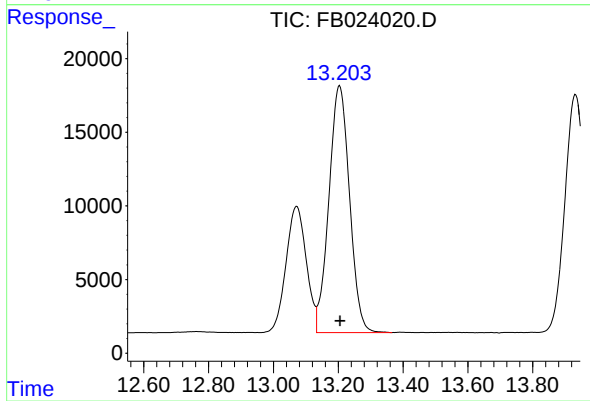

#8 m-Xylene

R.T.: 13.204 min
Delta R.T.: -0.002 min
Response: 741812
Conc: 19.32 ng/ml

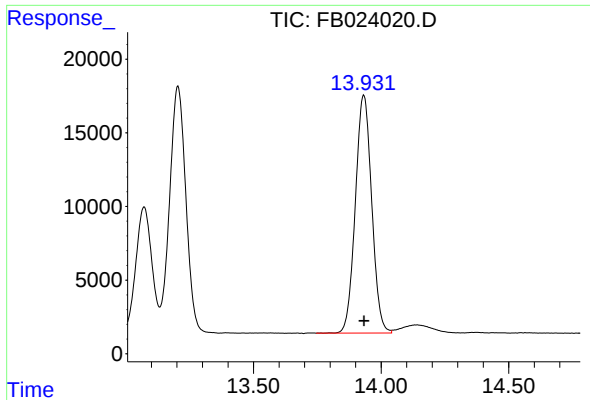

#9 O-Xylene


R.T.: 13.932 min

Delta R.T.: -0.001 min

Response: 719146

Conc: 19.34 ng/ml

Instrument :
FID_B
ClientSampleId :
FB032620GROICV

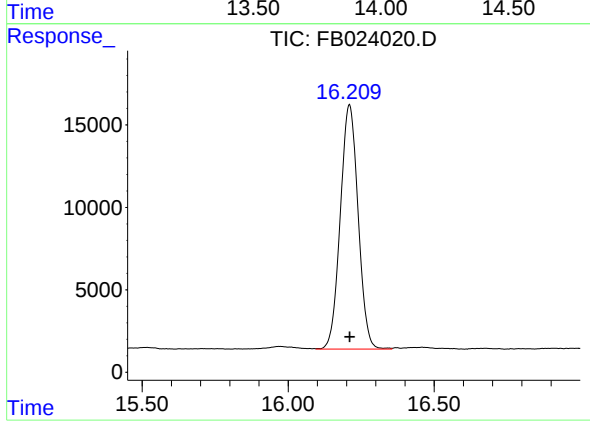

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min

Delta R.T.: -0.001 min

Response: 629145

Conc: 20.01 ng/ml