

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032719\
 Data File : FB020376.D
 Signal(s) : FID2B.CH
 Acq On : 27 Mar 2019 10:34
 Operator : MJ/SJ
 Sample : BSF0327S1
 Misc : 5.01gm/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 27 10:49:16 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
 Quant Title :
 QLast Update : Tue Mar 26 12:48:09 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.039	411687	21.368 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.901	871472	31.441 ng/ml
2) t 2,2,4-Trimethylpentane	7.665	779680	32.514 ng/ml
3) t n-Heptane	7.995	343607	10.510 ng/ml
4) t Benzene	8.133	360682	10.415 ng/ml
6) t Toluene	10.886	784195	30.235 ng/ml
7) t Ethylbenzene	13.338	197549	10.035 ng/ml
8) t m-Xylene	13.472	406229	20.009 ng/ml
9) t O-Xylene	14.203	403268	19.911 ng/ml
10) t 1,2,4-Trimethylbenzene	16.488	414466	19.921 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032719\
Data File : FB020376.D
Signal(s) : FID2B.CH
Acq On : 27 Mar 2019 10:34
Operator : MJ/SJ
Sample : BSF0327S1
Misc : 5.01gm/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 27 10:49:16 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
Quant Title :
QLast Update : Tue Mar 26 12:48:09 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

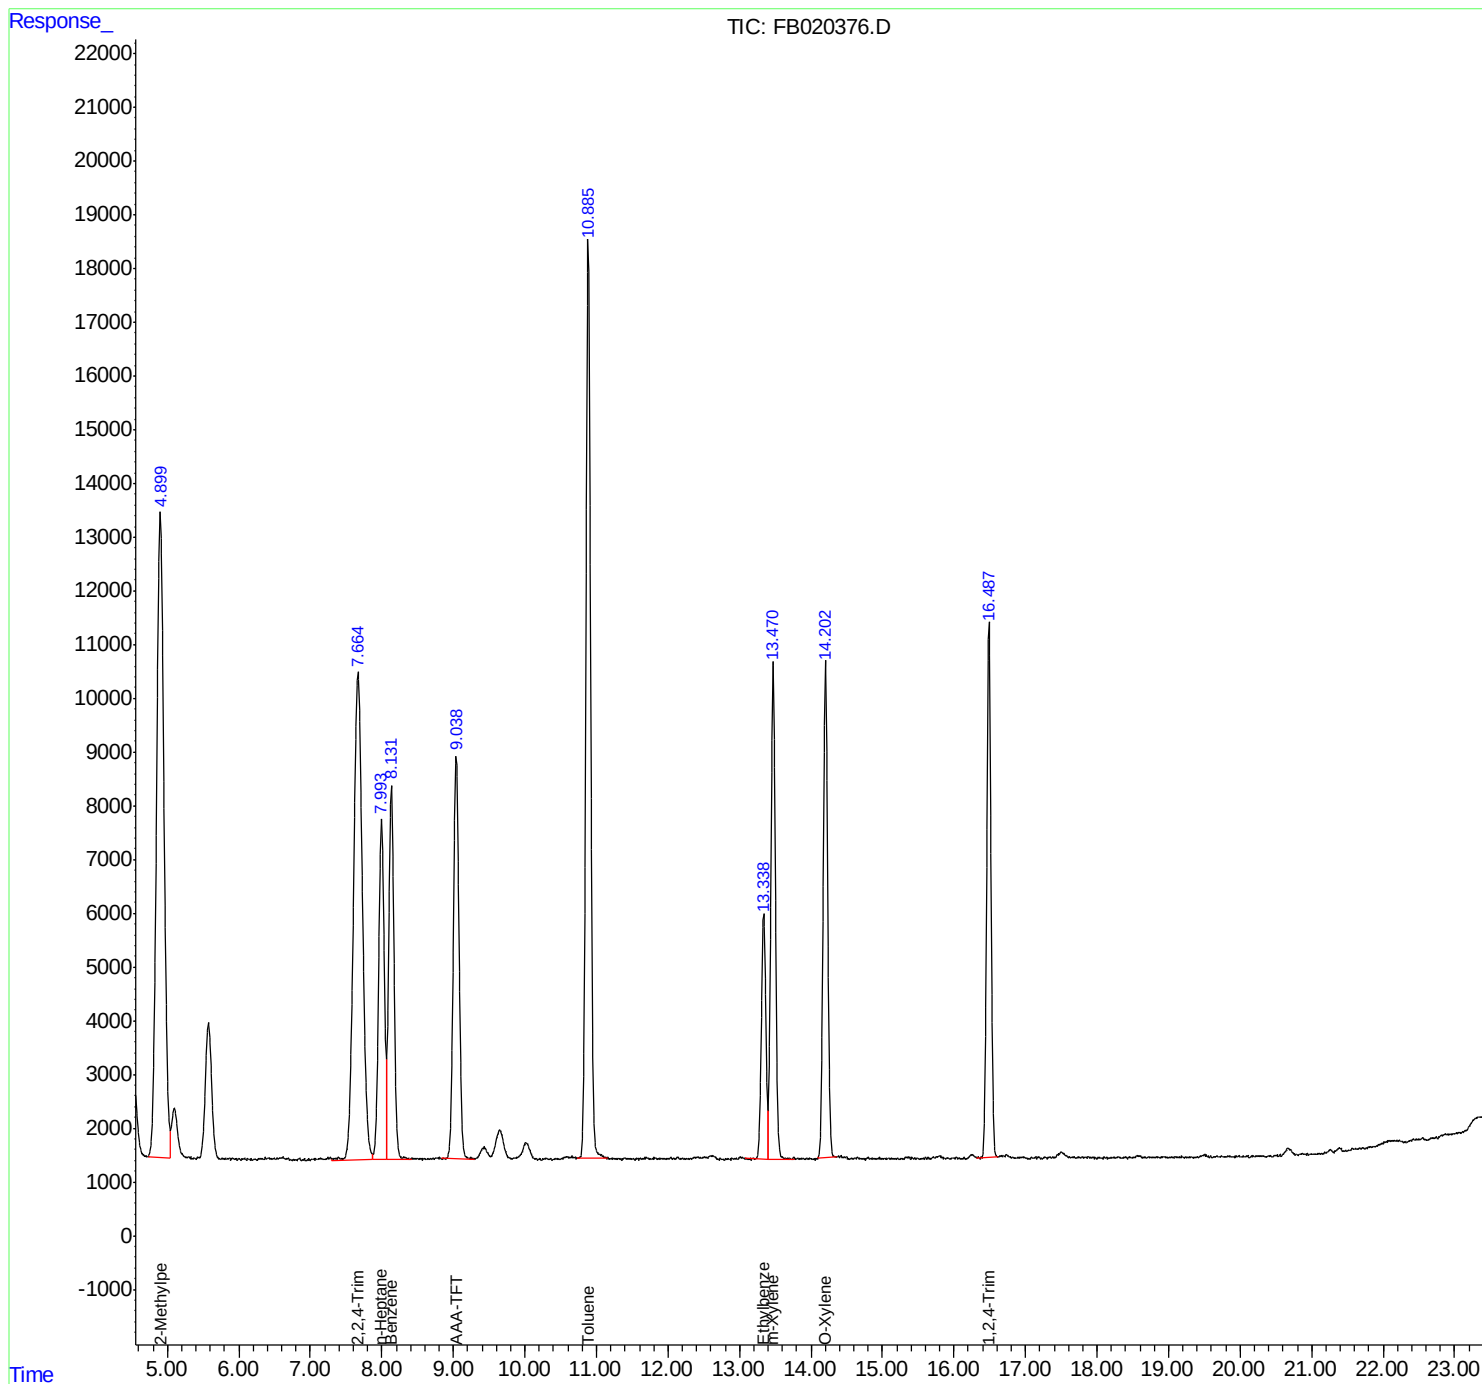

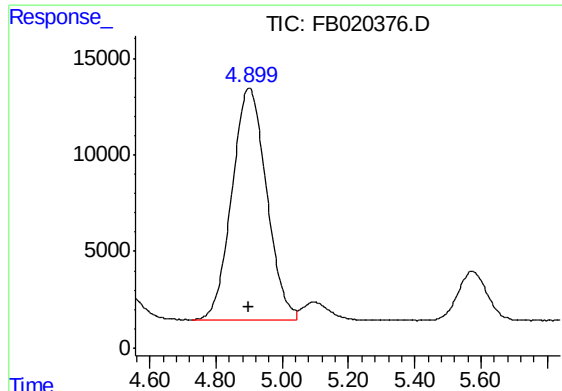


#1 2-Methylpentane

R.T.: 4.901 min
Delta R.T.: 0.002 min
Response: 871472
Conc: 31.44 ng/ml

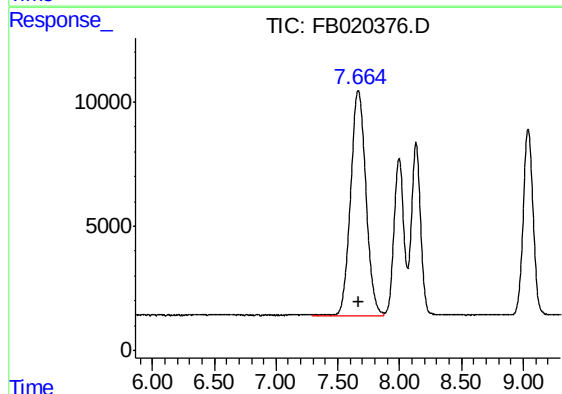


#2 2,2,4-Trimethylpentane

R.T.: 7.665 min
Delta R.T.: -0.001 min
Response: 779680
Conc: 32.51 ng/ml

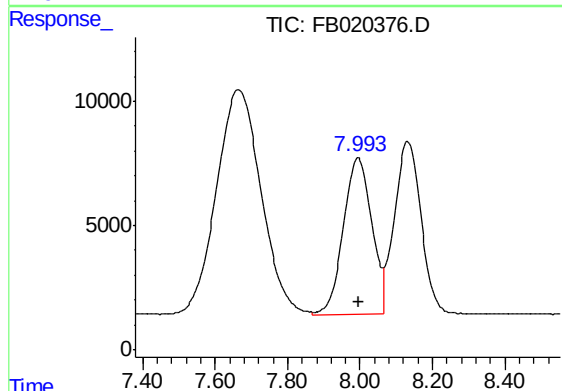


#3 n-Heptane

R.T.: 7.995 min
Delta R.T.: 0.000 min
Response: 343607
Conc: 10.51 ng/ml

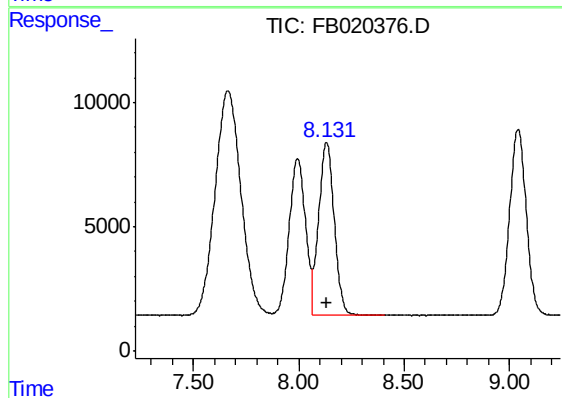


#4 Benzene

R.T.: 8.133 min
Delta R.T.: 0.000 min
Response: 360682
Conc: 10.41 ng/ml

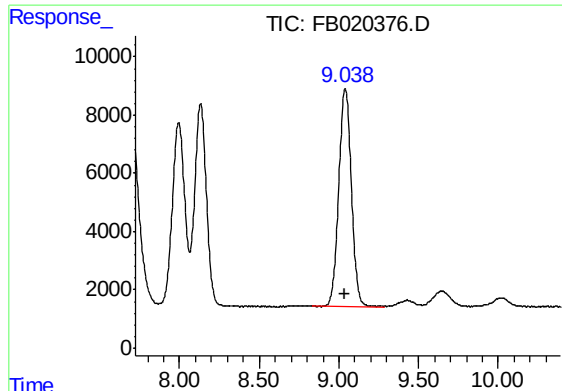


#5 AAA-TFT

R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 411687
Conc: 21.37 ng/ml

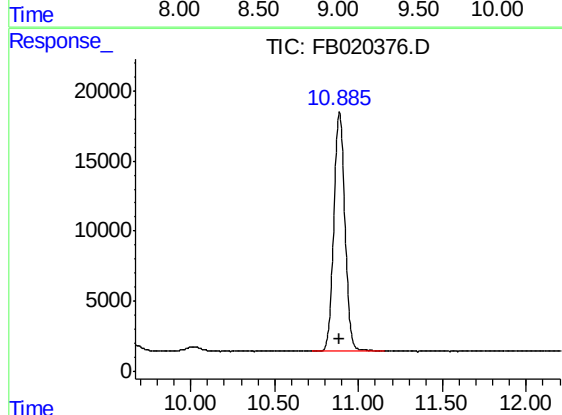


#6 Toluene

R.T.: 10.886 min
Delta R.T.: -0.001 min
Response: 784195
Conc: 30.23 ng/ml

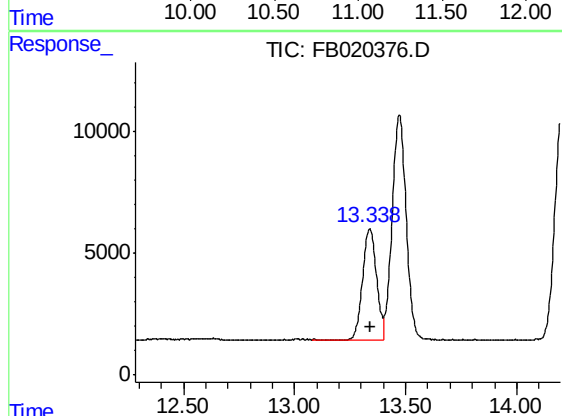


#7 Ethylbenzene

R.T.: 13.338 min
Delta R.T.: -0.002 min
Response: 197549
Conc: 10.03 ng/ml

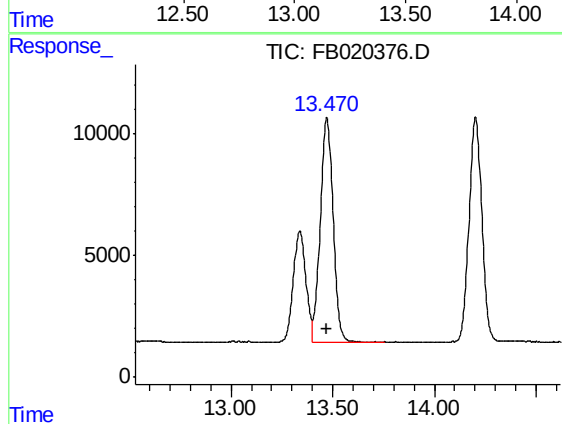


#8 m-Xylene

R.T.: 13.472 min
Delta R.T.: -0.002 min
Response: 406229
Conc: 20.01 ng/ml

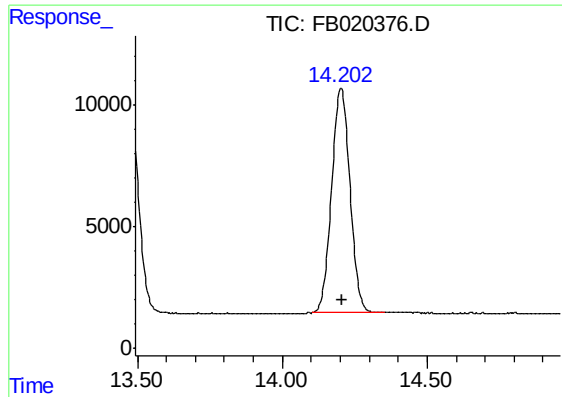

#9 O-Xylene

R.T.: 14.203 min
Delta R.T.: -0.001 min
Response: 403268
Conc: 19.91 ng/ml

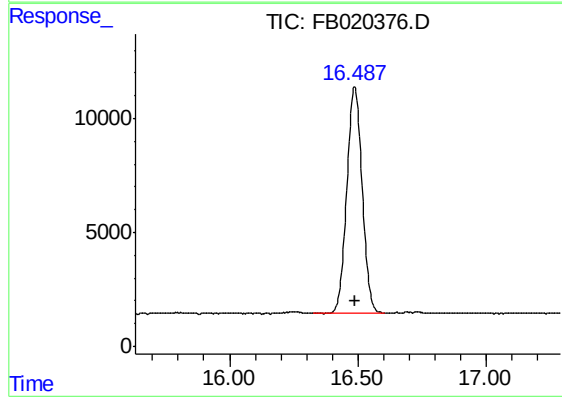

#10 1,2,4-Trimethylbenzene

R.T.: 16.488 min
Delta R.T.: -0.003 min
Response: 414466
Conc: 19.92 ng/ml