

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032719\
 Data File : FB020380.D
 Signal(s) : FID2B.CH
 Acq On : 27 Mar 2019 12:35
 Operator : MJ/SJ
 Sample : K1560-02
 Misc : 5.00gm/5.00ml DI WATER (10 PPB LOQ)
 ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 27 12:50:42 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
 Quant Title :
 QLast Update : Tue Mar 26 12:48:09 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.039	412890	21.431 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.899	397190	14.330 ng/ml
2) t 2,2,4-Trimethylpentane	7.664	350917	14.634 ng/ml
3) t n-Heptane	7.994	153912	4.708 ng/ml
4) t Benzene	8.132	166829	4.817 ng/ml
6) t Toluene	10.886	368313	14.200 ng/ml
7) t Ethylbenzene	13.338	93696	4.759 ng/ml
8) t m-Xylene	13.472	192047	9.459 ng/ml
9) t O-Xylene	14.203	190239	9.393 ng/ml
10) t 1,2,4-Trimethylbenzene	16.489	196567	9.448 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032719\
Data File : FB020380.D
Signal(s) : FID2B.CH
Acq On : 27 Mar 2019 12:35
Operator : MJ/SJ
Sample : K1560-02
Misc : 5.00gm/5.00ml DI WATER (10 PPB LOQ)
ALS Vial : 7 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 27 12:50:42 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
Quant Title :
QLast Update : Tue Mar 26 12:48:09 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

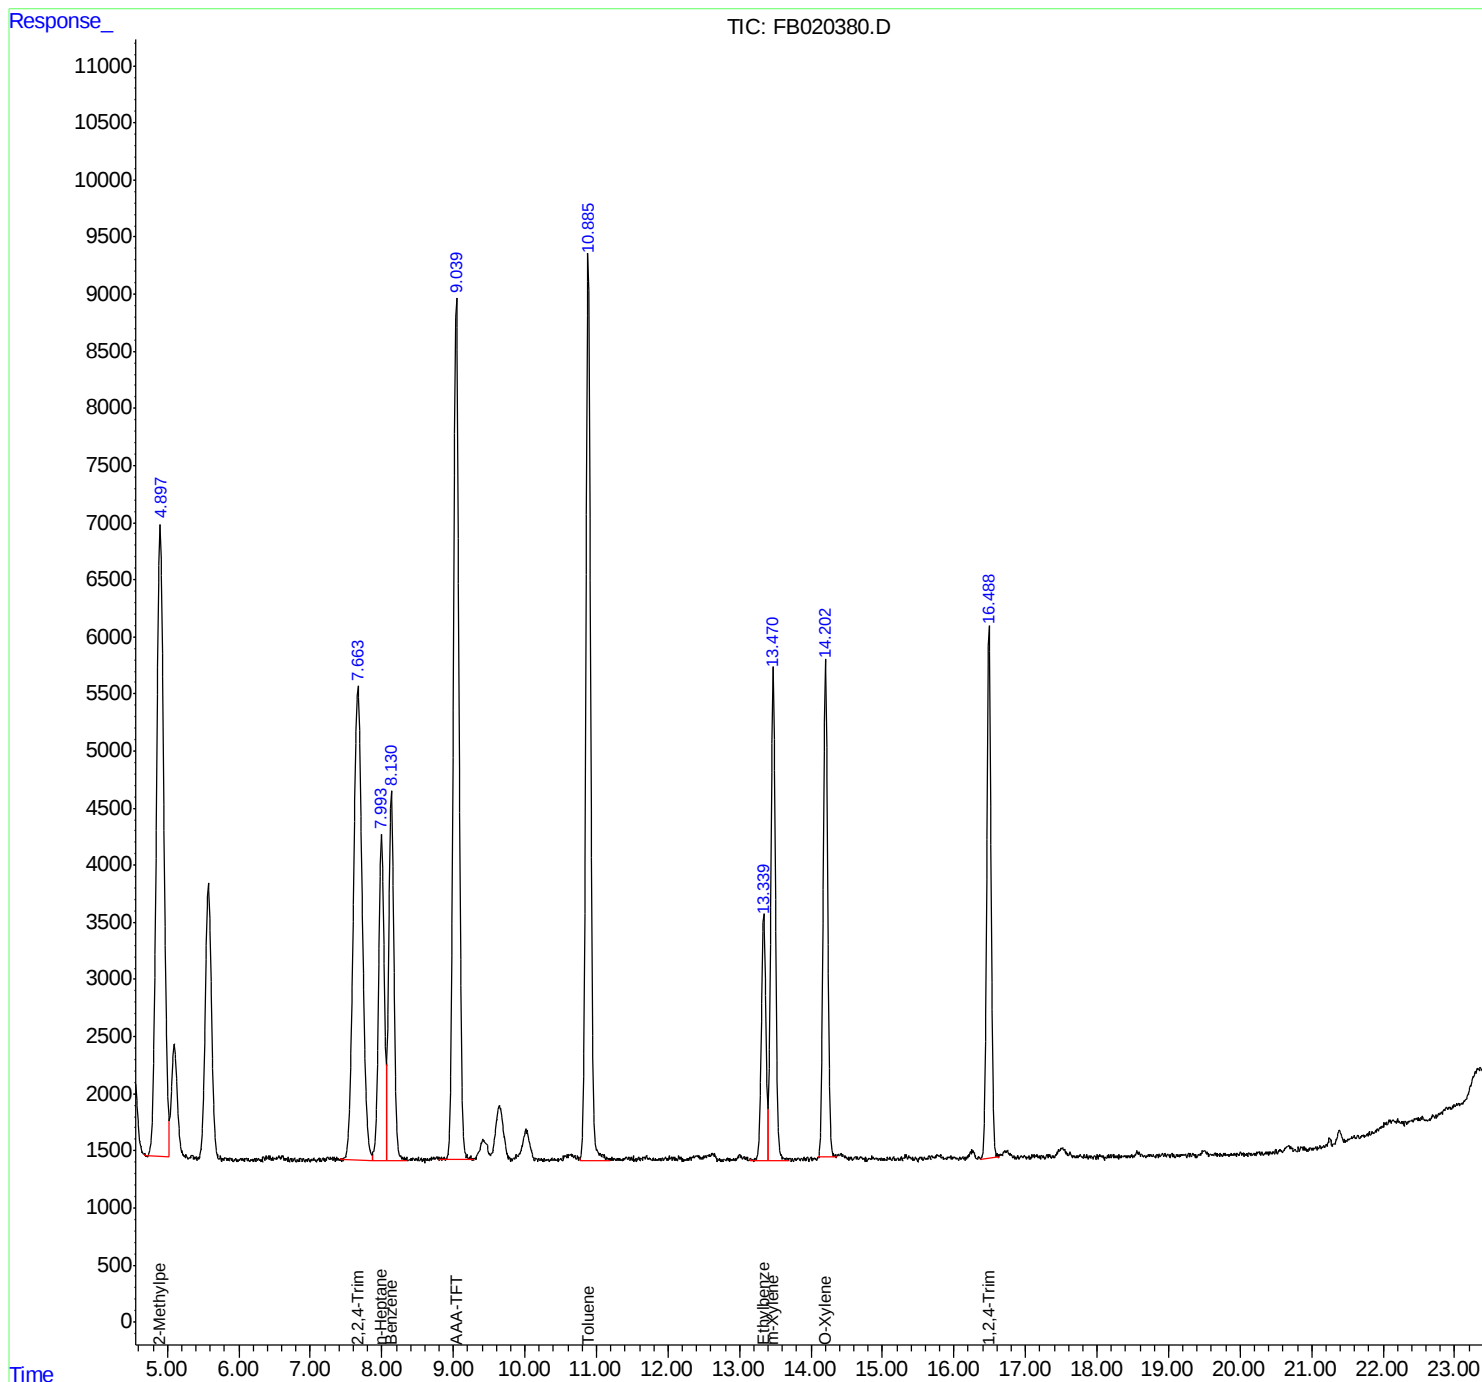

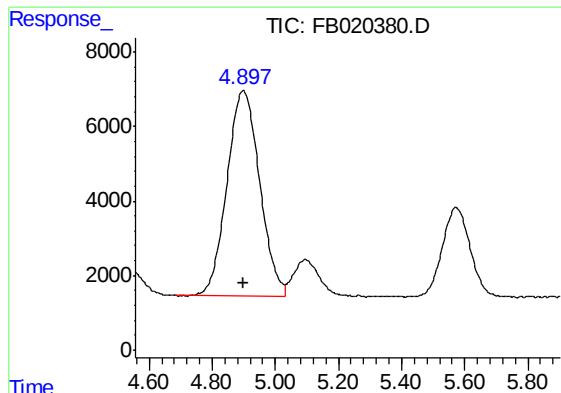


#1 2-Methylpentane

R.T.: 4.899 min
Delta R.T.: 0.000 min
Response: 397190
Conc: 14.33 ng/ml

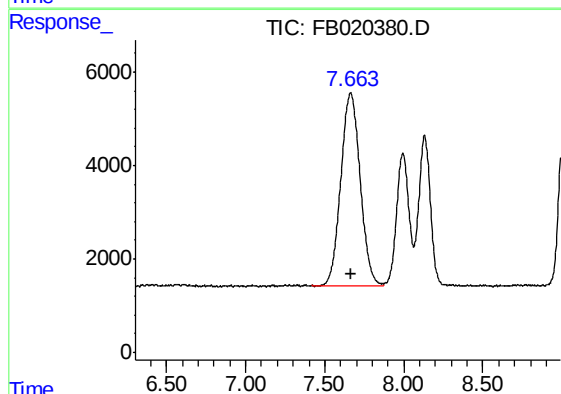


#2 2,2,4-Trimethylpentane

R.T.: 7.664 min
Delta R.T.: -0.002 min
Response: 350917
Conc: 14.63 ng/ml

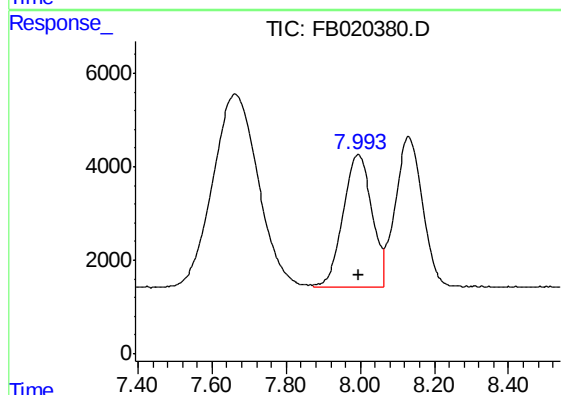


#3 n-Heptane

R.T.: 7.994 min
Delta R.T.: -0.001 min
Response: 153912
Conc: 4.71 ng/ml

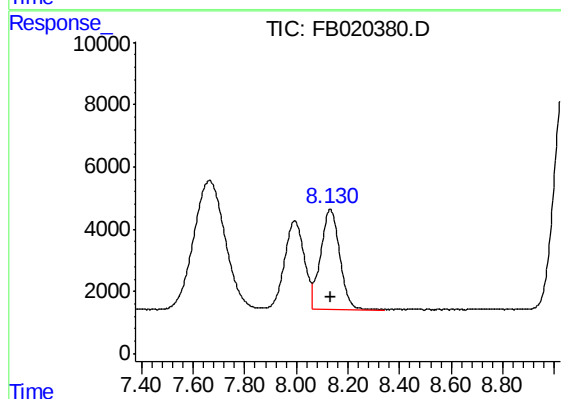


#4 Benzene

R.T.: 8.132 min
Delta R.T.: -0.001 min
Response: 166829
Conc: 4.82 ng/ml

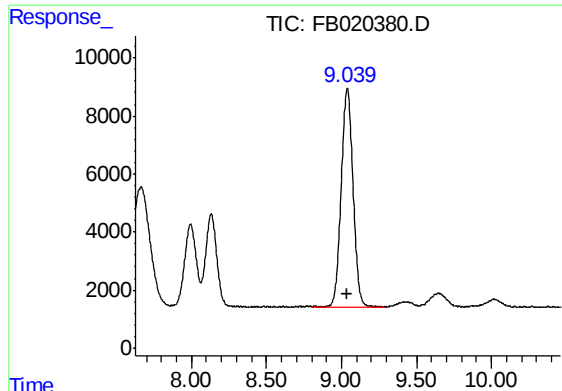


#5 AAA-TFT

R.T.: 9.039 min
Delta R.T.: -0.001 min
Response: 412890
Conc: 21.43 ng/ml

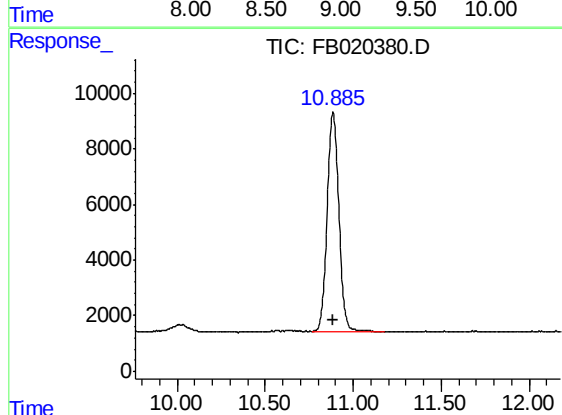


#6 Toluene

R.T.: 10.886 min
Delta R.T.: -0.001 min
Response: 368313
Conc: 14.20 ng/ml

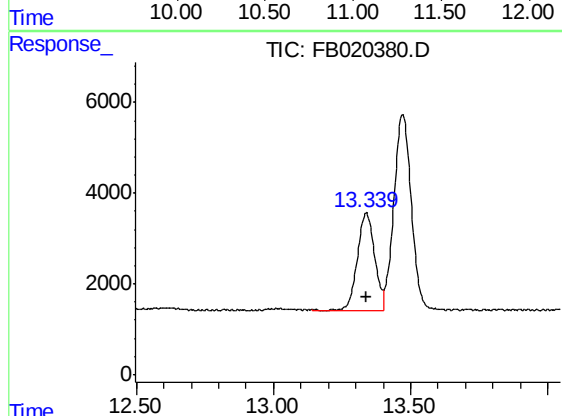


#7 Ethylbenzene

R.T.: 13.338 min
Delta R.T.: -0.002 min
Response: 93696
Conc: 4.76 ng/ml

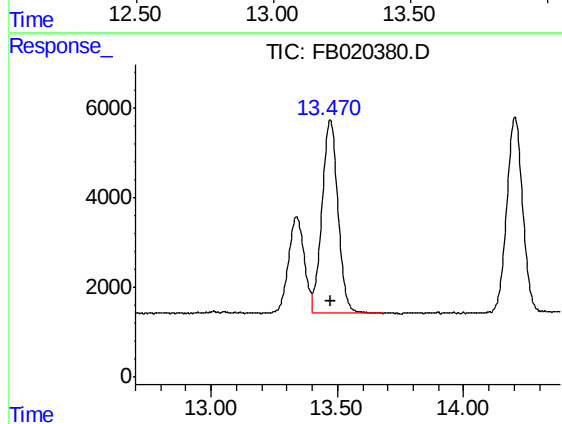


#8 m-Xylene

R.T.: 13.472 min
Delta R.T.: -0.002 min
Response: 192047
Conc: 9.46 ng/ml

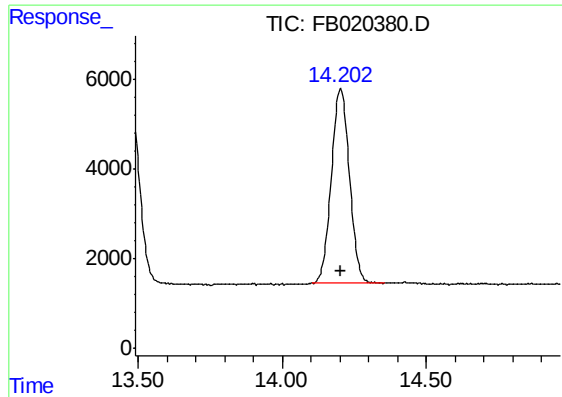

#9 O-Xylene

R.T.: 14.203 min
Delta R.T.: -0.002 min
Response: 190239
Conc: 9.39 ng/ml

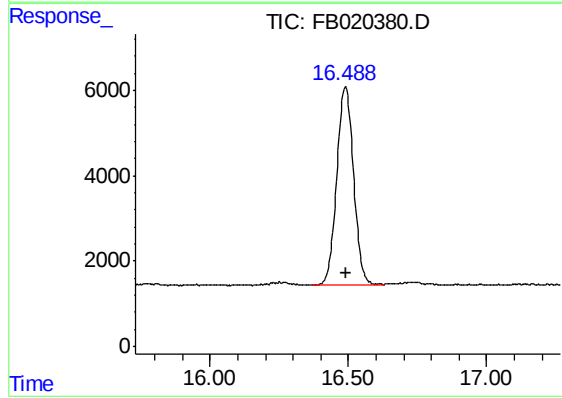

#10 1,2,4-Trimethylbenzene

R.T.: 16.489 min
Delta R.T.: -0.002 min
Response: 196567
Conc: 9.45 ng/ml