

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032719\
 Data File : FB020381.D
 Signal(s) : FID2B.CH
 Acq On : 27 Mar 2019 13:05
 Operator : MJ/SJ
 Sample : K1560-08
 Misc : 5.00ml DI WATER (10 PPB LOQ)
 ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 27 13:38:38 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
 Quant Title :
 QLast Update : Tue Mar 26 12:48:09 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.040	424191	22.017 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.901	417261	15.054 ng/ml
2) t 2,2,4-Trimethylpentane	7.665	382056	15.932 ng/ml
3) t n-Heptane	7.995	166325	5.087 ng/ml
4) t Benzene	8.133	177015	5.111 ng/ml
6) t Toluene	10.887	388756	14.989 ng/ml
7) t Ethylbenzene	13.339	97780	4.967 ng/ml
8) t m-Xylene	13.472	197314	9.719 ng/ml
9) t O-Xylene	14.203	194995	9.628 ng/ml
10) t 1,2,4-Trimethylbenzene	16.489	202616	9.738 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032719\
Data File : FB020381.D
Signal(s) : FID2B.CH
Acq On : 27 Mar 2019 13:05
Operator : MJ/SJ
Sample : K1560-08
Misc : 5.00ml DI WATER (10 PPB LOQ)
ALS Vial : 8 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 27 13:38:38 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
Quant Title :
QLast Update : Tue Mar 26 12:48:09 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

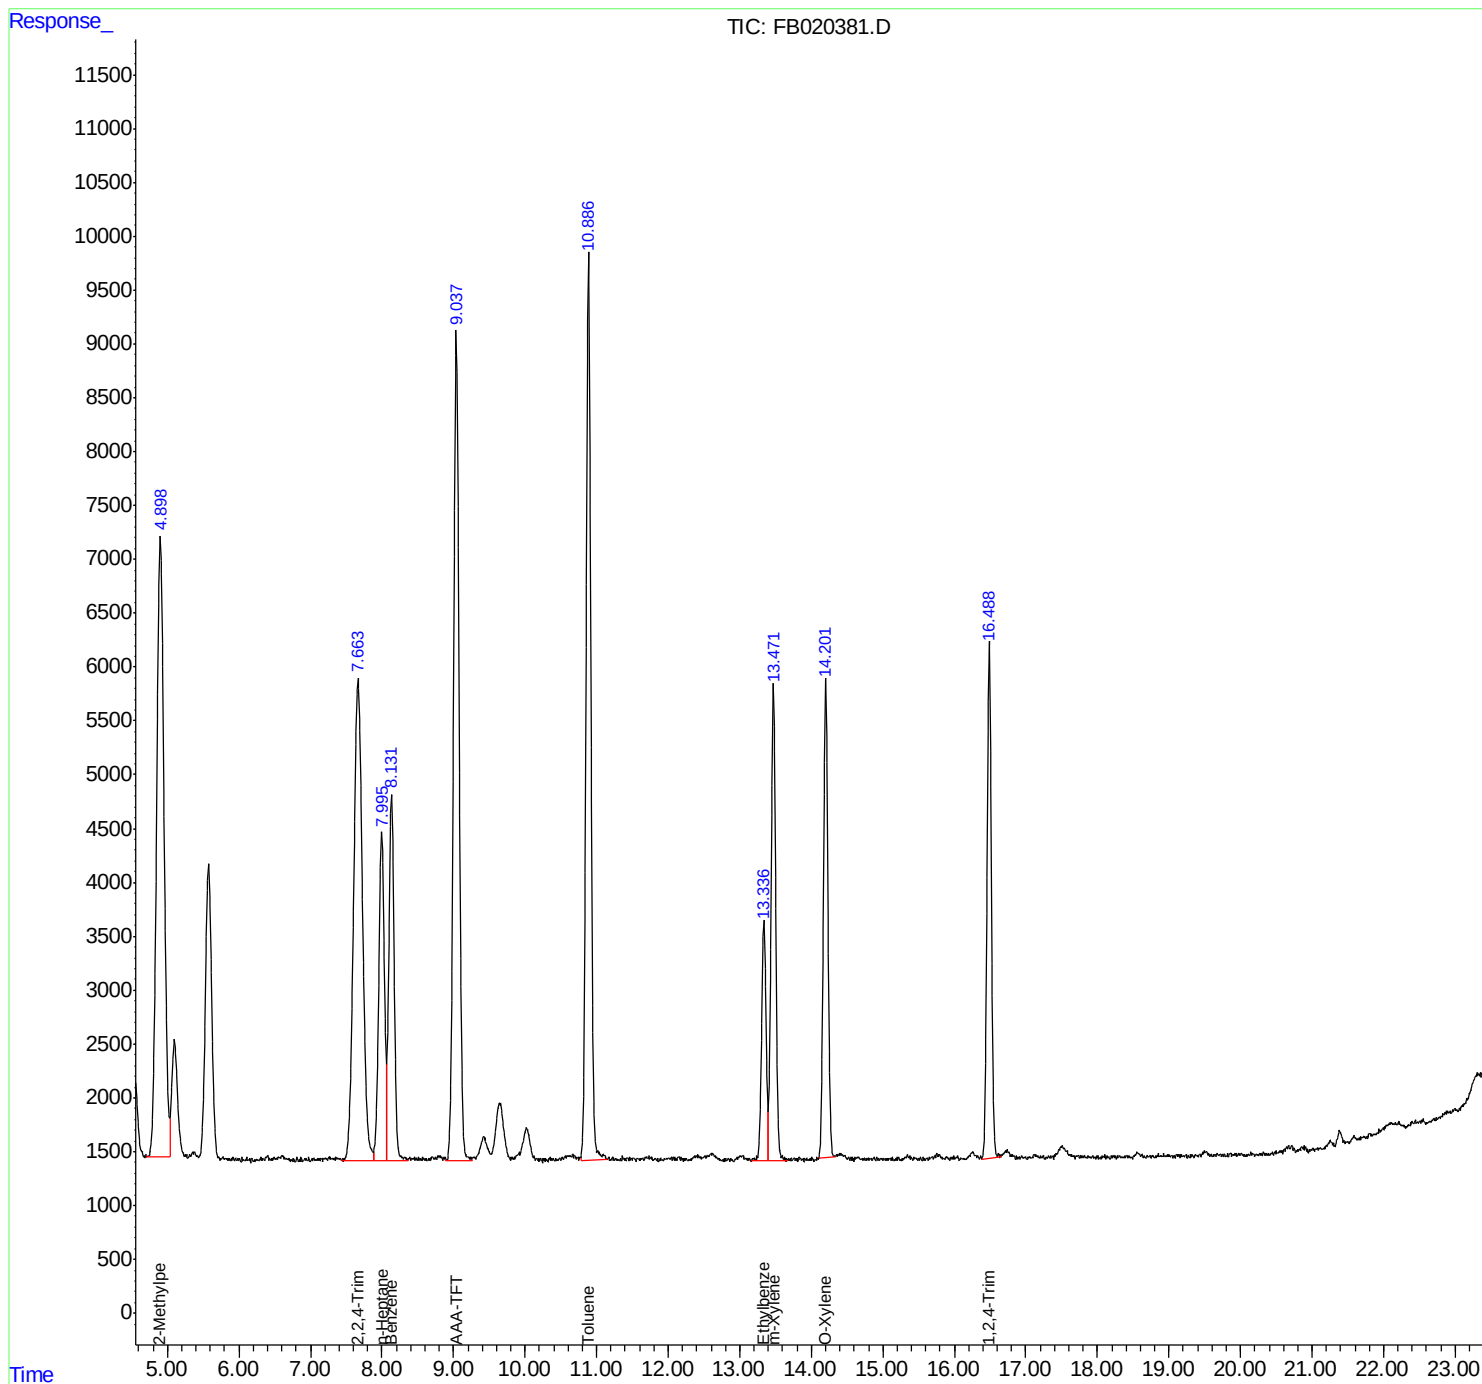

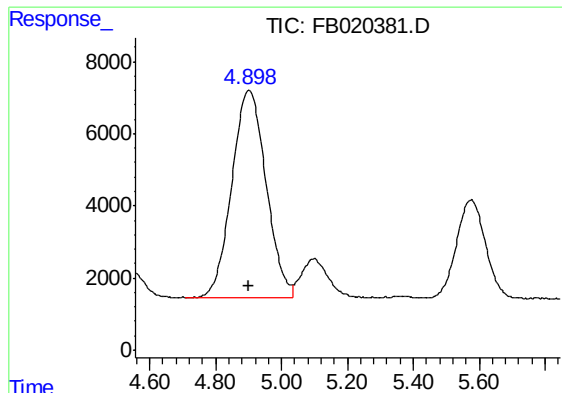


#1 2-Methylpentane

R.T.: 4.901 min
Delta R.T.: 0.002 min
Response: 417261
Conc: 15.05 ng/ml

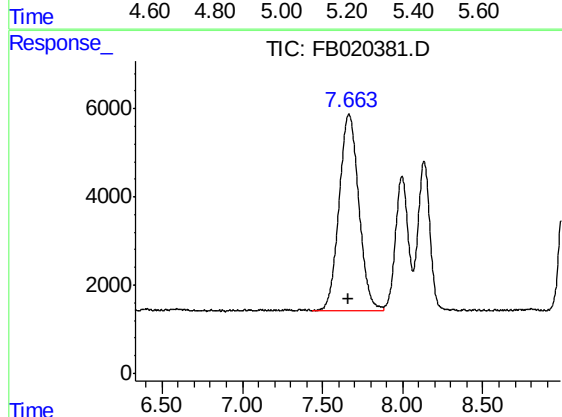


#2 2,2,4-Trimethylpentane

R.T.: 7.665 min
Delta R.T.: 0.000 min
Response: 382056
Conc: 15.93 ng/ml

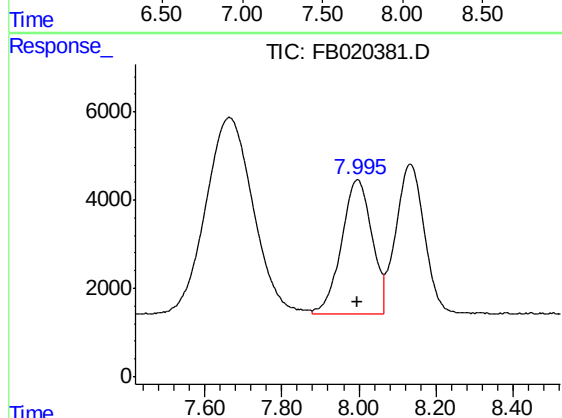


#3 n-Heptane

R.T.: 7.995 min
Delta R.T.: 0.000 min
Response: 166325
Conc: 5.09 ng/ml

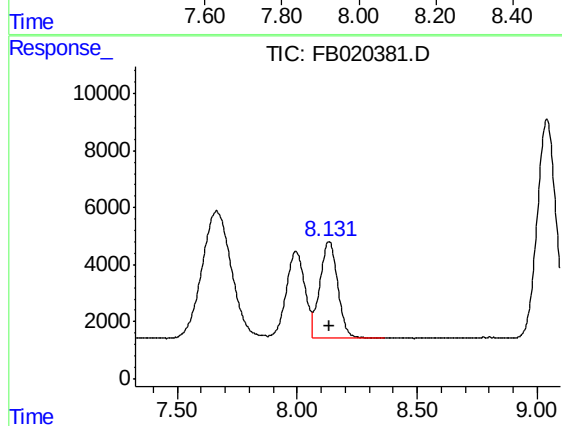


#4 Benzene

R.T.: 8.133 min
Delta R.T.: 0.000 min
Response: 177015
Conc: 5.11 ng/ml

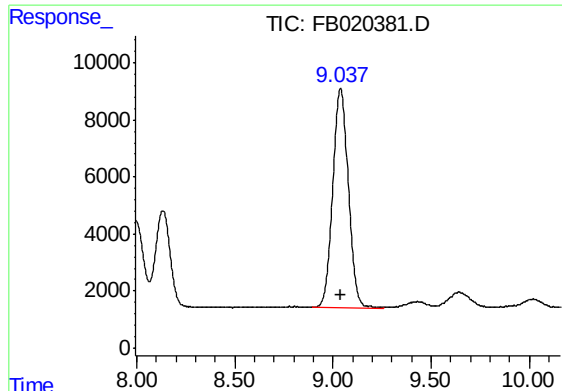


#5 AAA-TFT

R.T.: 9.040 min
Delta R.T.: 0.000 min
Response: 424191
Conc: 22.02 ng/ml

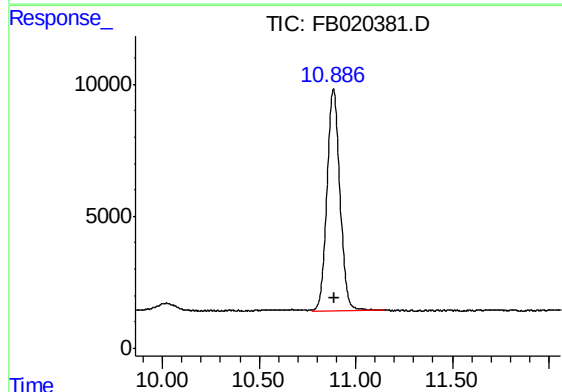


#6 Toluene

R.T.: 10.887 min
Delta R.T.: 0.000 min
Response: 388756
Conc: 14.99 ng/ml

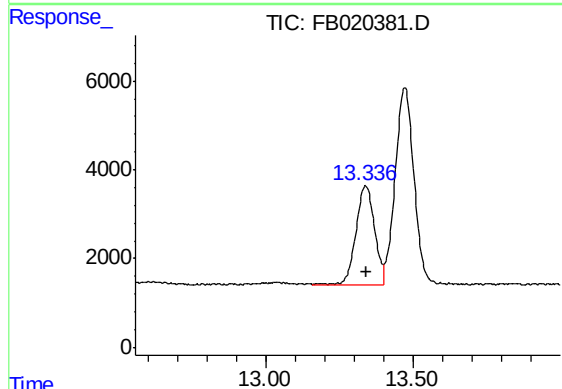


#7 Ethylbenzene

R.T.: 13.339 min
Delta R.T.: -0.002 min
Response: 97780
Conc: 4.97 ng/ml

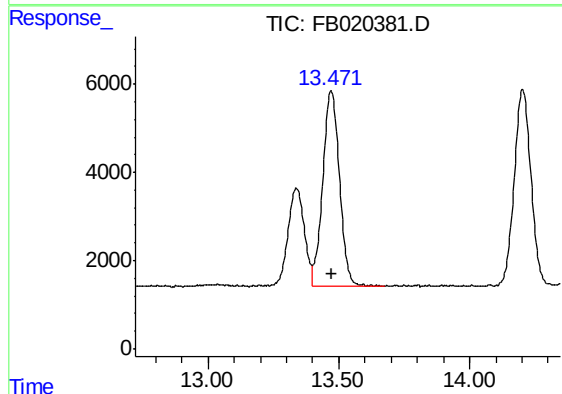


#8 m-Xylene

R.T.: 13.472 min
Delta R.T.: -0.002 min
Response: 197314
Conc: 9.72 ng/ml

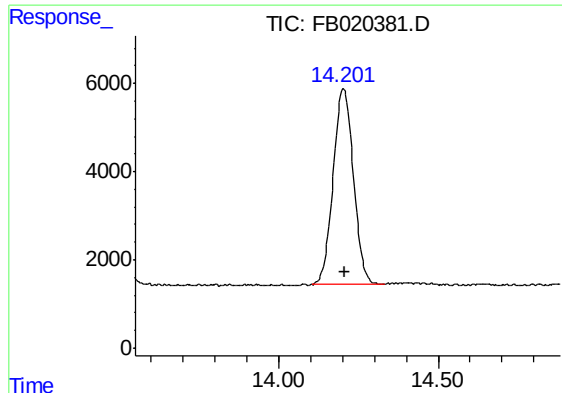

#9 O-Xylene

R.T.: 14.203 min
Delta R.T.: -0.002 min
Response: 194995
Conc: 9.63 ng/ml

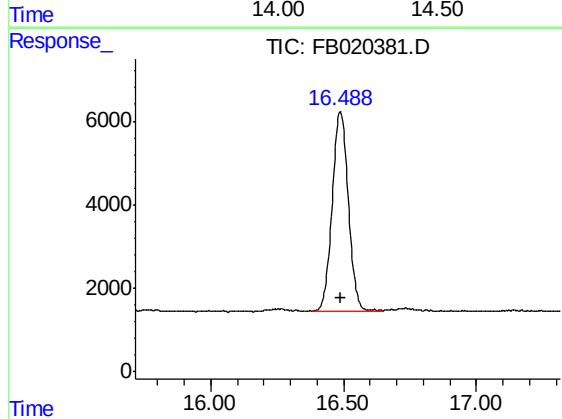

#10 1,2,4-Trimethylbenzene

R.T.: 16.489 min
Delta R.T.: -0.002 min
Response: 202616
Conc: 9.74 ng/ml