

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032719\
 Data File : FB020382.D
 Signal(s) : FID2B.CH
 Acq On : 27 Mar 2019 13:35
 Operator : MJ/SJ
 Sample : K1560-03
 Misc : 5.00gm/5.00ml DI WATER (1 PPB MDL)
 ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 27 14:10:37 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
 Quant Title :
 QLast Update : Tue Mar 26 12:48:09 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.041	385404	20.004 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.894	43452	1.568 ng/mlm
2) t 2,2,4-Trimethylpentane	7.673	42235	1.761 ng/ml
3) t n-Heptane	7.996	16931	0.518 ng/ml
4) t Benzene	8.133	18764	0.542 ng/ml
6) t Toluene	10.890	40477	1.561 ng/ml
7) t Ethylbenzene	13.338	11963	0.608 ng/ml
8) t m-Xylene	13.475	22008	1.084 ng/ml
9) t O-Xylene	14.208	22388	1.105 ng/ml
10) t 1,2,4-Trimethylbenzene	16.495	24698	1.187 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032719\
Data File : FB020382.D
Signal(s) : FID2B.CH
Acq On : 27 Mar 2019 13:35
Operator : MJ/SJ
Sample : K1560-03
Misc : 5.00gm/5.00ml DI WATER (1 PPB MDL)
ALS Vial : 9 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 27 14:10:37 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
Quant Title :
QLast Update : Tue Mar 26 12:48:09 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

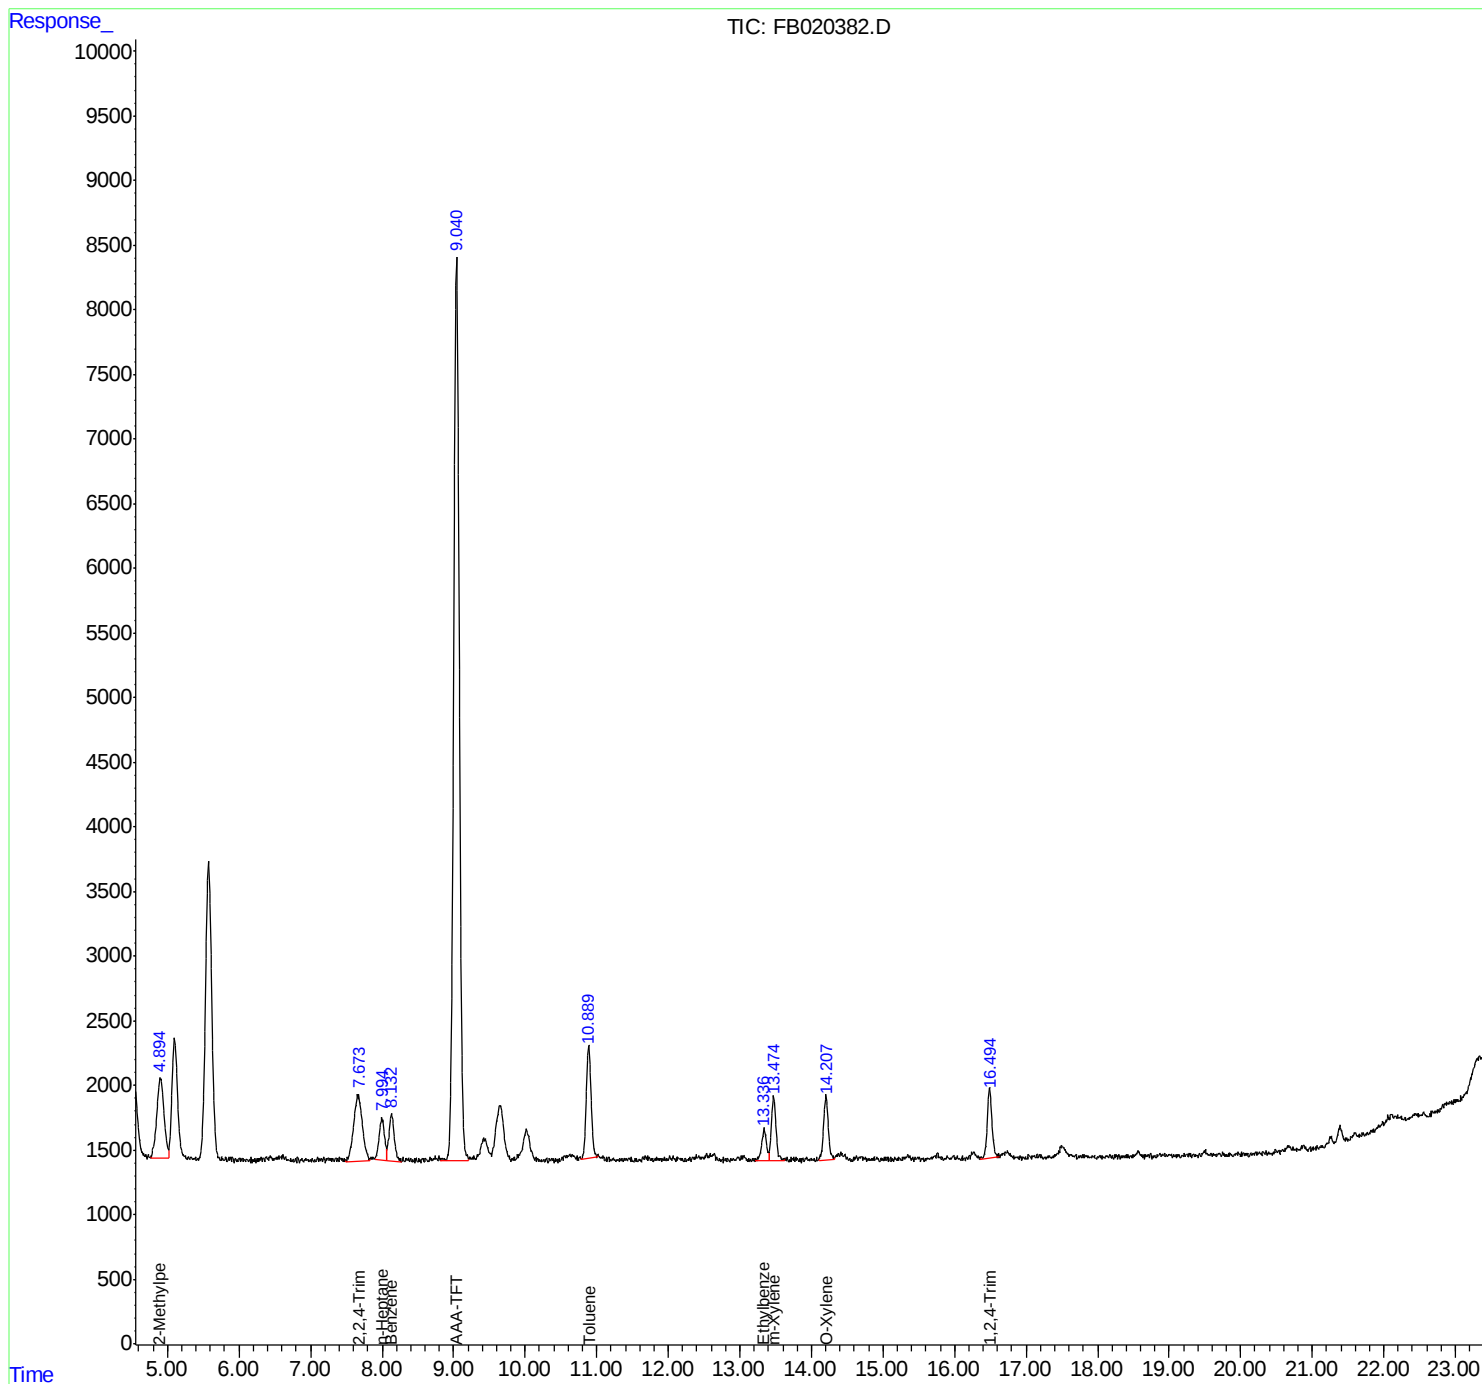

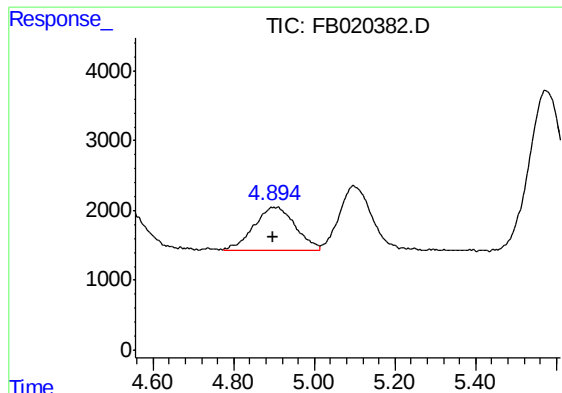


#1 2-Methylpentane

R.T.: 4.894 min
Delta R.T.: -0.005 min
Response: 43452
Conc: 1.57 ng/ml m

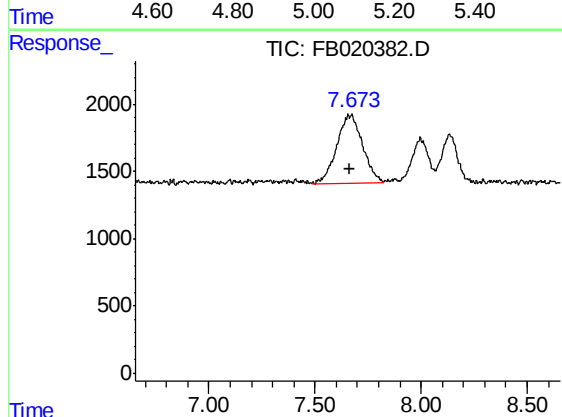


#2 2,2,4-Trimethylpentane

R.T.: 7.673 min
Delta R.T.: 0.007 min
Response: 42235
Conc: 1.76 ng/ml

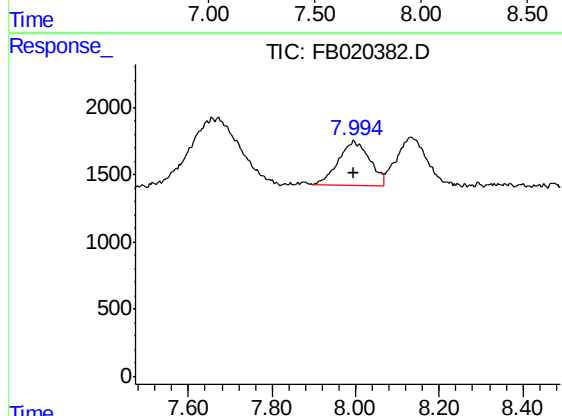


#3 n-Heptane

R.T.: 7.996 min
Delta R.T.: 0.001 min
Response: 16931
Conc: 0.52 ng/ml

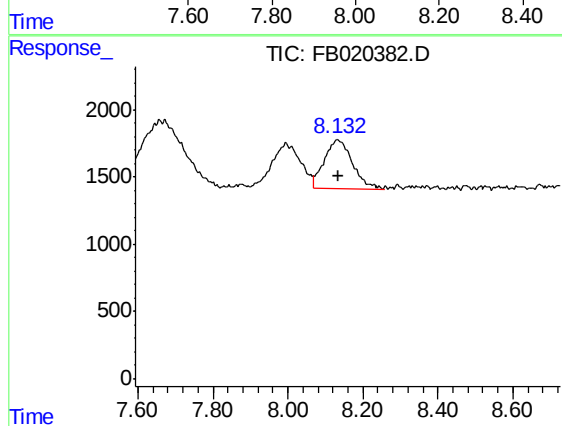


#4 Benzene

R.T.: 8.133 min
Delta R.T.: 0.000 min
Response: 18764
Conc: 0.54 ng/ml

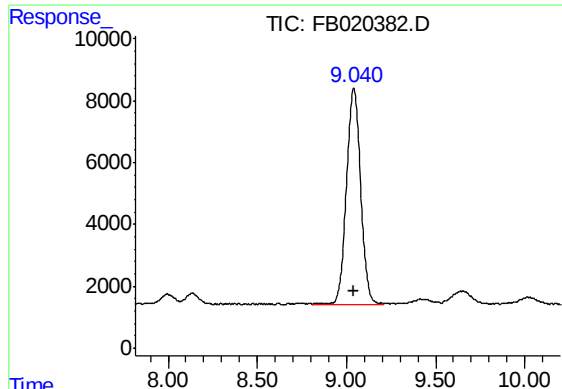


#5 AAA-TFT

R.T.: 9.041 min
Delta R.T.: 0.000 min
Response: 385404
Conc: 20.00 ng/ml

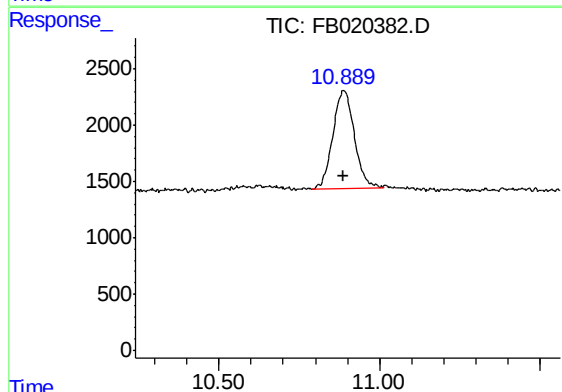


#6 Toluene

R.T.: 10.890 min
Delta R.T.: 0.002 min
Response: 40477
Conc: 1.56 ng/ml

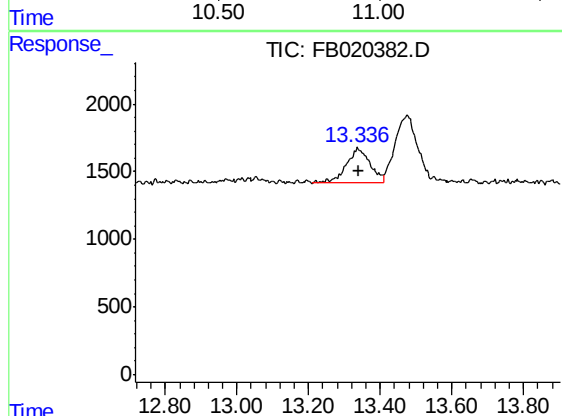


#7 Ethylbenzene

R.T.: 13.338 min
Delta R.T.: -0.002 min
Response: 11963
Conc: 0.61 ng/ml

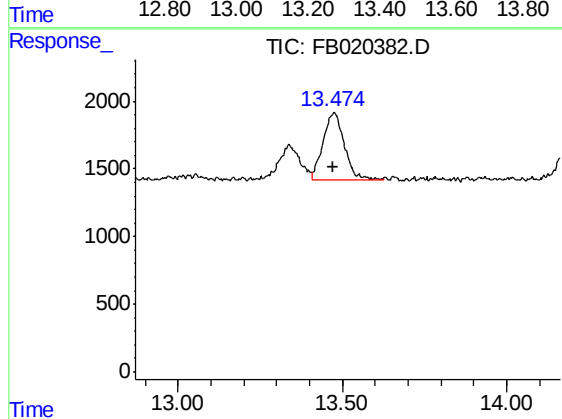


#8 m-Xylene

R.T.: 13.475 min
Delta R.T.: 0.002 min
Response: 22008
Conc: 1.08 ng/ml

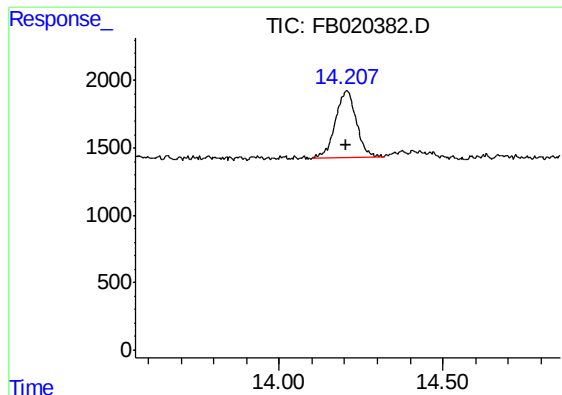

#9 O-Xylene

R.T.: 14.208 min
Delta R.T.: 0.003 min
Response: 22388
Conc: 1.11 ng/ml

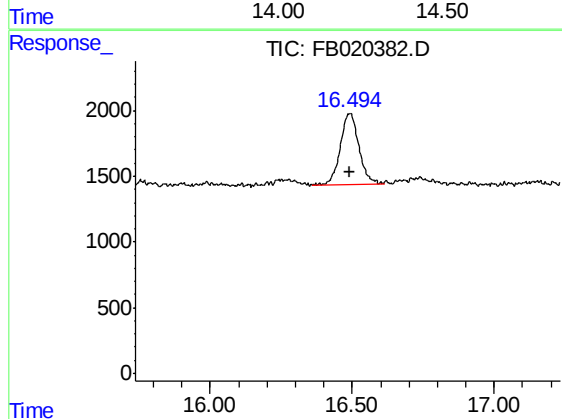

#10 1,2,4-Trimethylbenzene

R.T.: 16.495 min
Delta R.T.: 0.004 min
Response: 24698
Conc: 1.19 ng/ml