

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032719\
 Data File : FB020386.D
 Signal(s) : FID2B.CH
 Acq On : 27 Mar 2019 15:37
 Operator : MJ/SJ
 Sample : K2107-18MSD
 Misc : 5.01gm/5.00ml DI WATER
 ALS Vial : 13 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 27 15:52:11 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
 Quant Title :
 QLast Update : Tue Mar 26 12:48:09 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.040	477855	24.802 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.901	867521	31.298 ng/ml
2) t 2,2,4-Trimethylpentane	7.667	759995	31.693 ng/ml
3) t n-Heptane	7.996	348140	10.649 ng/ml
4) t Benzene	8.133	383623	11.077 ng/ml
6) t Toluene	10.887	848569	32.717 ng/ml
7) t Ethylbenzene	13.340	202439	10.283 ng/ml
8) t m-Xylene	13.473	407233	20.058 ng/ml
9) t O-Xylene	14.205	401356	19.817 ng/ml
10) t 1,2,4-Trimethylbenzene	16.490	416901	20.038 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032719\
Data File : FB020386.D
Signal(s) : FID2B.CH
Acq On : 27 Mar 2019 15:37
Operator : MJ/SJ
Sample : K2107-18MSD
Misc : 5.01gm/5.00ml DI WATER
ALS Vial : 13 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 27 15:52:11 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
Quant Title :
QLast Update : Tue Mar 26 12:48:09 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

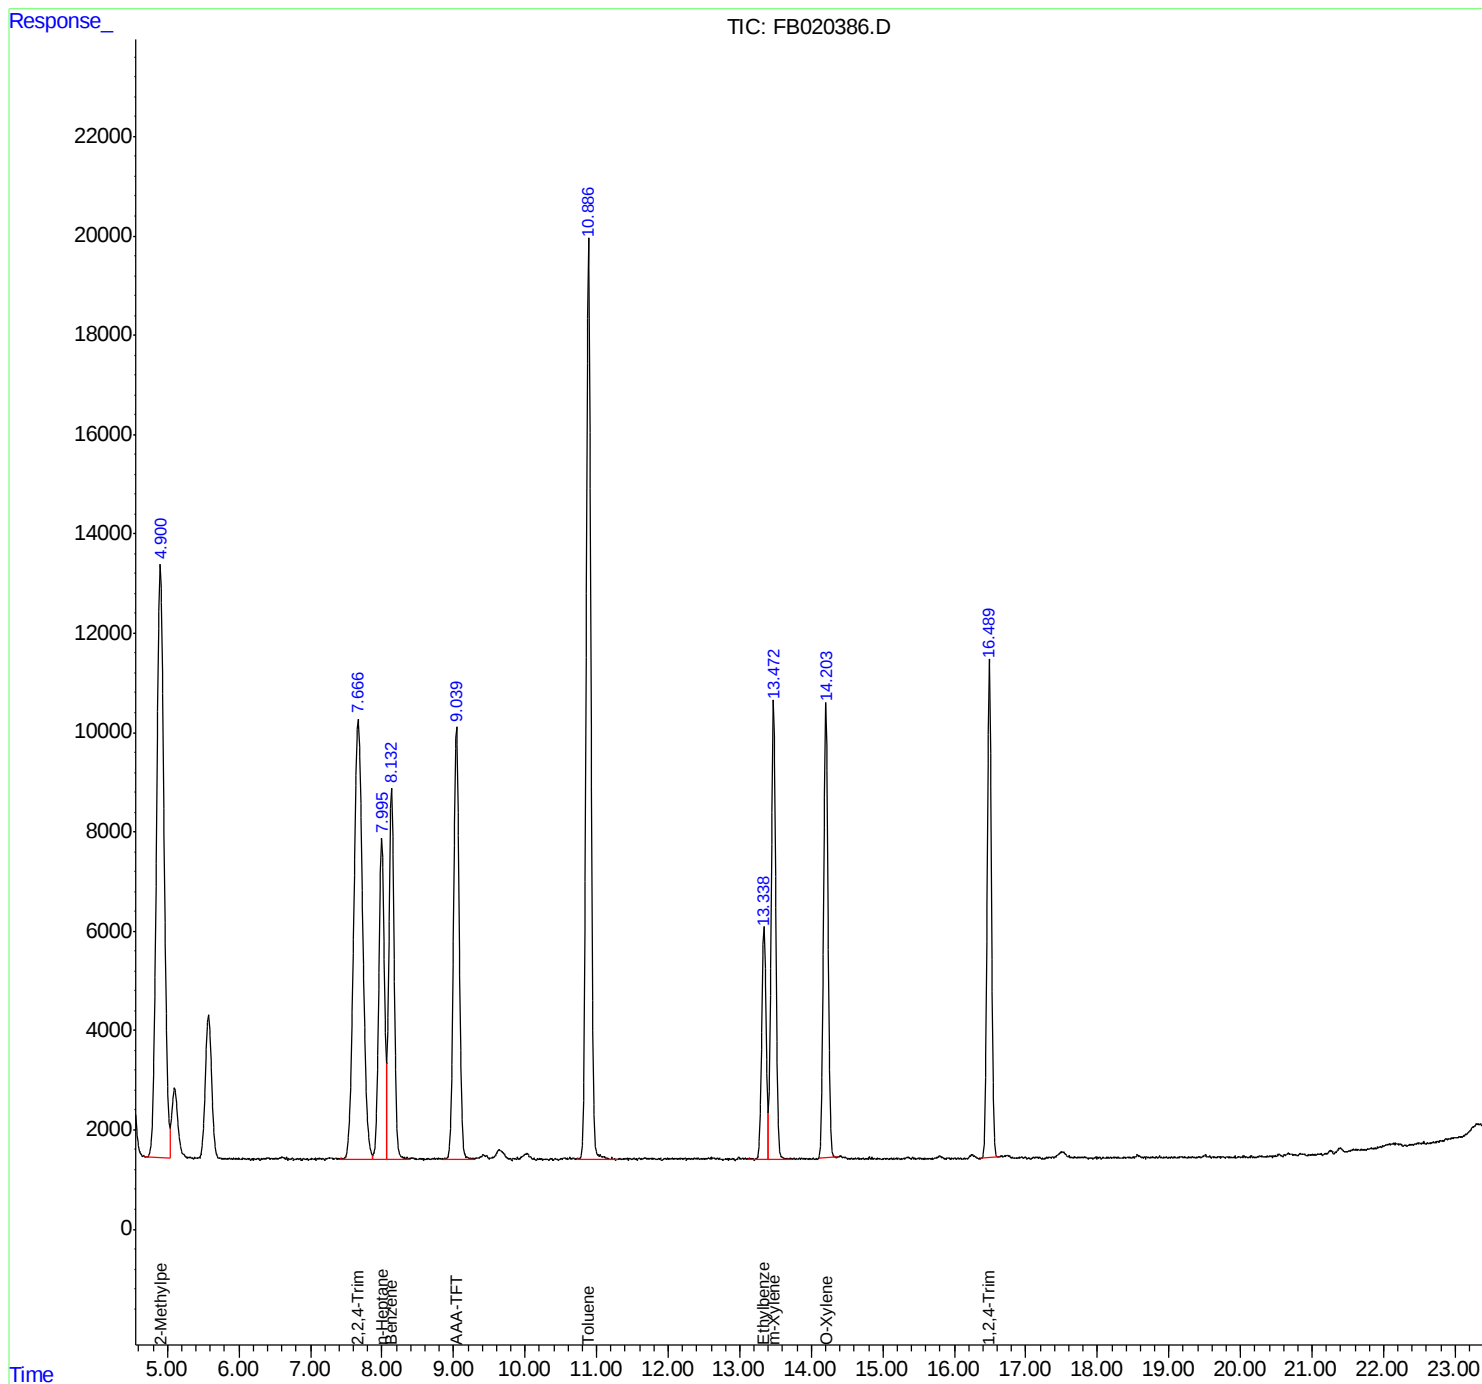

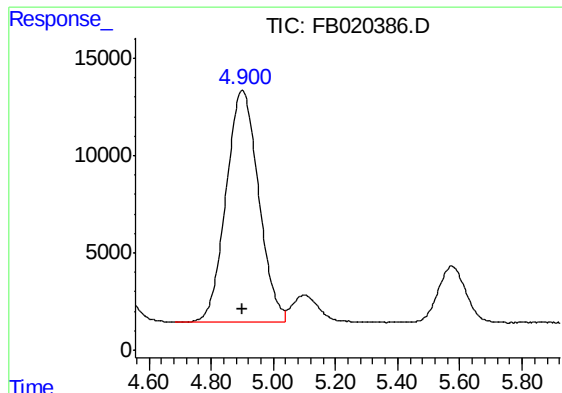


#1 2-Methylpentane

R.T.: 4.901 min
Delta R.T.: 0.002 min
Response: 867521
Conc: 31.30 ng/ml

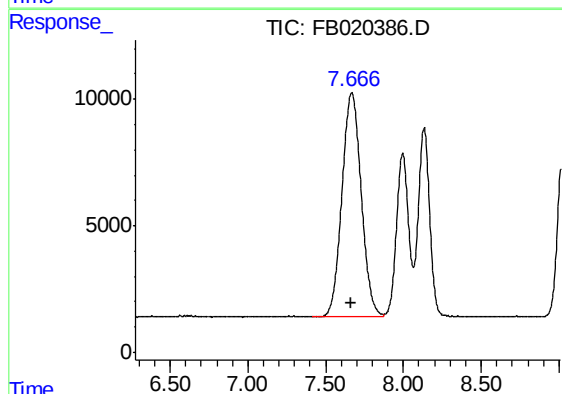


#2 2,2,4-Trimethylpentane

R.T.: 7.667 min
Delta R.T.: 0.000 min
Response: 759995
Conc: 31.69 ng/ml

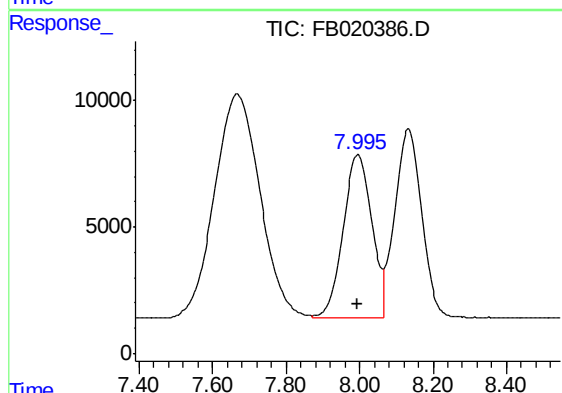


#3 n-Heptane

R.T.: 7.996 min
Delta R.T.: 0.000 min
Response: 348140
Conc: 10.65 ng/ml

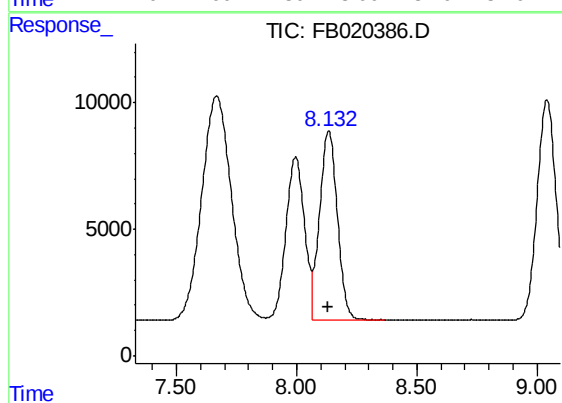


#4 Benzene

R.T.: 8.133 min
Delta R.T.: 0.000 min
Response: 383623
Conc: 11.08 ng/ml

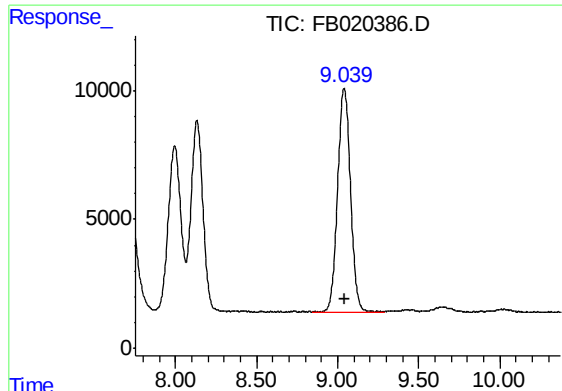


#5 AAA-TFT

R.T.: 9.040 min
Delta R.T.: 0.000 min
Response: 477855
Conc: 24.80 ng/ml

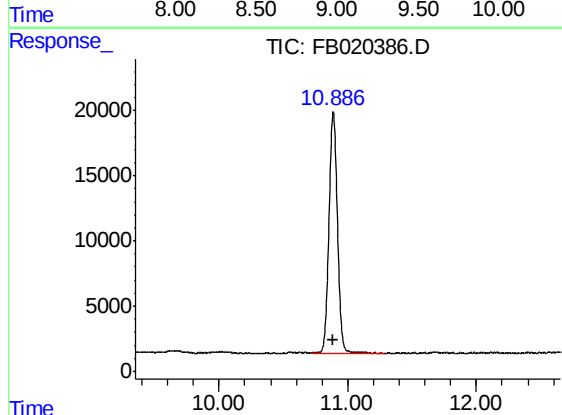


#6 Toluene

R.T.: 10.887 min
Delta R.T.: 0.000 min
Response: 848569
Conc: 32.72 ng/ml

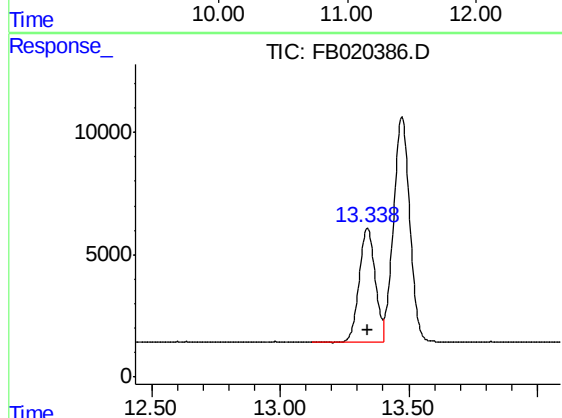


#7 Ethylbenzene

R.T.: 13.340 min
Delta R.T.: 0.000 min
Response: 202439
Conc: 10.28 ng/ml

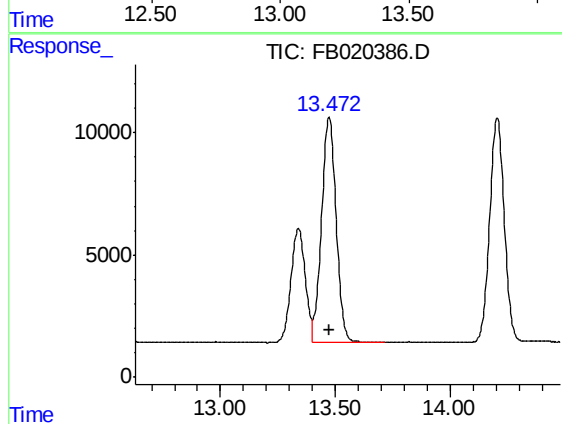


#8 m-Xylene

R.T.: 13.473 min
Delta R.T.: 0.000 min
Response: 407233
Conc: 20.06 ng/ml

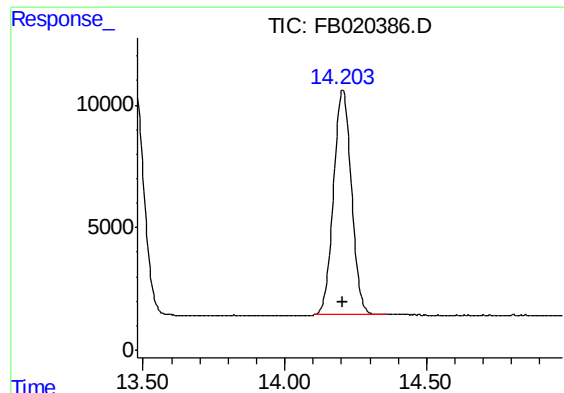

#9 O-Xylene

R.T.: 14.205 min
Delta R.T.: 0.000 min
Response: 401356
Conc: 19.82 ng/ml

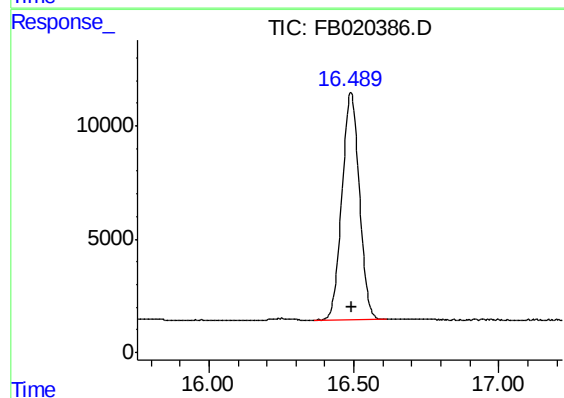

#10 1,2,4-Trimethylbenzene

R.T.: 16.490 min
Delta R.T.: 0.000 min
Response: 416901
Conc: 20.04 ng/ml