

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032720\
 Data File : FB024027.D
 Signal(s) : FID2B.CH
 Acq On : 27 Mar 2020 16:18
 Operator : DD/AJ
 Sample : L1753-10
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 28 01:12:18 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032620.M
 Quant Title :
 QLast Update : Fri Mar 27 11:16:49 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.803	423416	18.538 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.687	9127	0.264 ng/ml
2) t 2,2,4-Trimethylpentane	7.429	1542	0.042 ng/ml
6) t Toluene	10.631	3722	0.084 ng/ml
7) t Ethylbenzene	13.039	988	0.025 ng/ml
8) t m-Xylene	13.211	3505	0.091 ng/ml
9) t O-Xylene	13.944	1178	0.032 ng/ml
10) t 1,2,4-Trimethylbenzene	16.234	3120	0.098 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032720\
Data File : FB024027.D
Signal(s) : FID2B.CH
Acq On : 27 Mar 2020 16:18
Operator : DD/AJ
Sample : L1753-10
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 28 01:12:18 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032620.M
Quant Title :
QLast Update : Fri Mar 27 11:16:49 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

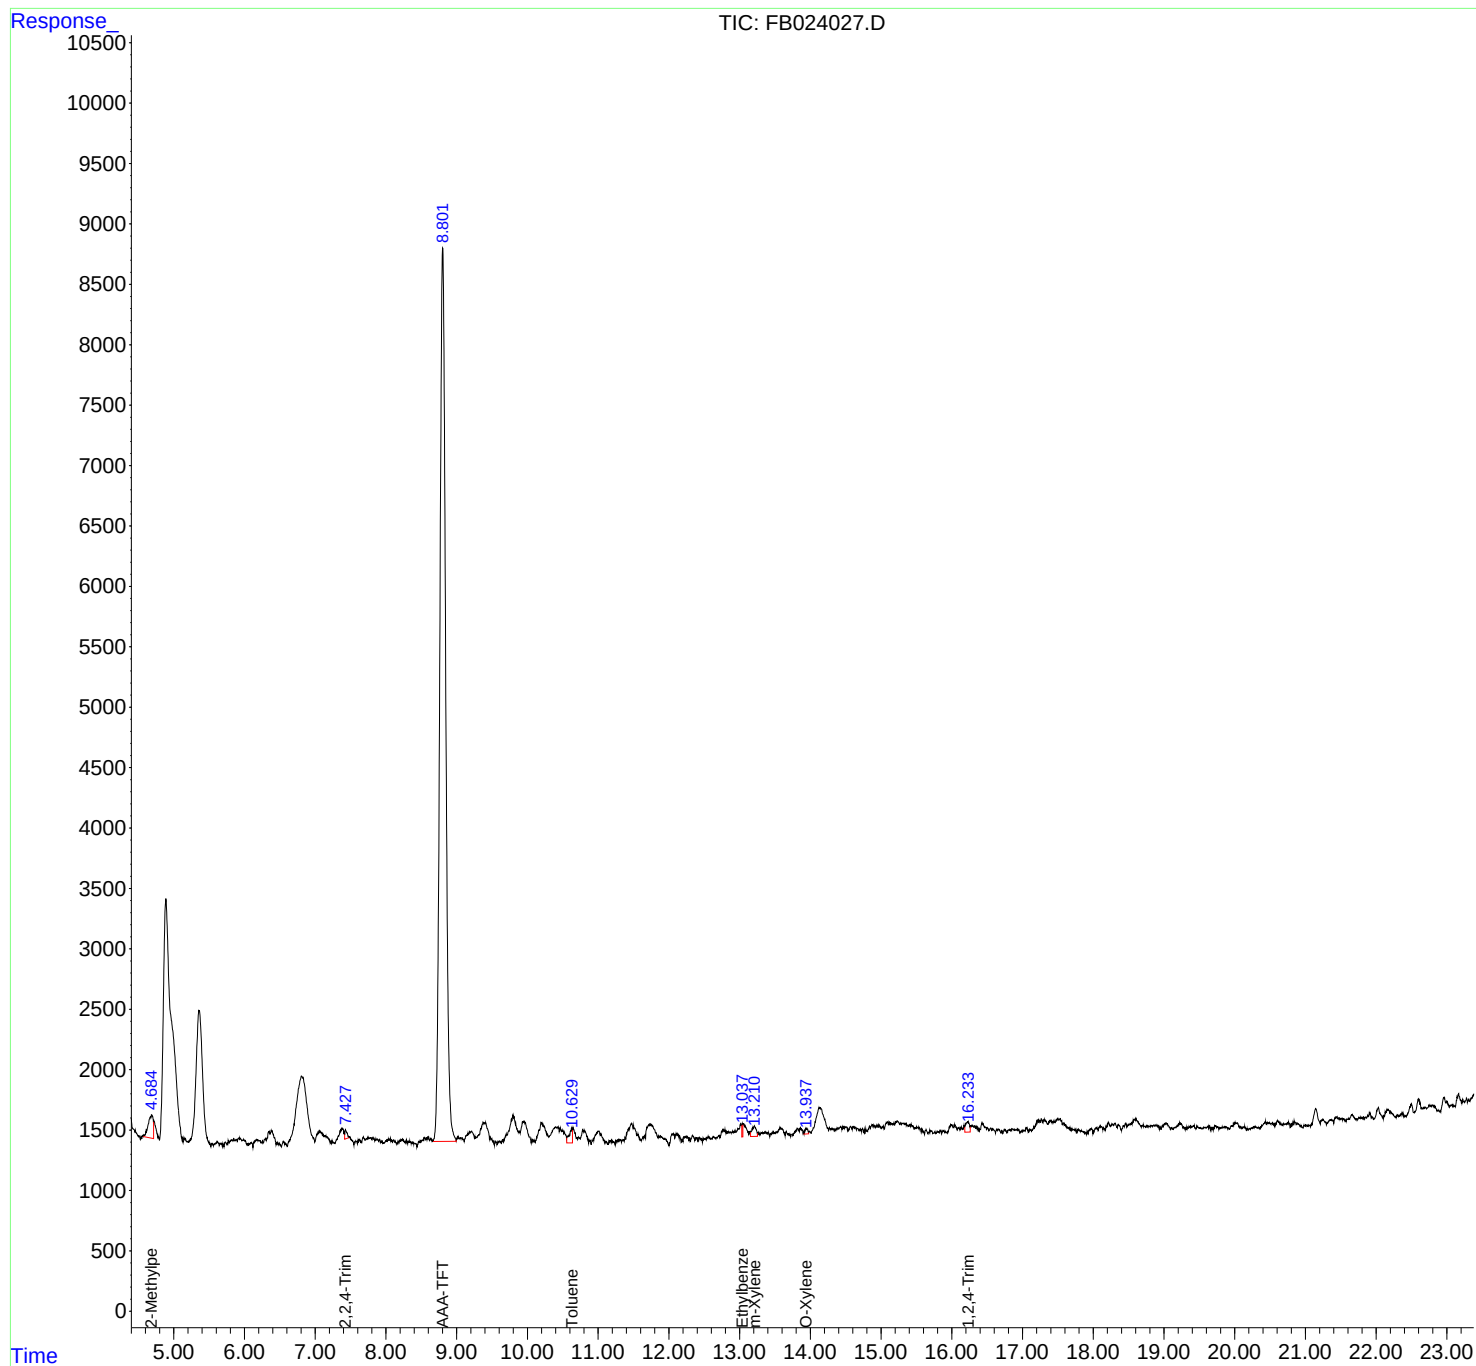


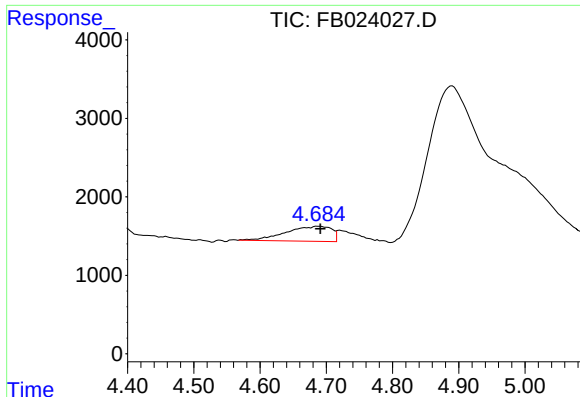

#1 2-Methylpentane


R.T.: 4.687 min
Delta R.T.: -0.004 min
Response: 9127
Conc: 0.26 ng/ml

Instrument :
FID_B
ClientSampleId :

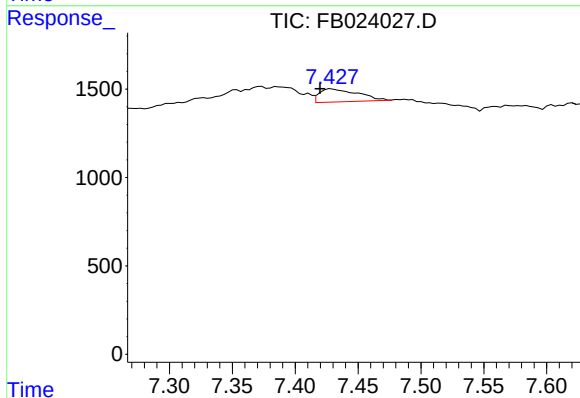


#2 2,2,4-Trimethylpentane

R.T.: 7.429 min
Delta R.T.: 0.009 min
Response: 1542
Conc: 0.04 ng/ml

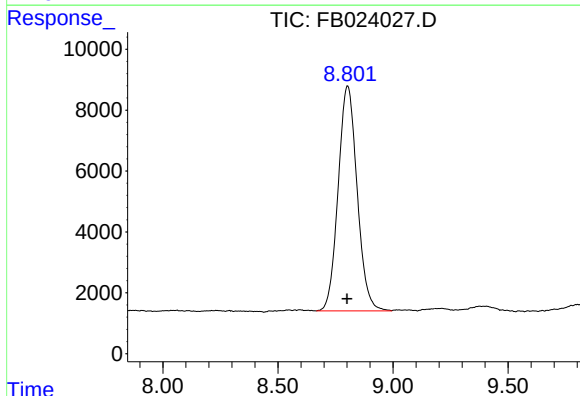


#5 AAA-TFT

R.T.: 8.803 min
Delta R.T.: 0.002 min
Response: 423416
Conc: 18.54 ng/ml

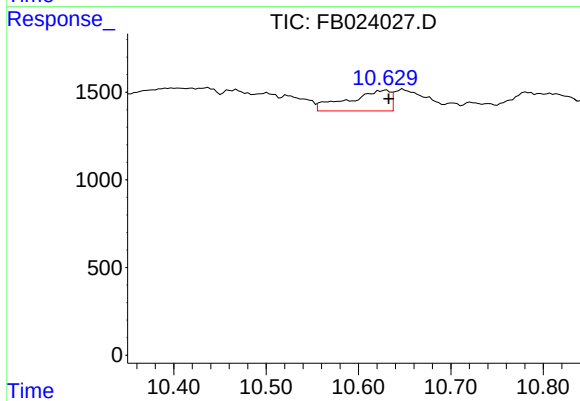

#6 Toluene


R.T.: 10.631 min
Delta R.T.: -0.002 min
Response: 3722
Conc: 0.08 ng/ml

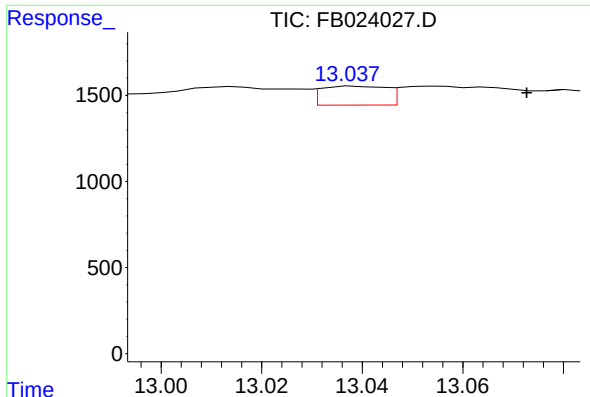

#7 Ethylbenzene


R.T.: 13.039 min
Delta R.T.: -0.034 min
Response: 988
Conc: 0.02 ng/ml

Instrument :
FID_B
ClientSampleId :

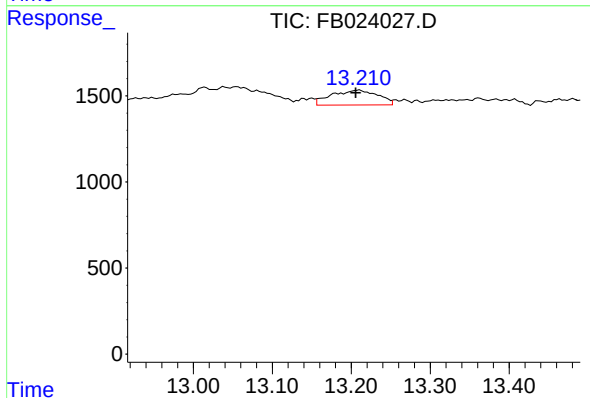


#8 m-Xylene

R.T.: 13.211 min
Delta R.T.: 0.005 min
Response: 3505
Conc: 0.09 ng/ml

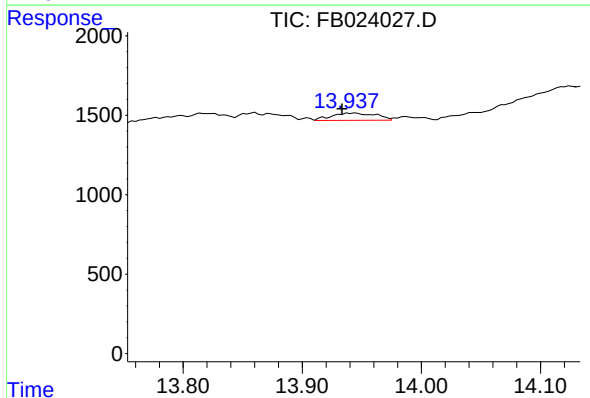

#9 o-Xylene

R.T.: 13.944 min
Delta R.T.: 0.010 min
Response: 1178
Conc: 0.03 ng/ml

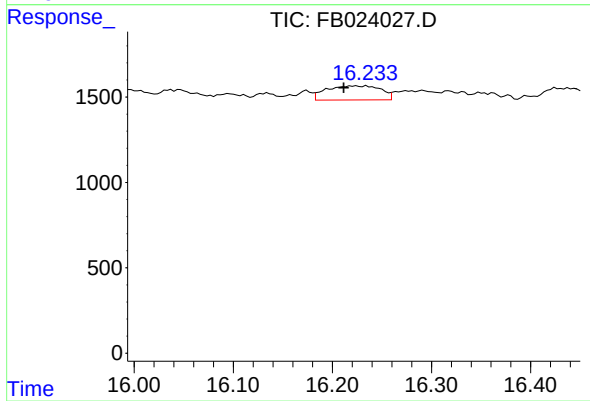

#10 1,2,4-Trimethylbenzene

R.T.: 16.234 min
Delta R.T.: 0.023 min
Response: 3120
Conc: 0.10 ng/ml