

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032720\
Data File : FB024030.D
Signal(s) : FID2B.CH
Acq On : 27 Mar 2020 17:50
Operator : DD/AJ
Sample : L2043-03
Misc : 5.08g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 28 01:12:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032620.M
Quant Title :
QLast Update : Fri Mar 27 11:16:49 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.802	475915	20.837 ng/ml
Target Compounds			
6) t Toluene	10.637	652	0.015 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032720\
Data File : FB024030.D
Signal(s) : FID2B.CH
Acq On : 27 Mar 2020 17:50
Operator : DD/AJ
Sample : L2043-03
Misc : 5.08g/5.00ml DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 28 01:12:44 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032620.M
Quant Title :
QLast Update : Fri Mar 27 11:16:49 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

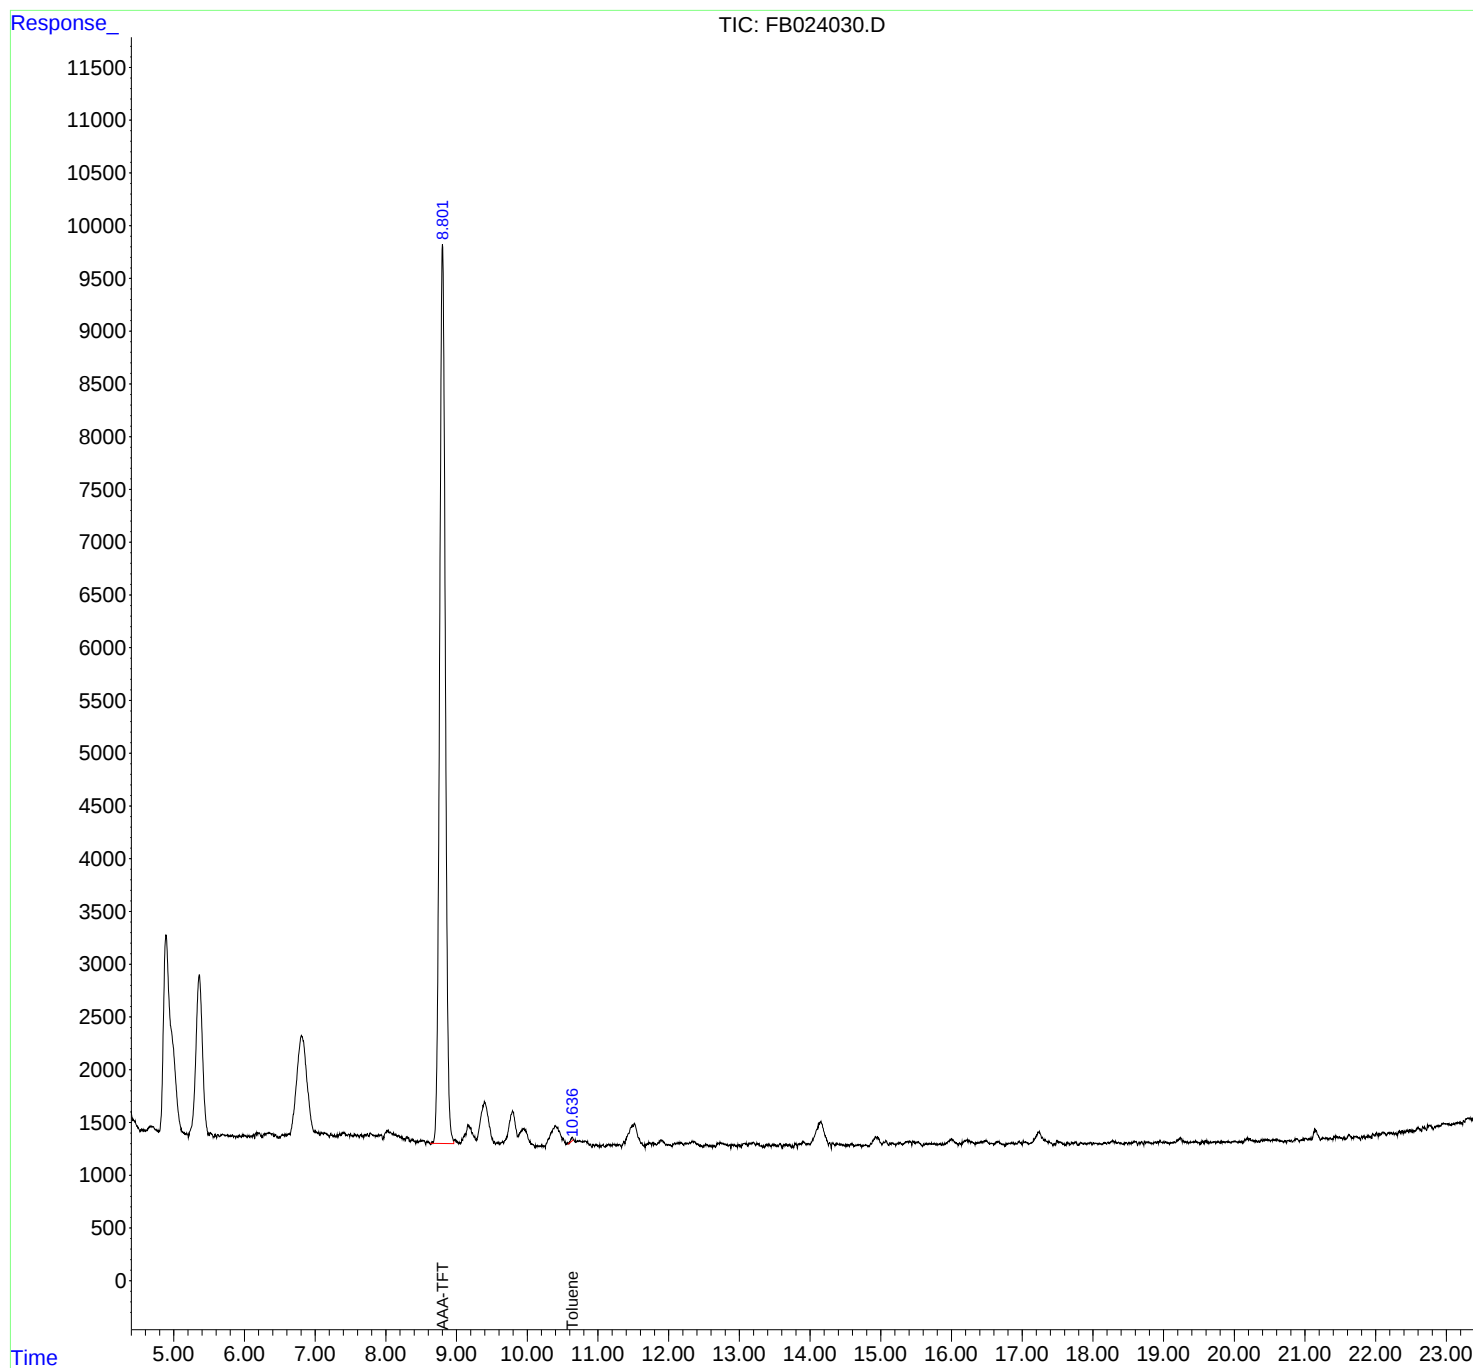


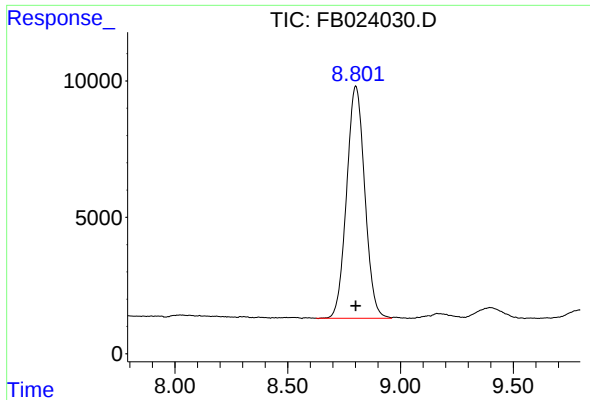

#5 AAA-TFT

R.T.: 8.802 min
Delta R.T.: 0.000 min
Response: 475915
Conc: 20.84 ng/ml

Instrument :
FID_B
ClientSampleId :

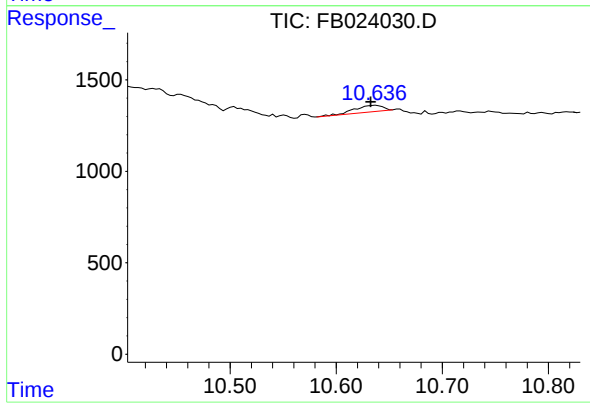

#6 Toluene

R.T.: 10.637 min
Delta R.T.: 0.005 min
Response: 652
Conc: 0.01 ng/ml