

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032720\
 Data File : FB024040.D
 Signal(s) : FID2B.CH
 Acq On : 27 Mar 2020 23:28
 Operator : DD/AJ
 Sample : L1762-24
 Misc : 5.04g/5.00ml DI WATER
 ALS Vial : 21 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 28 01:14:13 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032620.M
 Quant Title :
 QLast Update : Fri Mar 27 11:16:49 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.798	428488	18.760 ng/ml
Target Compounds			
2) t 2,2,4-Trimethylpentane	7.385	1375	0.037 ng/ml
4) t Benzene	7.882	5285	0.119 ng/ml
6) t Toluene	10.629	24131	0.548 ng/ml
7) t Ethylbenzene	13.075	4477	0.112 ng/ml
8) t m-Xylene	13.201	17100	0.445 ng/ml
9) t O-Xylene	13.935	5562	0.150 ng/ml
10) t 1,2,4-Trimethylbenzene	16.213	799	0.025 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032720\
Data File : FB024040.D
Signal(s) : FID2B.CH
Acq On : 27 Mar 2020 23:28
Operator : DD/AJ
Sample : L1762-24
Misc : 5.04g/5.00ml DI WATER
ALS Vial : 21 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 28 01:14:13 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032620.M
Quant Title :
QLast Update : Fri Mar 27 11:16:49 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

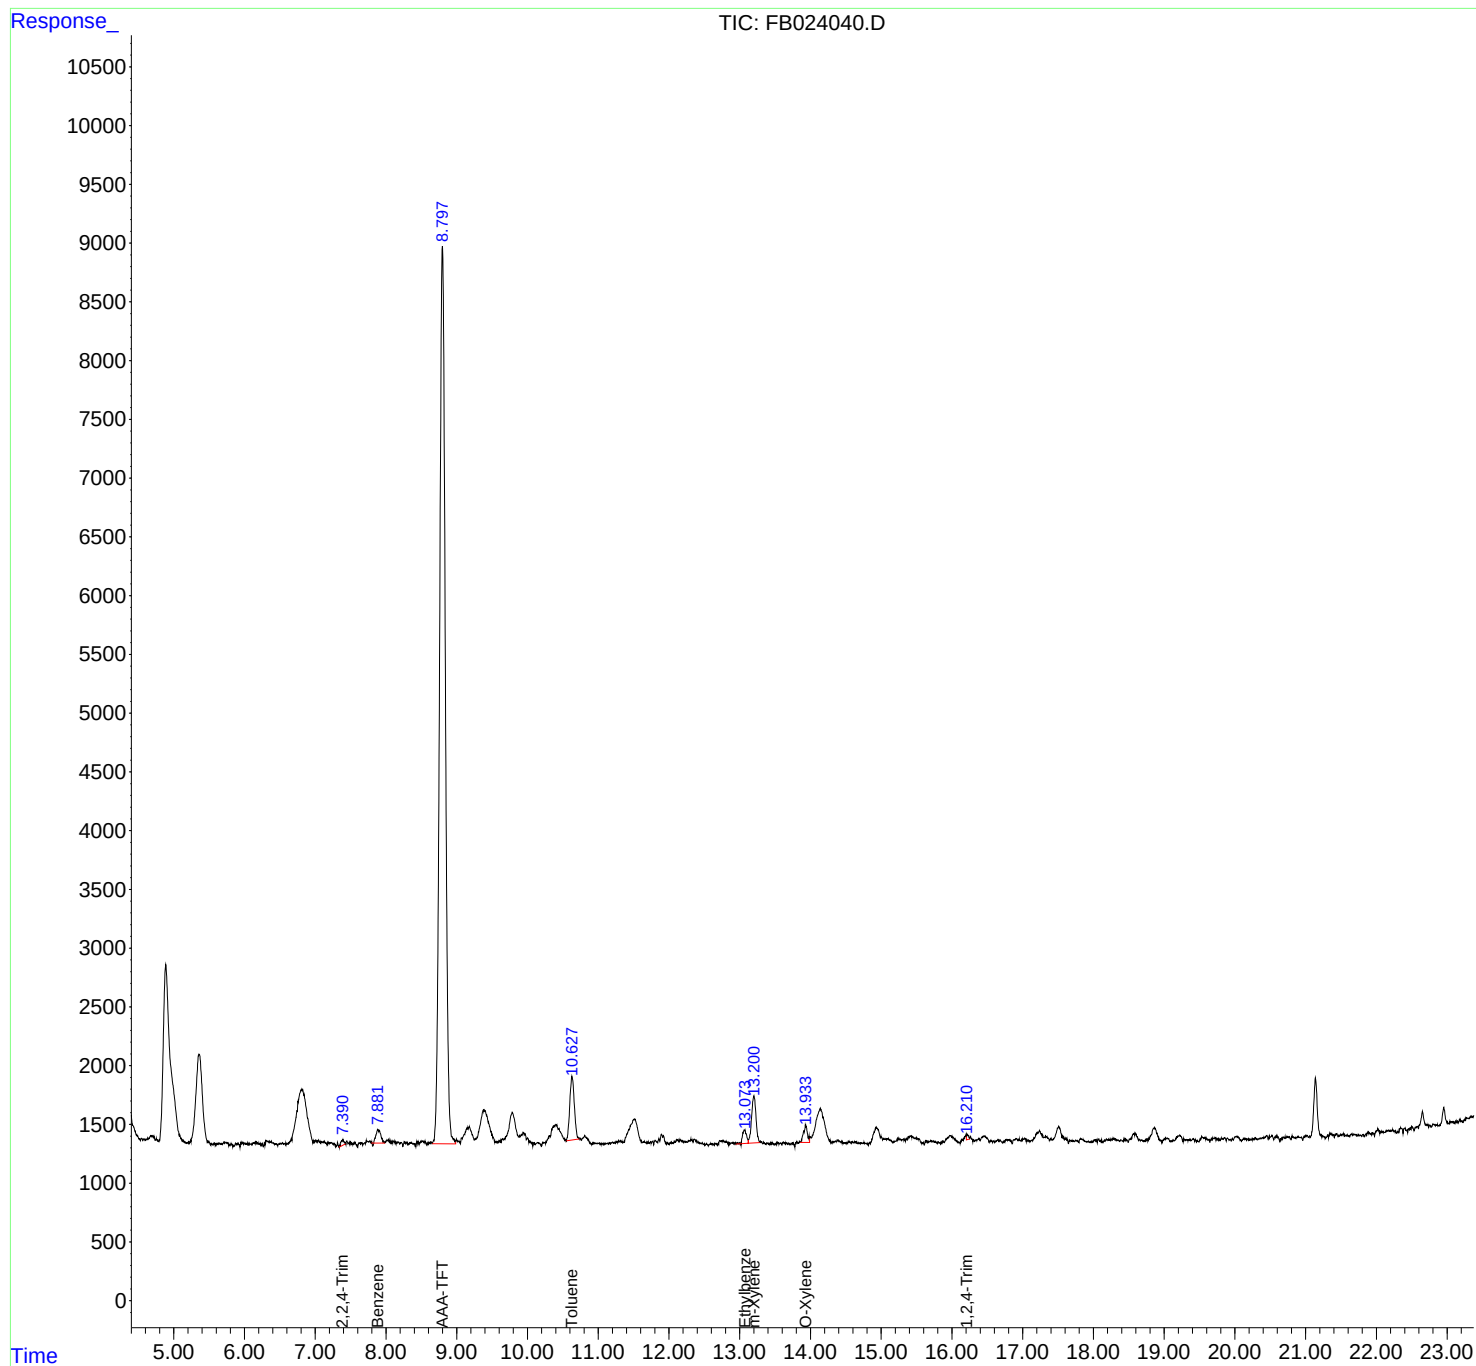


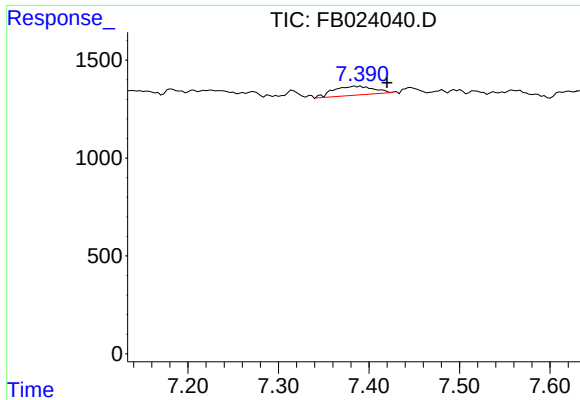

#2 2,2,4-Trimethylpentane


R.T.: 7.385 min
Delta R.T.: -0.035 min
Response: 1375
Conc: 0.04 ng/ml

Instrument :
FID_B
ClientSampleId :

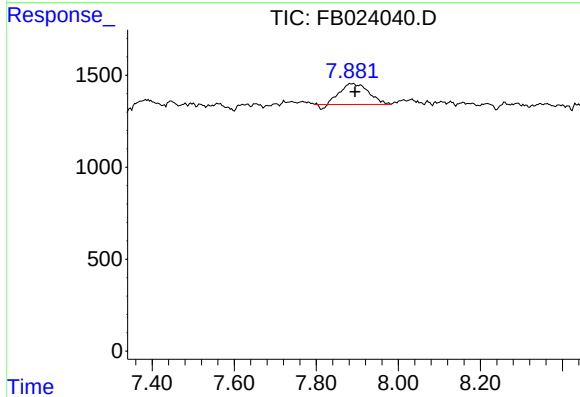


#4 Benzene

R.T.: 7.882 min
Delta R.T.: -0.012 min
Response: 5285
Conc: 0.12 ng/ml

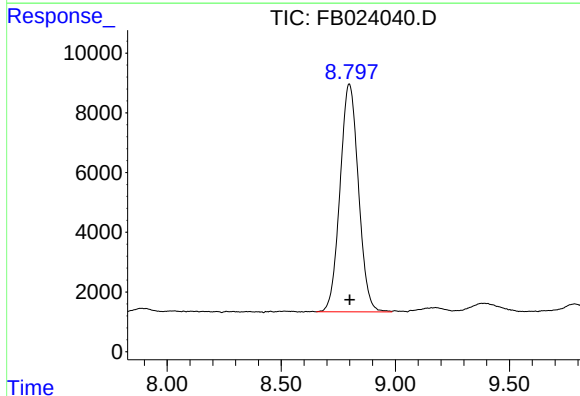


#5 AAA-TFT

R.T.: 8.798 min
Delta R.T.: -0.003 min
Response: 428488
Conc: 18.76 ng/ml

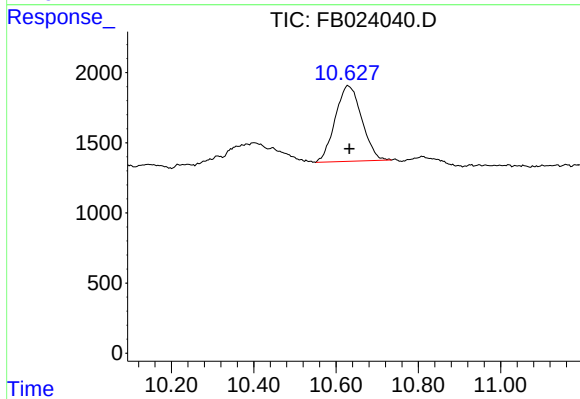

#6 Toluene


R.T.: 10.629 min
Delta R.T.: -0.003 min
Response: 24131
Conc: 0.55 ng/ml

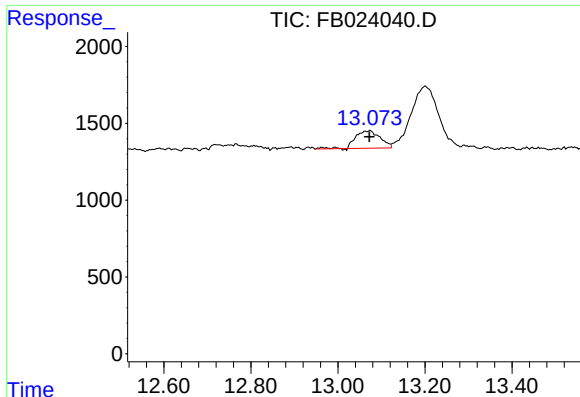

#7 Ethylbenzene


R.T.: 13.075 min
Delta R.T.: 0.002 min
Response: 4477
Conc: 0.11 ng/ml

Instrument :
FID_B
ClientSampleId :

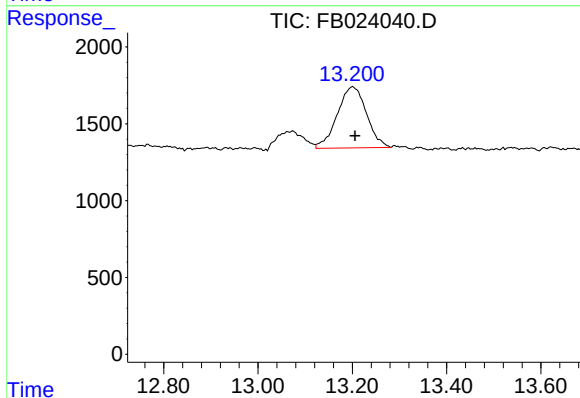


#8 m-Xylene

R.T.: 13.201 min
Delta R.T.: -0.005 min
Response: 17100
Conc: 0.44 ng/ml

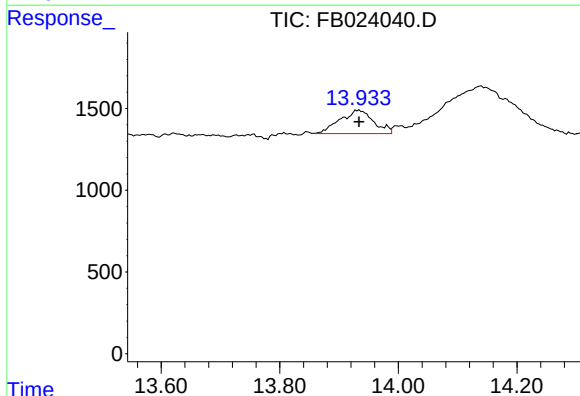

#9 O-Xylene

R.T.: 13.935 min
Delta R.T.: 0.001 min
Response: 5562
Conc: 0.15 ng/ml

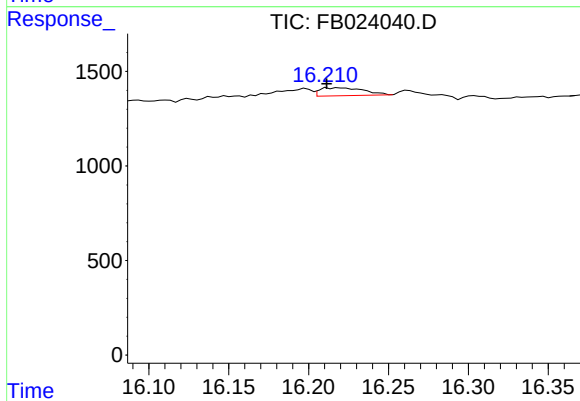

#10 1,2,4-Trimethylbenzene

R.T.: 16.213 min
Delta R.T.: 0.001 min
Response: 799
Conc: 0.03 ng/ml