

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032720\
 Data File : FB024023.D
 Signal(s) : FID2B.CH
 Acq On : 27 Mar 2020 14:15
 Operator : DD/AJ
 Sample : BSF0327S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0327S1

Integration File: Calibration.e
 Quant Time: Mar 27 15:55:20 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032620.M
 Quant Title :
 QLast Update : Fri Mar 27 11:16:49 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	445564	19.508 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.690	1023110	29.561 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	1145246	31.206 ng/ml
3) t n-Heptane	7.759	371335	10.295 ng/ml
4) t Benzene	7.893	445098	10.035 ng/ml
6) t Toluene	10.632	1315544	29.849 ng/ml
7) t Ethylbenzene	13.072	409031	10.265 ng/ml
8) t m-Xylene	13.205	792615	20.606 ng/ml
9) t O-Xylene	13.933	763697	20.662 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	666241	20.966 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032720\
Data File : FB024023.D
Signal(s) : FID2B.CH
Acq On : 27 Mar 2020 14:15
Operator : DD/AJ
Sample : BSF0327S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0327S1

Integration File: Calibration.e
Quant Time: Mar 27 15:55:20 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032620.M
Quant Title :
QLast Update : Fri Mar 27 11:16:49 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

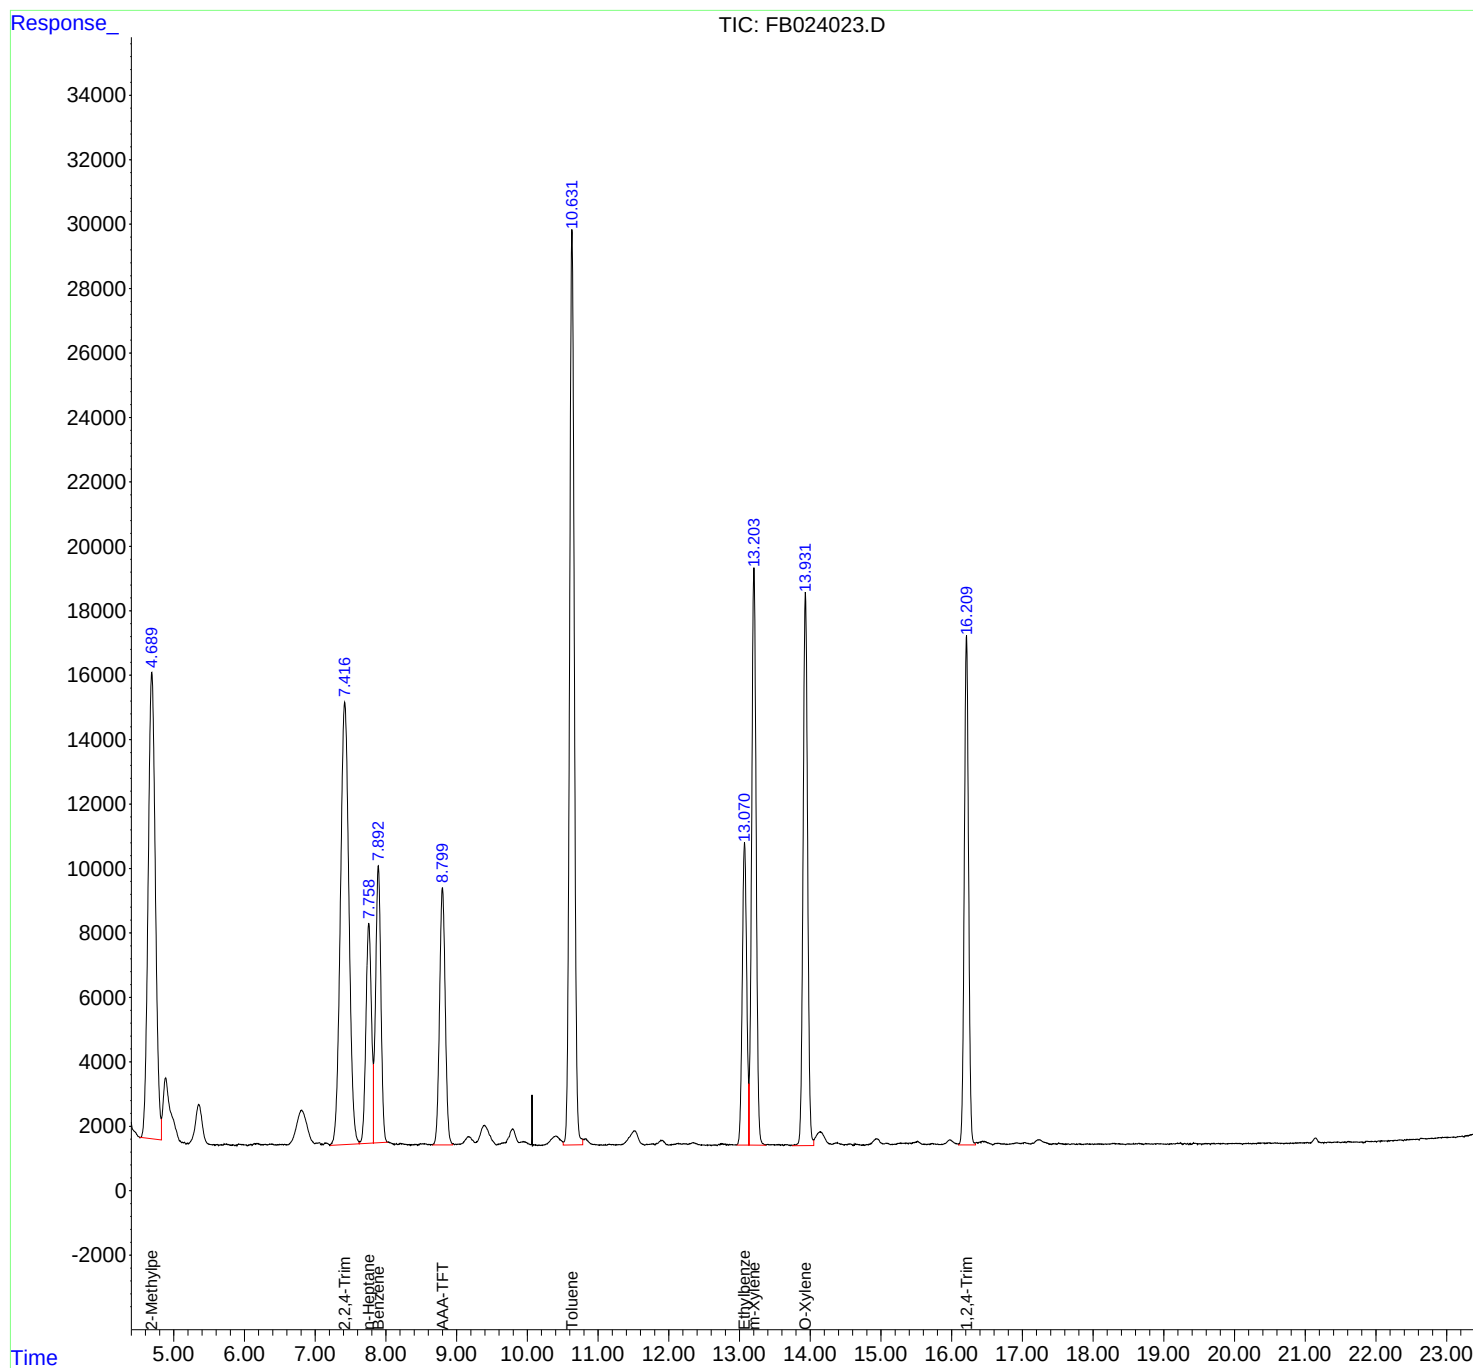


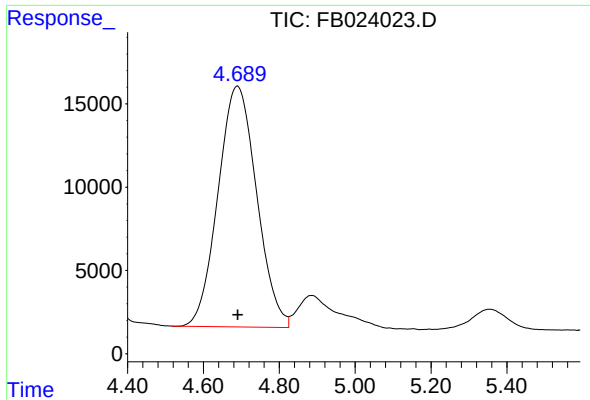

#1 2-Methylpentane


R.T.: 4.690 min
Delta R.T.: 0.000 min
Response: 1023110
Conc: 29.56 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0327S1

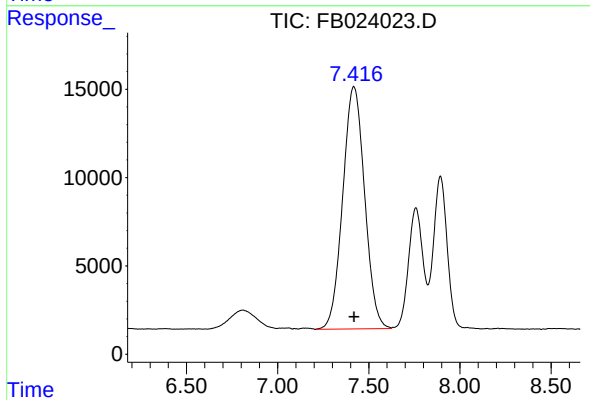


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: -0.002 min
Response: 1145246
Conc: 31.21 ng/ml

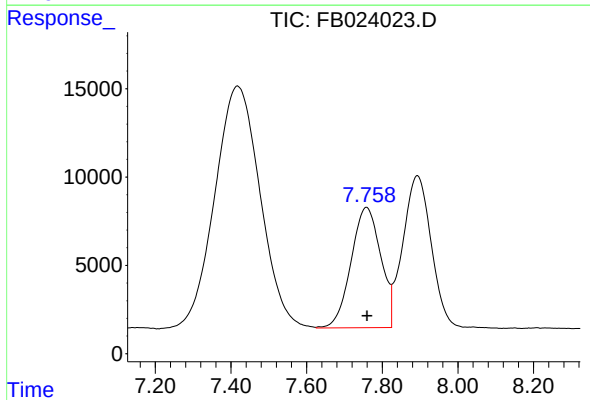


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: -0.001 min
Response: 371335
Conc: 10.30 ng/ml

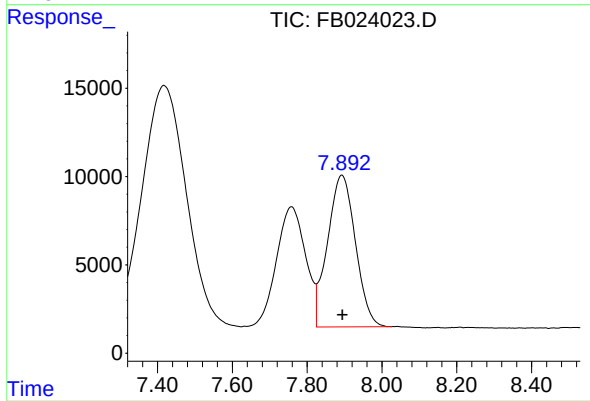

#4 Benzene


R.T.: 7.893 min
Delta R.T.: -0.001 min
Response: 445098
Conc: 10.04 ng/ml

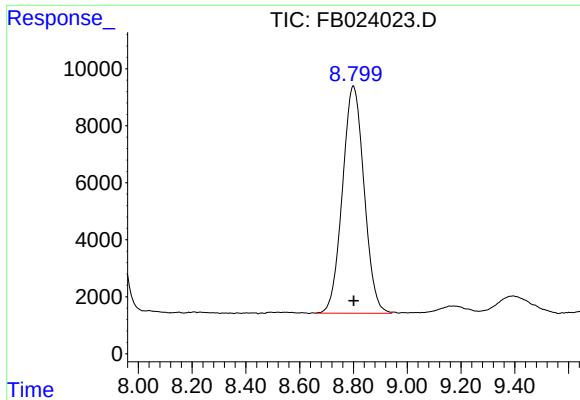

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: -0.001 min
Response: 445564
Conc: 19.51 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0327S1

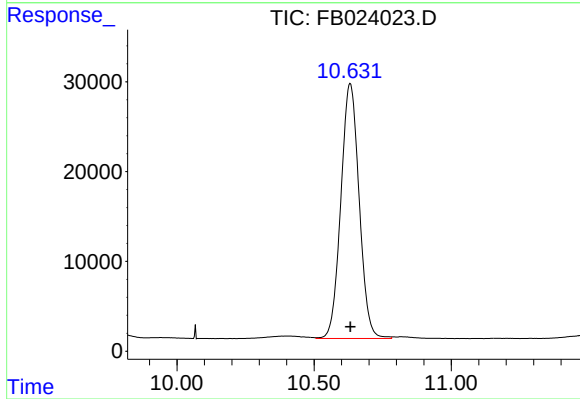


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.000 min
Response: 1315544
Conc: 29.85 ng/ml

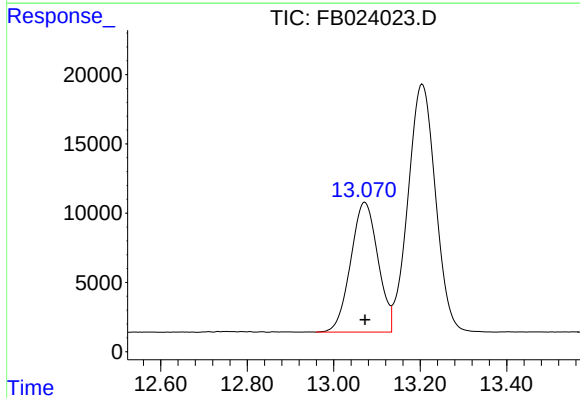


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.000 min
Response: 409031
Conc: 10.26 ng/ml

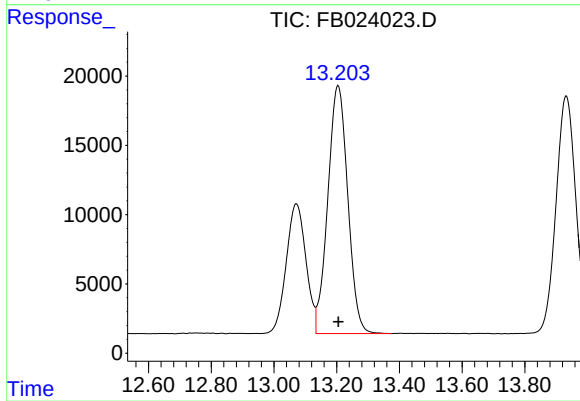

#8 m-Xylene


R.T.: 13.205 min
Delta R.T.: 0.000 min
Response: 792615
Conc: 20.61 ng/ml

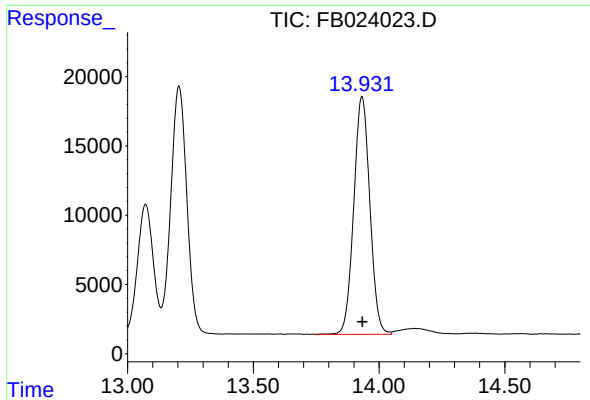

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.000 min
Response: 763697
Conc: 20.66 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0327S1

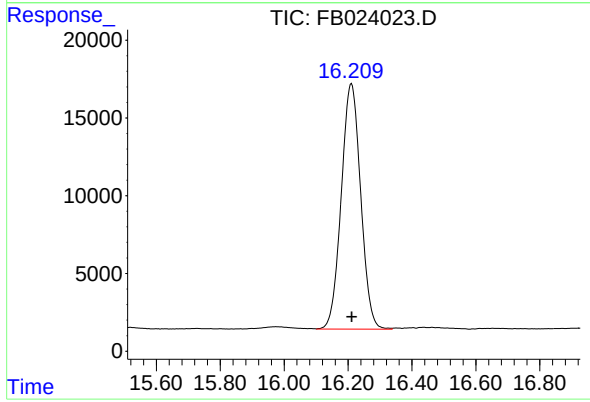

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.000 min
Response: 666241
Conc: 20.97 ng/ml