

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032720\
 Data File : FB024034.D
 Signal(s) : FID2B.CH
 Acq On : 27 Mar 2020 19:53
 Operator : DD/AJ
 Sample : L1753-10MSD
 Misc : 5.03g/5.00ml DI WATER
 ALS Vial : 14 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 CL-02-032520MSD

Integration File: Calibration.e
 Quant Time: Mar 28 01:13:17 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032620.M
 Quant Title :
 QLast Update : Fri Mar 27 11:16:49 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	431698	18.901 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.692	919287	26.561 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	1016189	27.689 ng/ml
3) t n-Heptane	7.759	330388	9.160 ng/ml
4) t Benzene	7.894	399391	9.005 ng/ml
6) t Toluene	10.632	1162142	26.368 ng/ml
7) t Ethylbenzene	13.072	356198	8.939 ng/ml
8) t m-Xylene	13.205	689396	17.923 ng/ml
9) t O-Xylene	13.933	661792	17.905 ng/ml
10) t 1,2,4-Trimethylbenzene	16.211	574432	18.076 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032720\
Data File : FB024034.D
Signal(s) : FID2B.CH
Acq On : 27 Mar 2020 19:53
Operator : DD/AJ
Sample : L1753-10MSD
Misc : 5.03g/5.00ml DI WATER
ALS Vial : 14 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
CL-02-032520MSD

Integration File: Calibration.e
Quant Time: Mar 28 01:13:17 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032620.M
Quant Title :
QLast Update : Fri Mar 27 11:16:49 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

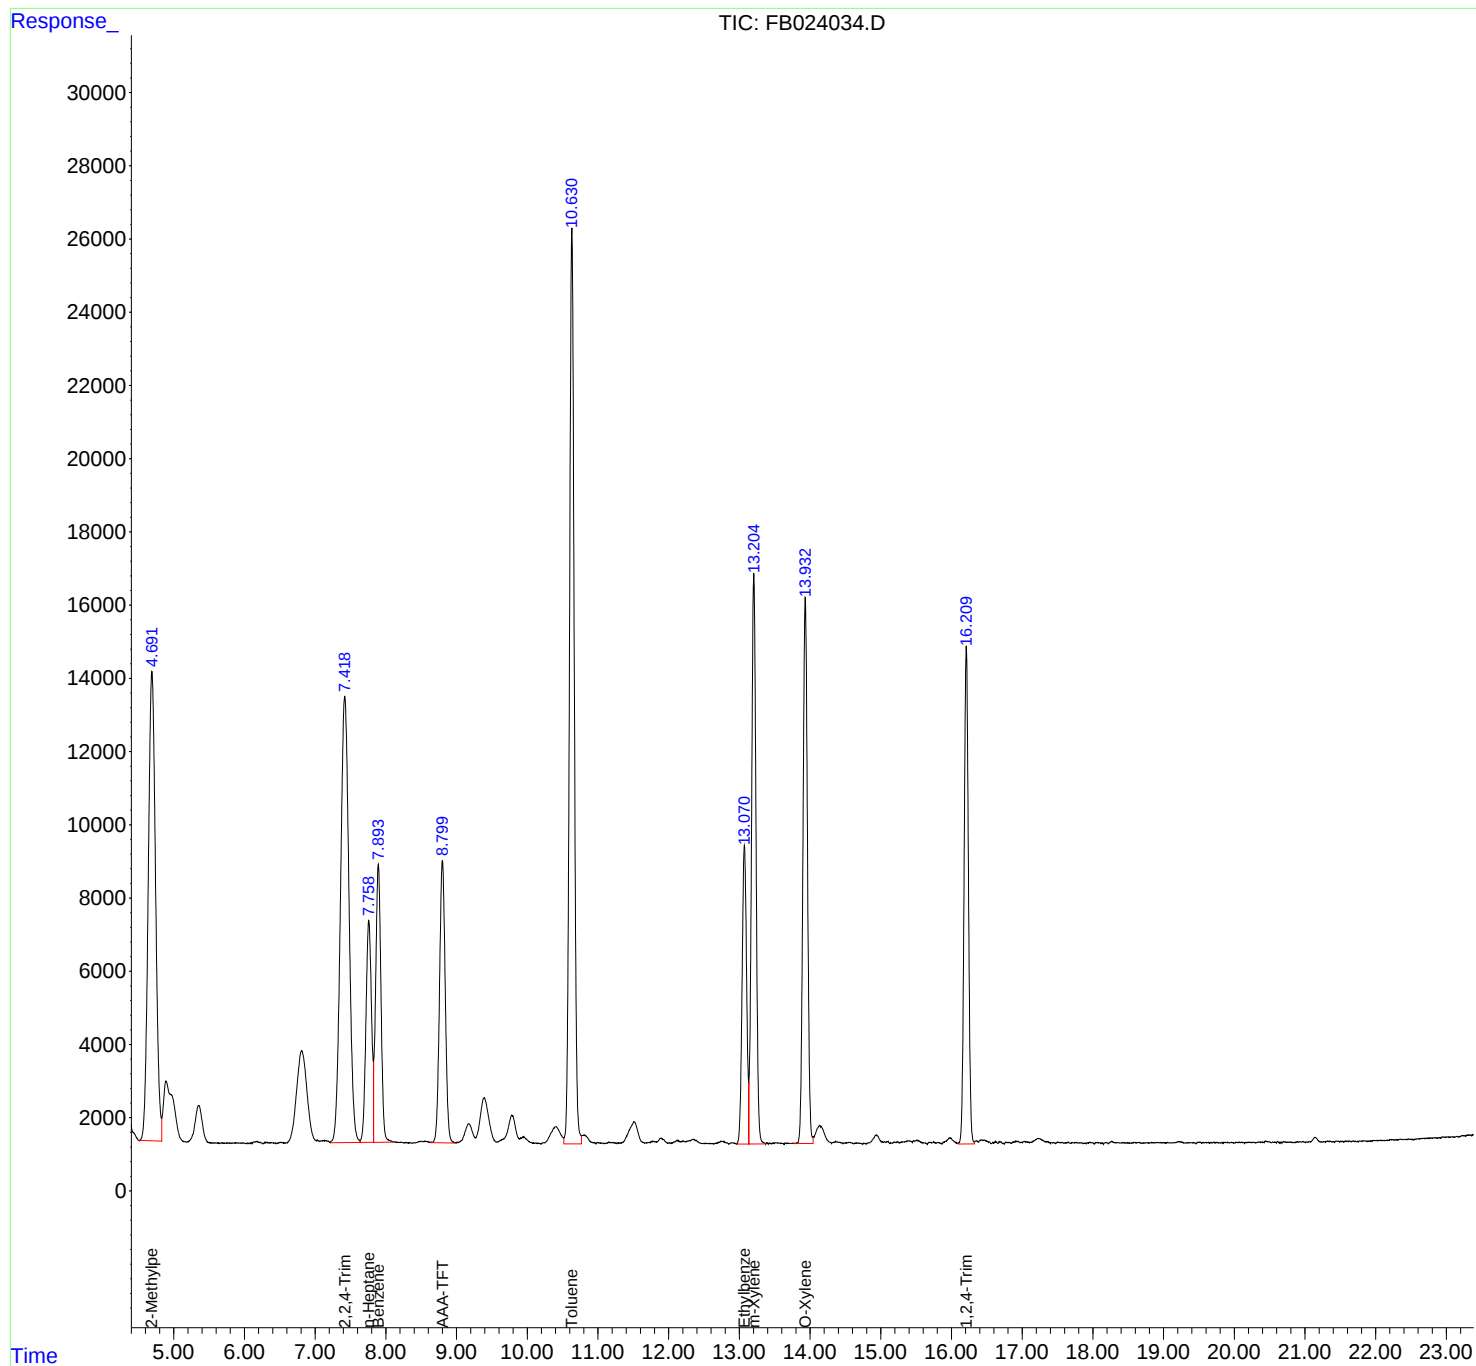


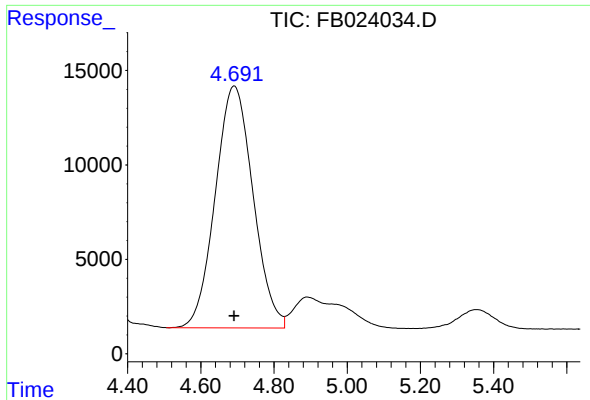

#1 2-Methylpentane


R.T.: 4.692 min
Delta R.T.: 0.001 min
Response: 919287
Conc: 26.56 ng/ml

Instrument :
FID_B
ClientSampleId :
CL-02-032520MSD

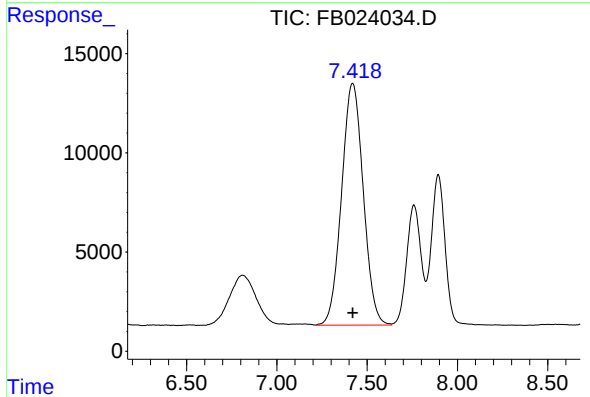


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: 0.000 min
Response: 1016189
Conc: 27.69 ng/ml

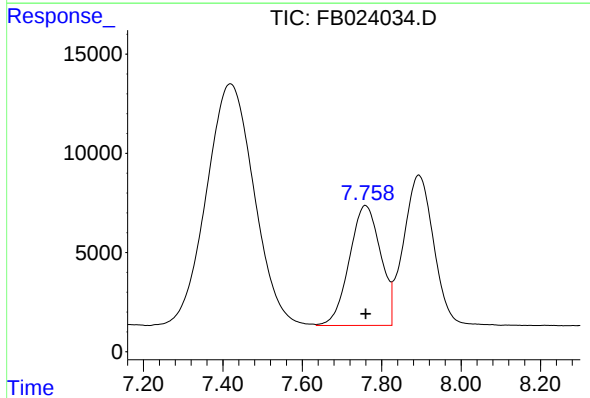


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.000 min
Response: 330388
Conc: 9.16 ng/ml

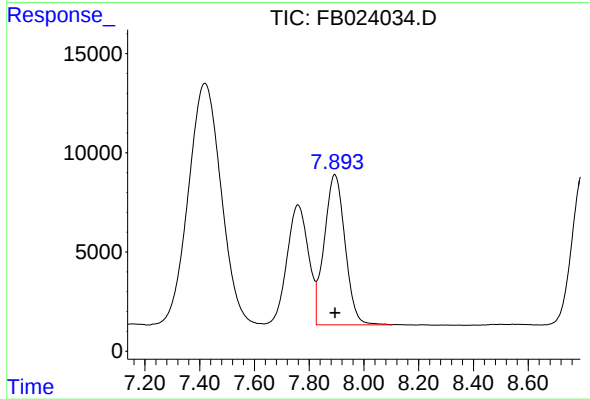

#4 Benzene


R.T.: 7.894 min
Delta R.T.: 0.000 min
Response: 399391
Conc: 9.00 ng/ml

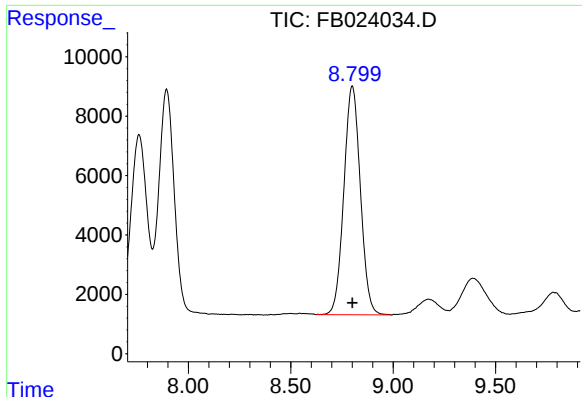

#5 AAA-TFT


R.T.: 8.801 min
Delta R.T.: 0.000 min
Response: 431698
Conc: 18.90 ng/ml

Instrument :
FID_B
ClientSampleId :
CL-02-032520MSD

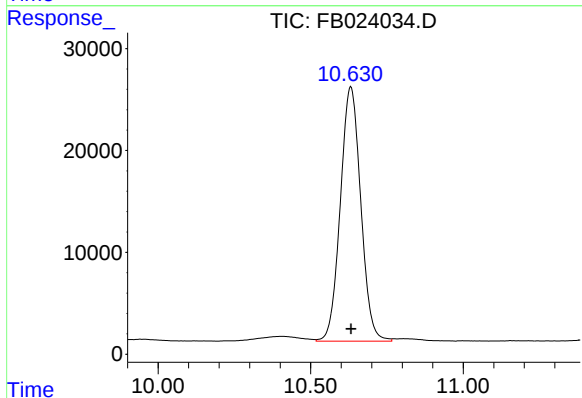


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.000 min
Response: 1162142
Conc: 26.37 ng/ml

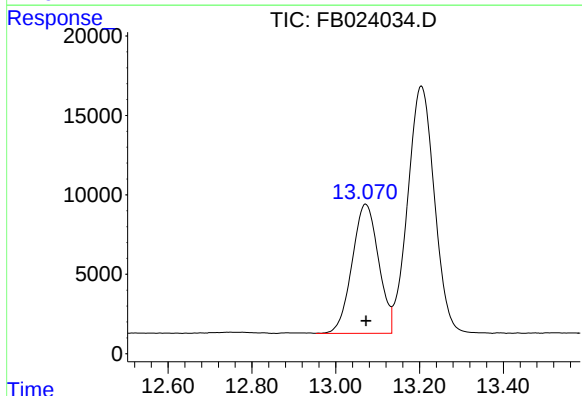


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.000 min
Response: 356198
Conc: 8.94 ng/ml

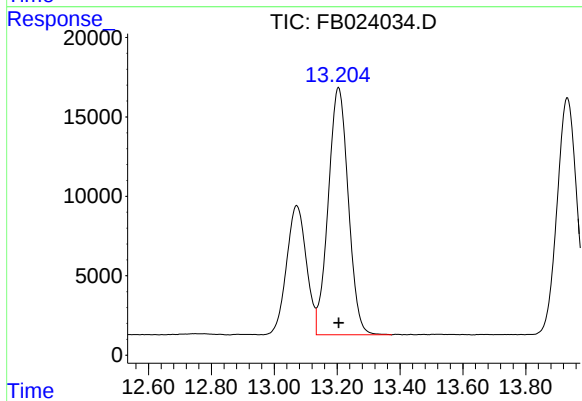

#8 m-Xylene


R.T.: 13.205 min
Delta R.T.: 0.000 min
Response: 689396
Conc: 17.92 ng/ml

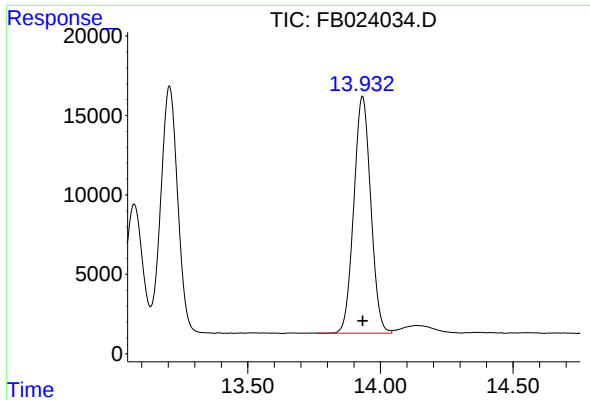

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.000 min
Response: 661792
Conc: 17.90 ng/ml

Instrument :
FID_B
ClientSampleId :
CL-02-032520MSD

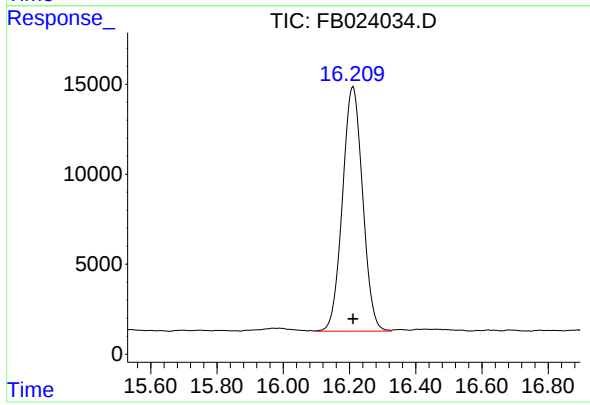

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.000 min
Response: 574432
Conc: 18.08 ng/ml