

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032720\
 Data File : FB024036.D
 Signal(s) : FID2B.CH
 Acq On : 27 Mar 2020 20:55
 Operator : DD/AJ
 Sample : BSF0327W1
 Misc :
 ALS Vial : 16 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0327W1

Integration File: Calibration.e
 Quant Time: Mar 28 01:13:34 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032620.M
 Quant Title :
 QLast Update : Fri Mar 27 11:16:49 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.800	417592	18.283 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.690	989551	28.592 ng/ml
2) t 2,2,4-Trimethylpentane	7.418	1084187	29.542 ng/ml
3) t n-Heptane	7.759	354231	9.821 ng/ml
4) t Benzene	7.893	432372	9.748 ng/ml
6) t Toluene	10.631	1242061	28.182 ng/ml
7) t Ethylbenzene	13.072	367145	9.214 ng/ml
8) t m-Xylene	13.205	715437	18.600 ng/ml
9) t O-Xylene	13.932	689246	18.648 ng/ml
10) t 1,2,4-Trimethylbenzene	16.210	598889	18.846 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032720\
Data File : FB024036.D
Signal(s) : FID2B.CH
Acq On : 27 Mar 2020 20:55
Operator : DD/AJ
Sample : BSF0327W1
Misc :
ALS Vial : 16 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0327W1

Integration File: Calibration.e
Quant Time: Mar 28 01:13:34 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032620.M
Quant Title :
QLast Update : Fri Mar 27 11:16:49 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

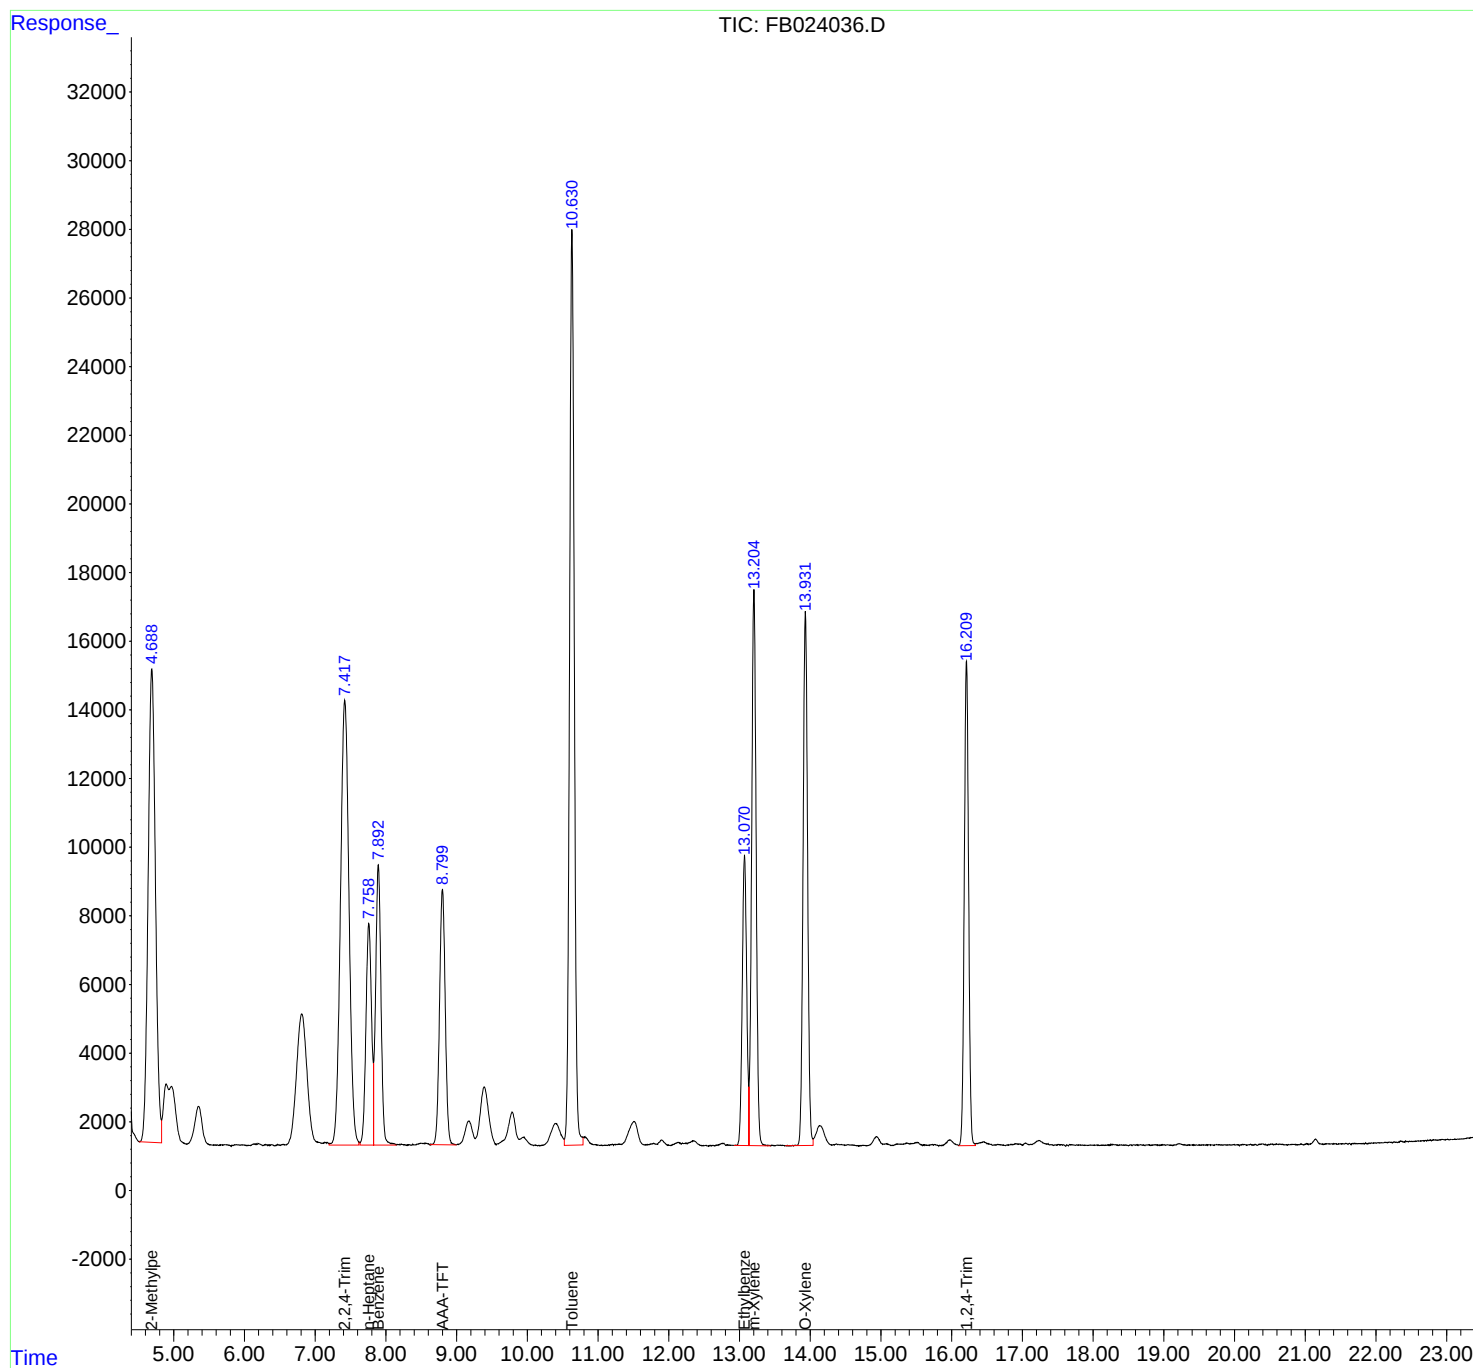


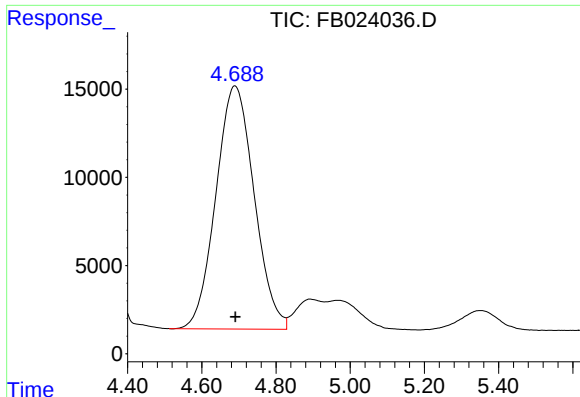

#1 2-Methylpentane


R.T.: 4.690 min
Delta R.T.: -0.001 min
Response: 989551
Conc: 28.59 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0327W1

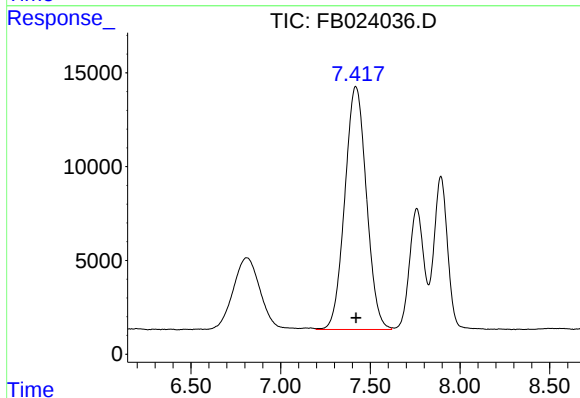


#2 2,2,4-Trimethylpentane

R.T.: 7.418 min
Delta R.T.: -0.002 min
Response: 1084187
Conc: 29.54 ng/ml

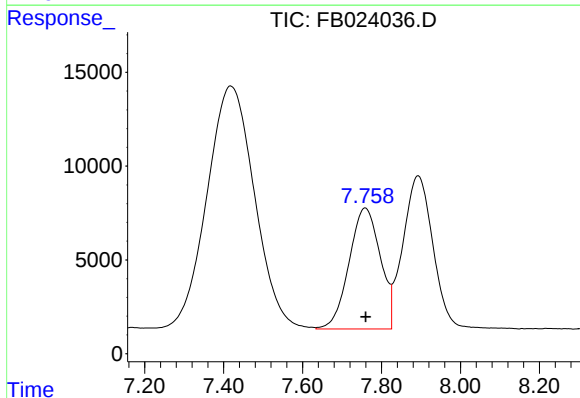


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: -0.001 min
Response: 354231
Conc: 9.82 ng/ml

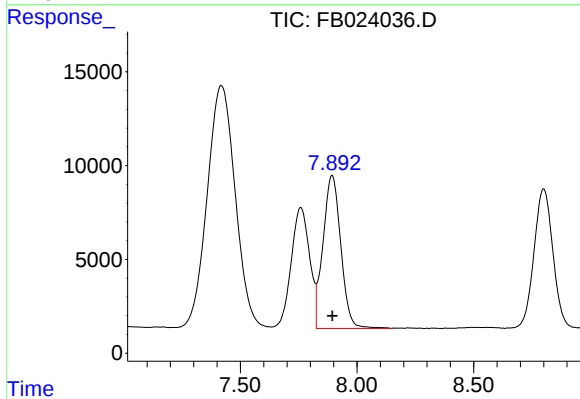

#4 Benzene


R.T.: 7.893 min
Delta R.T.: -0.001 min
Response: 432372
Conc: 9.75 ng/ml

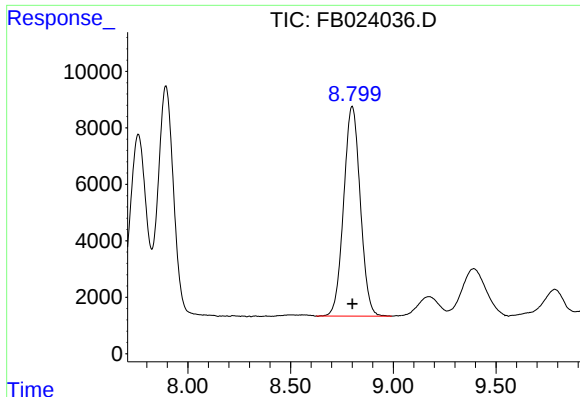

#5 AAA-TFT


R.T.: 8.800 min
Delta R.T.: -0.001 min
Response: 417592
Conc: 18.28 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0327W1

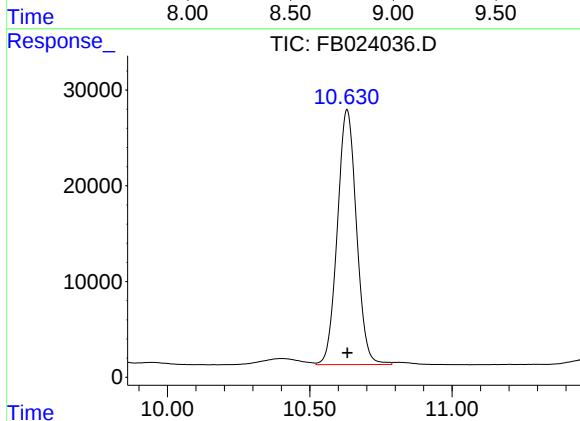


#6 Toluene

R.T.: 10.631 min
Delta R.T.: -0.001 min
Response: 1242061
Conc: 28.18 ng/ml

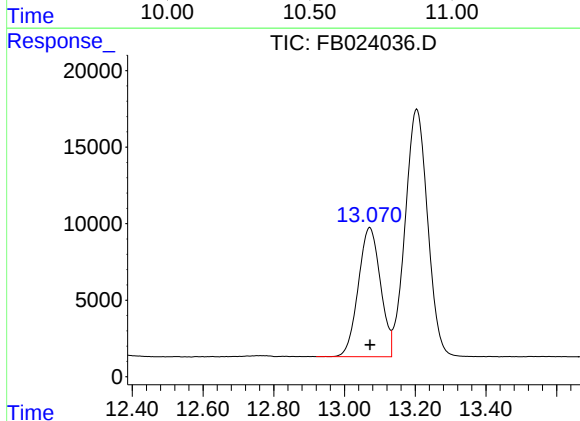


#7 Ethylbenzene

R.T.: 13.072 min
Delta R.T.: 0.000 min
Response: 367145
Conc: 9.21 ng/ml

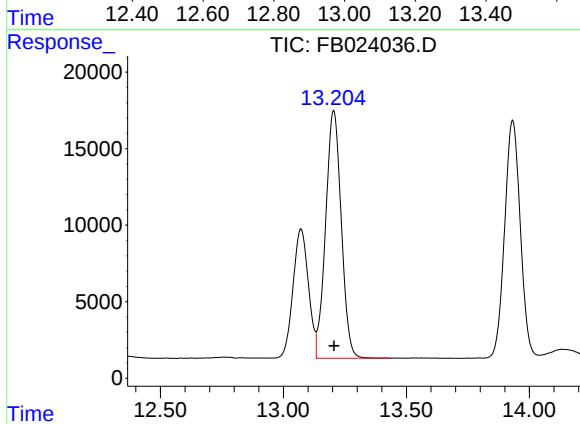

#8 m-Xylene


R.T.: 13.205 min
Delta R.T.: 0.000 min
Response: 715437
Conc: 18.60 ng/ml

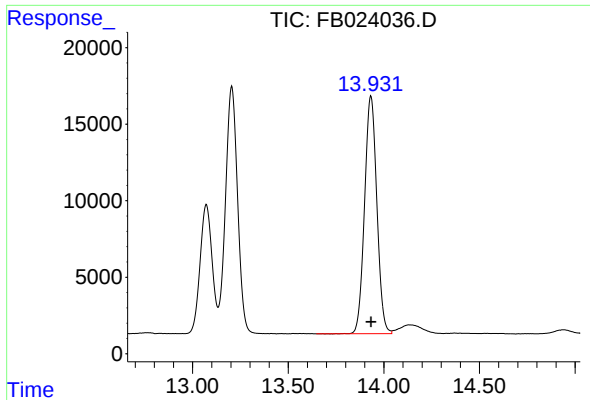

#9 O-Xylene

R.T.: 13.932 min
Delta R.T.: -0.001 min
Response: 689246
Conc: 18.65 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0327W1

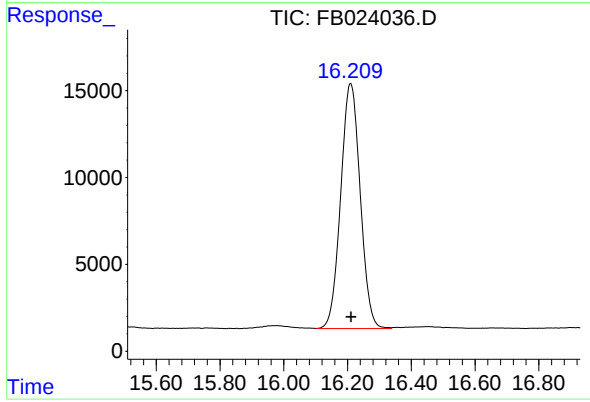

#10 1,2,4-Trimethylbenzene

R.T.: 16.210 min
Delta R.T.: -0.001 min
Response: 598889
Conc: 18.85 ng/ml