

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032720\
 Data File : FB024046.D
 Signal(s) : FID2B.CH
 Acq On : 28 Mar 2020 2:30
 Operator : DD/AJ
 Sample : 20 PPB GRO STD
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 27 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 28 06:51:04 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032620.M
 Quant Title :
 QLast Update : Fri Mar 27 11:16:49 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.797	416758	18.247 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	968575	27.986 ng/ml
2) t 2,2,4-Trimethylpentane	7.416	1042713	28.412 ng/ml
3) t n-Heptane	7.756	339793	9.421 ng/ml
4) t Benzene	7.890	435407	9.817 ng/ml
6) t Toluene	10.628	1250298	28.369 ng/ml
7) t Ethylbenzene	13.068	390790	9.807 ng/ml
8) t m-Xylene	13.201	763401	19.847 ng/ml
9) t O-Xylene	13.929	734226	19.865 ng/ml
10) t 1,2,4-Trimethylbenzene	16.207	602905	18.972 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032720\
Data File : FB024046.D
Signal(s) : FID2B.CH
Acq On : 28 Mar 2020 2:30
Operator : DD/AJ
Sample : 20 PPB GRO STD
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 27 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 28 06:51:04 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032620.M
Quant Title :
QLast Update : Fri Mar 27 11:16:49 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

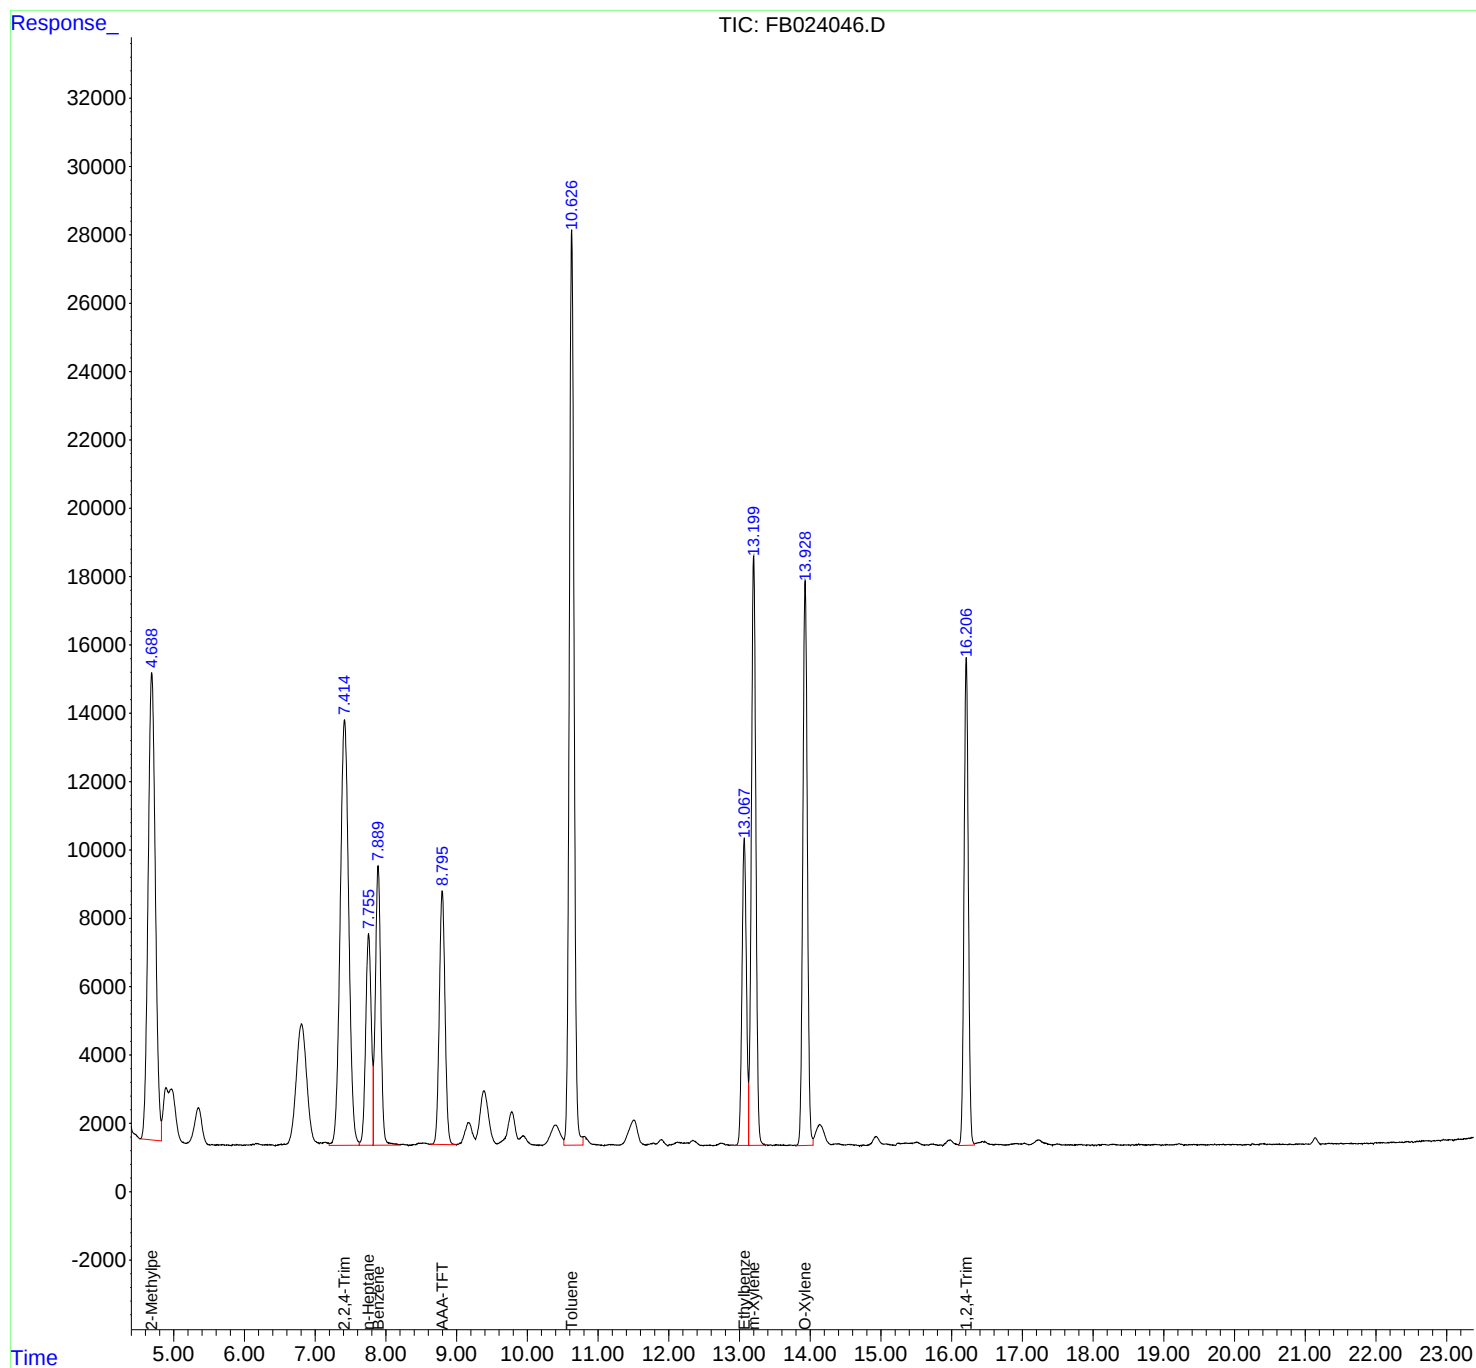


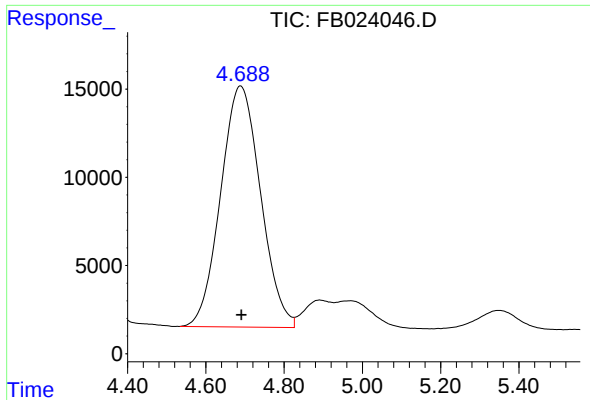

#1 2-Methylpentane


R.T.: 4.689 min
Delta R.T.: -0.002 min
Response: 968575
Conc: 27.99 ng/ml

Instrument :
FID_B
ClientSampleId :

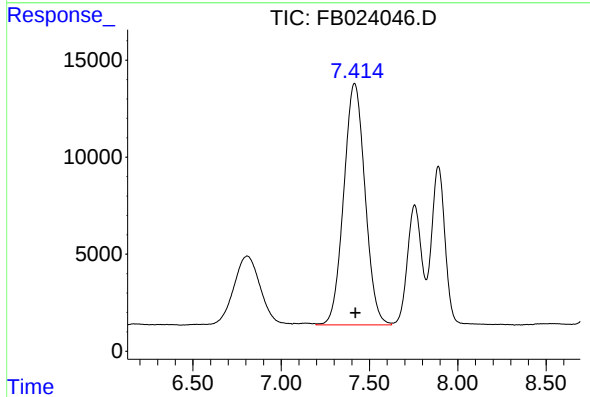


#2 2,2,4-Trimethylpentane

R.T.: 7.416 min
Delta R.T.: -0.004 min
Response: 1042713
Conc: 28.41 ng/ml

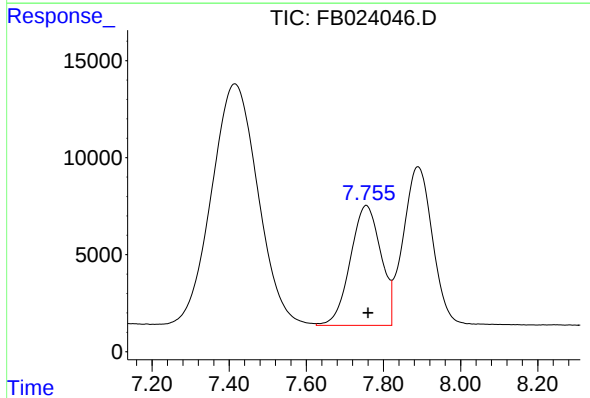


#3 n-Heptane

R.T.: 7.756 min
Delta R.T.: -0.004 min
Response: 339793
Conc: 9.42 ng/ml

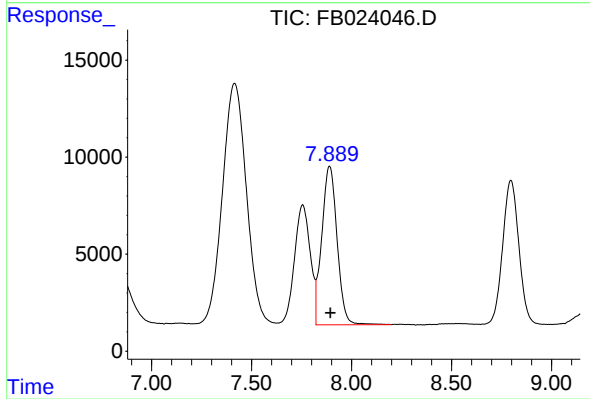

#4 Benzene


R.T.: 7.890 min
Delta R.T.: -0.004 min
Response: 435407
Conc: 9.82 ng/ml

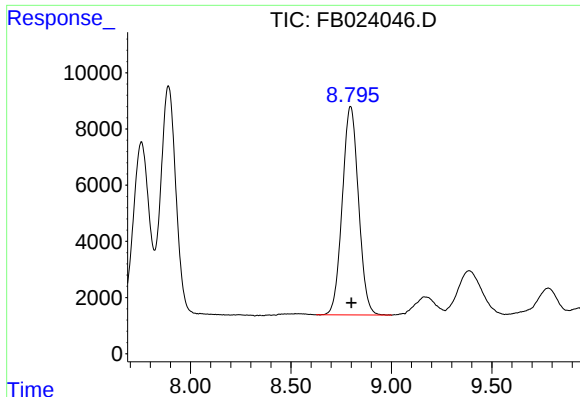

#5 AAA-TFT


R.T.: 8.797 min
Delta R.T.: -0.004 min
Response: 416758
Conc: 18.25 ng/ml

Instrument :
FID_B
ClientSampleId :

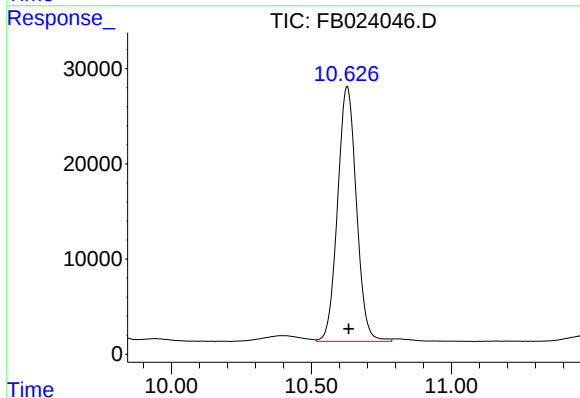


#6 Toluene

R.T.: 10.628 min
Delta R.T.: -0.005 min
Response: 1250298
Conc: 28.37 ng/ml

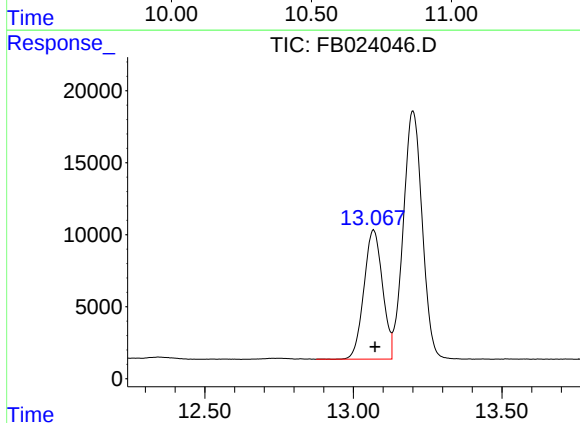


#7 Ethylbenzene

R.T.: 13.068 min
Delta R.T.: -0.005 min
Response: 390790
Conc: 9.81 ng/ml

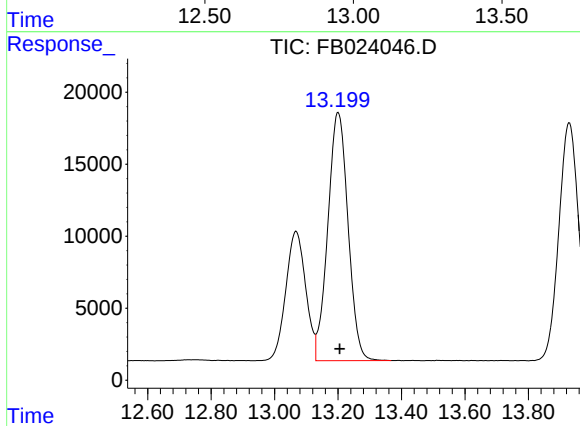

#8 m-Xylene


R.T.: 13.201 min
Delta R.T.: -0.005 min
Response: 763401
Conc: 19.85 ng/ml

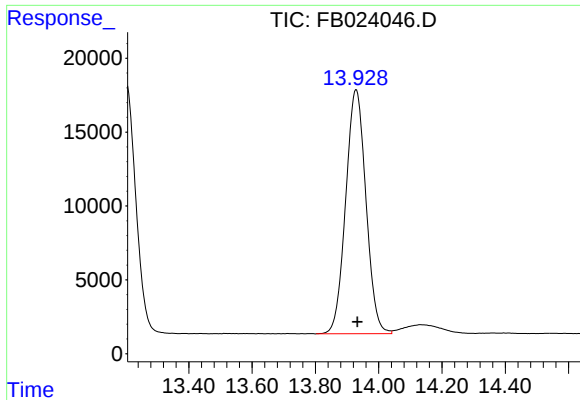

#9 O-Xylene

R.T.: 13.929 min
Delta R.T.: -0.004 min
Response: 734226
Conc: 19.86 ng/ml

Instrument :
FID_B
ClientSampleId :

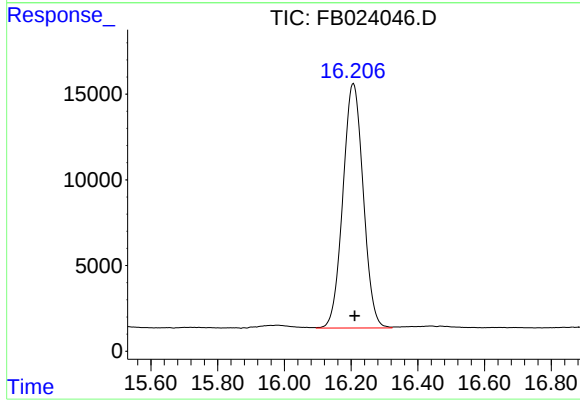

#10 1,2,4-Trimethylbenzene

R.T.: 16.207 min
Delta R.T.: -0.004 min
Response: 602905
Conc: 18.97 ng/ml