

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032723\
 Data File : FB029571.D
 Signal(s) : FID2B.CH
 Acq On : 27 Mar 2023 17:28
 Operator : YP/AJ
 Sample : 02100-01
 Misc :
 ALS Vial : 6 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Mar 28 02:15:20 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
 Quant Title :
 QLast Update : Thu Mar 23 11:44:29 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.788	265404	18.620 ng/ml
Target Compounds			
4) t Benzene	7.889	799	0.035 ng/ml
6) t Toluene	10.613	30755	1.395 ng/ml
7) t Ethylbenzene	13.055	3910	0.189 ng/ml
8) t m-Xylene	13.185	18553	0.907 ng/ml
9) t O-Xylene	13.912	10254	0.518 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	6467	0.339 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032723\
Data File : FB029571.D
Signal(s) : FID2B.CH
Acq On : 27 Mar 2023 17:28
Operator : YP/AJ
Sample : 02100-01
Misc :
ALS Vial : 6 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Mar 28 02:15:20 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
Quant Title :
QLast Update : Thu Mar 23 11:44:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

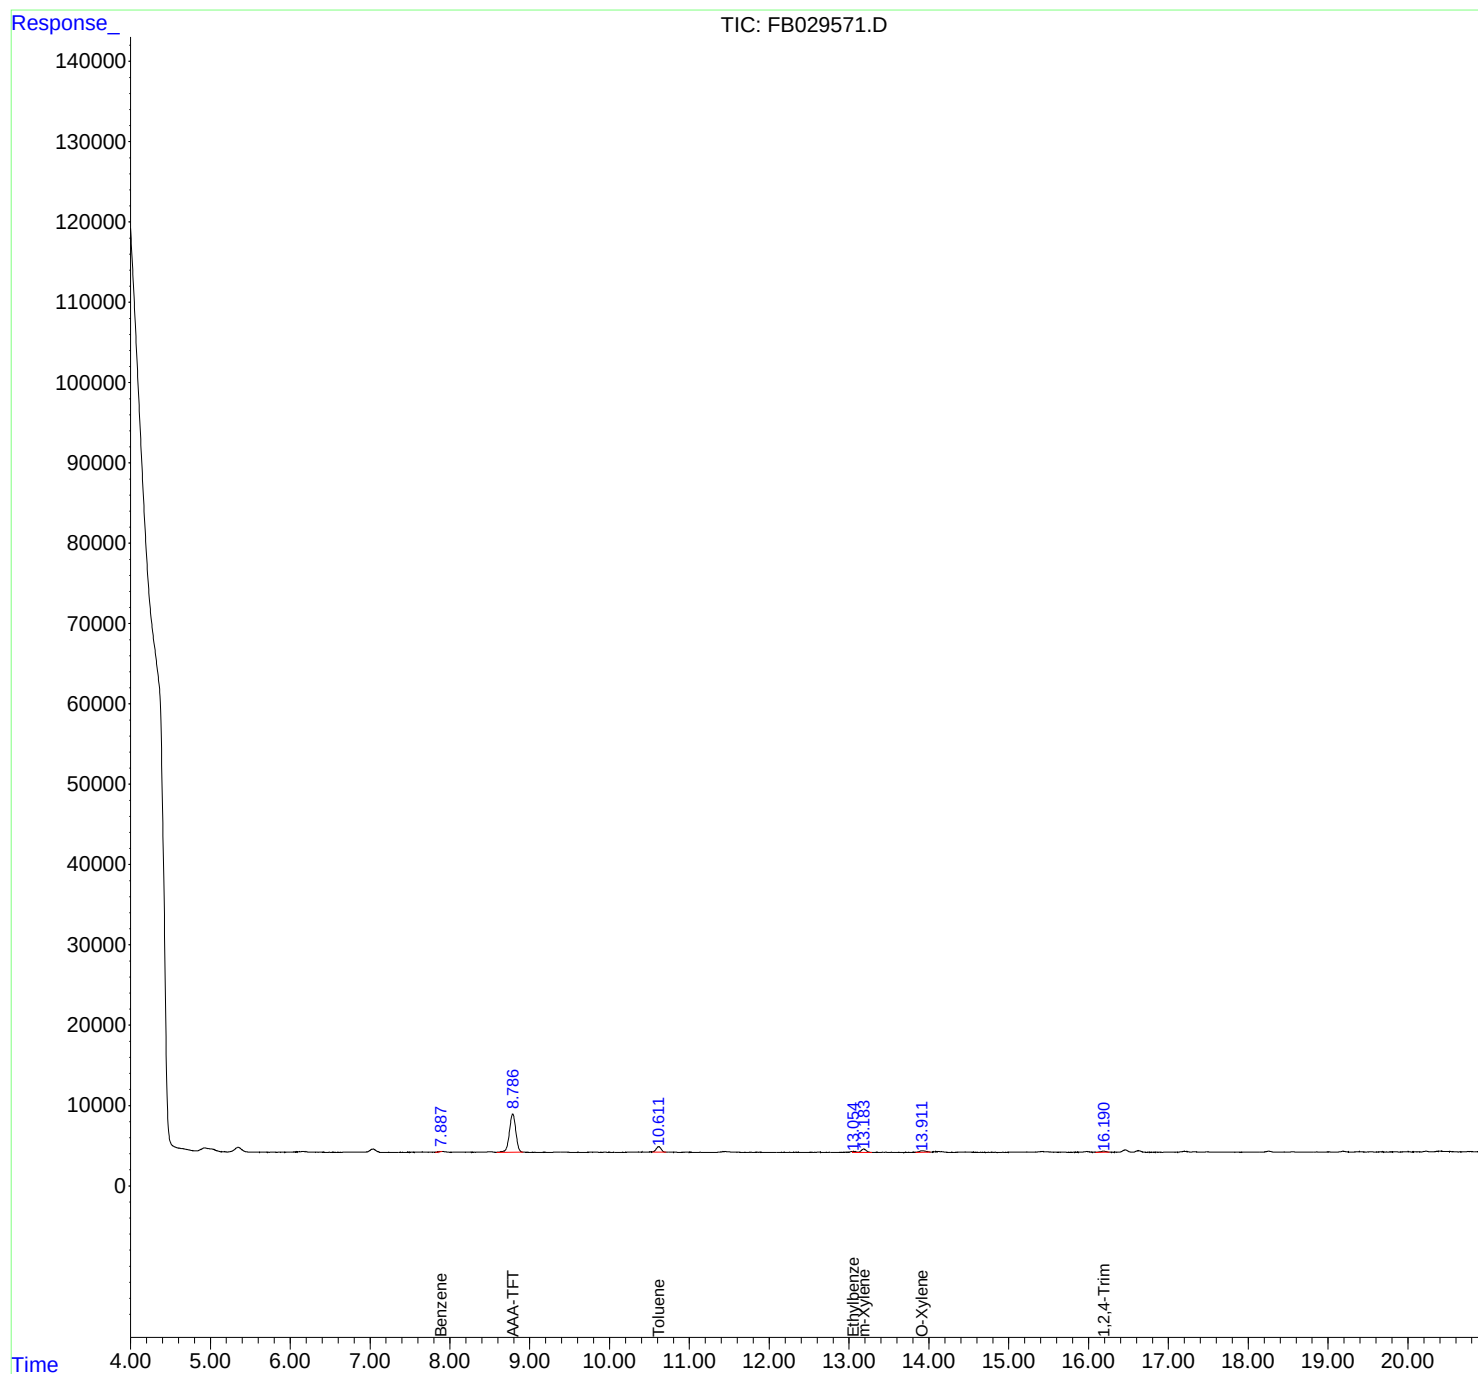


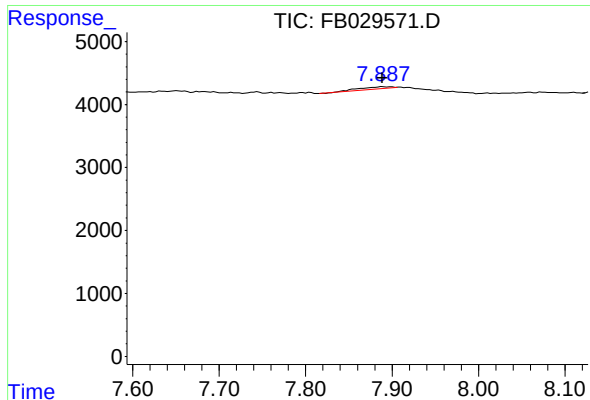

#4 Benzene


R.T.: 7.889 min
 Delta R.T.: 0.000 min
 Response: 799
 Conc: 0.04 ng/ml

Instrument : FID_B
 ClientSampleId :

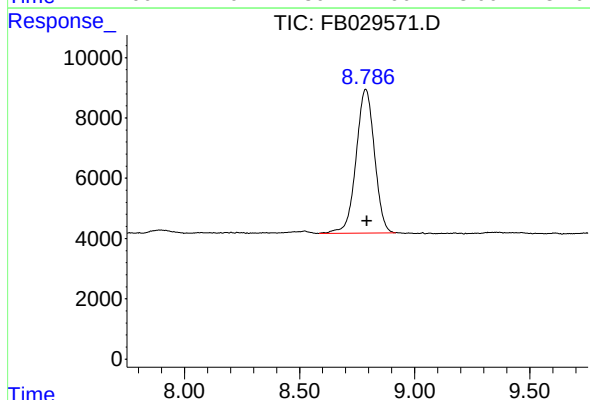


#5 AAA-TFT

R.T.: 8.788 min
 Delta R.T.: -0.006 min
 Response: 265404
 Conc: 18.62 ng/ml

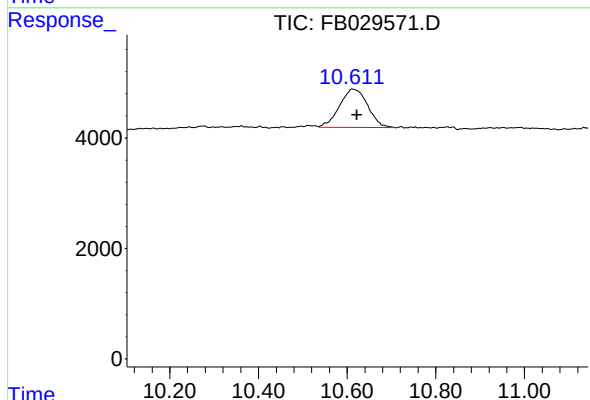


#6 Toluene

R.T.: 10.613 min
 Delta R.T.: -0.009 min
 Response: 30755
 Conc: 1.40 ng/ml

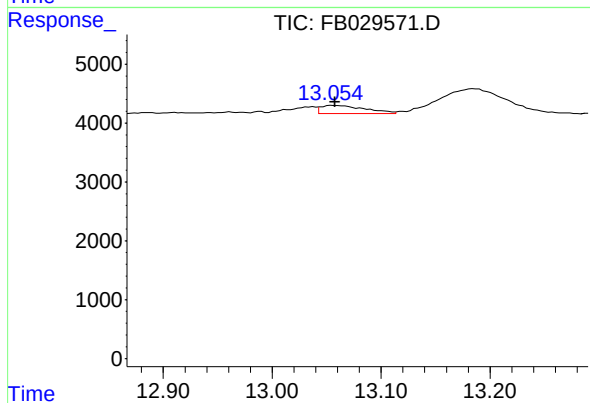

#7 Ethylbenzene


R.T.: 13.055 min
 Delta R.T.: -0.003 min
 Response: 3910
 Conc: 0.19 ng/ml

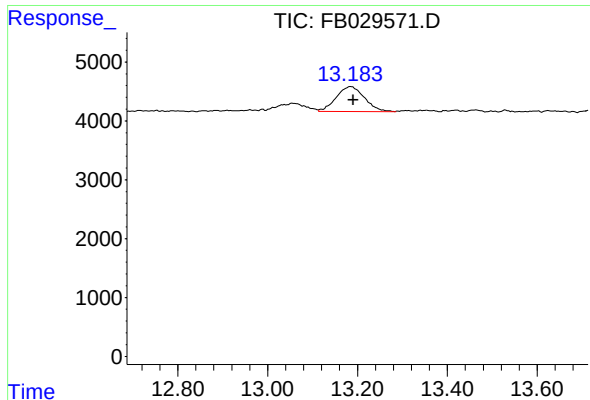

#8 m-Xylene


R.T.: 13.185 min
Delta R.T.: -0.005 min
Response: 18553
Conc: 0.91 ng/ml

Instrument :
FID_B
ClientSampleId :

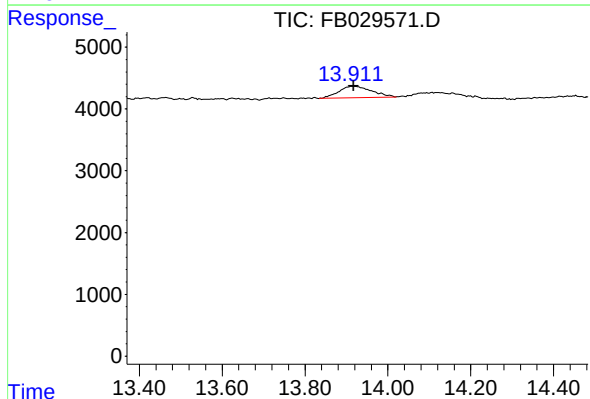

#9 O-Xylene

R.T.: 13.912 min
Delta R.T.: -0.005 min
Response: 10254
Conc: 0.52 ng/ml

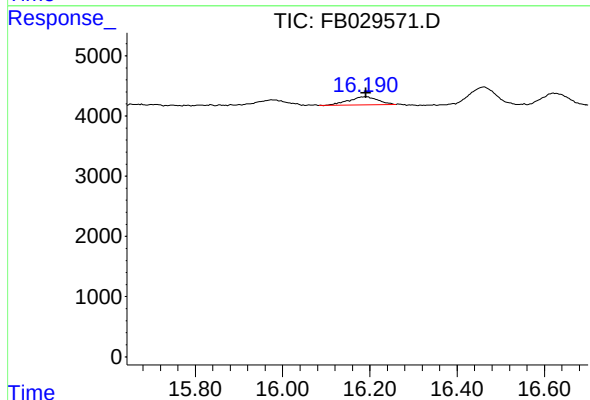

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: 0.000 min
Response: 6467
Conc: 0.34 ng/ml