

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032723\
 Data File : FB029569.D
 Signal(s) : FID2B.CH
 Acq On : 27 Mar 2023 16:12
 Operator : YP/AJ
 Sample : BSF0327W1
 Misc :
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0327W1

Integration File: Calibration.e
 Quant Time: Mar 28 02:15:10 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
 Quant Title :
 QLast Update : Thu Mar 23 11:44:29 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.793	334411	23.462 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.712	521169	31.043 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	585057	31.780 ng/ml
3) t n-Heptane	7.751	205605	10.555 ng/ml
4) t Benzene	7.888	242243	10.722 ng/ml
6) t Toluene	10.621	703662	31.920 ng/ml
7) t Ethylbenzene	13.058	215629	10.431 ng/ml
8) t m-Xylene	13.191	430800	21.054 ng/ml
9) t O-Xylene	13.918	419425	21.171 ng/ml
10) t 1,2,4-Trimethylbenzene	16.193	397345	20.813 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032723\
Data File : FB029569.D
Signal(s) : FID2B.CH
Acq On : 27 Mar 2023 16:12
Operator : YP/AJ
Sample : BSF0327W1
Misc :
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0327W1

Integration File: Calibration.e
Quant Time: Mar 28 02:15:10 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
Quant Title :
QLast Update : Thu Mar 23 11:44:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

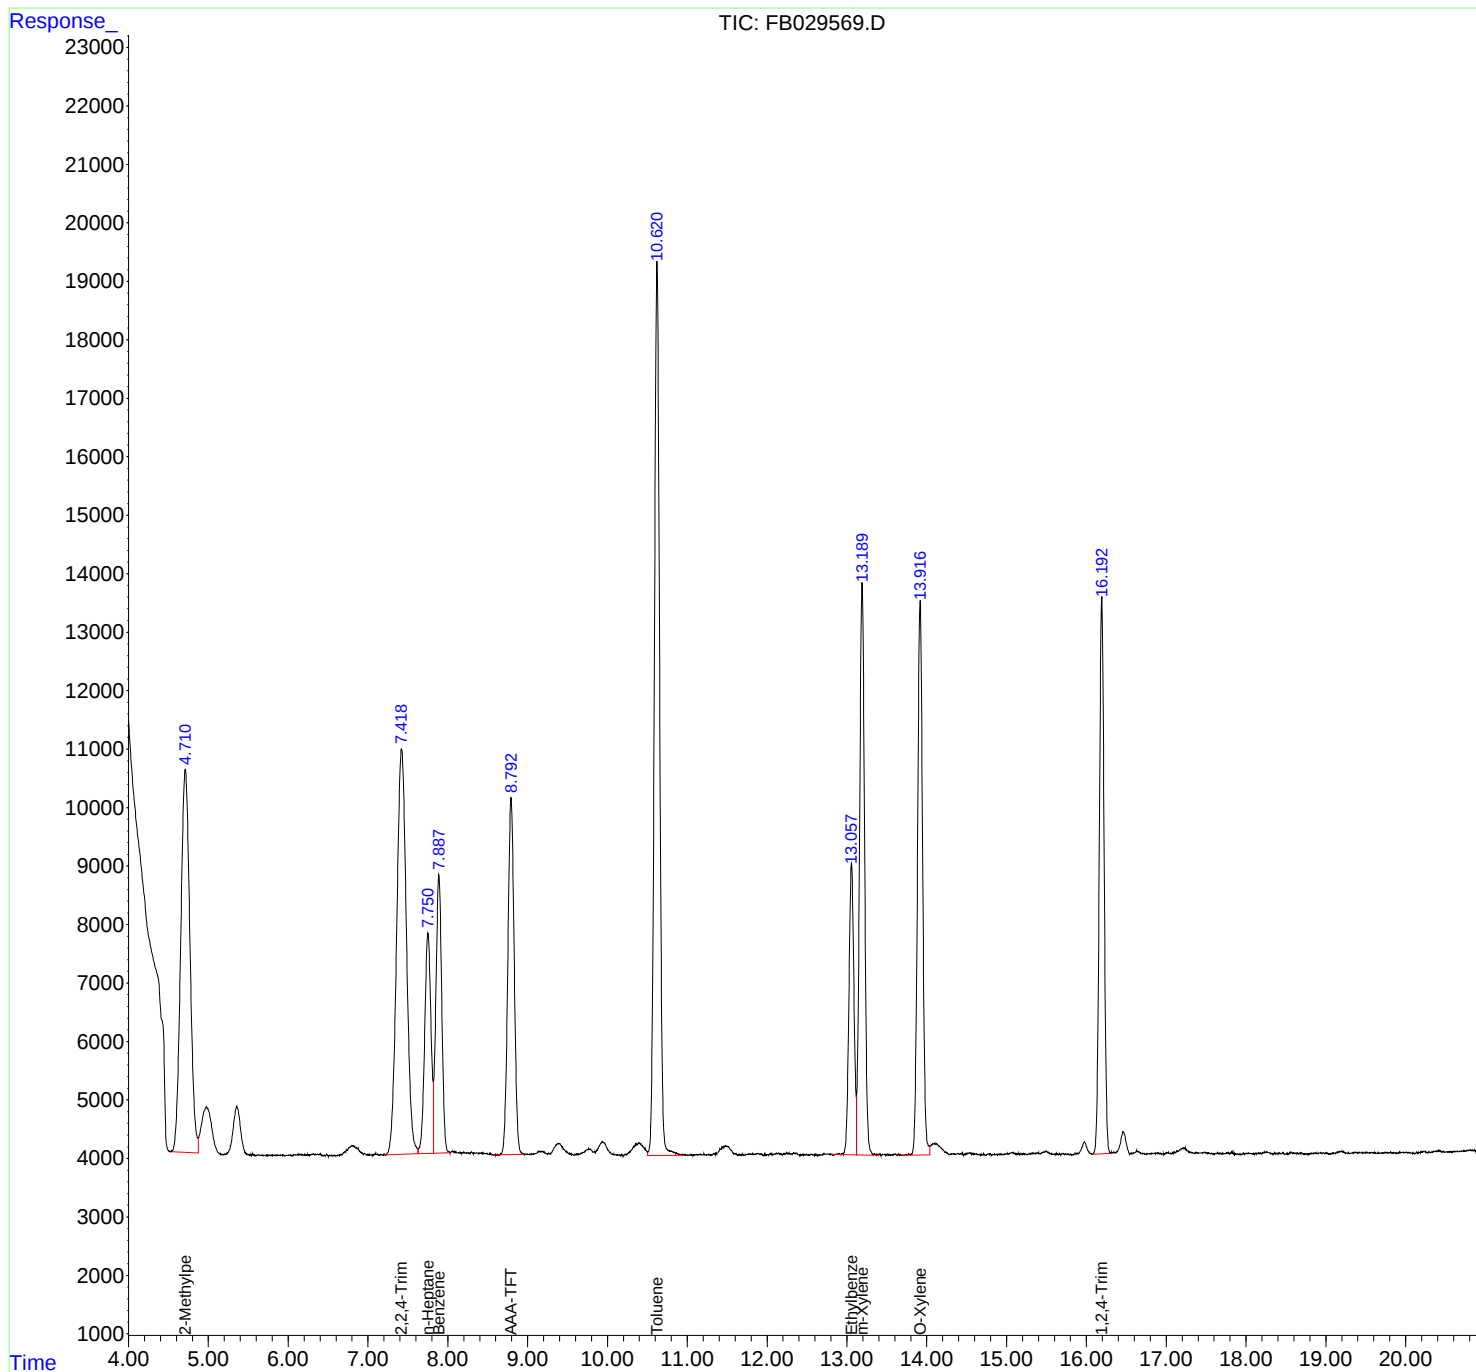


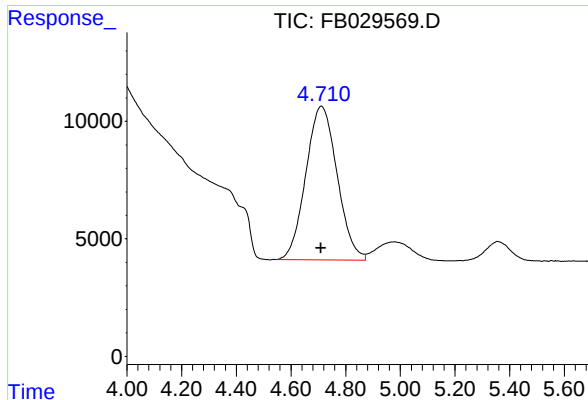

#1 2-Methylpentane


R.T.: 4.712 min
Delta R.T.: 0.002 min
Response: 521169
Conc: 31.04 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0327W1

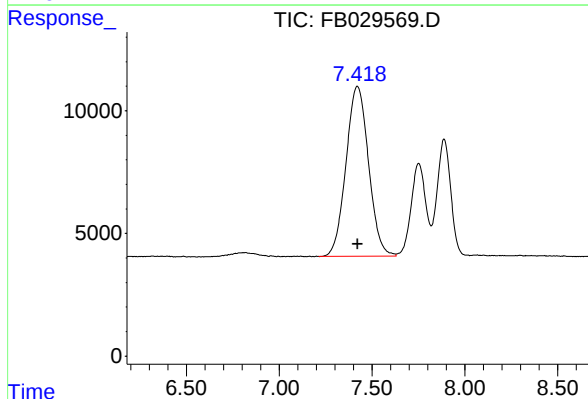


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: -0.003 min
Response: 585057
Conc: 31.78 ng/ml

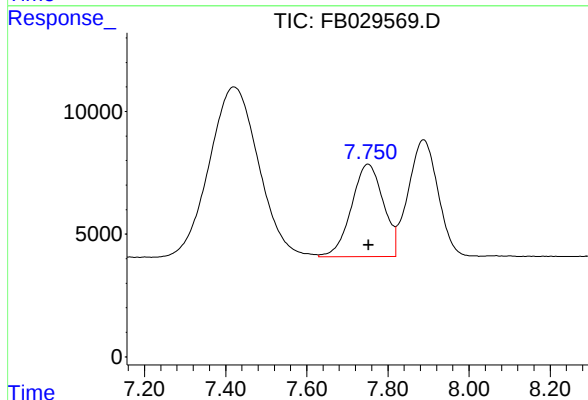


#3 n-Heptane

R.T.: 7.751 min
Delta R.T.: -0.001 min
Response: 205605
Conc: 10.55 ng/ml

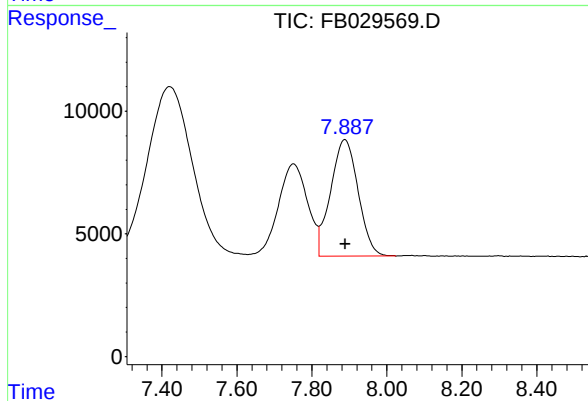

#4 Benzene


R.T.: 7.888 min
Delta R.T.: 0.000 min
Response: 242243
Conc: 10.72 ng/ml

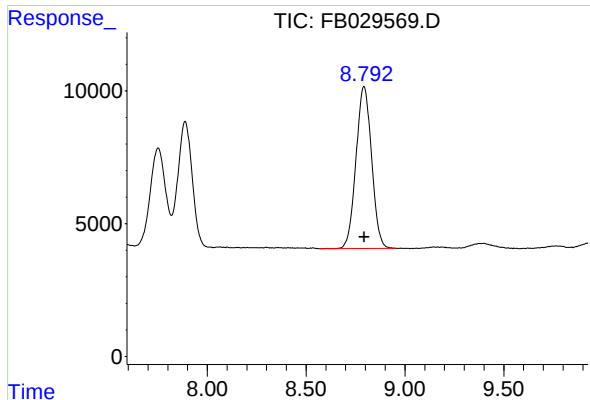

#5 AAA-TFT


R.T.: 8.793 min
Delta R.T.: 0.000 min
Response: 334411
Conc: 23.46 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0327W1

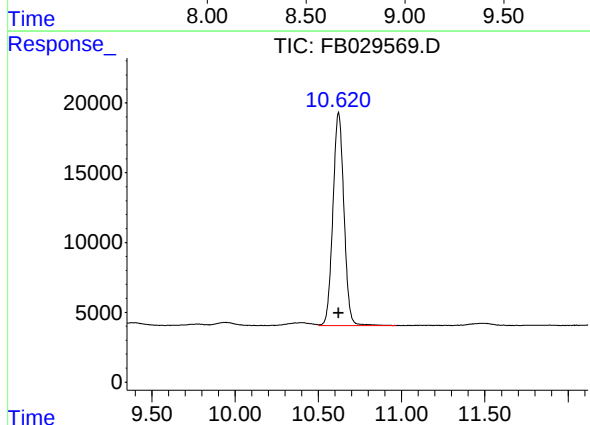


#6 Toluene

R.T.: 10.621 min
Delta R.T.: 0.000 min
Response: 703662
Conc: 31.92 ng/ml

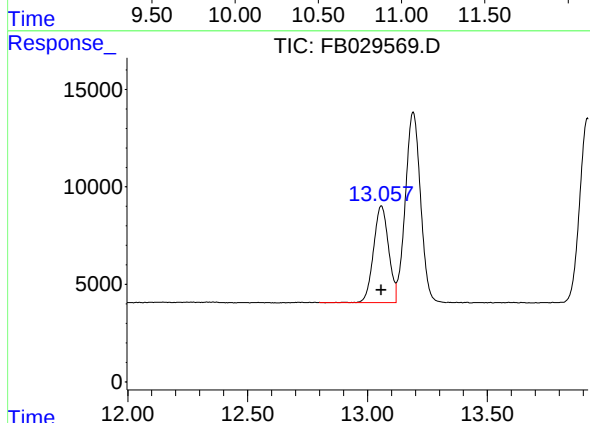


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: 0.000 min
Response: 215629
Conc: 10.43 ng/ml

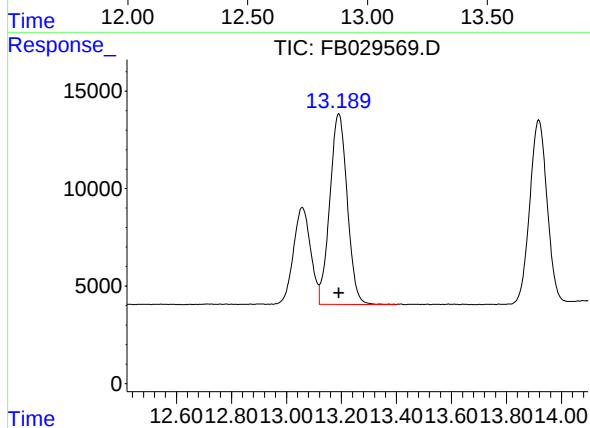

#8 m-Xylene


R.T.: 13.191 min
Delta R.T.: 0.000 min
Response: 430800
Conc: 21.05 ng/ml

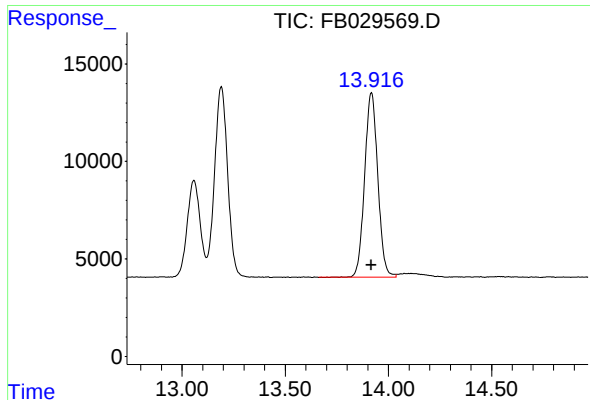

#9 O-Xylene

R.T.: 13.918 min
Delta R.T.: 0.000 min
Response: 419425
Conc: 21.17 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0327W1

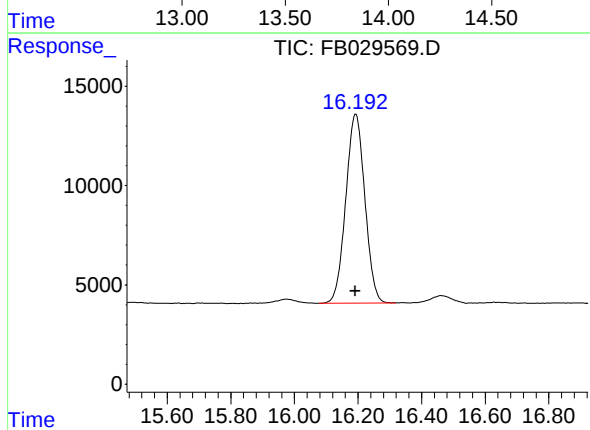

#10 1,2,4-Trimethylbenzene

R.T.: 16.193 min
Delta R.T.: 0.001 min
Response: 397345
Conc: 20.81 ng/ml