

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032723\
 Data File : FB029570.D
 Signal(s) : FID2B.CH
 Acq On : 27 Mar 2023 16:50
 Operator : YP/AJ
 Sample : BSF0327W2
 Misc :
 ALS Vial : 5 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0327W2

Integration File: Calibration.e
 Quant Time: Mar 28 02:15:15 2023
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
 Quant Title :
 QLast Update : Thu Mar 23 11:44:29 2023
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.792	261870	18.372 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.711	532912	31.742 ng/ml
2) t 2,2,4-Trimethylpentane	7.420	583301	31.685 ng/ml
3) t n-Heptane	7.750	205902	10.570 ng/ml
4) t Benzene	7.886	240364	10.639 ng/ml
6) t Toluene	10.620	689307	31.269 ng/ml
7) t Ethylbenzene	13.056	216617	10.479 ng/ml
8) t m-Xylene	13.189	430702	21.049 ng/ml
9) t O-Xylene	13.916	417679	21.083 ng/ml
10) t 1,2,4-Trimethylbenzene	16.191	400861	20.997 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032723\
Data File : FB029570.D
Signal(s) : FID2B.CH
Acq On : 27 Mar 2023 16:50
Operator : YP/AJ
Sample : BSF0327W2
Misc :
ALS Vial : 5 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0327W2

Integration File: Calibration.e
Quant Time: Mar 28 02:15:15 2023
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032323.M
Quant Title :
QLast Update : Thu Mar 23 11:44:29 2023
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

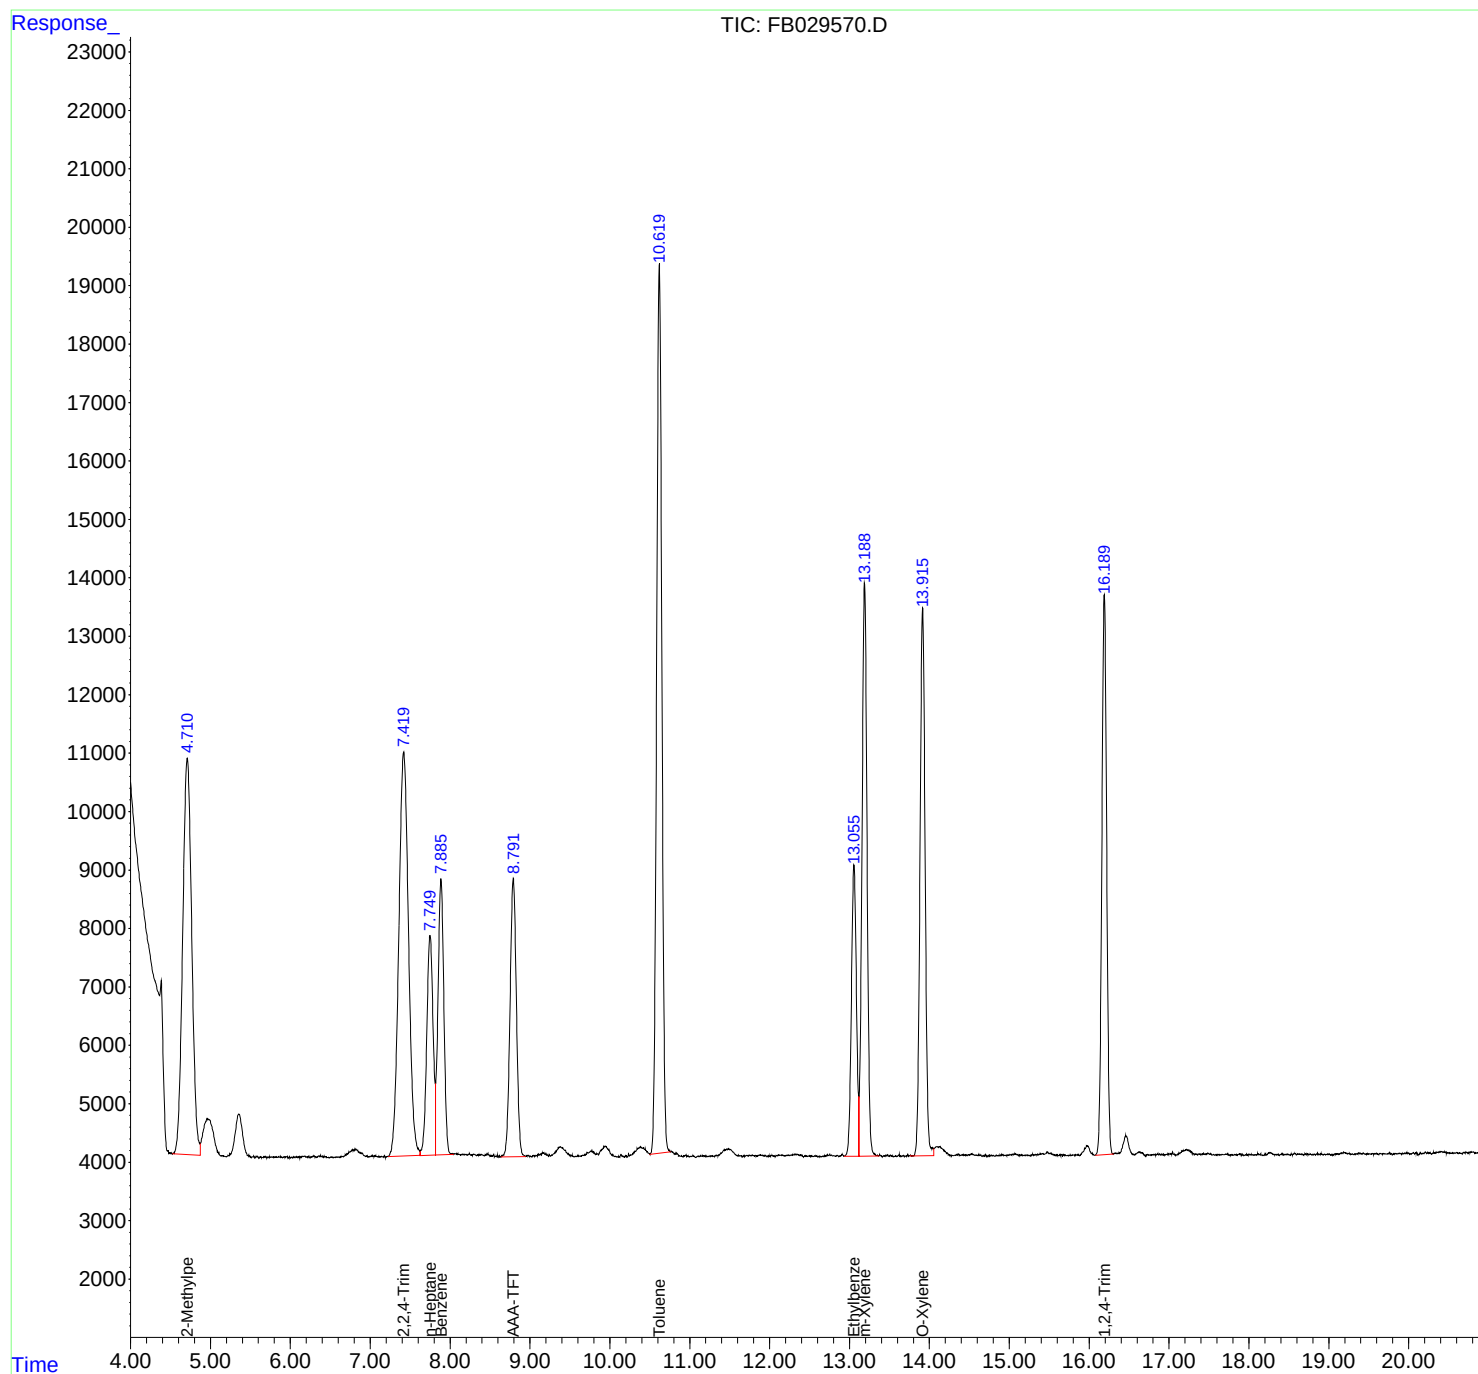


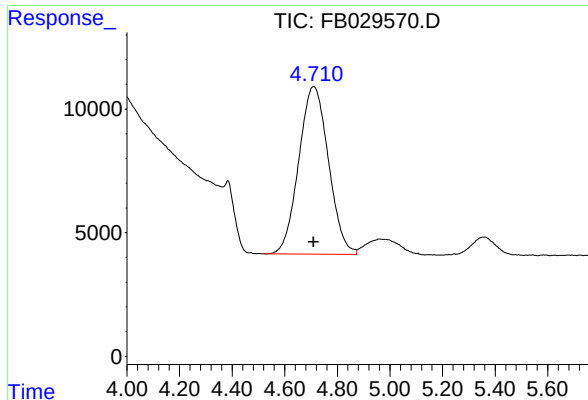

#1 2-Methylpentane


R.T.: 4.711 min
Delta R.T.: 0.001 min
Response: 532912
Conc: 31.74 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0327W2

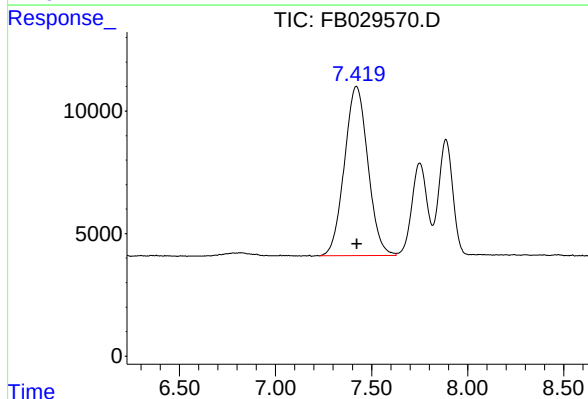


#2 2,2,4-Trimethylpentane

R.T.: 7.420 min
Delta R.T.: -0.003 min
Response: 583301
Conc: 31.68 ng/ml

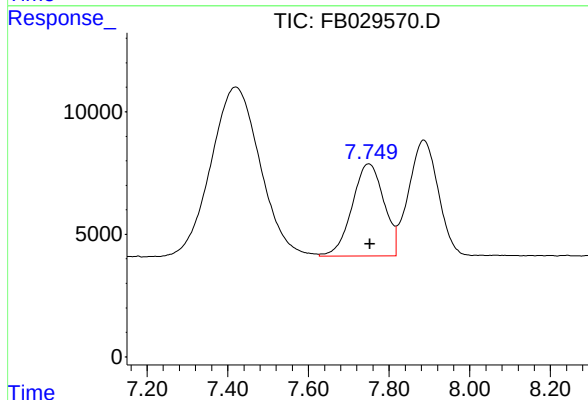


#3 n-Heptane

R.T.: 7.750 min
Delta R.T.: -0.003 min
Response: 205902
Conc: 10.57 ng/ml

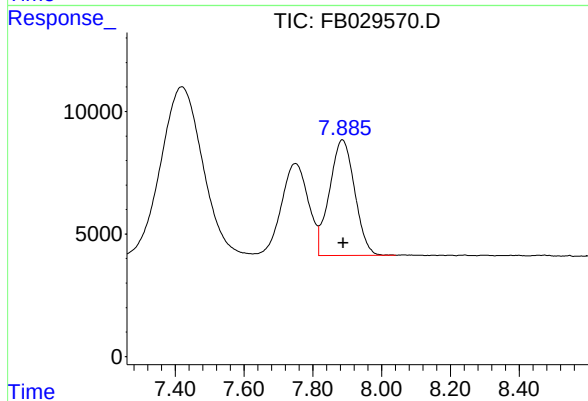

#4 Benzene


R.T.: 7.886 min
Delta R.T.: -0.003 min
Response: 240364
Conc: 10.64 ng/ml

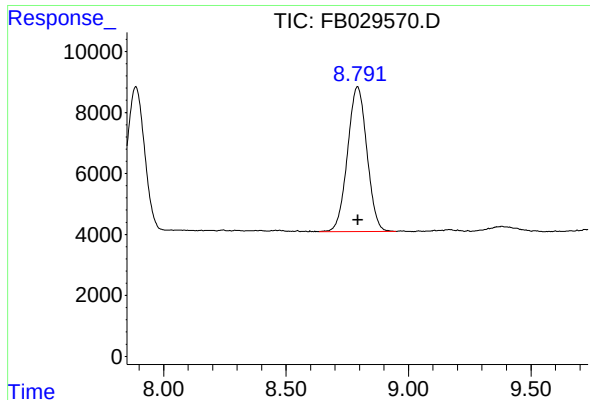

#5 AAA-TFT


R.T.: 8.792 min
Delta R.T.: -0.001 min
Response: 261870
Conc: 18.37 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0327W2

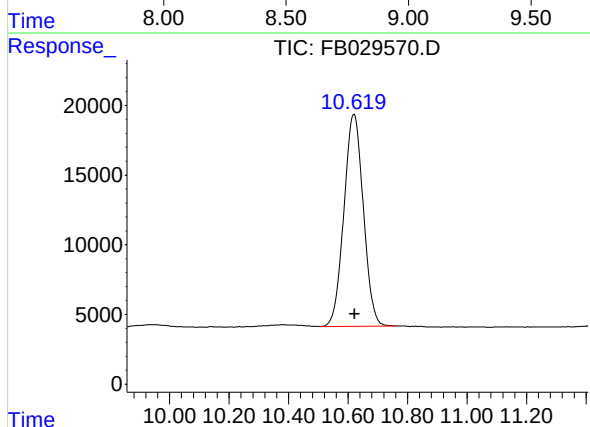


#6 Toluene

R.T.: 10.620 min
Delta R.T.: -0.001 min
Response: 689307
Conc: 31.27 ng/ml

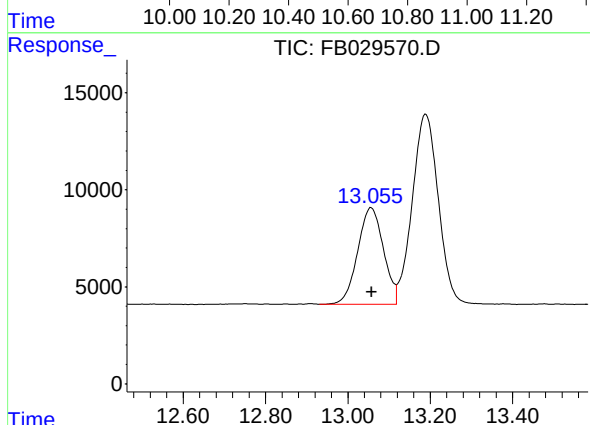


#7 Ethylbenzene

R.T.: 13.056 min
Delta R.T.: -0.001 min
Response: 216617
Conc: 10.48 ng/ml

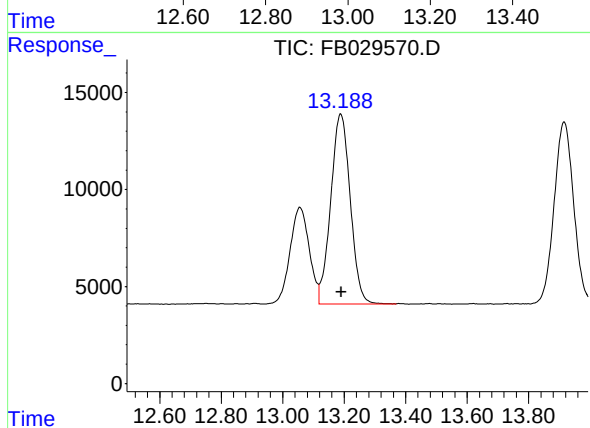

#8 m-Xylene


R.T.: 13.189 min
Delta R.T.: -0.001 min
Response: 430702
Conc: 21.05 ng/ml

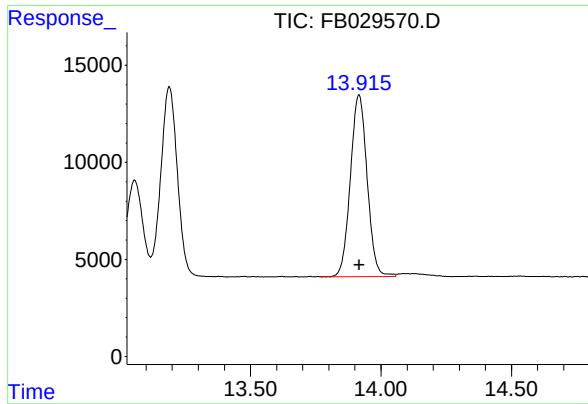

#9 O-Xylene

R.T.: 13.916 min
Delta R.T.: -0.001 min
Response: 417679
Conc: 21.08 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0327W2

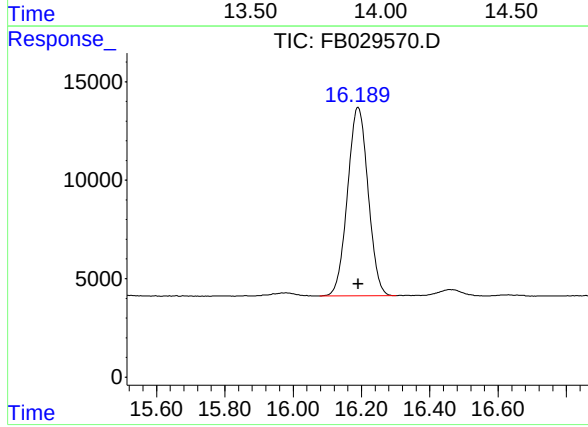

#10 1,2,4-Trimethylbenzene

R.T.: 16.191 min
Delta R.T.: -0.001 min
Response: 400861
Conc: 21.00 ng/ml