

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032819\
 Data File : FB020411.D
 Signal(s) : FID2B.CH
 Acq On : 28 Mar 2019 9:51
 Operator : MJ/SJ
 Sample : BSF0328S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0328S1

Integration File: Calibration.e
 Quant Time: Mar 29 00:56:13 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
 Quant Title :
 QLast Update : Tue Mar 26 12:48:09 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.038	477922	24.806 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.899	954096	34.422 ng/ml
2) t 2,2,4-Trimethylpentane	7.661	858965	35.820 ng/ml
3) t n-Heptane	7.993	370104	11.321 ng/ml
4) t Benzene	8.131	397766	11.485 ng/ml
6) t Toluene	10.885	878131	33.856 ng/ml
7) t Ethylbenzene	13.337	215856	10.965 ng/ml
8) t m-Xylene	13.470	435881	21.469 ng/ml
9) t O-Xylene	14.202	424221	20.946 ng/ml
10) t 1,2,4-Trimethylbenzene	16.488	429818	20.659 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032819\
Data File : FB020411.D
Signal(s) : FID2B.CH
Acq On : 28 Mar 2019 9:51
Operator : MJ/SJ
Sample : BSF0328S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0328S1

Integration File: Calibration.e
Quant Time: Mar 29 00:56:13 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
Quant Title :
QLast Update : Tue Mar 26 12:48:09 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

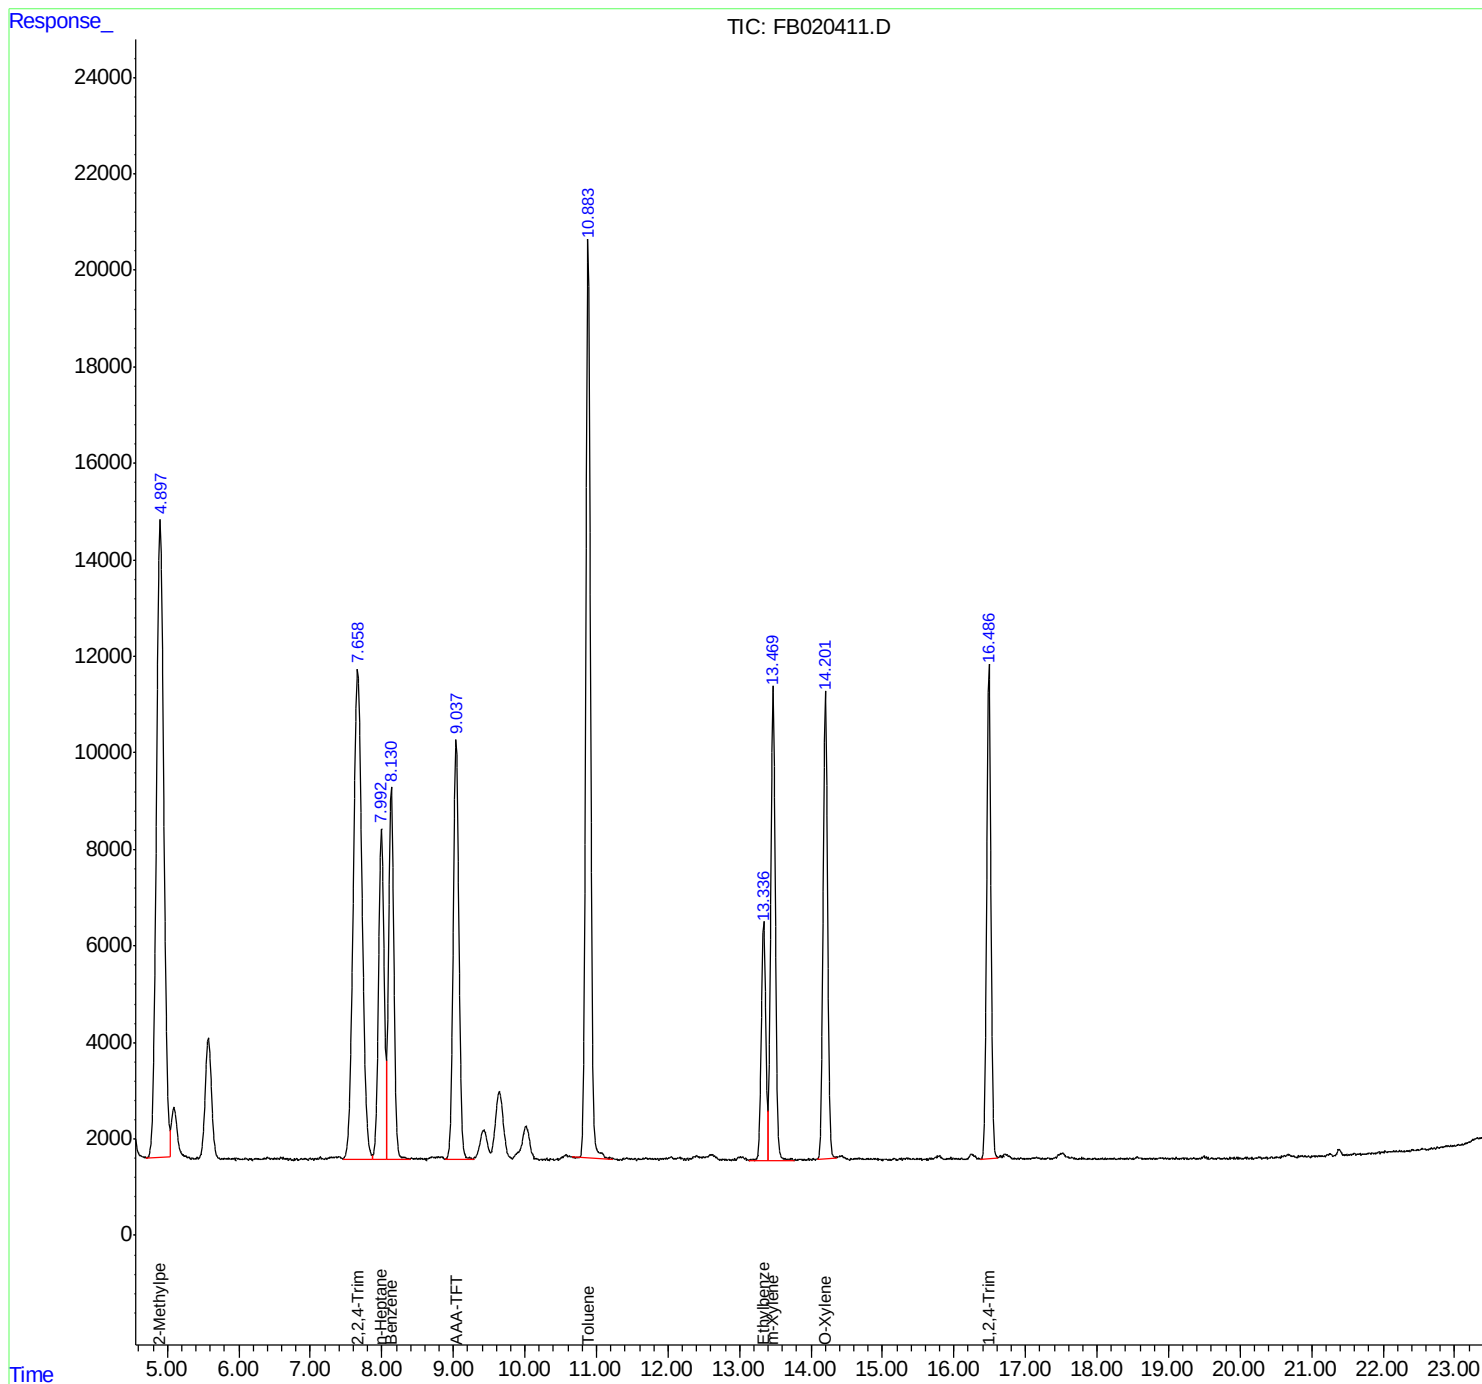


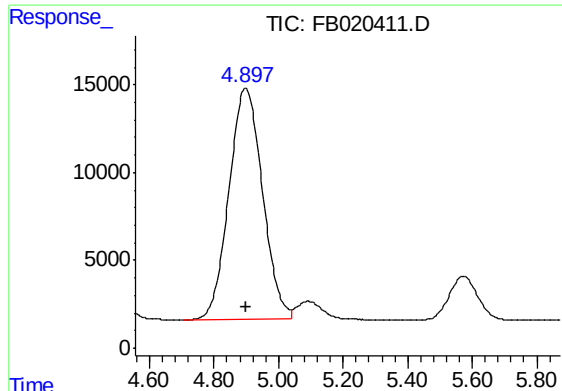

#1 2-Methylpentane


R.T.: 4.899 min
Delta R.T.: 0.000 min
Response: 954096
Conc: 34.42 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0328S1

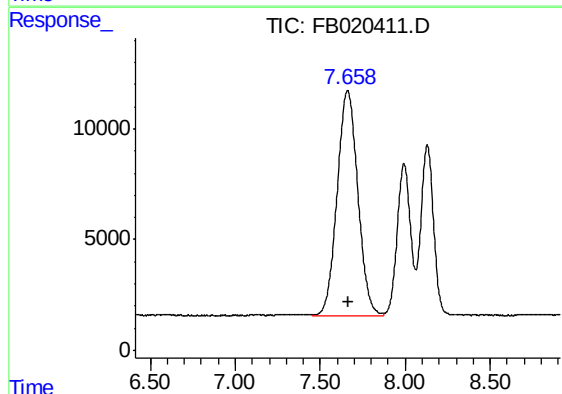


#2 2,2,4-Trimethylpentane

R.T.: 7.661 min
Delta R.T.: -0.005 min
Response: 858965
Conc: 35.82 ng/ml

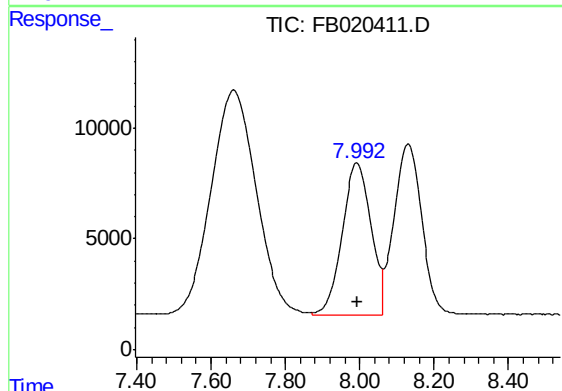


#3 n-Heptane

R.T.: 7.993 min
Delta R.T.: -0.002 min
Response: 370104
Conc: 11.32 ng/ml

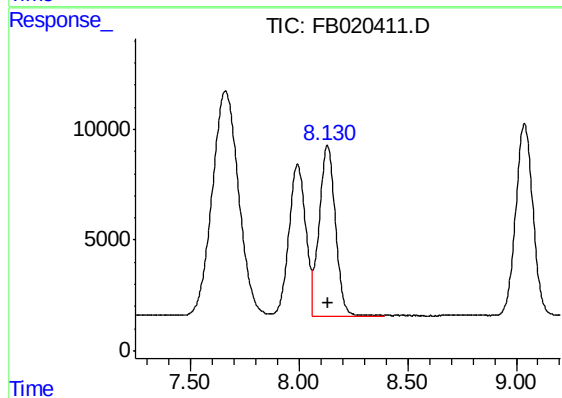

#4 Benzene


R.T.: 8.131 min
Delta R.T.: -0.002 min
Response: 397766
Conc: 11.49 ng/ml

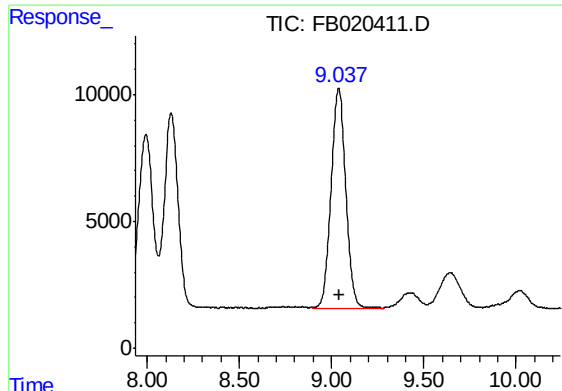

#5 AAA-TFT


R.T.: 9.038 min
Delta R.T.: -0.002 min
Response: 477922
Conc: 24.81 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0328S1

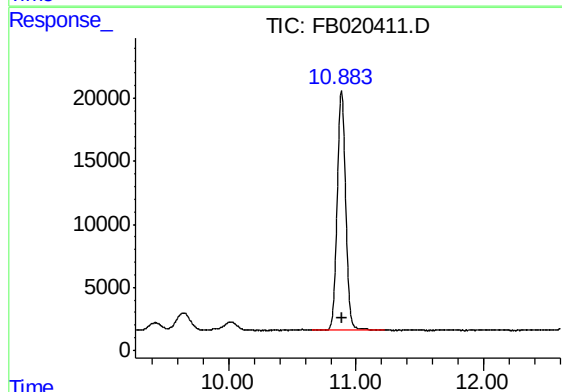


#6 Toluene

R.T.: 10.885 min
Delta R.T.: -0.003 min
Response: 878131
Conc: 33.86 ng/ml

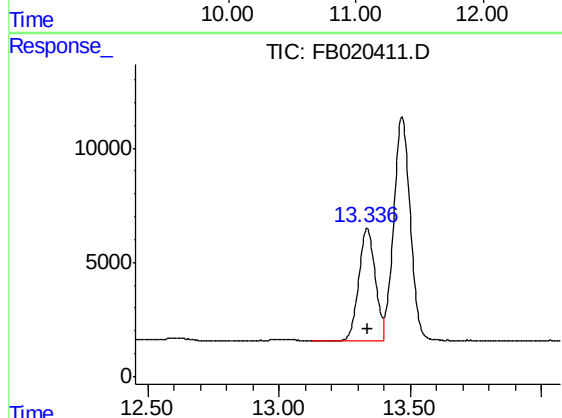


#7 Ethylbenzene

R.T.: 13.337 min
Delta R.T.: -0.003 min
Response: 215856
Conc: 10.96 ng/ml

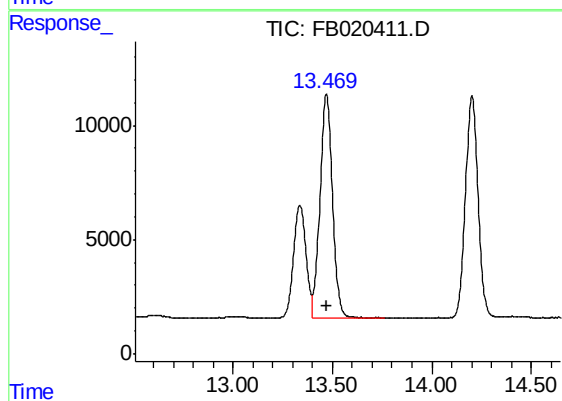

#8 m-Xylene


R.T.: 13.470 min
Delta R.T.: -0.004 min
Response: 435881
Conc: 21.47 ng/ml

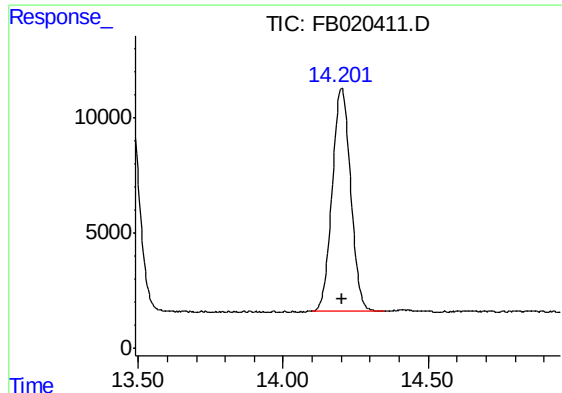

#9 O-Xylene

R.T.: 14.202 min
Delta R.T.: -0.003 min
Response: 424221
Conc: 20.95 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0328S1

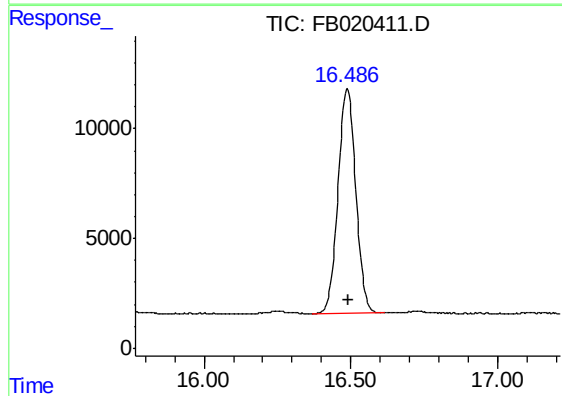

#10 1,2,4-Trimethylbenzene

R.T.: 16.488 min
Delta R.T.: -0.003 min
Response: 429818
Conc: 20.66 ng/ml