

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032919\
 Data File : FB020454.D
 Signal(s) : FID2B.CH
 Acq On : 29 Mar 2019 23:50
 Operator : MJ/SJ
 Sample : K2180-18
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 24 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Mar 30 02:28:58 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
 Quant Title :
 QLast Update : Tue Mar 26 12:48:09 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.062	1341259	69.616 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.899	336285	12.132 ng/ml
2) t 2,2,4-Trimethylpentane	7.676	1438345	59.982 ng/ml
3) t n-Heptane	7.997	1639993	50.163 ng/ml
6) t Toluene	10.930	597452	23.035 ng/ml
7) t Ethylbenzene	13.342	4844982	246.105 ng/ml
8) t m-Xylene	13.471	5160041	254.154 ng/ml
9) t O-Xylene	14.204	59186	2.922 ng/ml
10) t 1,2,4-Trimethylbenzene	16.493	9748811	468.561 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032919\
Data File : FB020454.D
Signal(s) : FID2B.CH
Acq On : 29 Mar 2019 23:50
Operator : MJ/SJ
Sample : K2180-18
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 24 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Mar 30 02:28:58 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
Quant Title :
QLast Update : Tue Mar 26 12:48:09 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

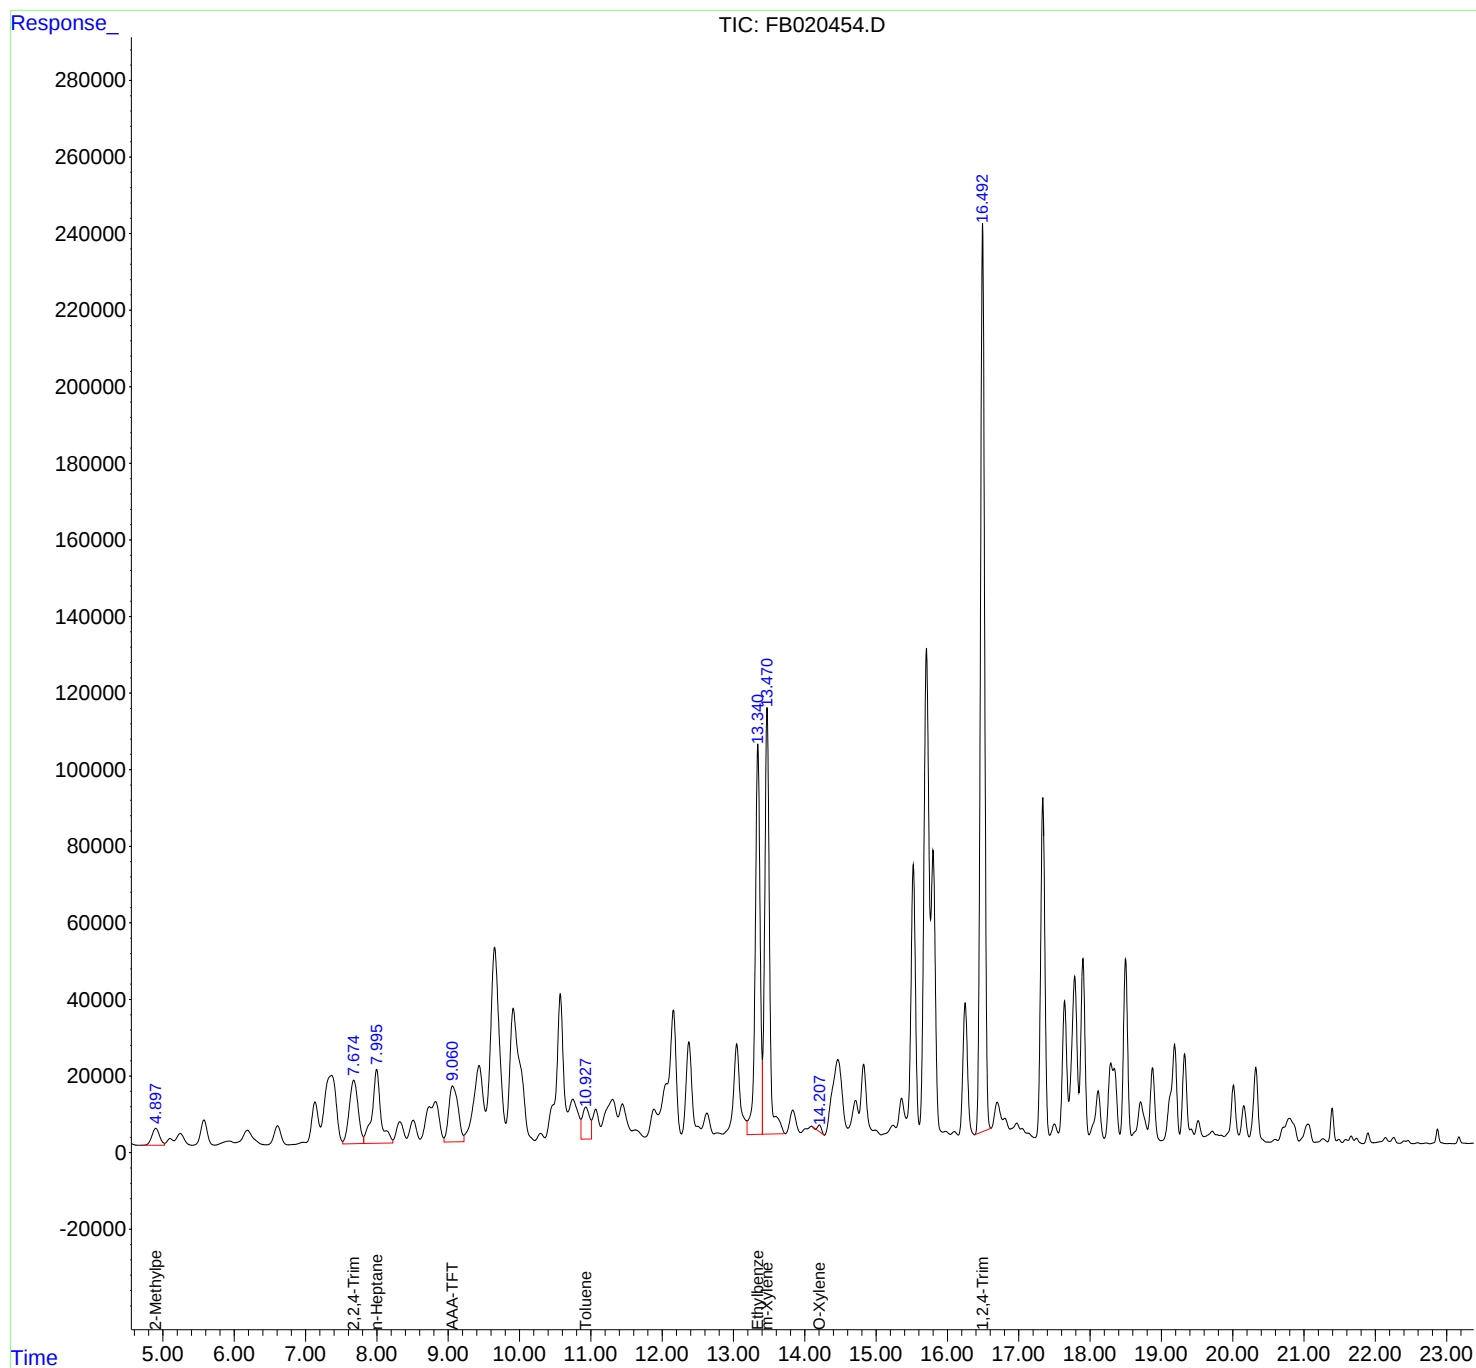

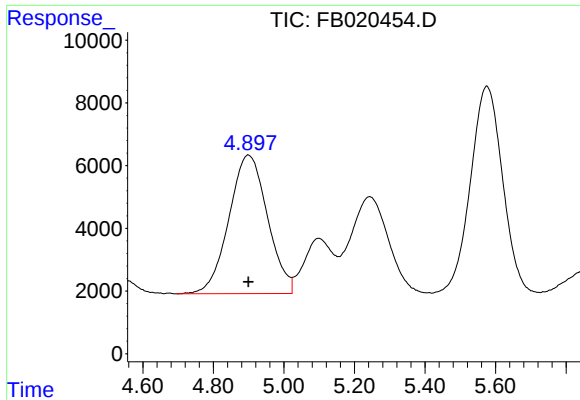


#1 2-Methylpentane

R.T.: 4.899 min
Delta R.T.: 0.000 min
Response: 336285
Conc: 12.13 ng/ml

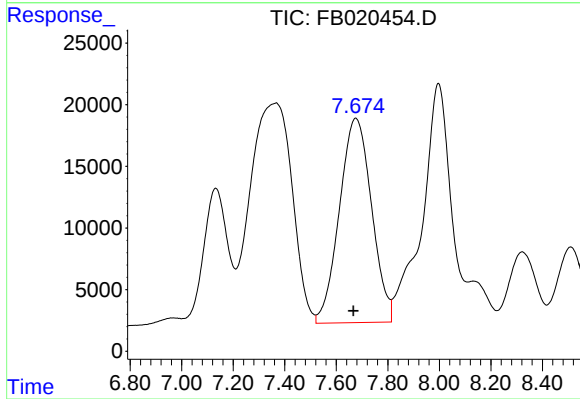


#2 2,2,4-Trimethylpentane

R.T.: 7.676 min
Delta R.T.: 0.010 min
Response: 1438345
Conc: 59.98 ng/ml

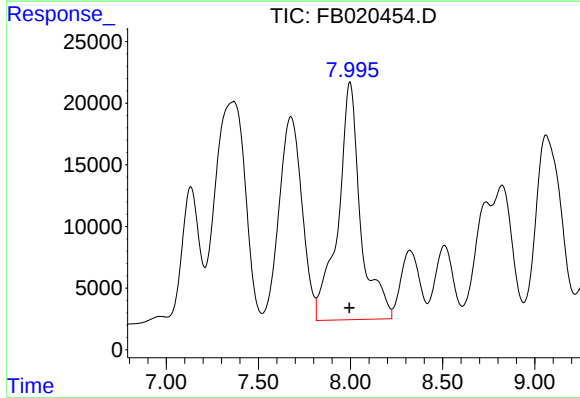


#3 n-Heptane

R.T.: 7.997 min
Delta R.T.: 0.002 min
Response: 1639993
Conc: 50.16 ng/ml

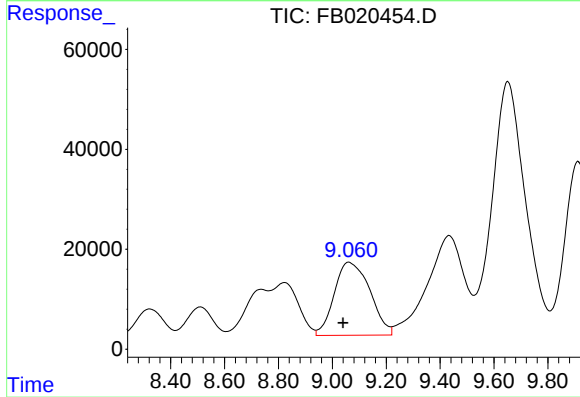


#5 AAA-TFT

R.T.: 9.062 min
Delta R.T.: 0.022 min
Response: 1341259
Conc: 69.62 ng/ml

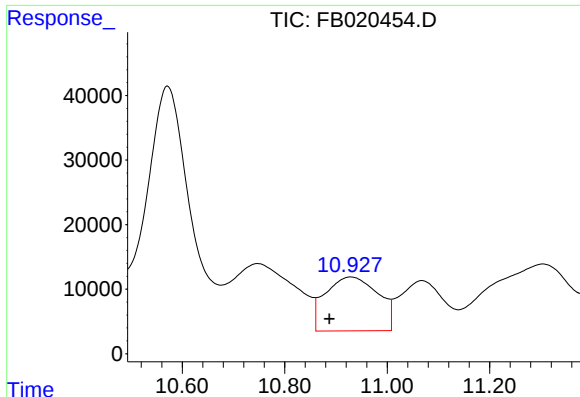


#6 Toluene

R.T.: 10.930 min
Delta R.T.: 0.042 min
Response: 597452
Conc: 23.03 ng/ml

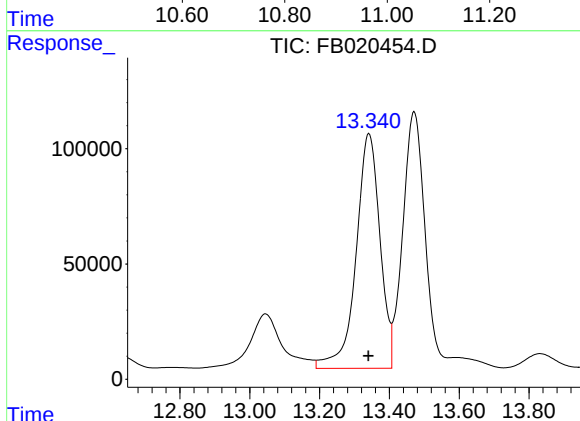


#7 Ethylbenzene

R.T.: 13.342 min
Delta R.T.: 0.002 min
Response: 4844982
Conc: 246.11 ng/ml

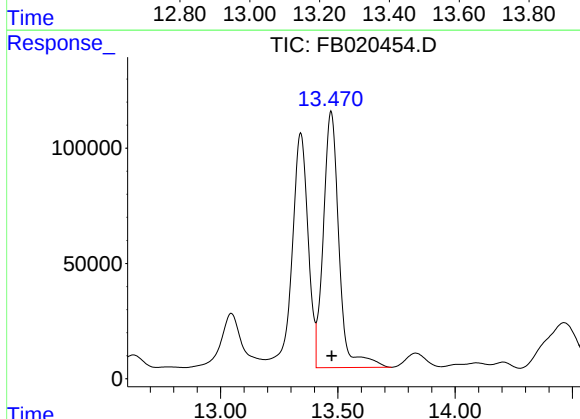


#8 m-Xylene

R.T.: 13.471 min
Delta R.T.: -0.002 min
Response: 5160041
Conc: 254.15 ng/ml

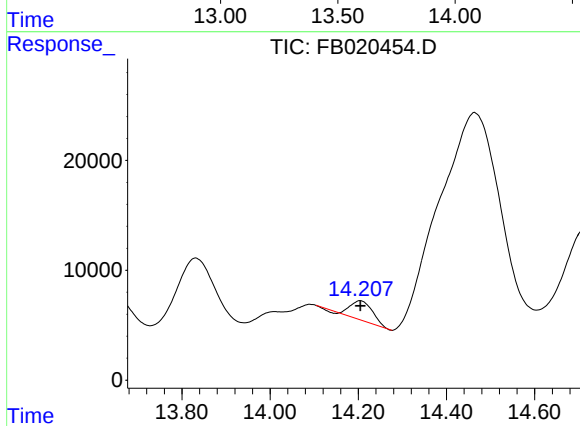

#9 O-Xylene

R.T.: 14.204 min
Delta R.T.: 0.000 min
Response: 59186
Conc: 2.92 ng/ml

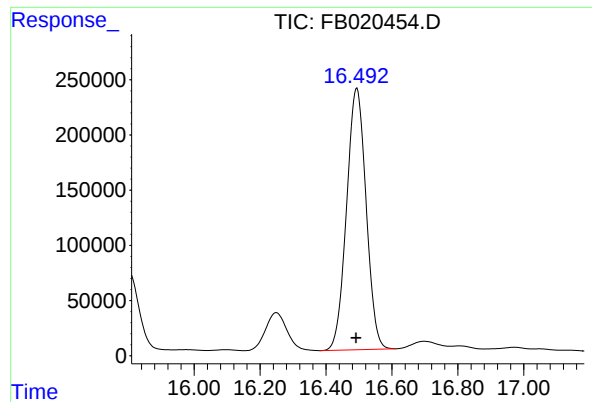

#10 1,2,4-Trimethylbenzene

R.T.: 16.493 min
Delta R.T.: 0.002 min
Response: 9748811
Conc: 468.56 ng/ml