

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032919\
 Data File : FB020460.D
 Signal(s) : FID2B.CH
 Acq On : 30 Mar 2019 3:51
 Operator : MJ/SJ
 Sample : K2180-29
 Misc : 5.06g/5.00ml DI WATER
 ALS Vial : 32 Sample Multiplier: 1

Integration File: SAMPLE.e
 Quant Time: Mar 30 07:04:52 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
 Quant Title :
 QLast Update : Tue Mar 26 12:48:09 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	9.044	418312	21.712 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.898	583	0.021 ng/ml
2) t	2,2,4-Trimethylpentane	7.674	5151	0.215 ng/ml
3) t	n-Heptane	8.003	625	0.019 ng/ml
4) t	Benzene	8.151	2921	0.084 ng/ml
6) t	Toluene	10.936	8473	0.327 ng/ml
7) t	Ethylbenzene	13.337	2790	0.142 ng/ml
8) t	m-Xylene	13.474	3524	0.174 ng/ml
9) t	O-Xylene	14.191	2319	0.114 ng/ml
10) t	1,2,4-Trimethylbenzene	16.526	5382	0.259 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB032919\
Data File : FB020460.D
Signal(s) : FID2B.CH
Acq On : 30 Mar 2019 3:51
Operator : MJ/SJ
Sample : K2180-29
Misc : 5.06g/5.00ml DI WATER
ALS Vial : 32 Sample Multiplier: 1

Integration File: SAMPLE.e
Quant Time: Mar 30 07:04:52 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
Quant Title :
QLast Update : Tue Mar 26 12:48:09 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

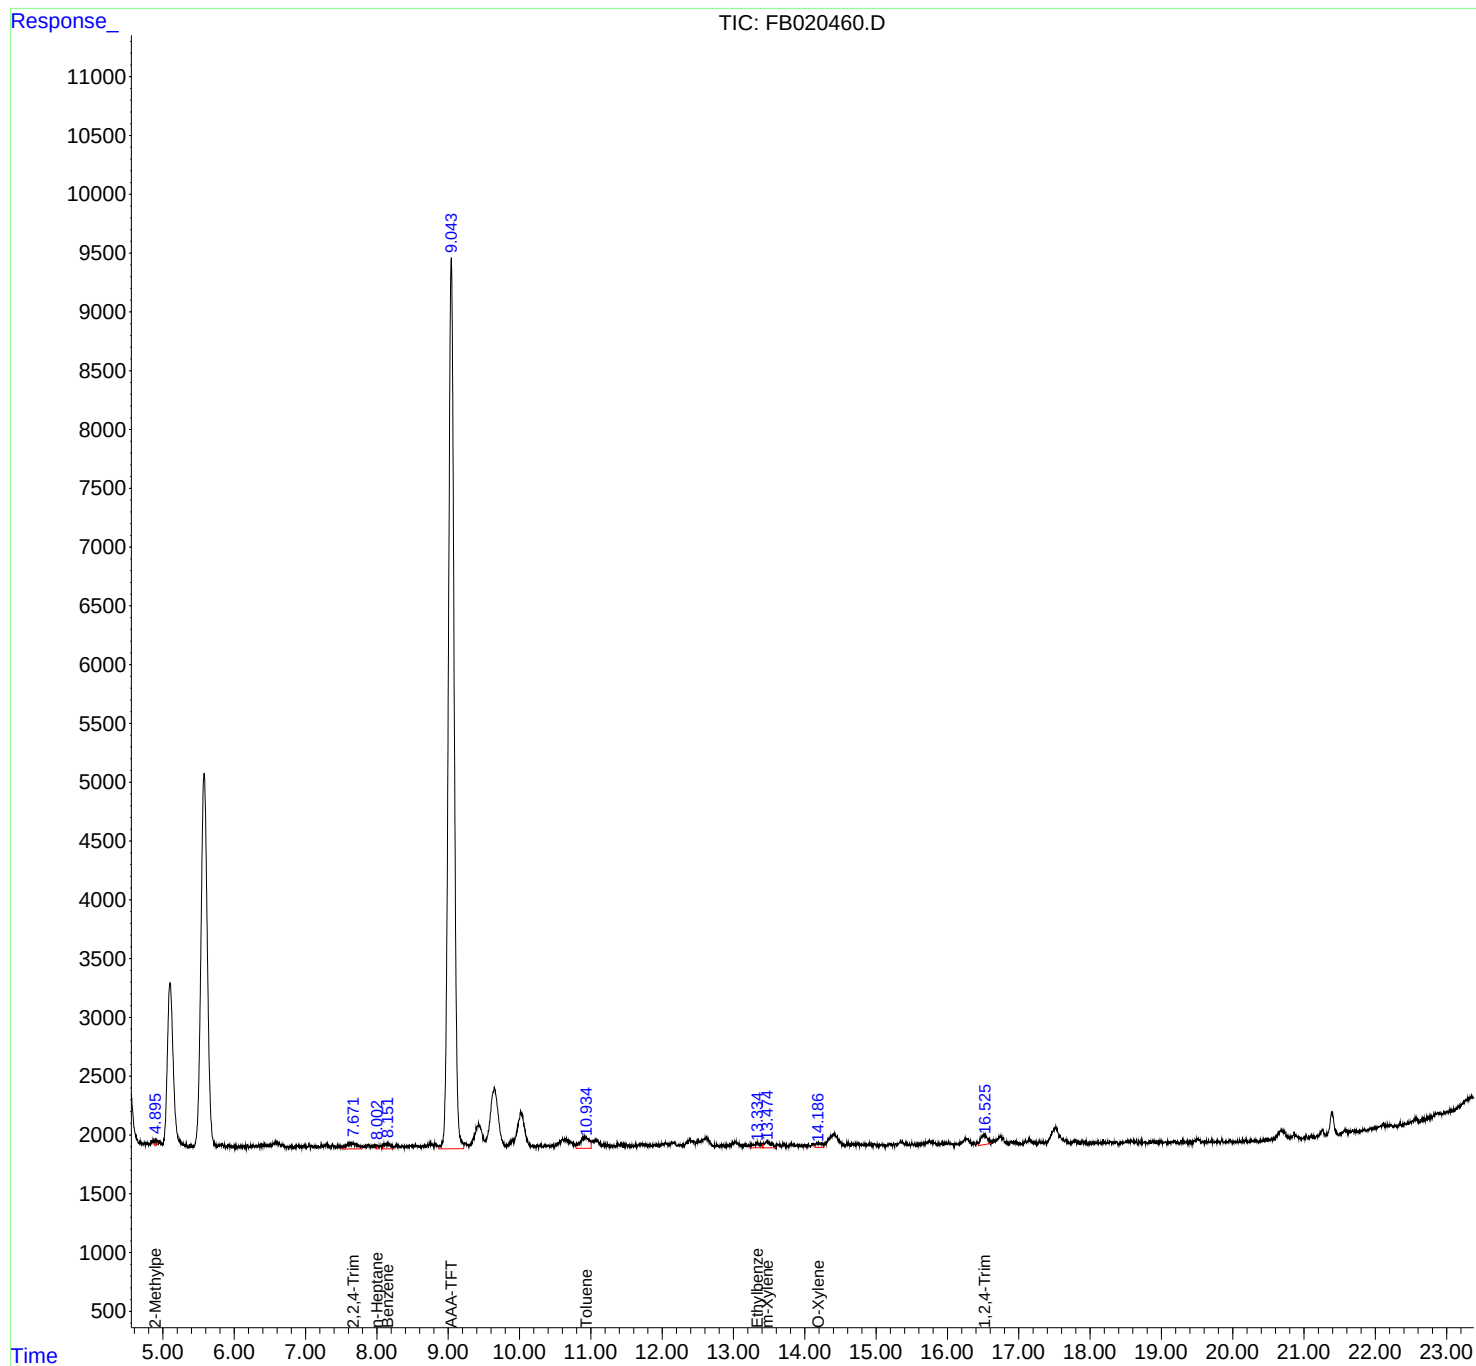

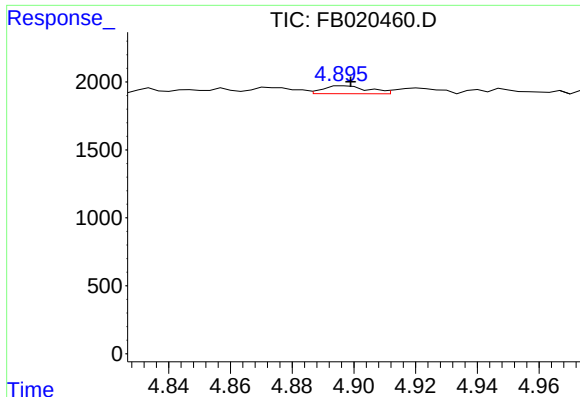


#1 2-Methylpentane

R.T.: 4.898 min
Delta R.T.: -0.001 min
Response: 583
Conc: 0.02 ng/ml

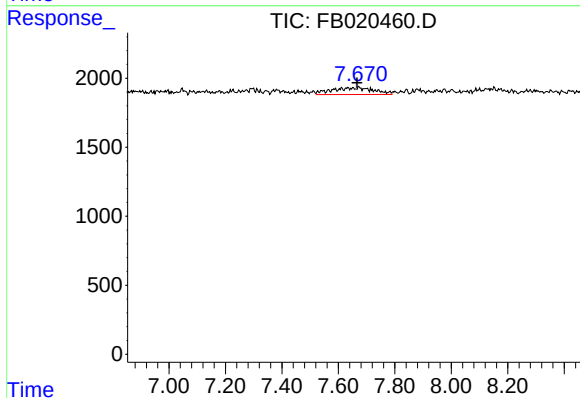


#2 2,2,4-Trimethylpentane

R.T.: 7.674 min
Delta R.T.: 0.008 min
Response: 5151
Conc: 0.21 ng/ml

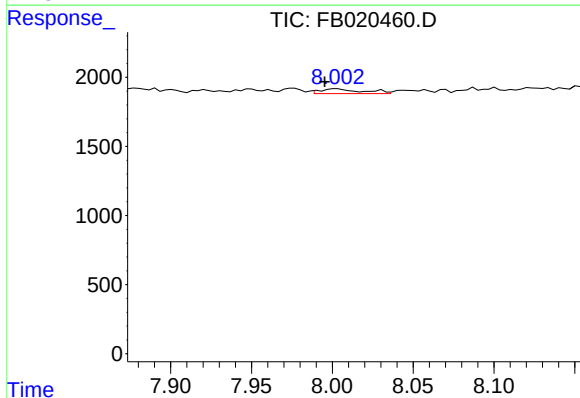


#3 n-Heptane

R.T.: 8.003 min
Delta R.T.: 0.008 min
Response: 625
Conc: 0.02 ng/ml

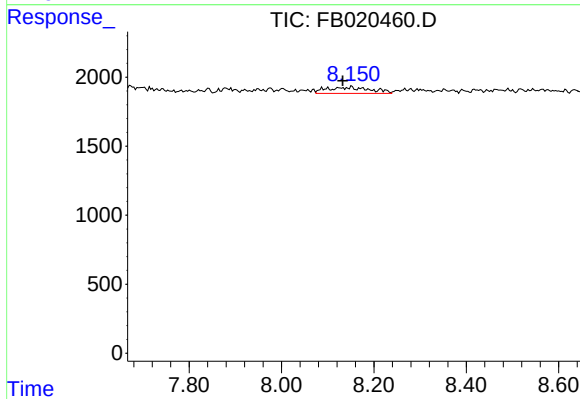


#4 Benzene

R.T.: 8.151 min
Delta R.T.: 0.018 min
Response: 2921
Conc: 0.08 ng/ml

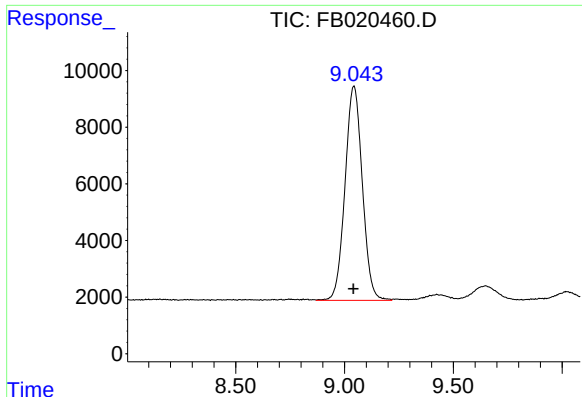


#5 AAA-TFT

R.T.: 9.044 min
Delta R.T.: 0.003 min
Response: 418312
Conc: 21.71 ng/ml

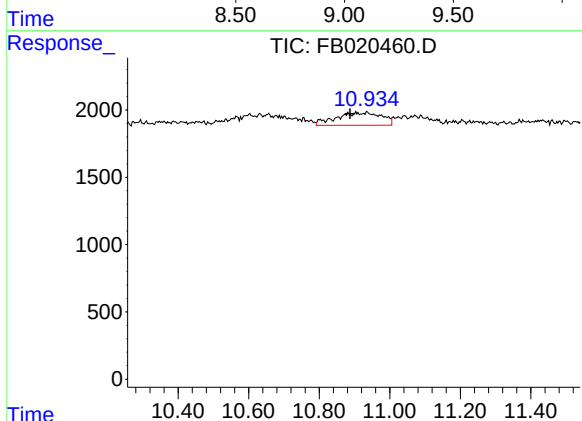


#6 Toluene

R.T.: 10.936 min
Delta R.T.: 0.049 min
Response: 8473
Conc: 0.33 ng/ml

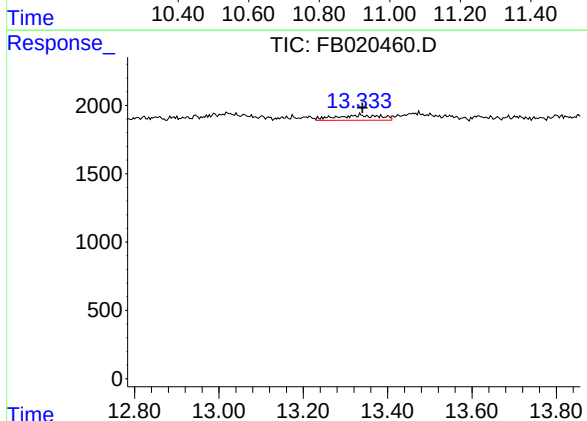


#7 Ethylbenzene

R.T.: 13.337 min
Delta R.T.: -0.003 min
Response: 2790
Conc: 0.14 ng/ml

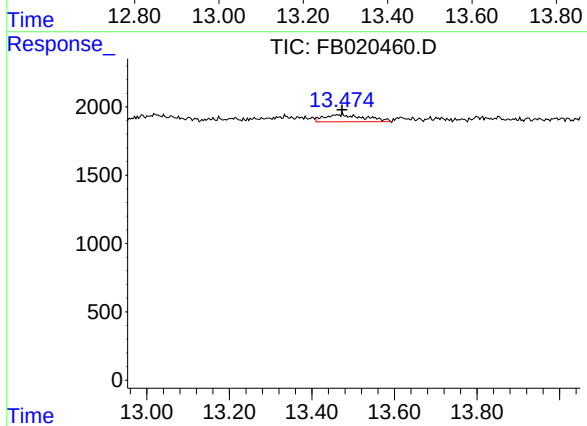


#8 m-Xylene

R.T.: 13.474 min
Delta R.T.: 0.000 min
Response: 3524
Conc: 0.17 ng/ml

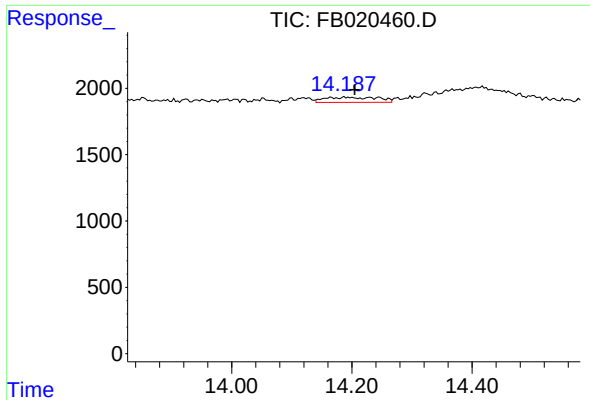

#9 O-Xylene

R.T.: 14.191 min
Delta R.T.: -0.014 min
Response: 2319
Conc: 0.11 ng/ml

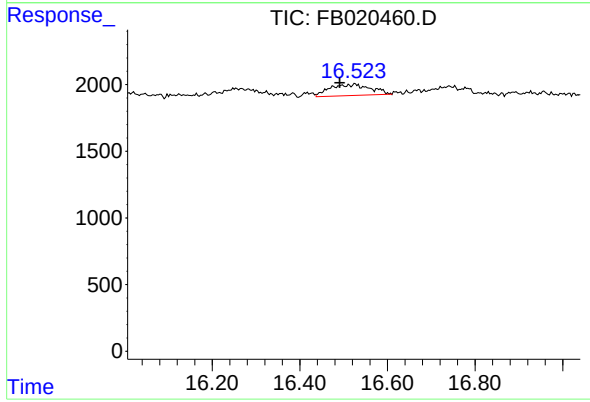

#10 1,2,4-Trimethylbenzene

R.T.: 16.526 min
Delta R.T.: 0.035 min
Response: 5382
Conc: 0.26 ng/ml