

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040119\
Data File : FB020474.D
Signal(s) : FID2B.CH
Acq On : 1 Apr 2019 13:05
Operator : MJ/SJ
Sample : VBF0401S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF0401S1

Integration File: Calibration.e
Quant Time: Apr 02 01:34:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
Quant Title :
QLast Update : Tue Mar 26 12:48:09 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.040	353255	18.335 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.893	7549	0.272 ng/ml
2) t 2,2,4-Trimethylpentane	7.655	10047	0.419 ng/ml
6) t Toluene	10.885	9895	0.381 ng/ml
8) t m-Xylene	13.475	6732	0.332 ng/ml
9) t O-Xylene	14.204	6499	0.321 ng/ml
10) t 1,2,4-Trimethylbenzene	16.499	10942	0.526 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040119\
Data File : FB020474.D
Signal(s) : FID2B.CH
Acq On : 1 Apr 2019 13:05
Operator : MJ/SJ
Sample : VBF0401S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 2 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
VBF0401S1

Integration File: Calibration.e
Quant Time: Apr 02 01:34:34 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
Quant Title :
QLast Update : Tue Mar 26 12:48:09 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

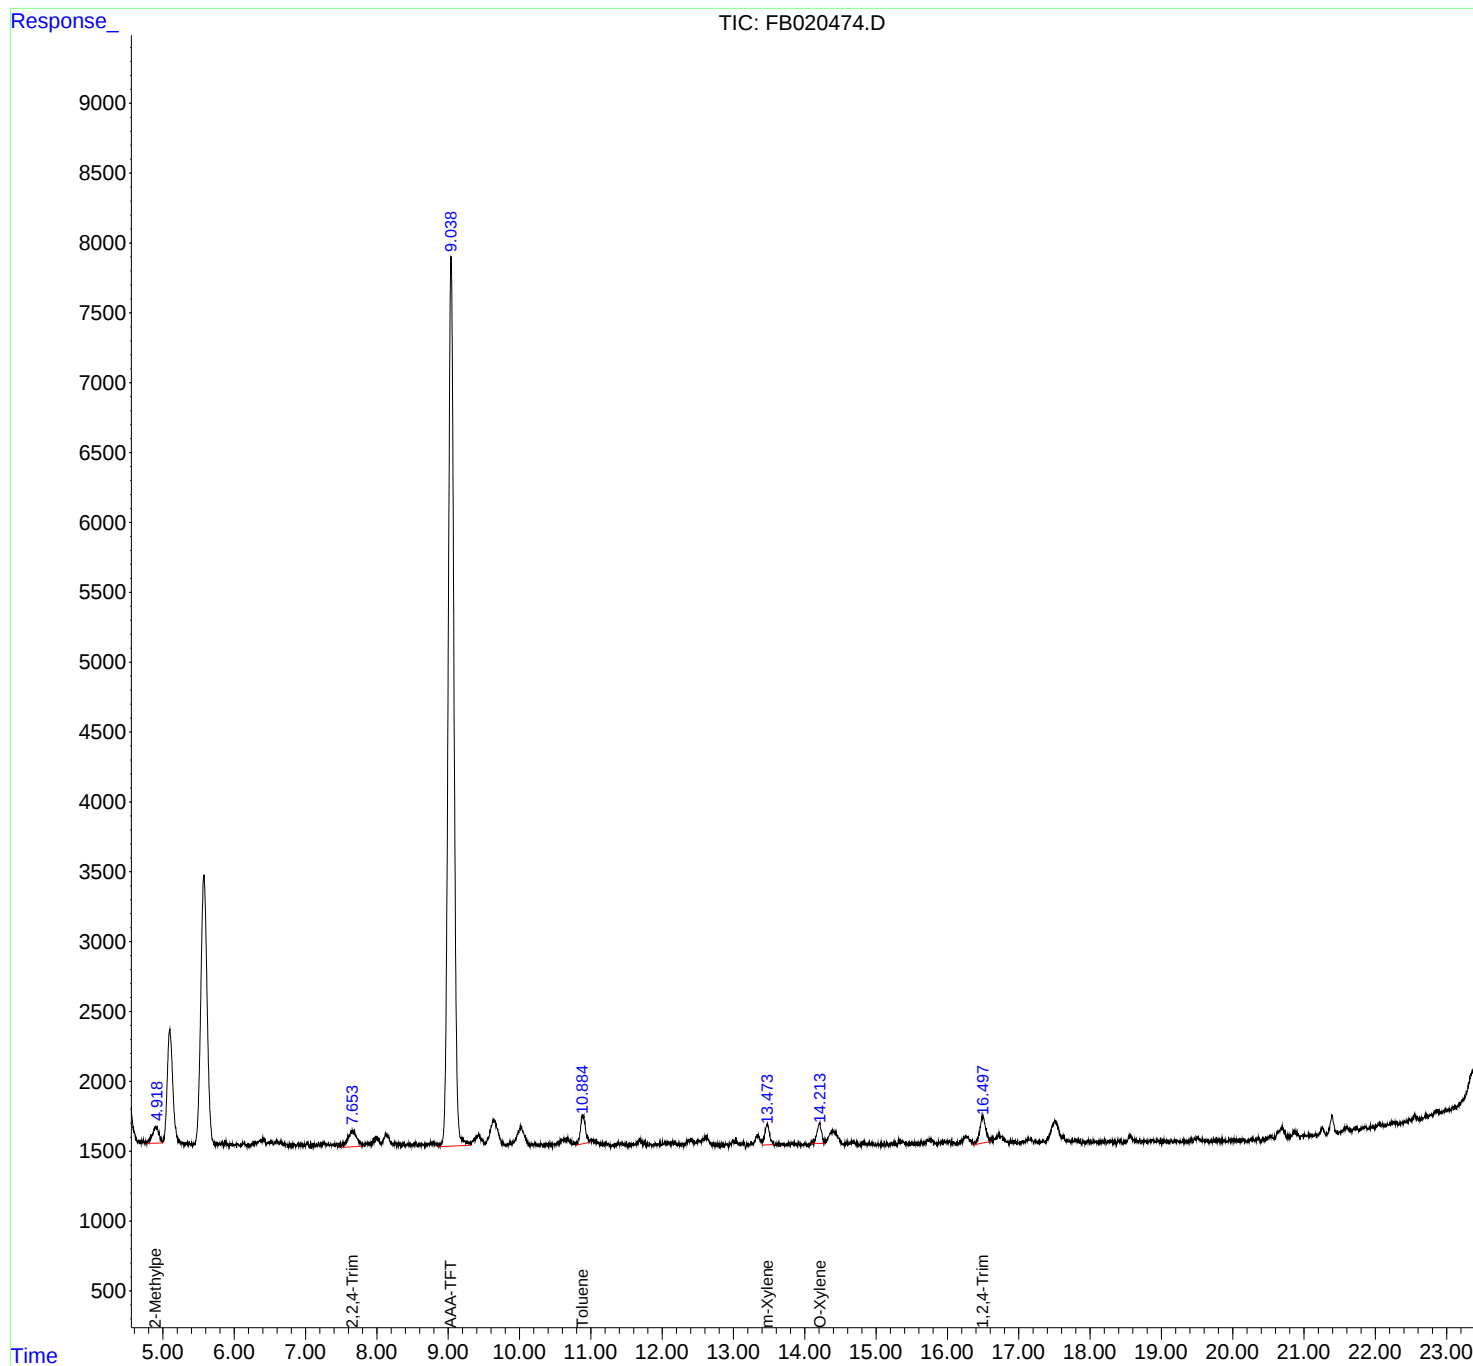


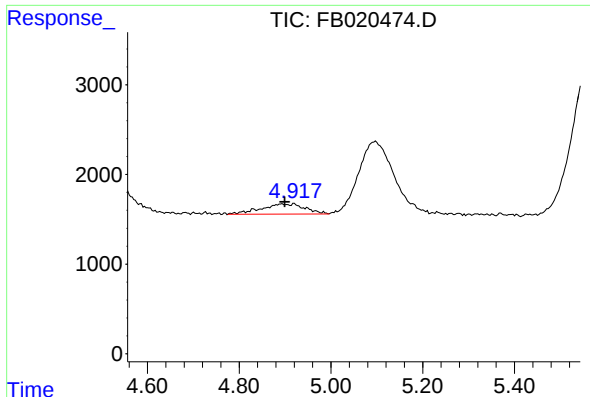

#1 2-Methylpentane


R.T.: 4.893 min
Delta R.T.: -0.006 min
Response: 7549
Conc: 0.27 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF0401S1

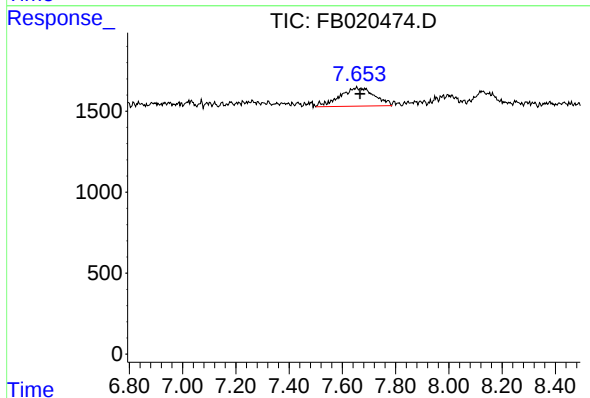


#2 2,2,4-Trimethylpentane

R.T.: 7.655 min
Delta R.T.: -0.011 min
Response: 10047
Conc: 0.42 ng/ml

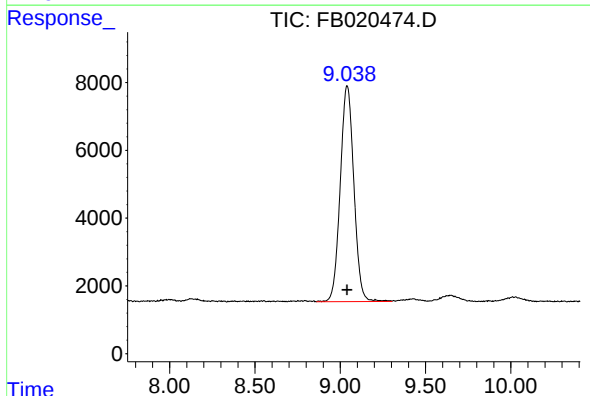


#5 AAA-TFT

R.T.: 9.040 min
Delta R.T.: 0.000 min
Response: 353255
Conc: 18.34 ng/ml

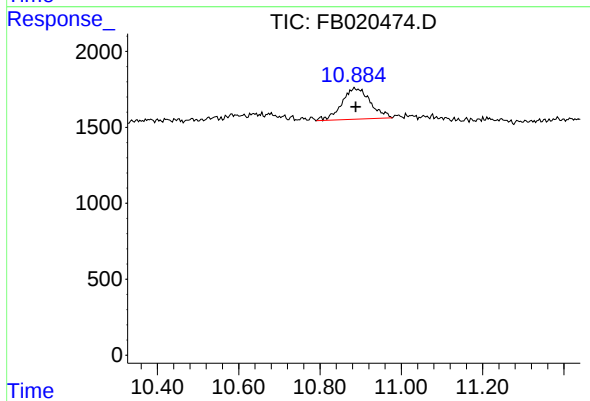

#6 Toluene


R.T.: 10.885 min
Delta R.T.: -0.002 min
Response: 9895
Conc: 0.38 ng/ml

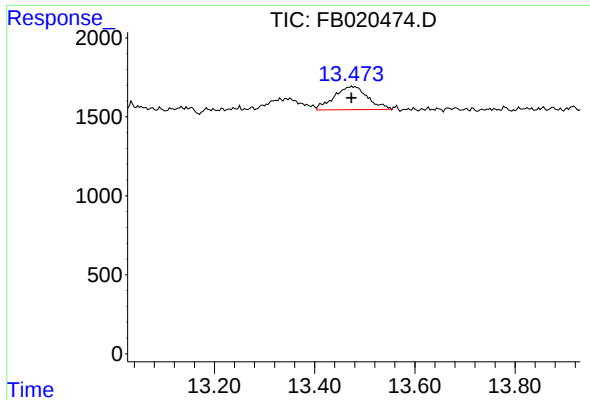

#8 m-Xylene


R.T.: 13.475 min
Delta R.T.: 0.002 min
Response: 6732
Conc: 0.33 ng/ml

Instrument :
FID_B
ClientSampleId :
VBF0401S1

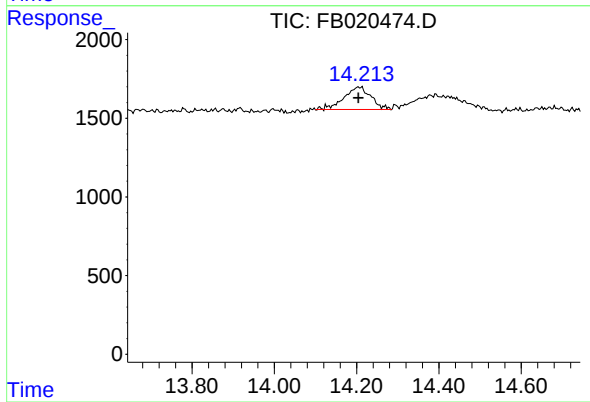

#9 O-Xylene

R.T.: 14.204 min
Delta R.T.: 0.000 min
Response: 6499
Conc: 0.32 ng/ml

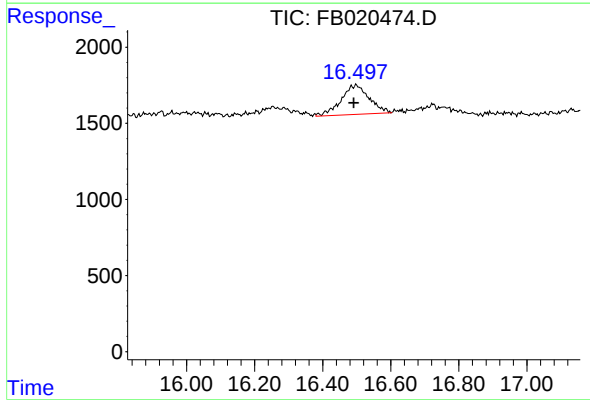

#10 1,2,4-Trimethylbenzene

R.T.: 16.499 min
Delta R.T.: 0.008 min
Response: 10942
Conc: 0.53 ng/ml