

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040119\
 Data File : FB020475.D
 Signal(s) : FID2B.CH
 Acq On : 1 Apr 2019 13:35
 Operator : MJ/SJ
 Sample : BSF0401S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0401S1

Integration File: Calibration.e
 Quant Time: Apr 02 01:34:45 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
 Quant Title :
 QLast Update : Tue Mar 26 12:48:09 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.040	444231	23.057 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.900	859217	30.999 ng/ml
2) t 2,2,4-Trimethylpentane	7.662	786778	32.810 ng/ml
3) t n-Heptane	7.996	327403	10.014 ng/ml
4) t Benzene	8.133	353762	10.215 ng/ml
6) t Toluene	10.887	779404	30.050 ng/ml
7) t Ethylbenzene	13.340	206330	10.481 ng/ml
8) t m-Xylene	13.473	426289	20.997 ng/ml
9) t O-Xylene	14.204	421793	20.826 ng/ml
10) t 1,2,4-Trimethylbenzene	16.491	422954	20.329 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040119\
Data File : FB020475.D
Signal(s) : FID2B.CH
Acq On : 1 Apr 2019 13:35
Operator : MJ/SJ
Sample : BSF0401S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0401S1

Integration File: Calibration.e
Quant Time: Apr 02 01:34:45 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
Quant Title :
QLast Update : Tue Mar 26 12:48:09 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

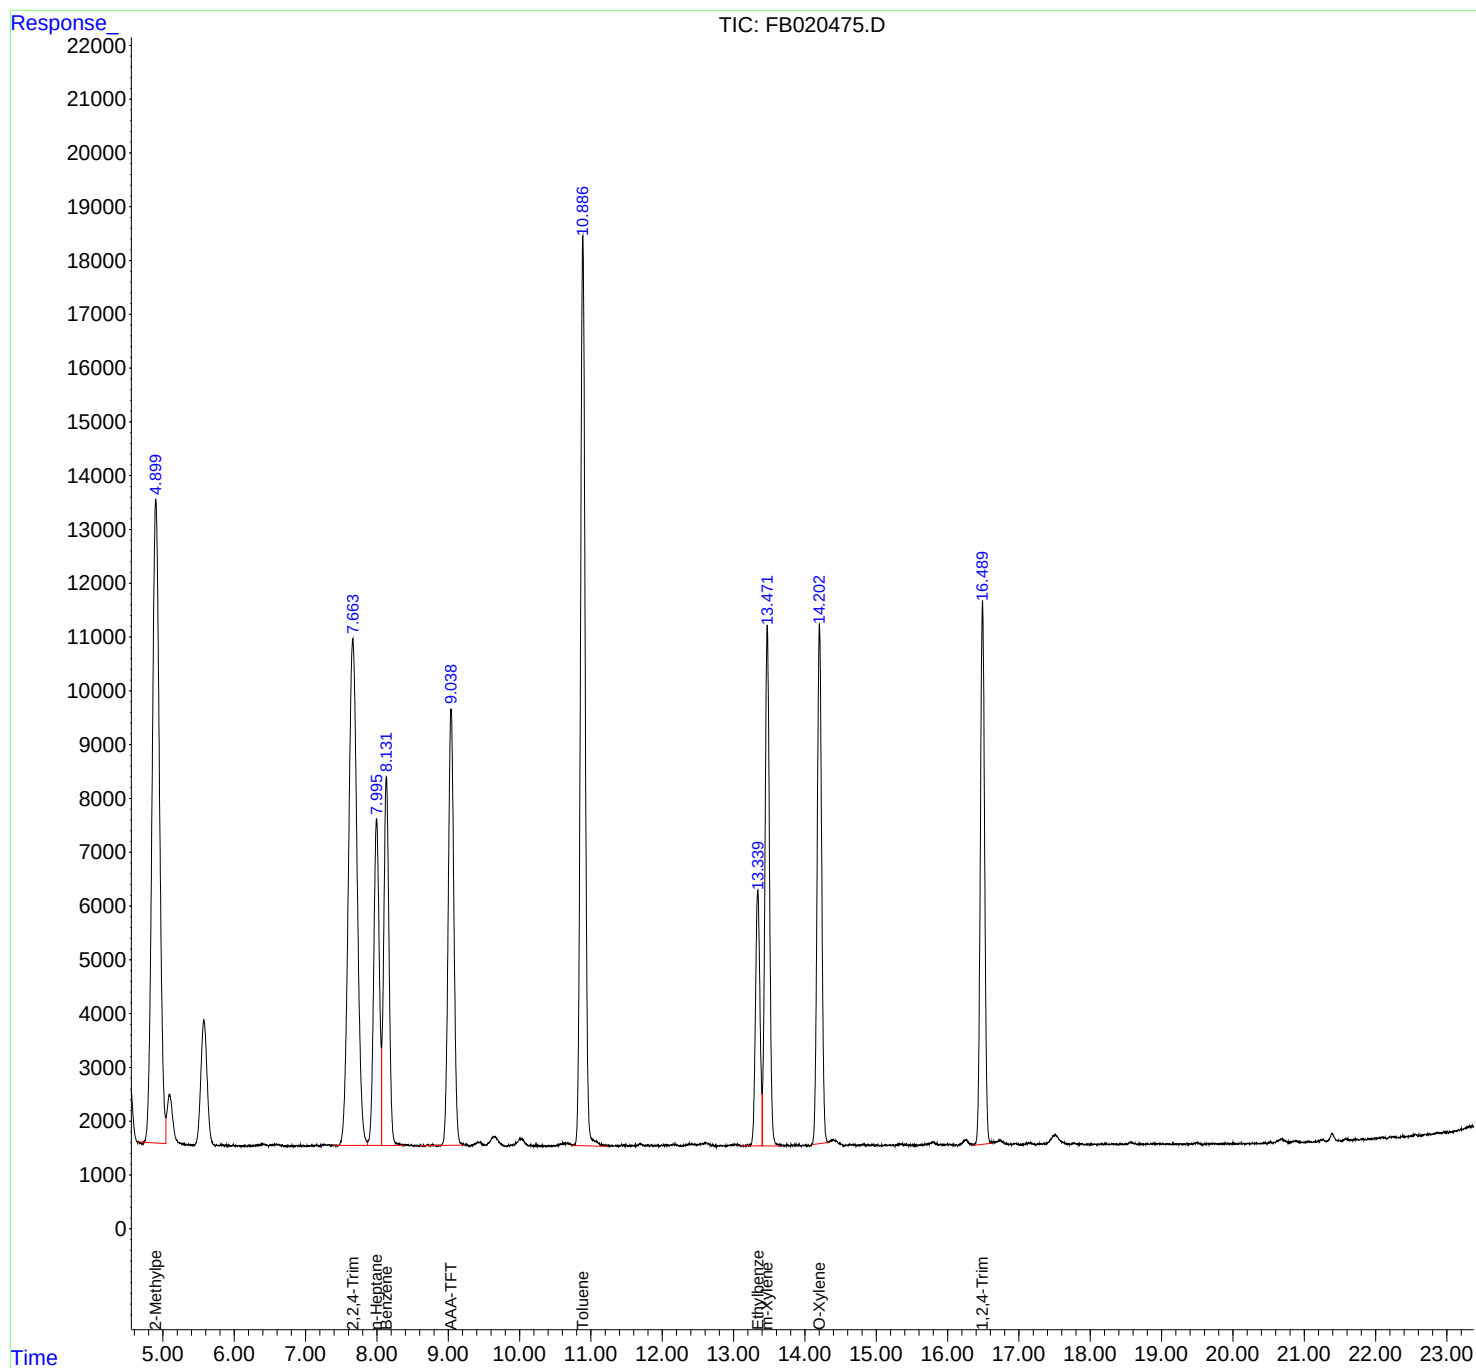


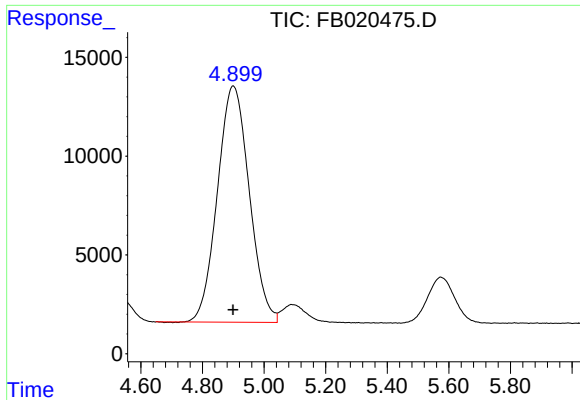

#1 2-Methylpentane


R.T.: 4.900 min
Delta R.T.: 0.001 min
Response: 859217
Conc: 31.00 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0401S1

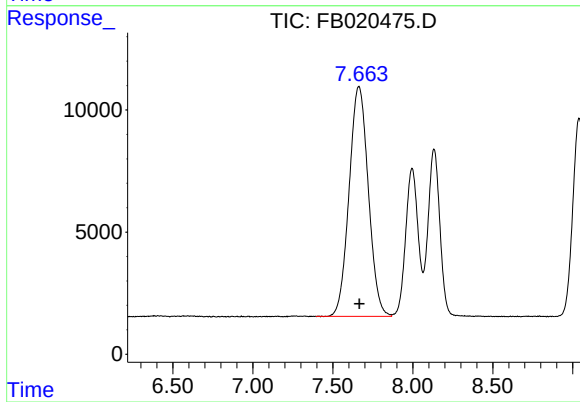


#2 2,2,4-Trimethylpentane

R.T.: 7.662 min
Delta R.T.: -0.004 min
Response: 786778
Conc: 32.81 ng/ml

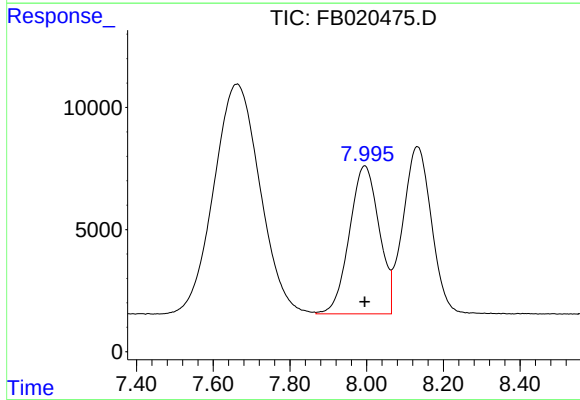


#3 n-Heptane

R.T.: 7.996 min
Delta R.T.: 0.000 min
Response: 327403
Conc: 10.01 ng/ml

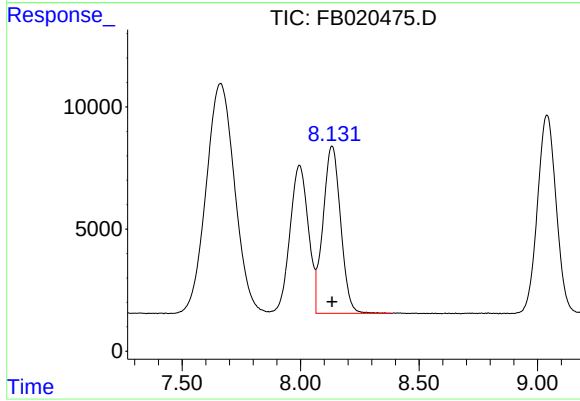

#4 Benzene


R.T.: 8.133 min
Delta R.T.: 0.000 min
Response: 353762
Conc: 10.21 ng/ml

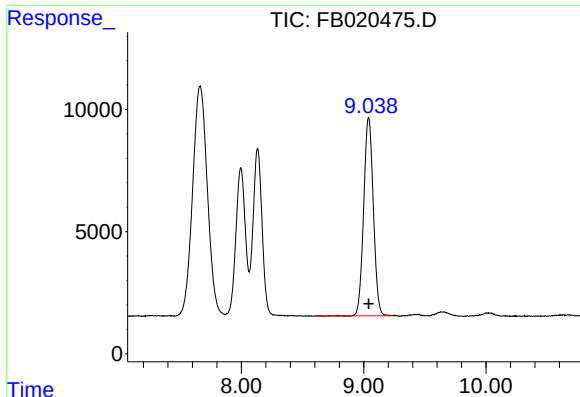

#5 AAA-TFT


R.T.: 9.040 min
Delta R.T.: 0.000 min
Response: 444231
Conc: 23.06 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0401S1

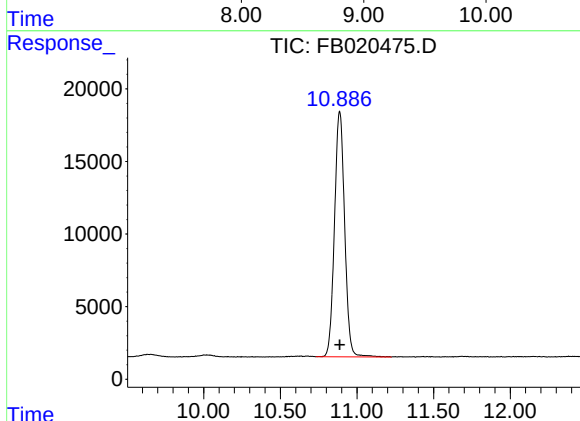


#6 Toluene

R.T.: 10.887 min
Delta R.T.: 0.000 min
Response: 779404
Conc: 30.05 ng/ml

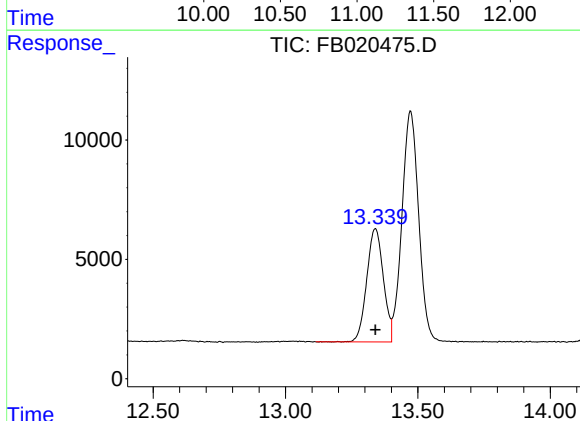


#7 Ethylbenzene

R.T.: 13.340 min
Delta R.T.: 0.000 min
Response: 206330
Conc: 10.48 ng/ml

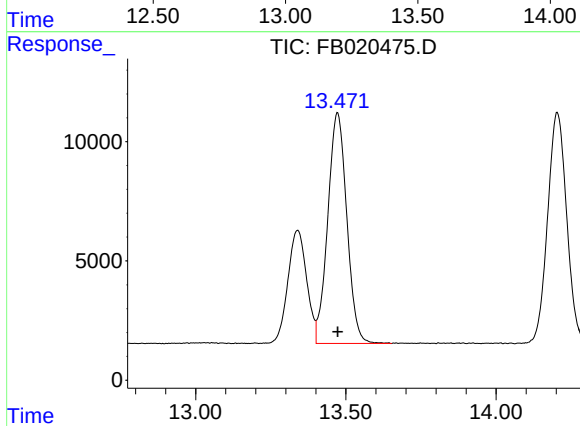

#8 m-Xylene


R.T.: 13.473 min
Delta R.T.: 0.000 min
Response: 426289
Conc: 21.00 ng/ml

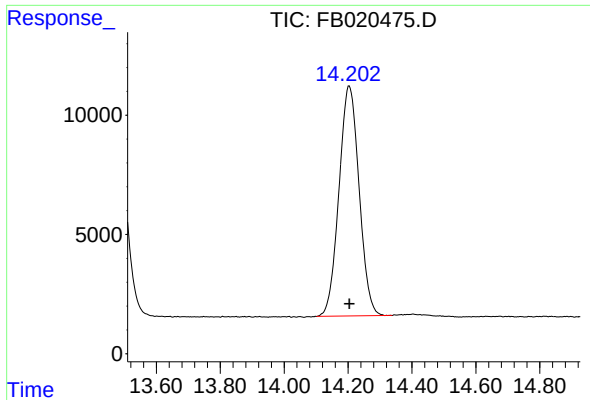

#9 O-Xylene

R.T.: 14.204 min
Delta R.T.: 0.000 min
Response: 421793
Conc: 20.83 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0401S1

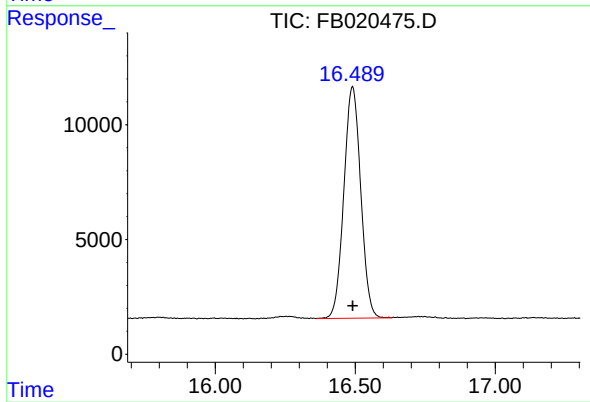

#10 1,2,4-Trimethylbenzene

R.T.: 16.491 min
Delta R.T.: 0.000 min
Response: 422954
Conc: 20.33 ng/ml