

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040119\
 Data File : FB020490.D
 Signal(s) : FID2B.CH
 Acq On : 1 Apr 2019 21:05
 Operator : MJ/SJ
 Sample : K2185-02MSD
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 18 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 P-4-OW(0-10)MSD

Integration File: Calibration.e
 Quant Time: Apr 02 01:45:19 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
 Quant Title :
 QLast Update : Tue Mar 26 12:48:09 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.039	352837	18.314 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.901	625997	22.585 ng/ml
2) t 2,2,4-Trimethylpentane	7.660	454843	18.968 ng/ml
3) t n-Heptane	7.995	182012	5.567 ng/ml
4) t Benzene	8.132	309643	8.941 ng/ml
6) t Toluene	10.885	635206	24.490 ng/ml
7) t Ethylbenzene	13.338	158690	8.061 ng/ml
8) t m-Xylene	13.471	322608	15.890 ng/ml
9) t O-Xylene	14.203	326237	16.108 ng/ml
10) t 1,2,4-Trimethylbenzene	16.489	299222	14.382 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040119\
Data File : FB020490.D
Signal(s) : FID2B.CH
Acq On : 1 Apr 2019 21:05
Operator : MJ/SJ
Sample : K2185-02MSD
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 18 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
P-4-OW(0-10)MSD

Integration File: Calibration.e
Quant Time: Apr 02 01:45:19 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
Quant Title :
QLast Update : Tue Mar 26 12:48:09 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

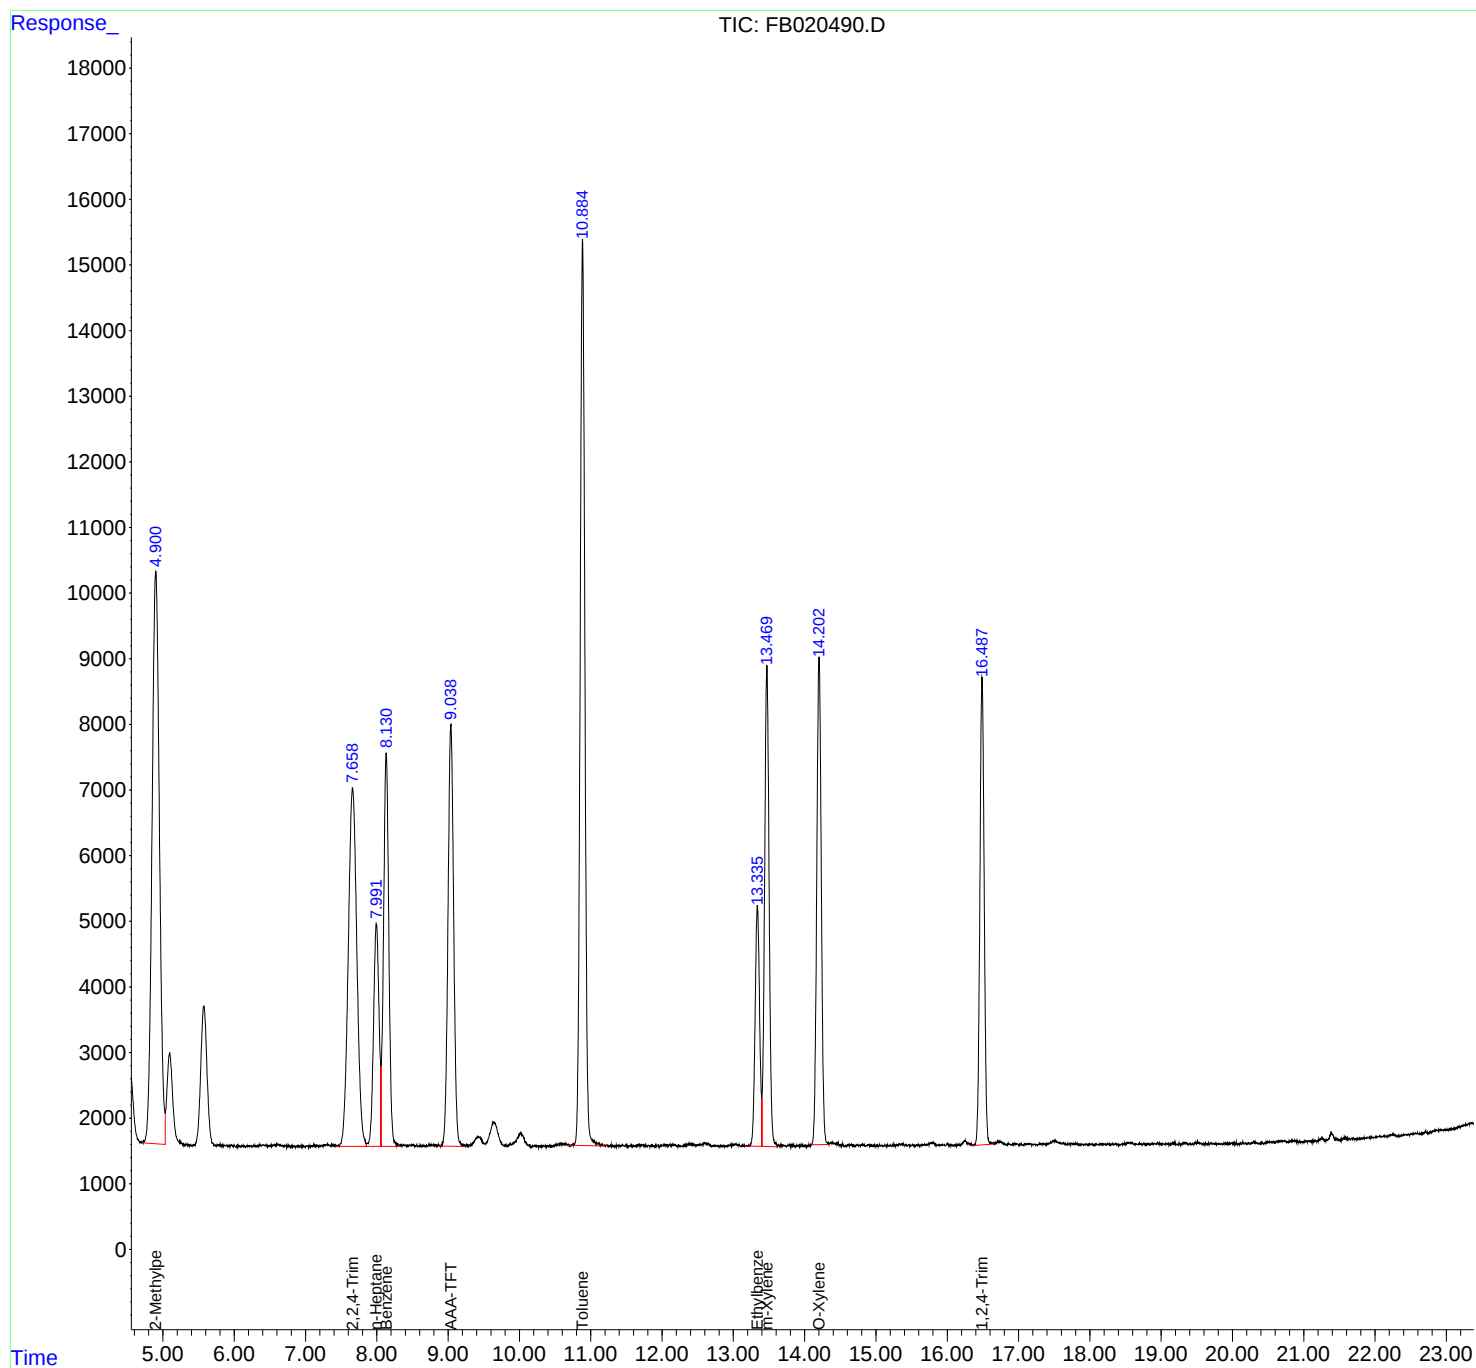


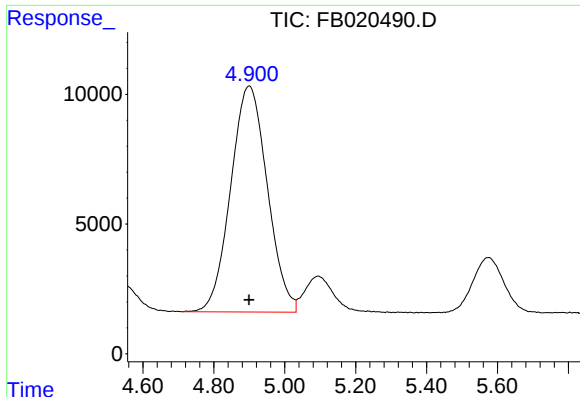

#1 2-Methylpentane


R.T.: 4.901 min
Delta R.T.: 0.002 min
Response: 625997
Conc: 22.58 ng/ml

Instrument :
FID_B
ClientSampleId :
P-4-OW(0-10)MSD

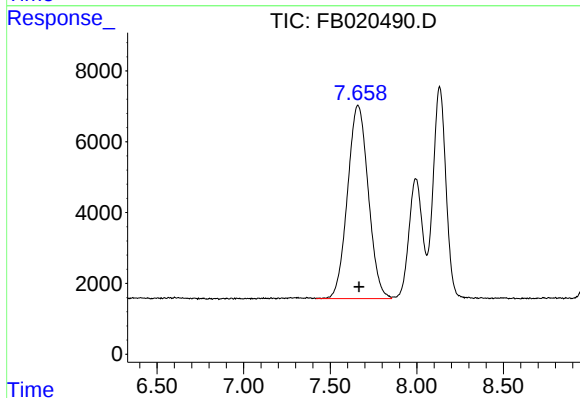


#2 2,2,4-Trimethylpentane

R.T.: 7.660 min
Delta R.T.: -0.006 min
Response: 454843
Conc: 18.97 ng/ml

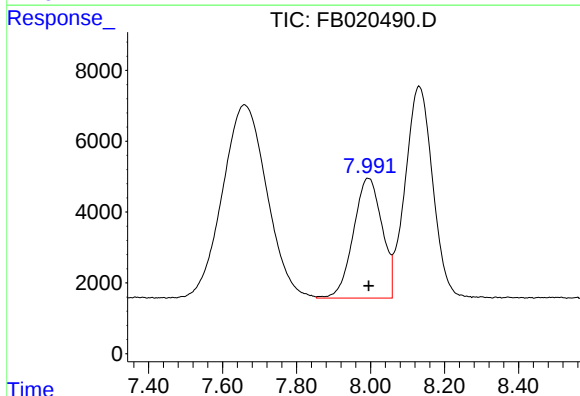


#3 n-Heptane

R.T.: 7.995 min
Delta R.T.: 0.000 min
Response: 182012
Conc: 5.57 ng/ml

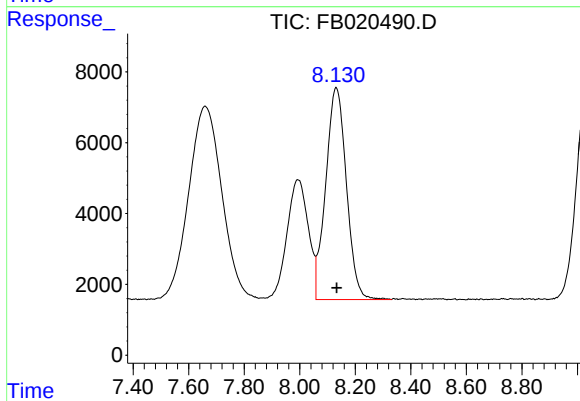

#4 Benzene


R.T.: 8.132 min
Delta R.T.: -0.001 min
Response: 309643
Conc: 8.94 ng/ml

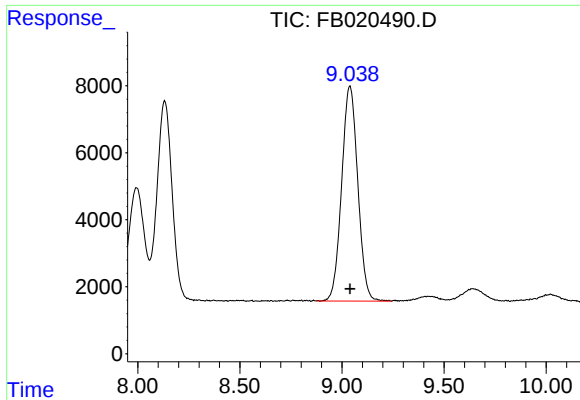

#5 AAA-TFT


R.T.: 9.039 min
Delta R.T.: -0.001 min
Response: 352837
Conc: 18.31 ng/ml

Instrument :
FID_B
ClientSampleId :
P-4-OW(0-10)MSD

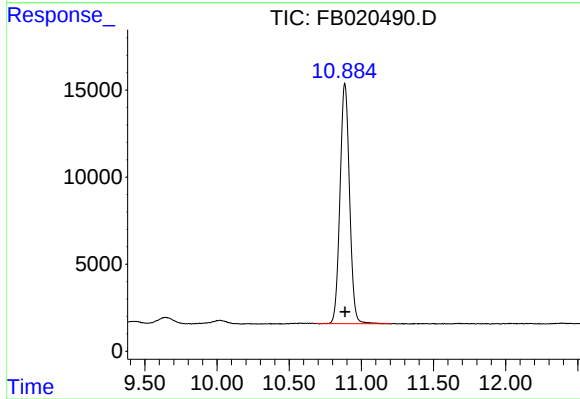


#6 Toluene

R.T.: 10.885 min
Delta R.T.: -0.002 min
Response: 635206
Conc: 24.49 ng/ml

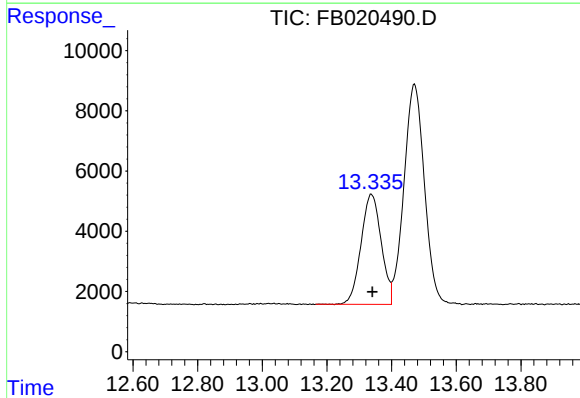


#7 Ethylbenzene

R.T.: 13.338 min
Delta R.T.: -0.002 min
Response: 158690
Conc: 8.06 ng/ml

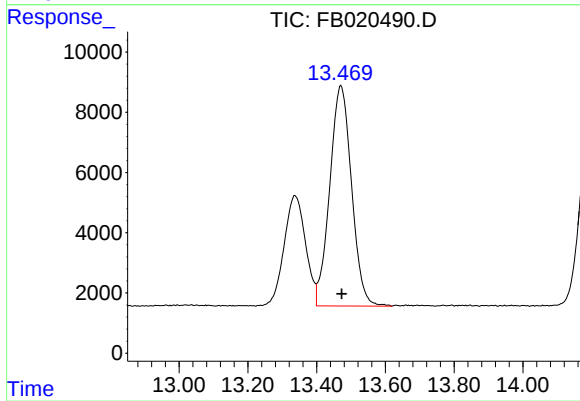

#8 m-Xylene


R.T.: 13.471 min
Delta R.T.: -0.002 min
Response: 322608
Conc: 15.89 ng/ml

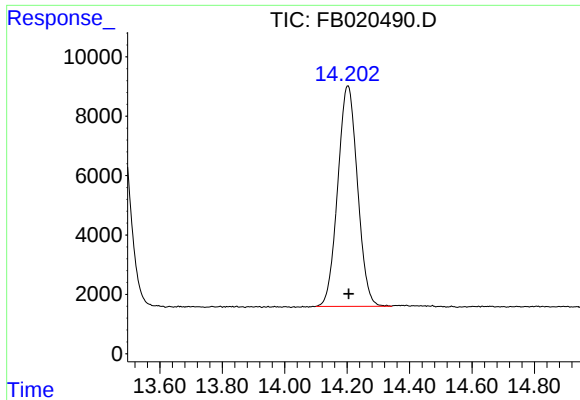

#9 O-Xylene

R.T.: 14.203 min
Delta R.T.: -0.002 min
Response: 326237
Conc: 16.11 ng/ml

Instrument :
FID_B
ClientSampleId :
P-4-OW(0-10)MSD

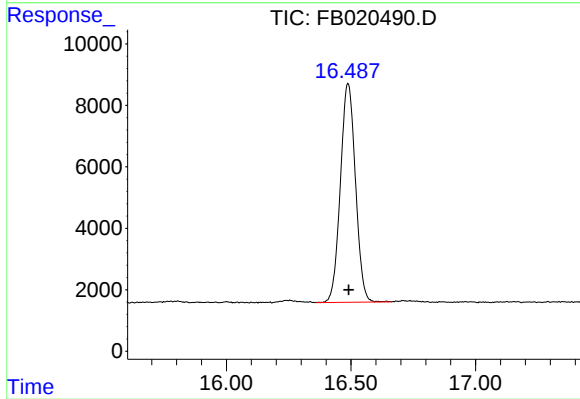

#10 1,2,4-Trimethylbenzene

R.T.: 16.489 min
Delta R.T.: -0.003 min
Response: 299222
Conc: 14.38 ng/ml