

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040119\
 Data File : FB020489.D
 Signal(s) : FID2B.CH
 Acq On : 1 Apr 2019 20:35
 Operator : MJ/SJ
 Sample : K2185-02MS
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 17 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 P-4-OW(0-10)MS

Integration File: Calibration.e
 Quant Time: Apr 02 01:45:07 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
 Quant Title :
 QLast Update : Tue Mar 26 12:48:09 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.039	380195	19.734 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.900	604689	21.816 ng/ml
2) t 2,2,4-Trimethylpentane	7.661	474792	19.800 ng/ml
3) t n-Heptane	7.995	190071	5.814 ng/ml
4) t Benzene	8.132	289789	8.368 ng/ml
6) t Toluene	10.886	609725	23.508 ng/ml
7) t Ethylbenzene	13.338	151957	7.719 ng/ml
8) t m-Xylene	13.472	309178	15.228 ng/ml
9) t O-Xylene	14.203	309756	15.294 ng/ml
10) t 1,2,4-Trimethylbenzene	16.489	289785	13.928 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040119\
Data File : FB020489.D
Signal(s) : FID2B.CH
Acq On : 1 Apr 2019 20:35
Operator : MJ/SJ
Sample : K2185-02MS
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 17 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
P-4-OW(0-10)MS

Integration File: Calibration.e
Quant Time: Apr 02 01:45:07 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
Quant Title :
QLast Update : Tue Mar 26 12:48:09 2019
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

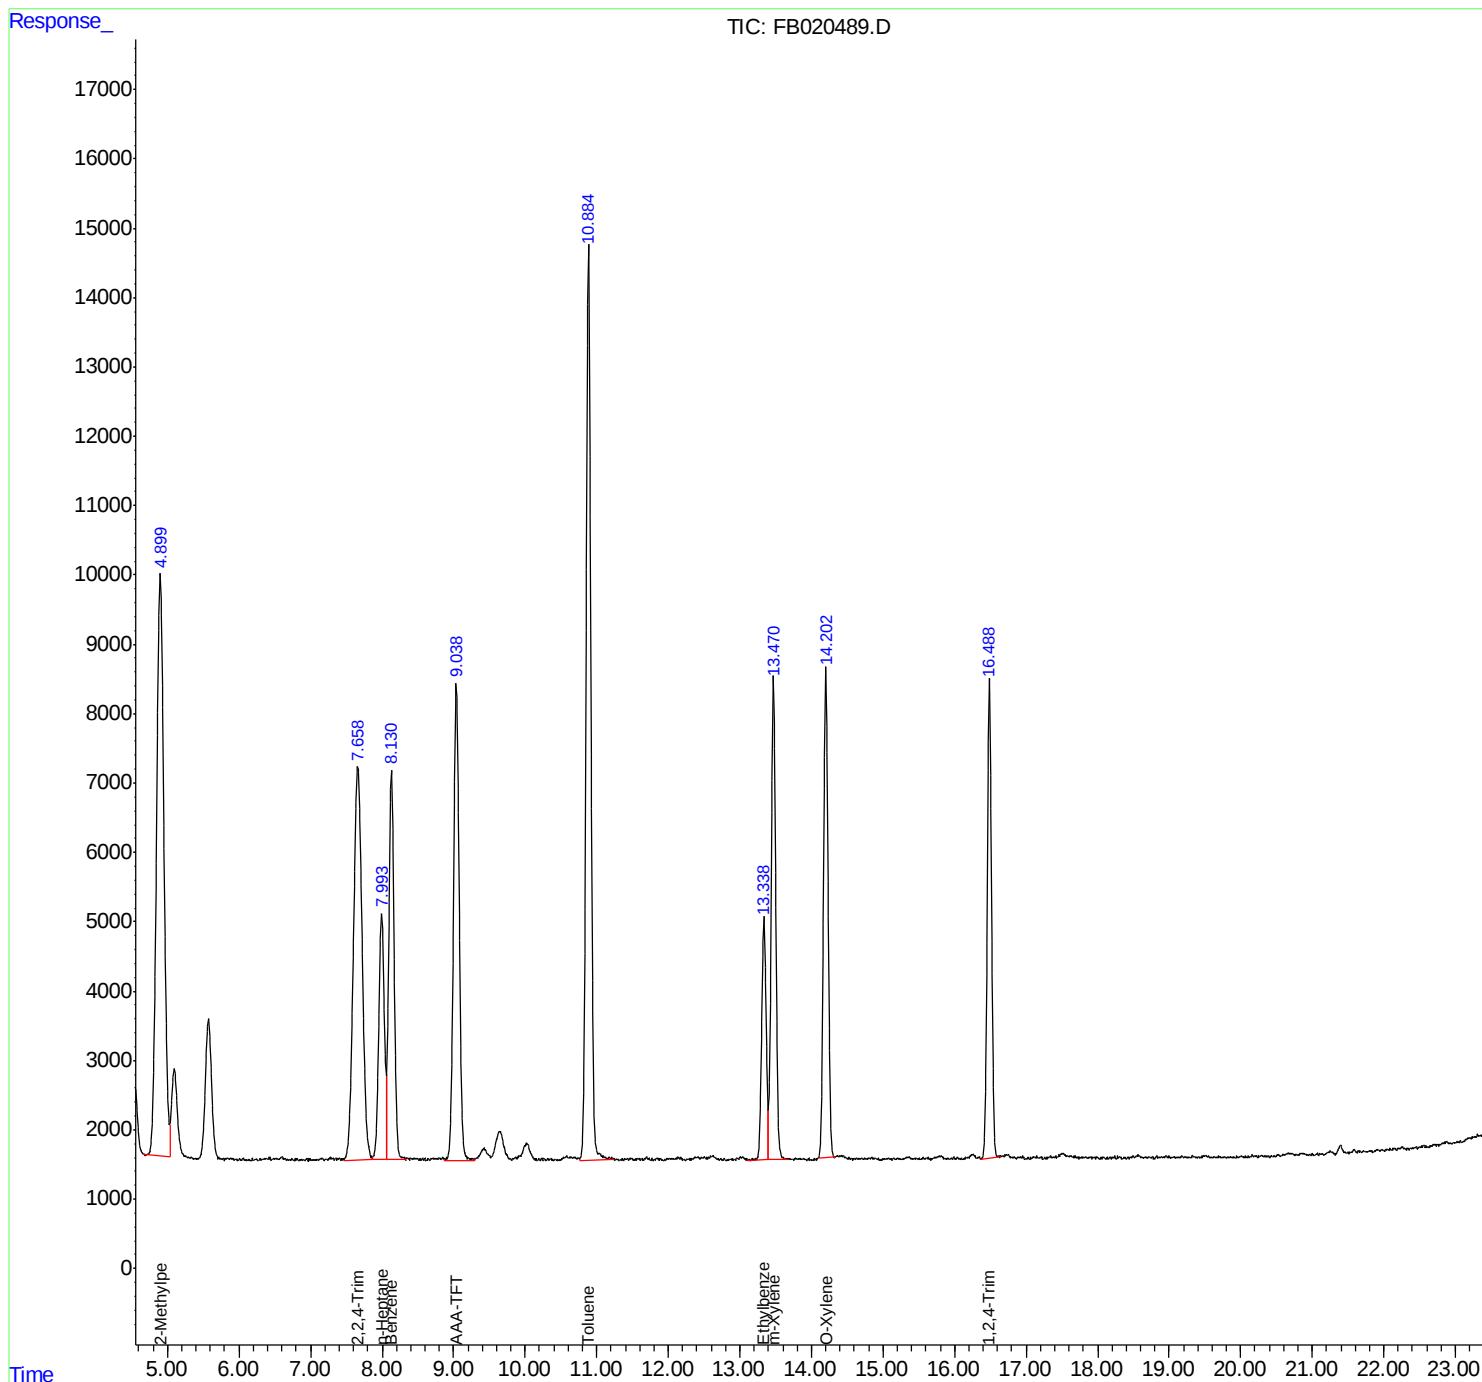


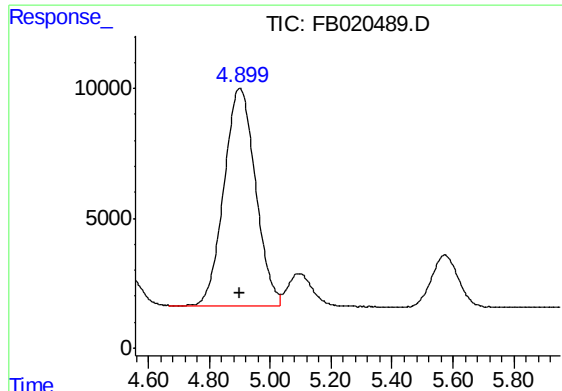

#1 2-Methylpentane


R.T.: 4.900 min
Delta R.T.: 0.001 min
Response: 604689
Conc: 21.82 ng/ml

Instrument :
FID_B
ClientSampleId :
P-4-OW(0-10)MS

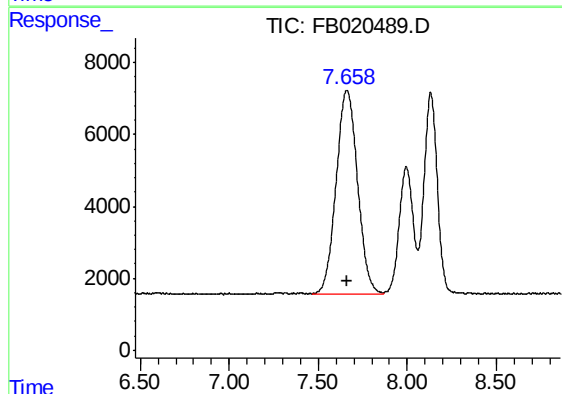


#2 2,2,4-Trimethylpentane

R.T.: 7.661 min
Delta R.T.: -0.005 min
Response: 474792
Conc: 19.80 ng/ml

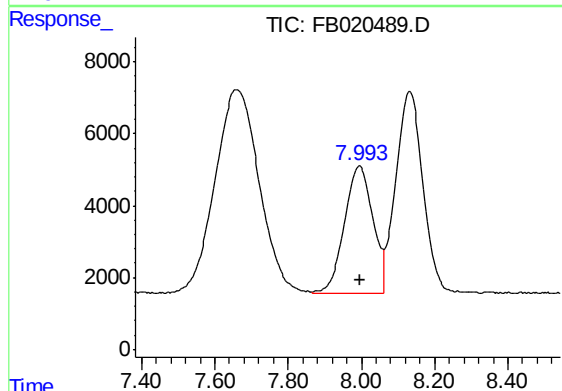


#3 n-Heptane

R.T.: 7.995 min
Delta R.T.: 0.000 min
Response: 190071
Conc: 5.81 ng/ml

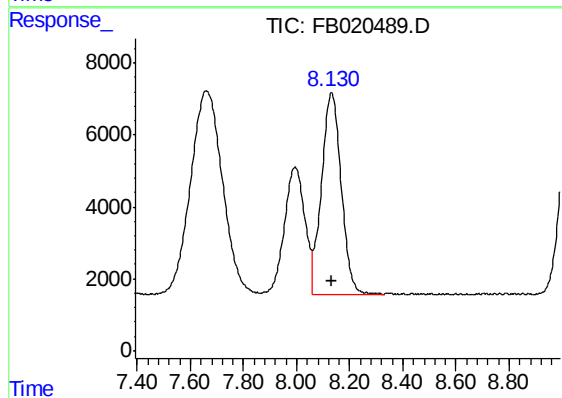

#4 Benzene


R.T.: 8.132 min
Delta R.T.: -0.001 min
Response: 289789
Conc: 8.37 ng/ml

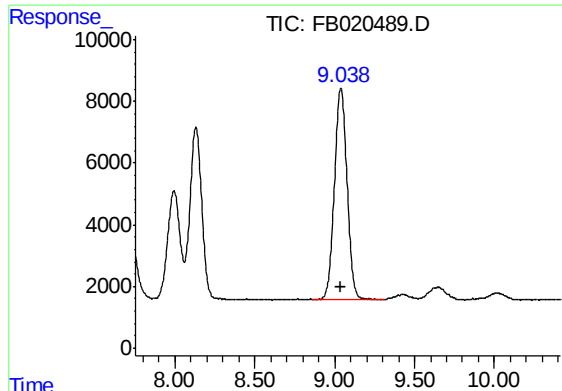

#5 AAA-TFT


R.T.: 9.039 min
Delta R.T.: 0.000 min
Response: 380195
Conc: 19.73 ng/ml

Instrument :
FID_B
ClientSampleId :
P-4-OW(0-10)MS

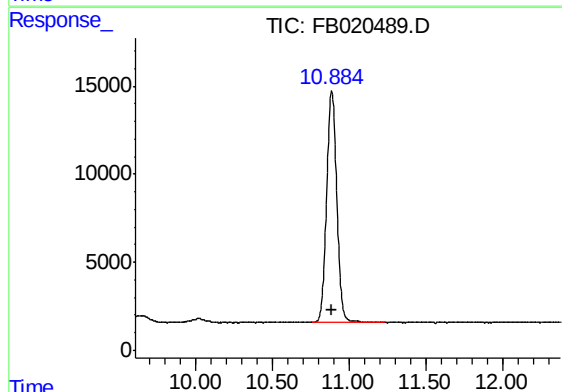


#6 Toluene

R.T.: 10.886 min
Delta R.T.: -0.002 min
Response: 609725
Conc: 23.51 ng/ml

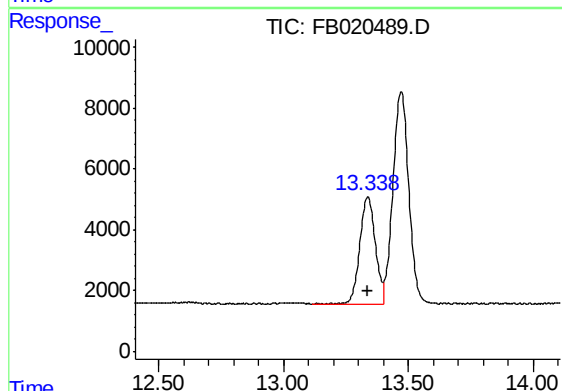


#7 Ethylbenzene

R.T.: 13.338 min
Delta R.T.: -0.002 min
Response: 151957
Conc: 7.72 ng/ml

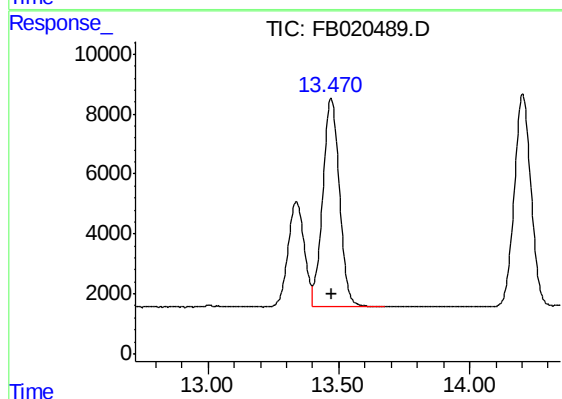

#8 m-Xylene


R.T.: 13.472 min
Delta R.T.: -0.002 min
Response: 309178
Conc: 15.23 ng/ml

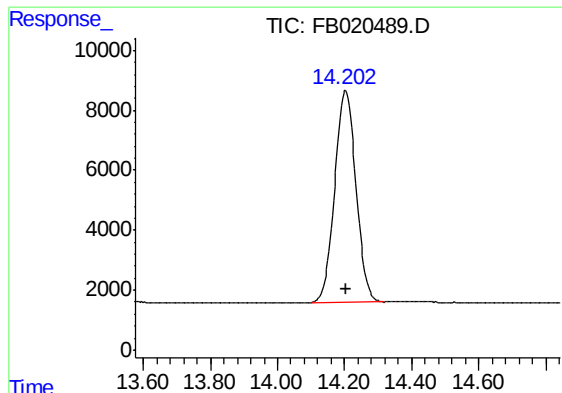

#9 O-Xylene

R.T.: 14.203 min
Delta R.T.: -0.001 min
Response: 309756
Conc: 15.29 ng/ml

Instrument :
FID_B
ClientSampleId :
P-4-OW(0-10)MS

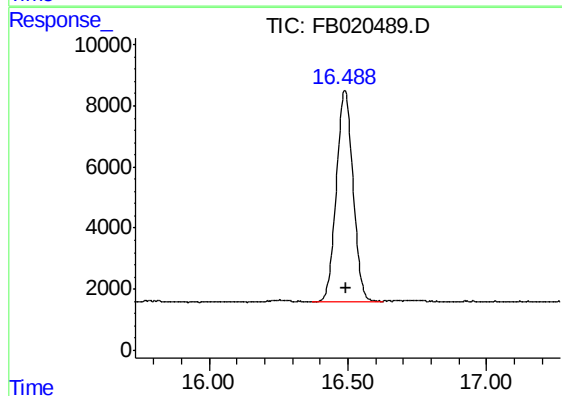

#10 1,2,4-Trimethylbenzene

R.T.: 16.489 min
Delta R.T.: -0.002 min
Response: 289785
Conc: 13.93 ng/ml