

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040219\
 Data File : FB020503.D
 Signal(s) : FID2B.CH
 Acq On : 2 Apr 2019 9:40
 Operator : MJ/SJ
 Sample : BSF0402S1
 Misc : 5.01g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 03 00:51:57 2019
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
 Quant Title :
 QLast Update : Tue Mar 26 12:48:09 2019
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	9.038	434382	22.546 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.899	836833	30.191 ng/ml
2) t 2,2,4-Trimethylpentane	7.662	783936	32.692 ng/ml
3) t n-Heptane	7.994	334331	10.226 ng/ml
4) t Benzene	8.131	357467	10.322 ng/ml
6) t Toluene	10.885	790867	30.492 ng/ml
7) t Ethylbenzene	13.338	207839	10.557 ng/ml
8) t m-Xylene	13.471	426709	21.017 ng/ml
9) t O-Xylene	14.203	422101	20.841 ng/ml
10) t 1,2,4-Trimethylbenzene	16.489	429224	20.630 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040219\
Data File : FB020503.D
Signal(s) : FID2B.CH
Acq On : 2 Apr 2019 9:40
Operator : MJ/SJ
Sample : BSF0402S1
Misc : 5.01g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 03 00:51:57 2019
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032619.M
Quant Title :
QLast Update : Tue Mar 26 12:48:09 2019
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

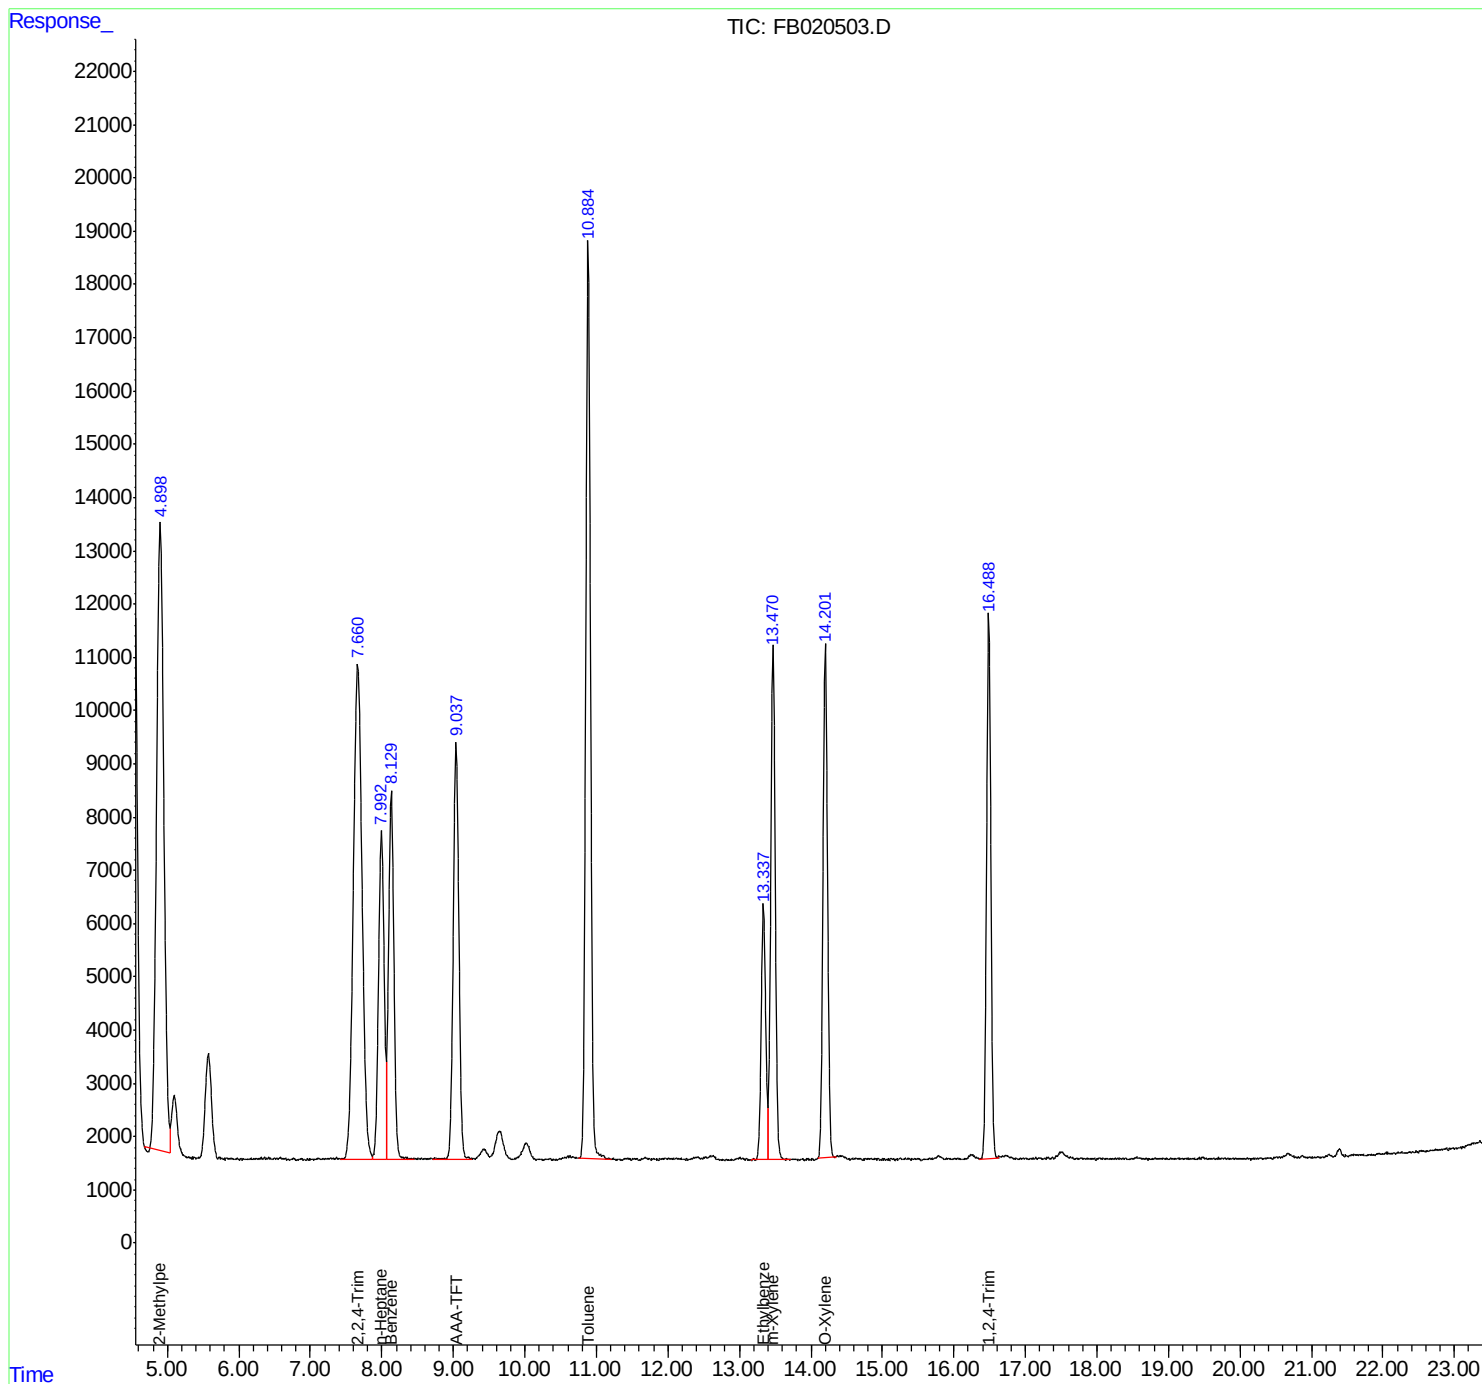

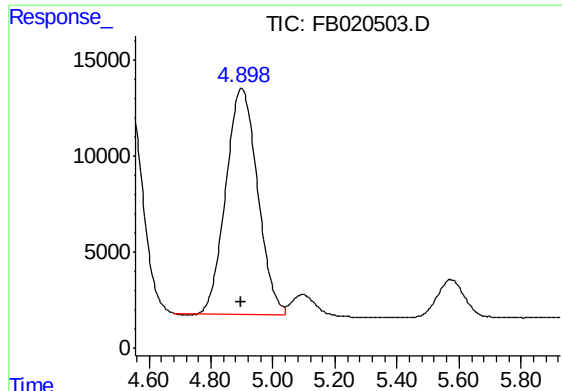


#1 2-Methylpentane

R.T.: 4.899 min
Delta R.T.: 0.000 min
Response: 836833
Conc: 30.19 ng/ml

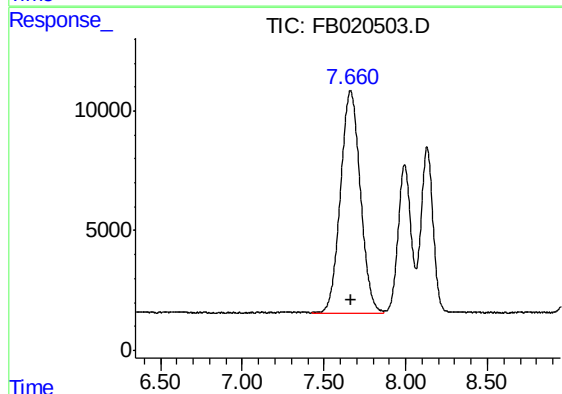


#2 2,2,4-Trimethylpentane

R.T.: 7.662 min
Delta R.T.: -0.004 min
Response: 783936
Conc: 32.69 ng/ml

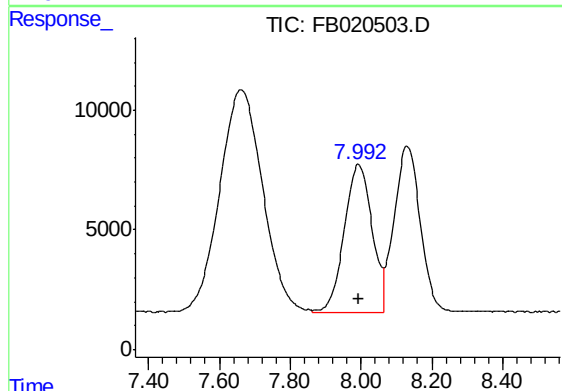


#3 n-Heptane

R.T.: 7.994 min
Delta R.T.: -0.001 min
Response: 334331
Conc: 10.23 ng/ml

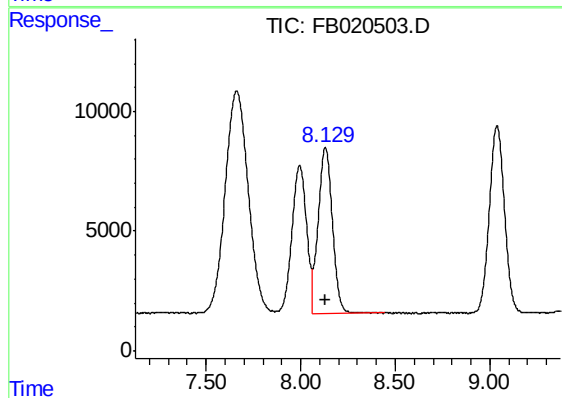


#4 Benzene

R.T.: 8.131 min
Delta R.T.: -0.002 min
Response: 357467
Conc: 10.32 ng/ml

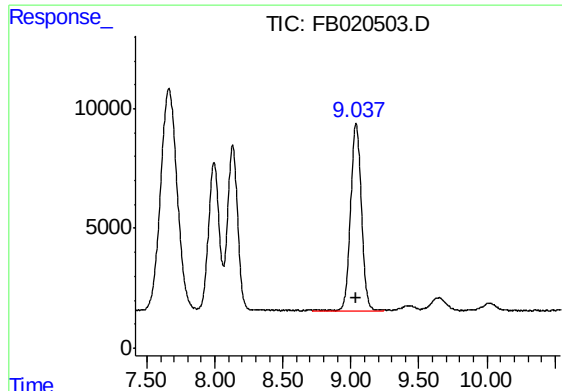


#5 AAA-TFT

R.T.: 9.038 min
Delta R.T.: -0.002 min
Response: 434382
Conc: 22.55 ng/ml

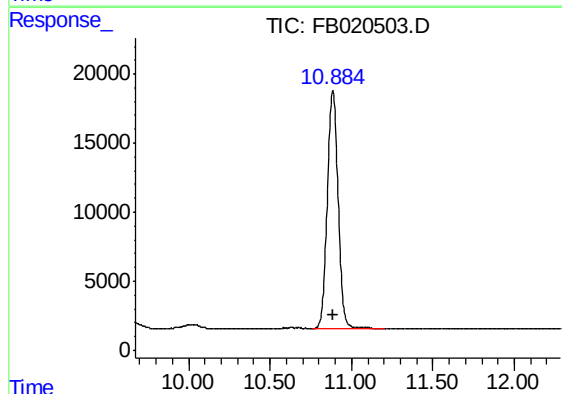


#6 Toluene

R.T.: 10.885 min
Delta R.T.: -0.002 min
Response: 790867
Conc: 30.49 ng/ml

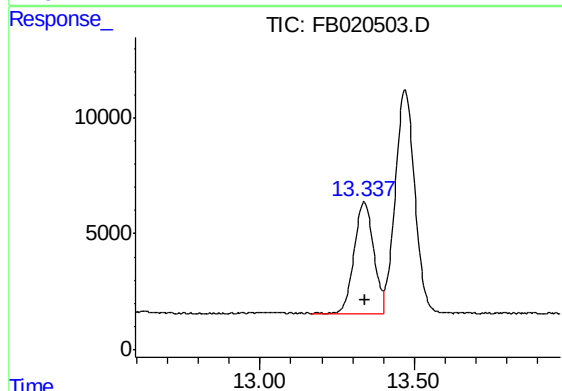


#7 Ethylbenzene

R.T.: 13.338 min
Delta R.T.: -0.002 min
Response: 207839
Conc: 10.56 ng/ml

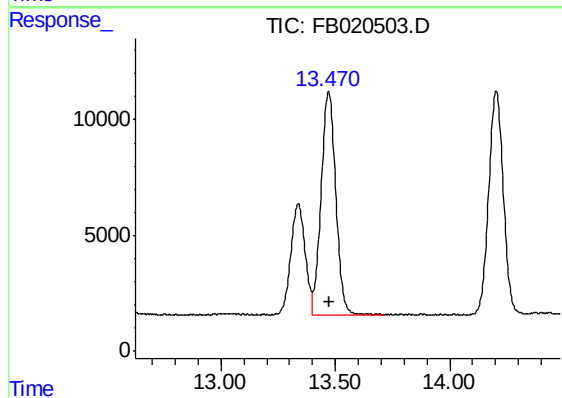


#8 m-Xylene

R.T.: 13.471 min
Delta R.T.: -0.002 min
Response: 426709
Conc: 21.02 ng/ml

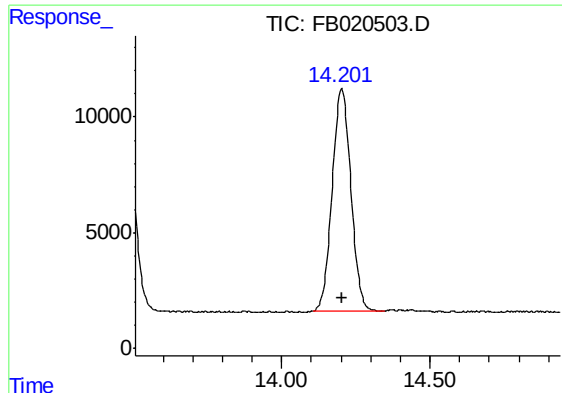

#9 O-Xylene

R.T.: 14.203 min
Delta R.T.: -0.002 min
Response: 422101
Conc: 20.84 ng/ml

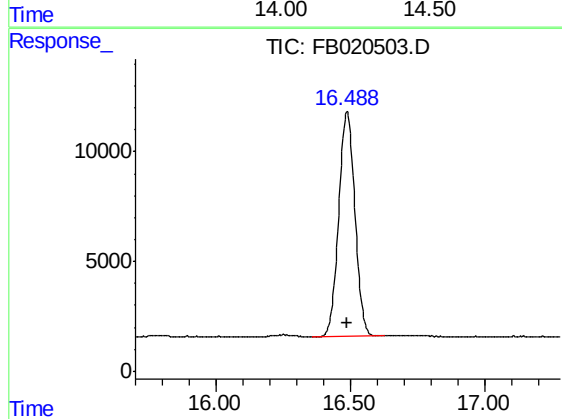

#10 1,2,4-Trimethylbenzene

R.T.: 16.489 min
Delta R.T.: -0.002 min
Response: 429224
Conc: 20.63 ng/ml