

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040220\
 Data File : FB024053.D
 Signal(s) : FID2B.CH
 Acq On : 2 Apr 2020 16:20
 Operator : DD/AJ
 Sample : L1758-02
 Misc : 5.00g/5.00ml DI WATER
 ALS Vial : 7 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :

Integration File: Calibration.e
 Quant Time: Apr 02 18:35:06 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032620.M
 Quant Title :
 QLast Update : Fri Mar 27 11:16:49 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.801	412938	18.079 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.689	2194	0.063 ng/ml
2) t 2,2,4-Trimethylpentane	7.419	648	0.018 ng/ml
3) t n-Heptane	7.765	1926	0.053 ng/ml
6) t Toluene	10.628	6929	0.157 ng/ml
7) t Ethylbenzene	13.058	50962	1.279 ng/ml
8) t m-Xylene	13.202	40761	1.060 ng/ml
9) t O-Xylene	13.934	96209	2.603 ng/ml
10) t 1,2,4-Trimethylbenzene	16.214	583186	18.352 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040220\
Data File : FB024053.D
Signal(s) : FID2B.CH
Acq On : 2 Apr 2020 16:20
Operator : DD/AJ
Sample : L1758-02
Misc : 5.00g/5.00ml DI WATER
ALS Vial : 7 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :

Integration File: Calibration.e
Quant Time: Apr 02 18:35:06 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032620.M
Quant Title :
QLast Update : Fri Mar 27 11:16:49 2020
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

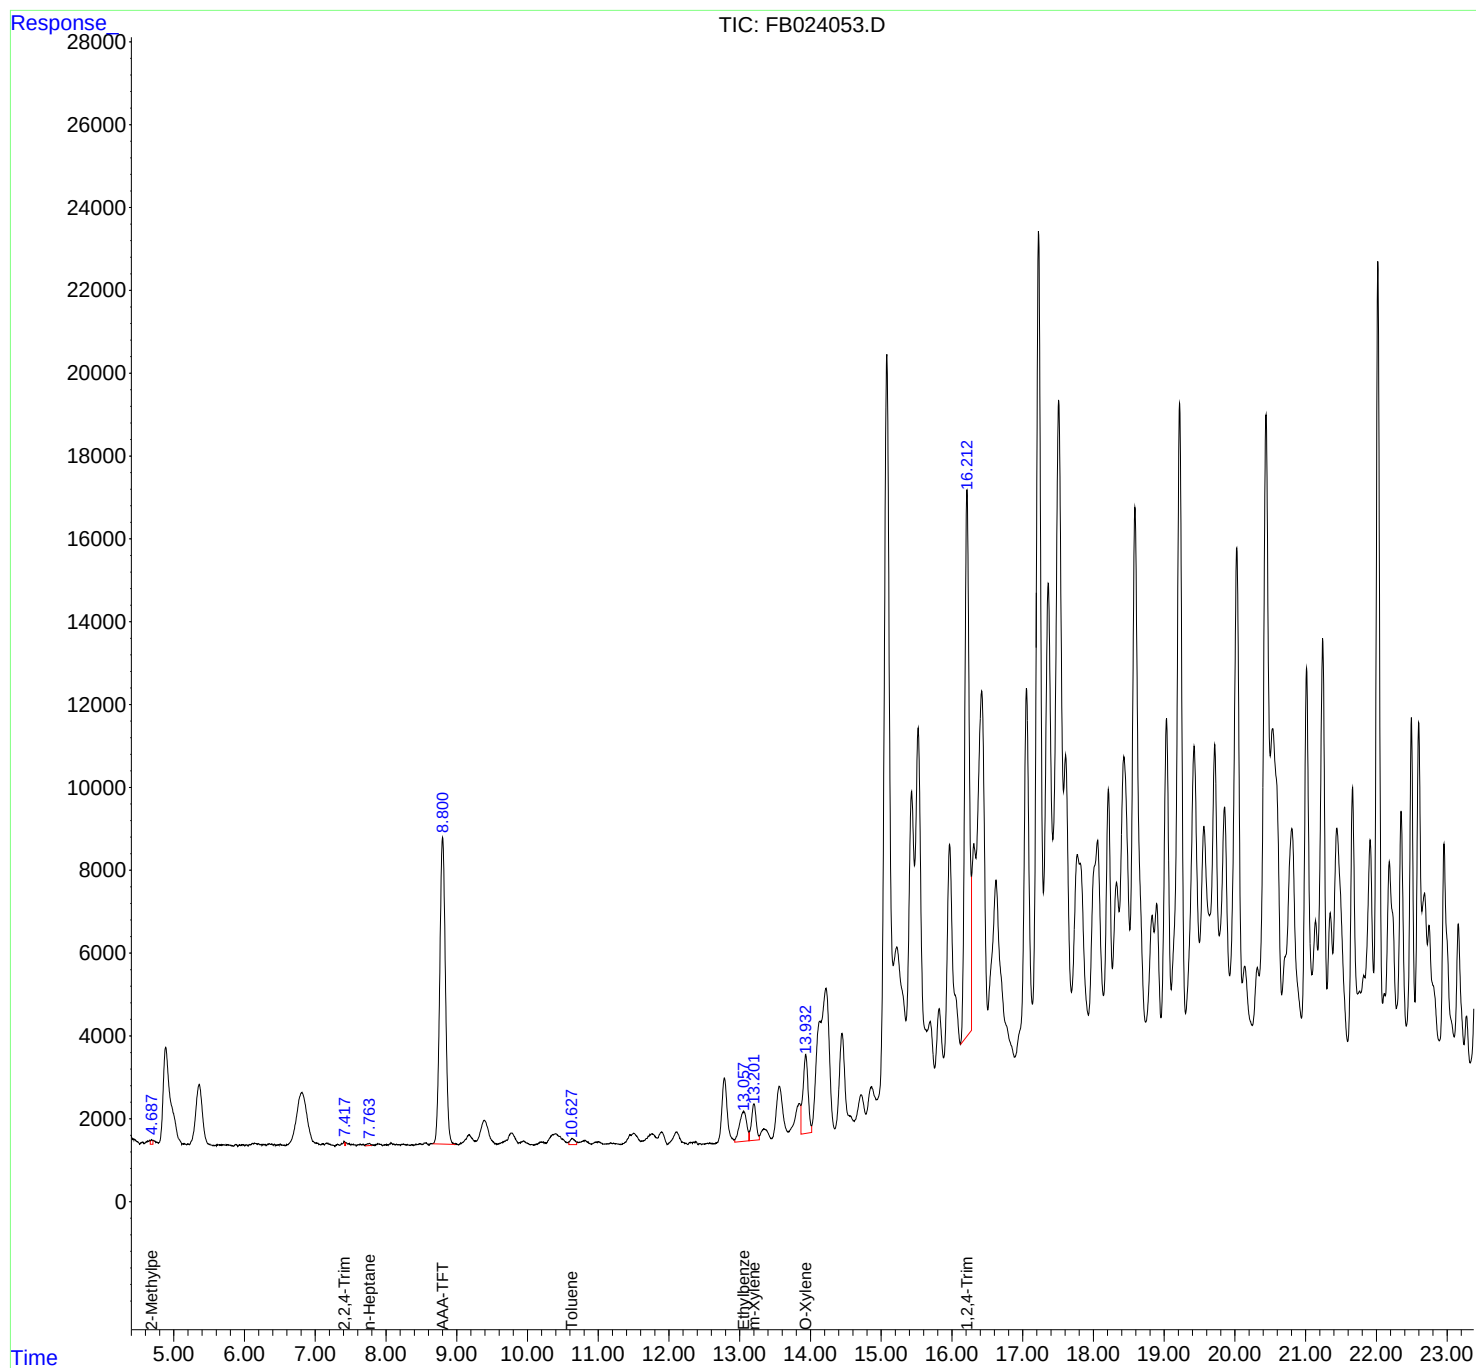


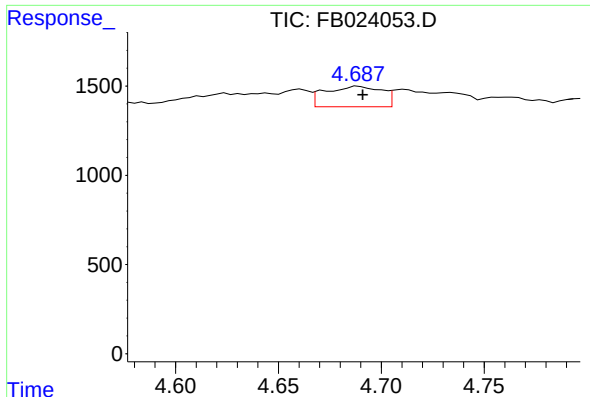

#1 2-Methylpentane


R.T.: 4.689 min
Delta R.T.: -0.002 min
Response: 2194
Conc: 0.06 ng/ml

Instrument :
FID_B
ClientSampleId :

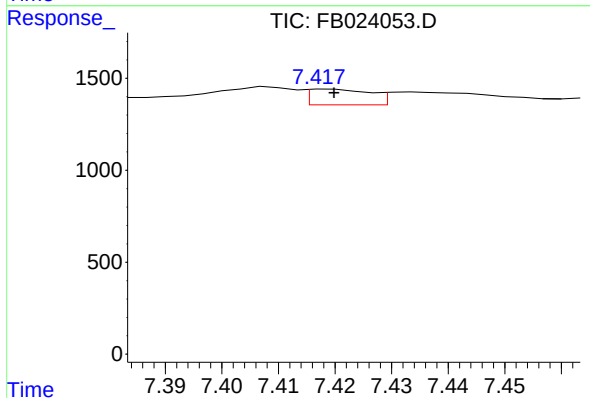


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.000 min
Response: 648
Conc: 0.02 ng/ml

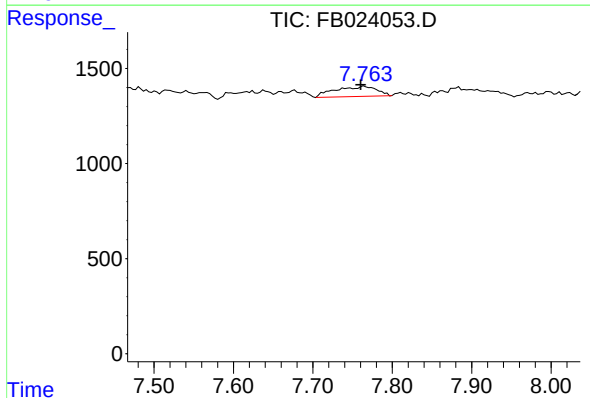


#3 n-Heptane

R.T.: 7.765 min
Delta R.T.: 0.004 min
Response: 1926
Conc: 0.05 ng/ml

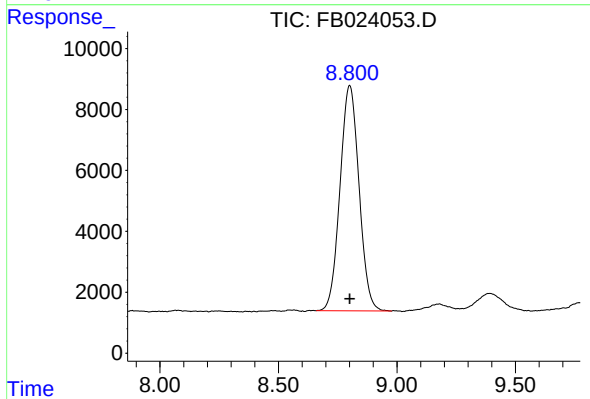

#5 AAA-TFT


R.T.: 8.801 min
Delta R.T.: 0.000 min
Response: 412938
Conc: 18.08 ng/ml

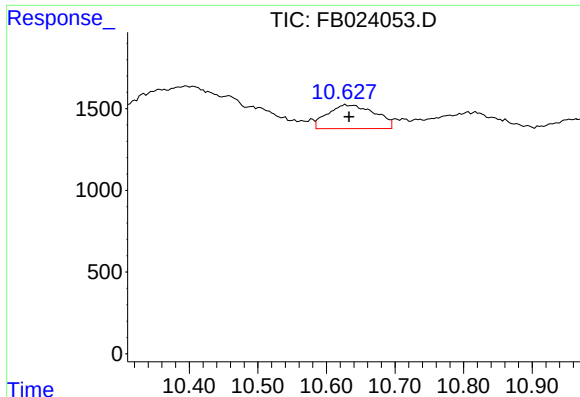

#6 Toluene


R.T.: 10.628 min
Delta R.T.: -0.005 min
Response: 6929
Conc: 0.16 ng/ml

Instrument :
FID_B
ClientSampleId :

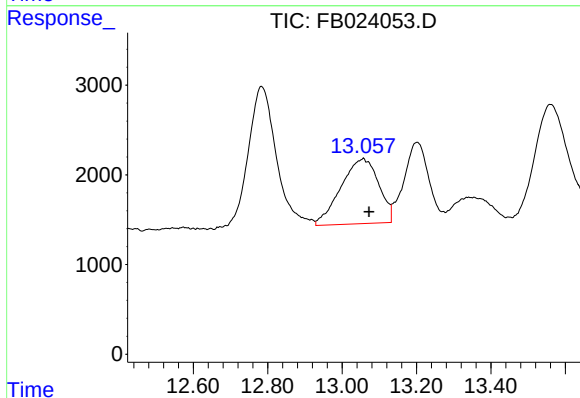


#7 Ethylbenzene

R.T.: 13.058 min
Delta R.T.: -0.015 min
Response: 50962
Conc: 1.28 ng/ml

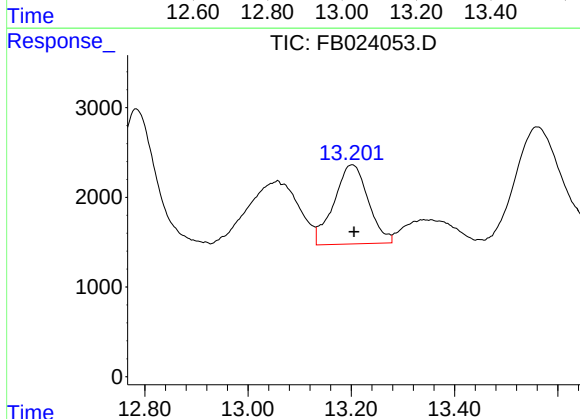


#8 m-Xylene

R.T.: 13.202 min
Delta R.T.: -0.003 min
Response: 40761
Conc: 1.06 ng/ml

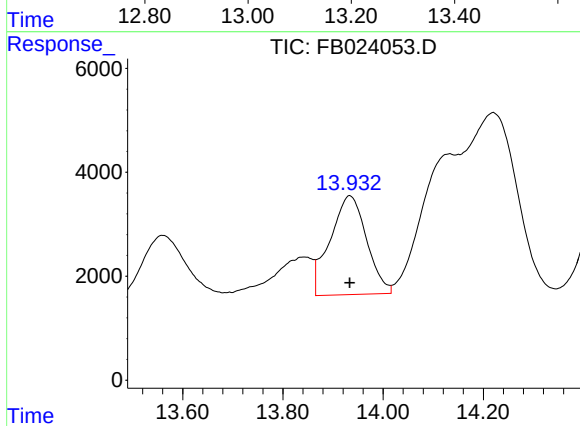

#9 O-Xylene

R.T.: 13.934 min
Delta R.T.: 0.000 min
Response: 96209
Conc: 2.60 ng/ml

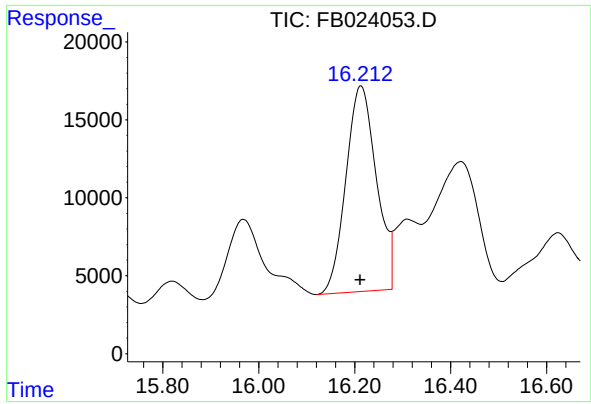

#10 1,2,4-Trimethylbenzene

R.T.: 16.214 min

Delta R.T.: 0.002 min

Response: 583186

Conc: 18.35 ng/ml

Instrument :
FID_B
ClientSampleId :