

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040320\
 Data File : FB024060.D
 Signal(s) : FID2B.CH
 Acq On : 3 Apr 2020 14:48
 Operator : DD/AJ
 Sample : BSF0403S1
 Misc : 5.02g/5.00ml DI WATER
 ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
 Quant Time: Apr 04 00:49:12 2020
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032620.M
 Quant Title :
 QLast Update : Fri Mar 27 11:16:49 2020
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound		R.T.	Response	Conc Units

System Monitoring Compounds				
5) s	AAA-TFT	8.800	410010	17.951 ng/ml
Target Compounds				
1) t	2-Methylpentane	4.690	910771	26.315 ng/ml
2) t	2,2,4-Trimethylpentane	7.419	1007115	27.442 ng/ml
3) t	n-Heptane	7.759	322391	8.938 ng/ml
4) t	Benzene	7.894	414936	9.355 ng/ml
6) t	Toluene	10.632	1224491	27.783 ng/ml
7) t	Ethylbenzene	13.073	386938	9.711 ng/ml
8) t	m-Xylene	13.205	762130	19.814 ng/ml
9) t	O-Xylene	13.933	737284	19.947 ng/ml
10) t	1,2,4-Trimethylbenzene	16.211	631159	19.862 ng/ml


(f)=RT Delta > 1/2 Window


(m)=manual int.

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040320\
Data File : FB024060.D
Signal(s) : FID2B.CH
Acq On : 3 Apr 2020 14:48
Operator : DD/AJ
Sample : BSF0403S1
Misc : 5.02g/5.00ml DI WATER
ALS Vial : 3 Sample Multiplier: 1

Integration File: Calibration.e
Quant Time: Apr 04 00:49:12 2020
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB032620.M
Quant Title :
QLast Update : Fri Mar 27 11:16:49 2020
Response via : Initial Calibration
Integrator: ChemStation


Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

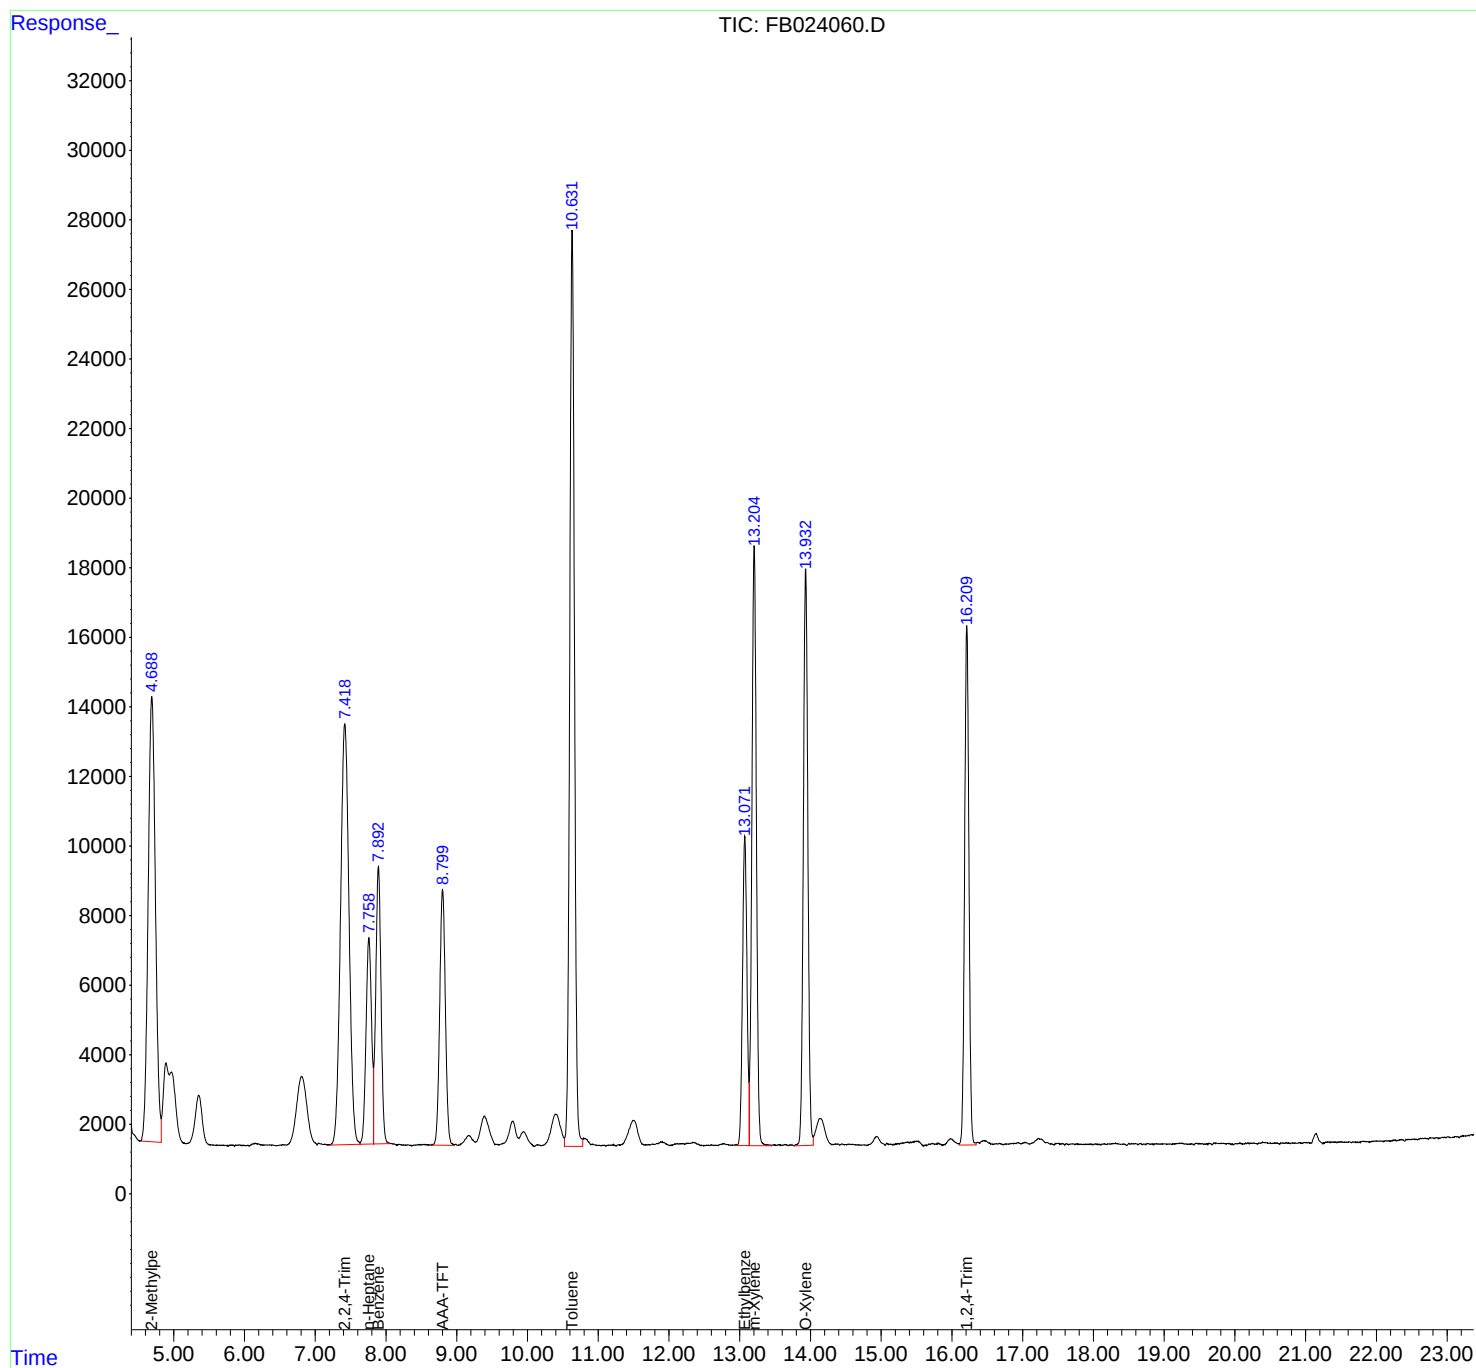

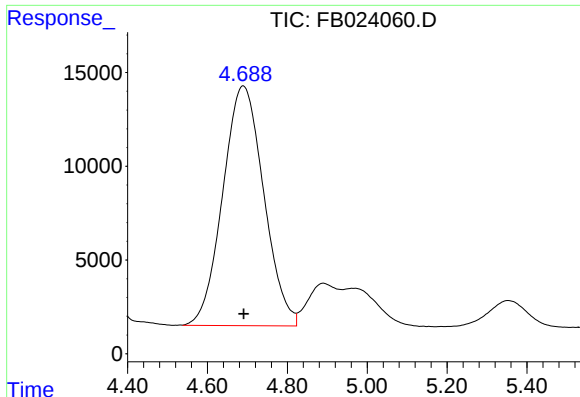


#1 2-Methylpentane

R.T.: 4.690 min
Delta R.T.: -0.001 min
Response: 910771
Conc: 26.32 ng/ml

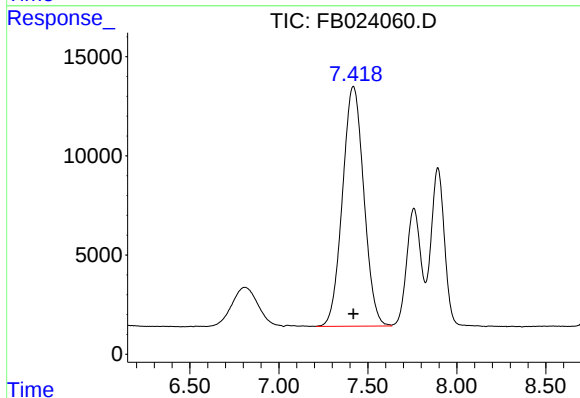


#2 2,2,4-Trimethylpentane

R.T.: 7.419 min
Delta R.T.: 0.000 min
Response: 1007115
Conc: 27.44 ng/ml

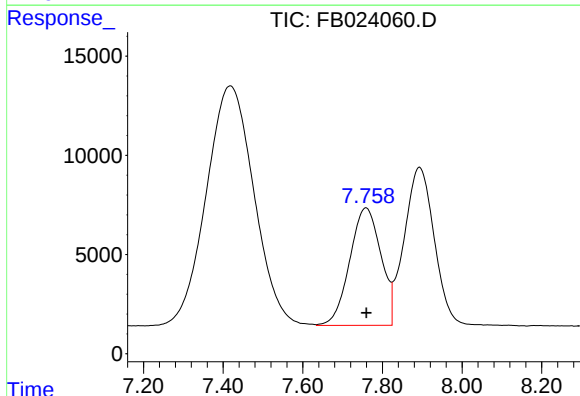


#3 n-Heptane

R.T.: 7.759 min
Delta R.T.: 0.000 min
Response: 322391
Conc: 8.94 ng/ml

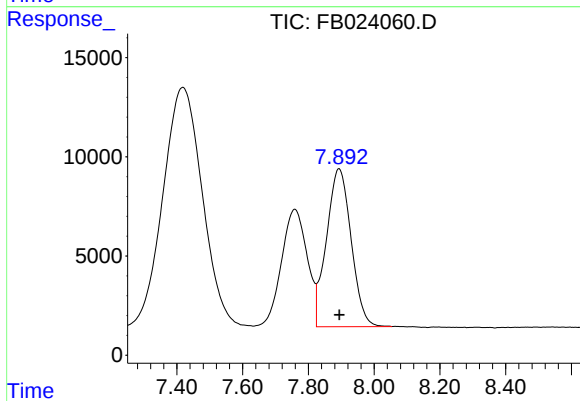


#4 Benzene

R.T.: 7.894 min
Delta R.T.: 0.000 min
Response: 414936
Conc: 9.36 ng/ml

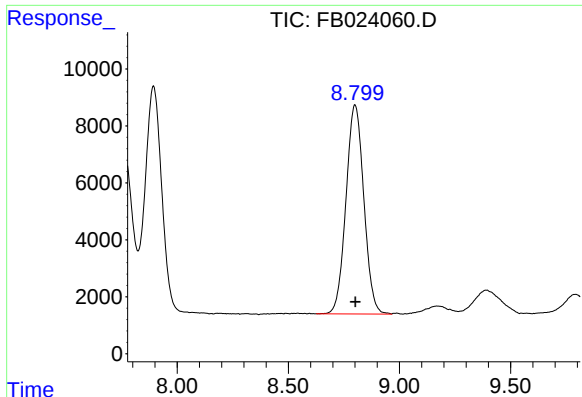


#5 AAA-TFT

R.T.: 8.800 min
Delta R.T.: -0.001 min
Response: 410010
Conc: 17.95 ng/ml

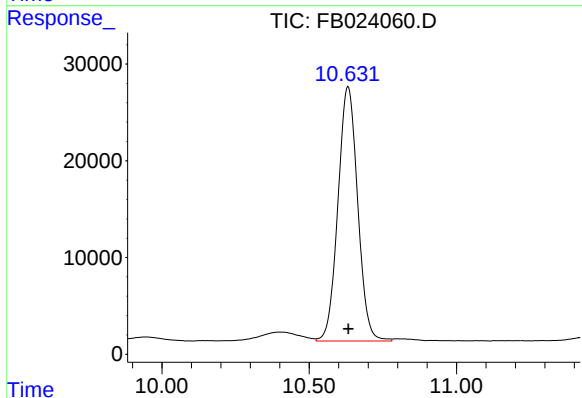


#6 Toluene

R.T.: 10.632 min
Delta R.T.: 0.000 min
Response: 1224491
Conc: 27.78 ng/ml

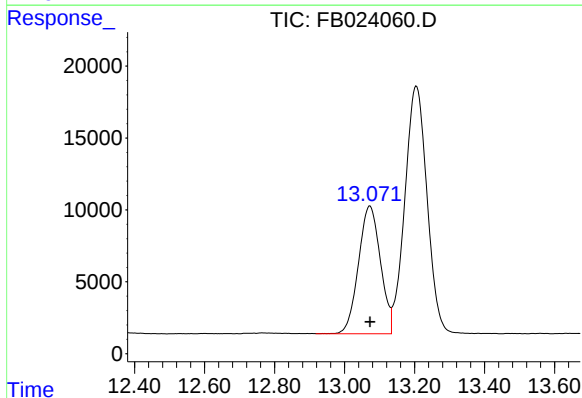


#7 Ethylbenzene

R.T.: 13.073 min
Delta R.T.: 0.000 min
Response: 386938
Conc: 9.71 ng/ml

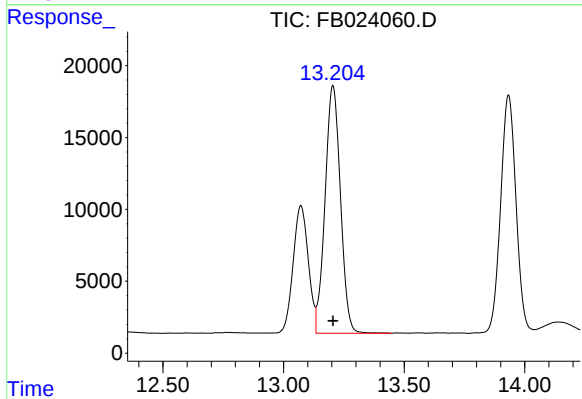


#8 m-Xylene

R.T.: 13.205 min
Delta R.T.: 0.000 min
Response: 762130
Conc: 19.81 ng/ml

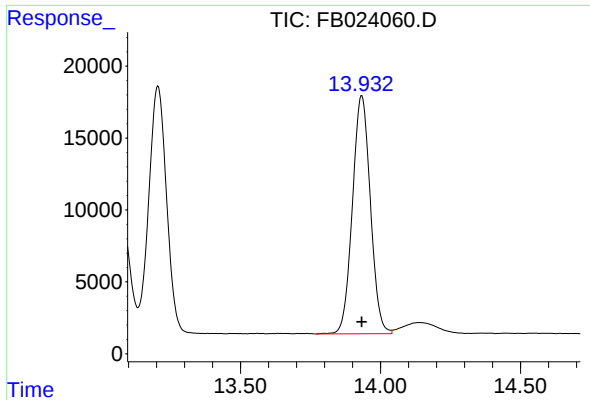

#9 O-Xylene

R.T.: 13.933 min
Delta R.T.: 0.000 min
Response: 737284
Conc: 19.95 ng/ml

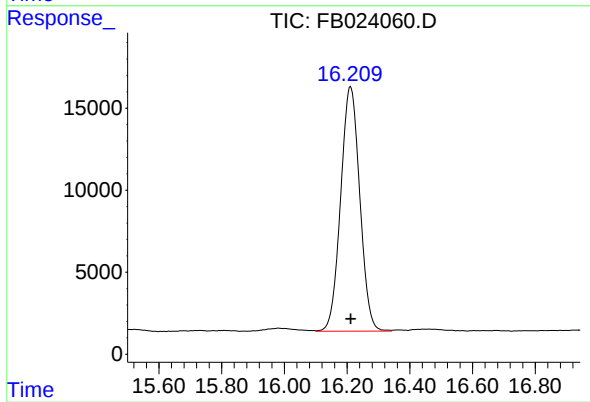

#10 1,2,4-Trimethylbenzene

R.T.: 16.211 min
Delta R.T.: 0.000 min
Response: 631159
Conc: 19.86 ng/ml