

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040422\
 Data File : FB026814.D
 Signal(s) : FID2B.CH
 Acq On : 4 Apr 2022 14:03
 Operator : AJ/MA
 Sample : BSF0404S1
 Misc : 5.02G/5.00 ML DI WATER
 ALS Vial : 4 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSF0404S1

Integration File: SAMPLE.e
 Quant Time: Apr 05 02:07:26 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.789	241836	23.046 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.709	368201	19.447 ng/ml
2) t 2,2,4-Trimethylpentane	7.425	462266	22.302 ng/ml
3) t n-Heptane	7.749	118221	5.973 ng/ml
4) t Benzene	7.885	178182	7.722 ng/ml
6) t Toluene	10.618	512759	23.421 ng/ml
7) t Ethylbenzene	13.055	164472	8.184 ng/ml
8) t m-Xylene	13.187	331618	16.455 ng/ml
9) t O-Xylene	13.914	333722	16.728 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	359519	18.044 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040422\
Data File : FB026814.D
Signal(s) : FID2B.CH
Acq On : 4 Apr 2022 14:03
Operator : AJ/MA
Sample : BSF0404S1
Misc : 5.02G/5.00 ML DI WATER
ALS Vial : 4 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSF0404S1

Integration File: SAMPLE.e
Quant Time: Apr 05 02:07:26 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

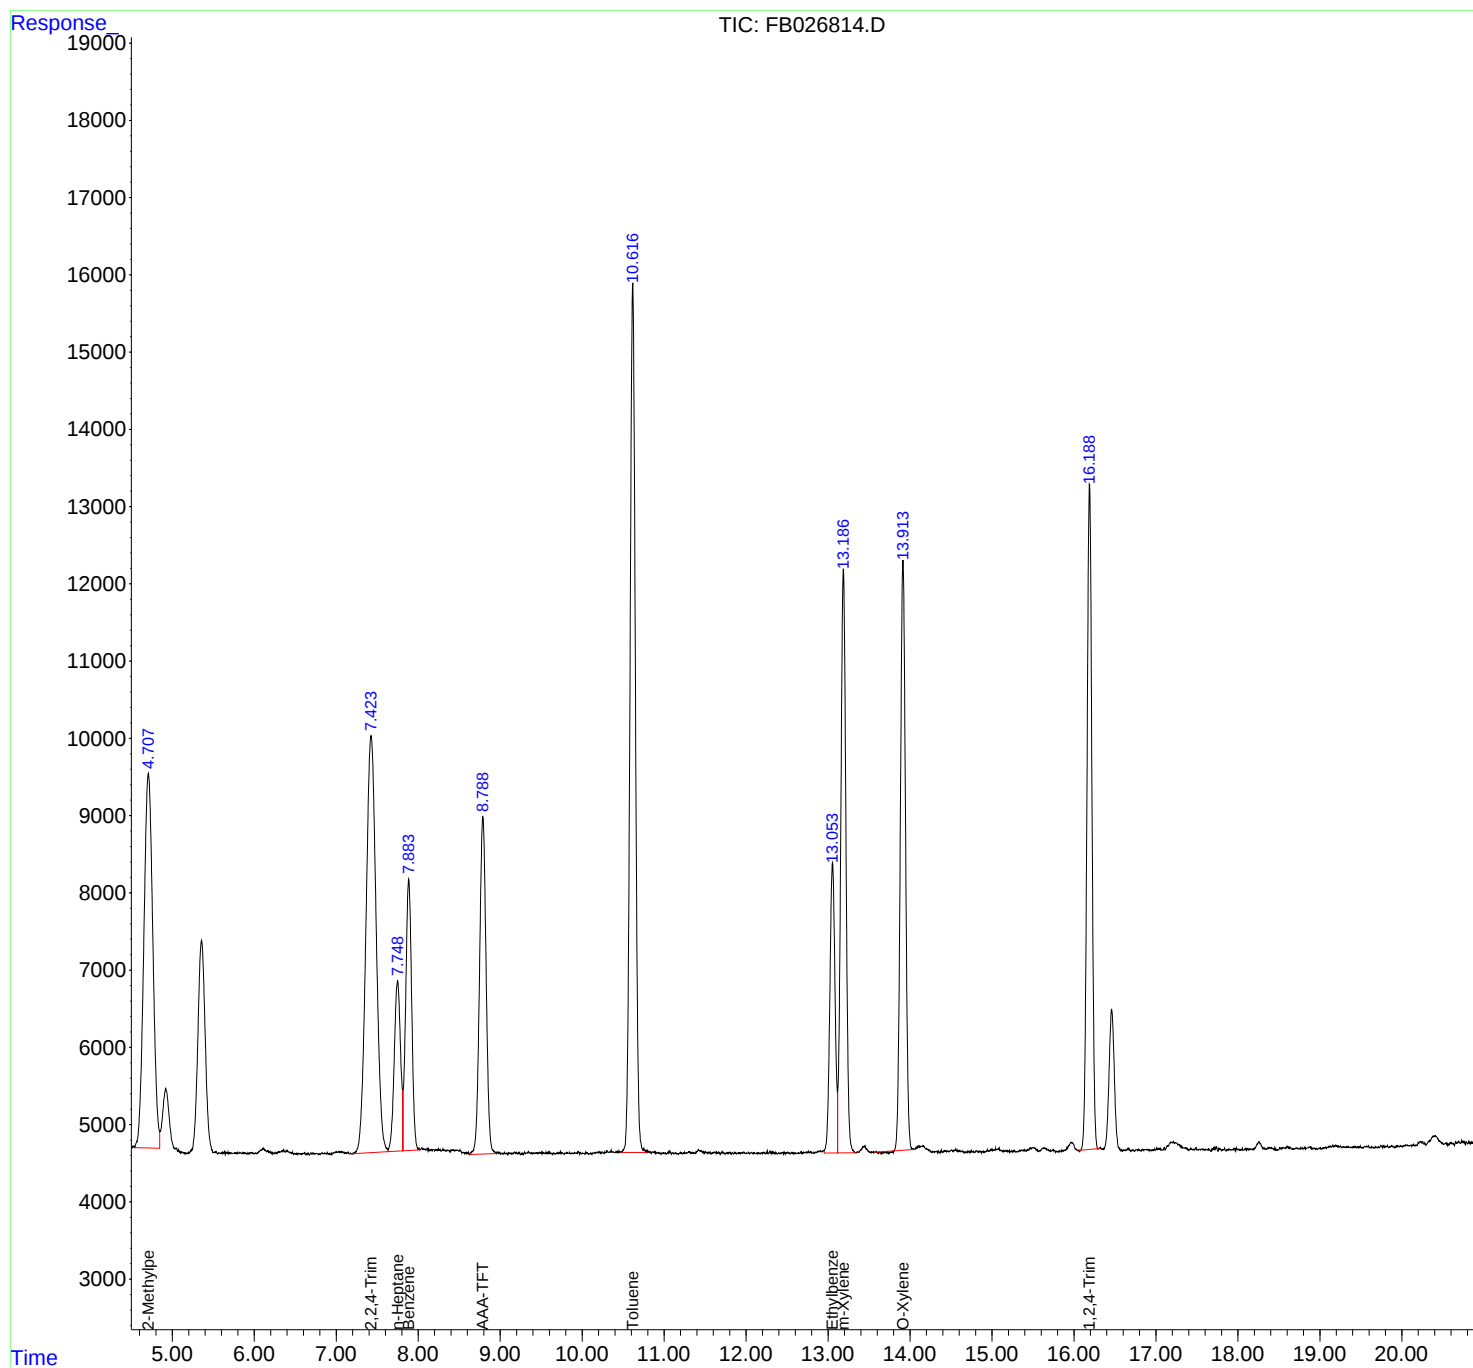


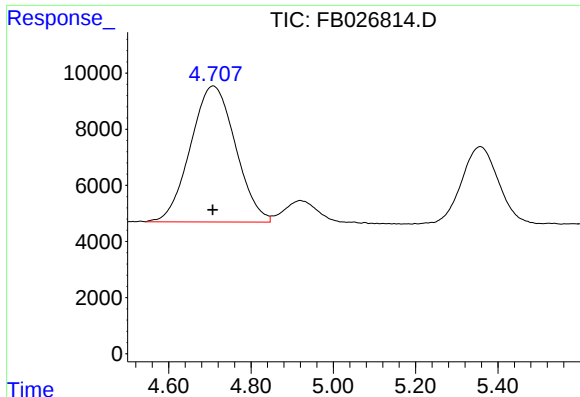

#1 2-Methylpentane


R.T.: 4.709 min
Delta R.T.: 0.002 min
Response: 368201
Conc: 19.45 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0404S1

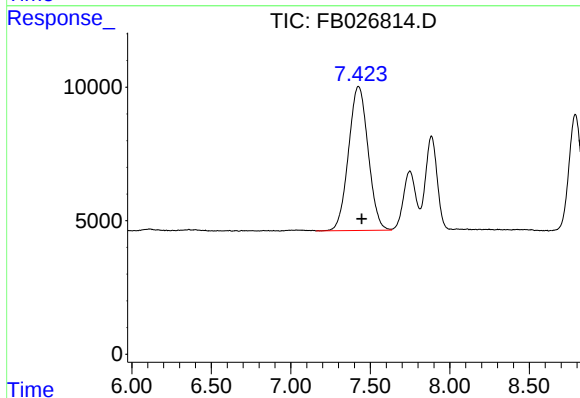


#2 2,2,4-Trimethylpentane

R.T.: 7.425 min
Delta R.T.: -0.023 min
Response: 462266
Conc: 22.30 ng/ml

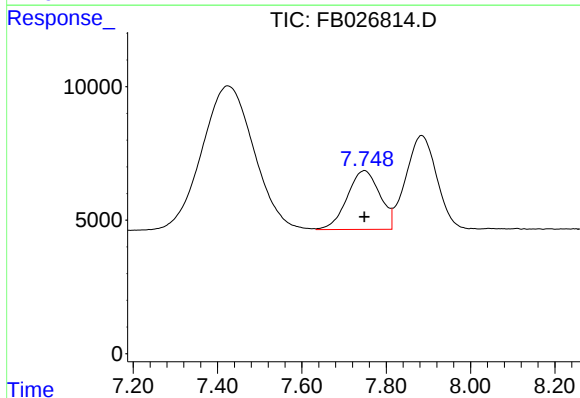


#3 n-Heptane

R.T.: 7.749 min
Delta R.T.: 0.000 min
Response: 118221
Conc: 5.97 ng/ml

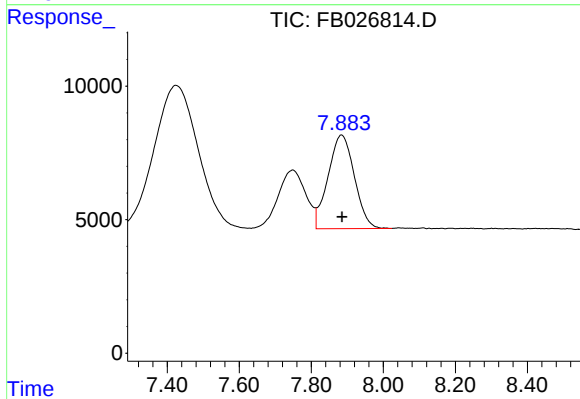

#4 Benzene


R.T.: 7.885 min
Delta R.T.: -0.001 min
Response: 178182
Conc: 7.72 ng/ml

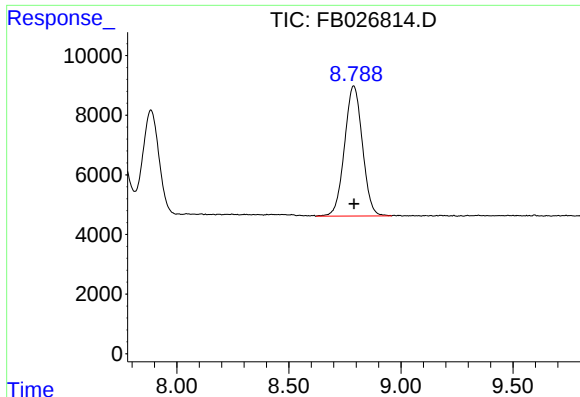

#5 AAA-TFT


R.T.: 8.789 min
Delta R.T.: -0.002 min
Response: 241836
Conc: 23.05 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0404S1

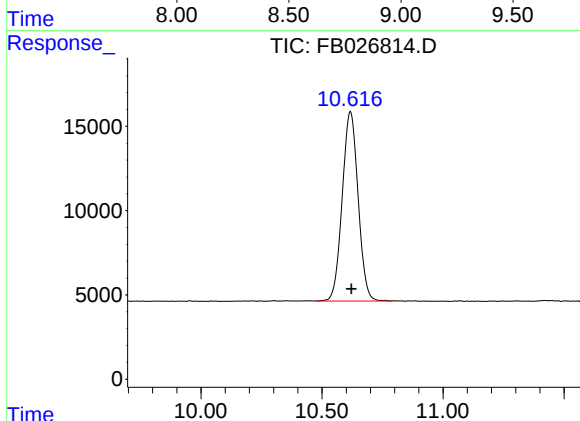


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.004 min
Response: 512759
Conc: 23.42 ng/ml

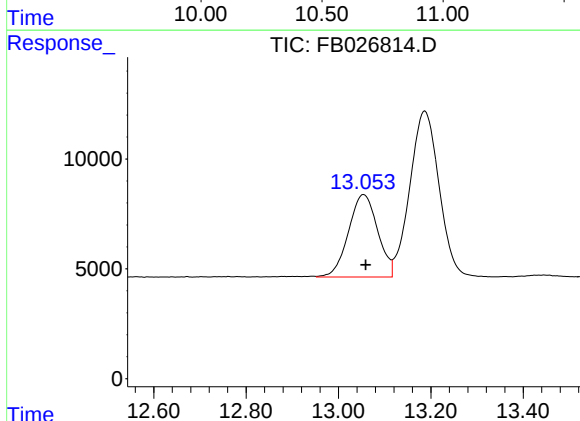


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: -0.004 min
Response: 164472
Conc: 8.18 ng/ml

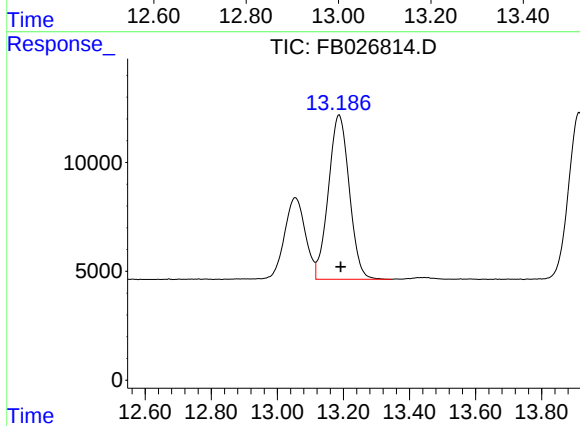

#8 m-Xylene


R.T.: 13.187 min
Delta R.T.: -0.004 min
Response: 331618
Conc: 16.46 ng/ml

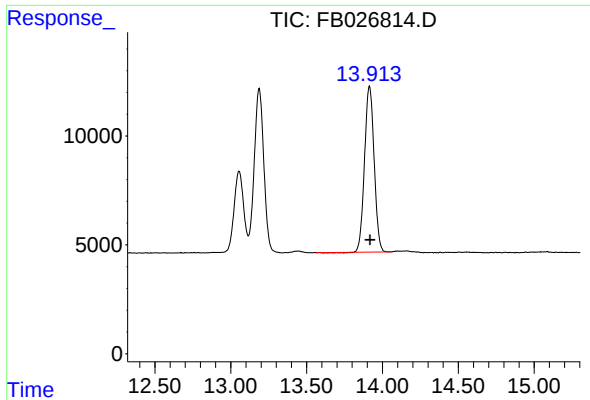

#9 O-Xylene

R.T.: 13.914 min
Delta R.T.: -0.004 min
Response: 333722
Conc: 16.73 ng/ml

Instrument :
FID_B
ClientSampleId :
BSF0404S1

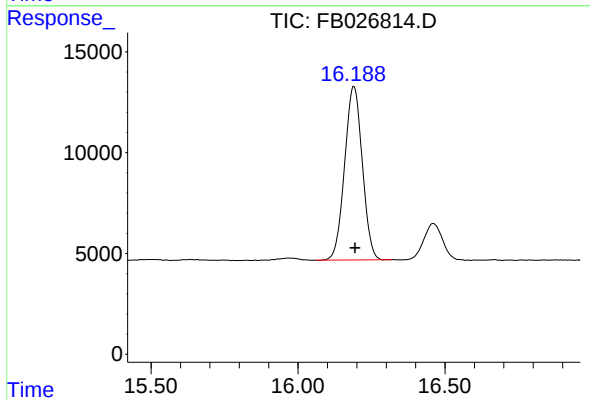

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: -0.004 min
Response: 359519
Conc: 18.04 ng/ml