

Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040422\
 Data File : FB026820.D
 Signal(s) : FID2B.CH
 Acq On : 4 Apr 2022 18:45
 Operator : AJ/MA
 Sample : BSDF0404S1
 Misc : 5.01G/5.00 ML DI WATER
 ALS Vial : 10 Sample Multiplier: 1

Instrument :
 FID_B
 ClientSampleId :
 BSDF0404S1

Integration File: SAMPLE.e
 Quant Time: Apr 05 02:08:12 2022
 Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
 Quant Title :
 QLast Update : Fri Mar 11 13:08:49 2022
 Response via : Initial Calibration
 Integrator: ChemStation

Volume Inj. : 5 g/ml
 Signal Phase : RTX-502.2
 Signal Info : 60mx0.53mmx3.00um

Compound	R.T.	Response	Conc Units

System Monitoring Compounds			
5) s AAA-TFT	8.790	249348	23.762 ng/ml
Target Compounds			
1) t 2-Methylpentane	4.706	383599	20.260 ng/ml
2) t 2,2,4-Trimethylpentane	7.428	453958	21.901 ng/ml
3) t n-Heptane	7.747	138182	6.981 ng/ml
4) t Benzene	7.886	188556	8.172 ng/ml
6) t Toluene	10.618	542736	24.791 ng/ml
7) t Ethylbenzene	13.055	170257	8.471 ng/ml
8) t m-Xylene	13.188	331732	16.461 ng/ml
9) t O-Xylene	13.915	326616	16.372 ng/ml
10) t 1,2,4-Trimethylbenzene	16.190	328648	16.495 ng/ml

(f)=RT Delta > 1/2 Window


(m)=manual int.


Data Path : Z:\pestpcbsrv\HPCHEM1\FID_B\Data\FB040422\
Data File : FB026820.D
Signal(s) : FID2B.CH
Acq On : 4 Apr 2022 18:45
Operator : AJ/MA
Sample : BSDF0404S1
Misc : 5.01G/5.00 ML DI WATER
ALS Vial : 10 Sample Multiplier: 1

Instrument :
FID_B
ClientSampleId :
BSDF0404S1

Integration File: SAMPLE.e
Quant Time: Apr 05 02:08:12 2022
Quant Method : Z:\pestpcbsrv\HPCHEM1\FID_B\Method\FB030822.M
Quant Title :
QLast Update : Fri Mar 11 13:08:49 2022
Response via : Initial Calibration
Integrator: ChemStation

Volume Inj. : 5 g/ml
Signal Phase : RTX-502.2
Signal Info : 60mx0.53mmx3.00um

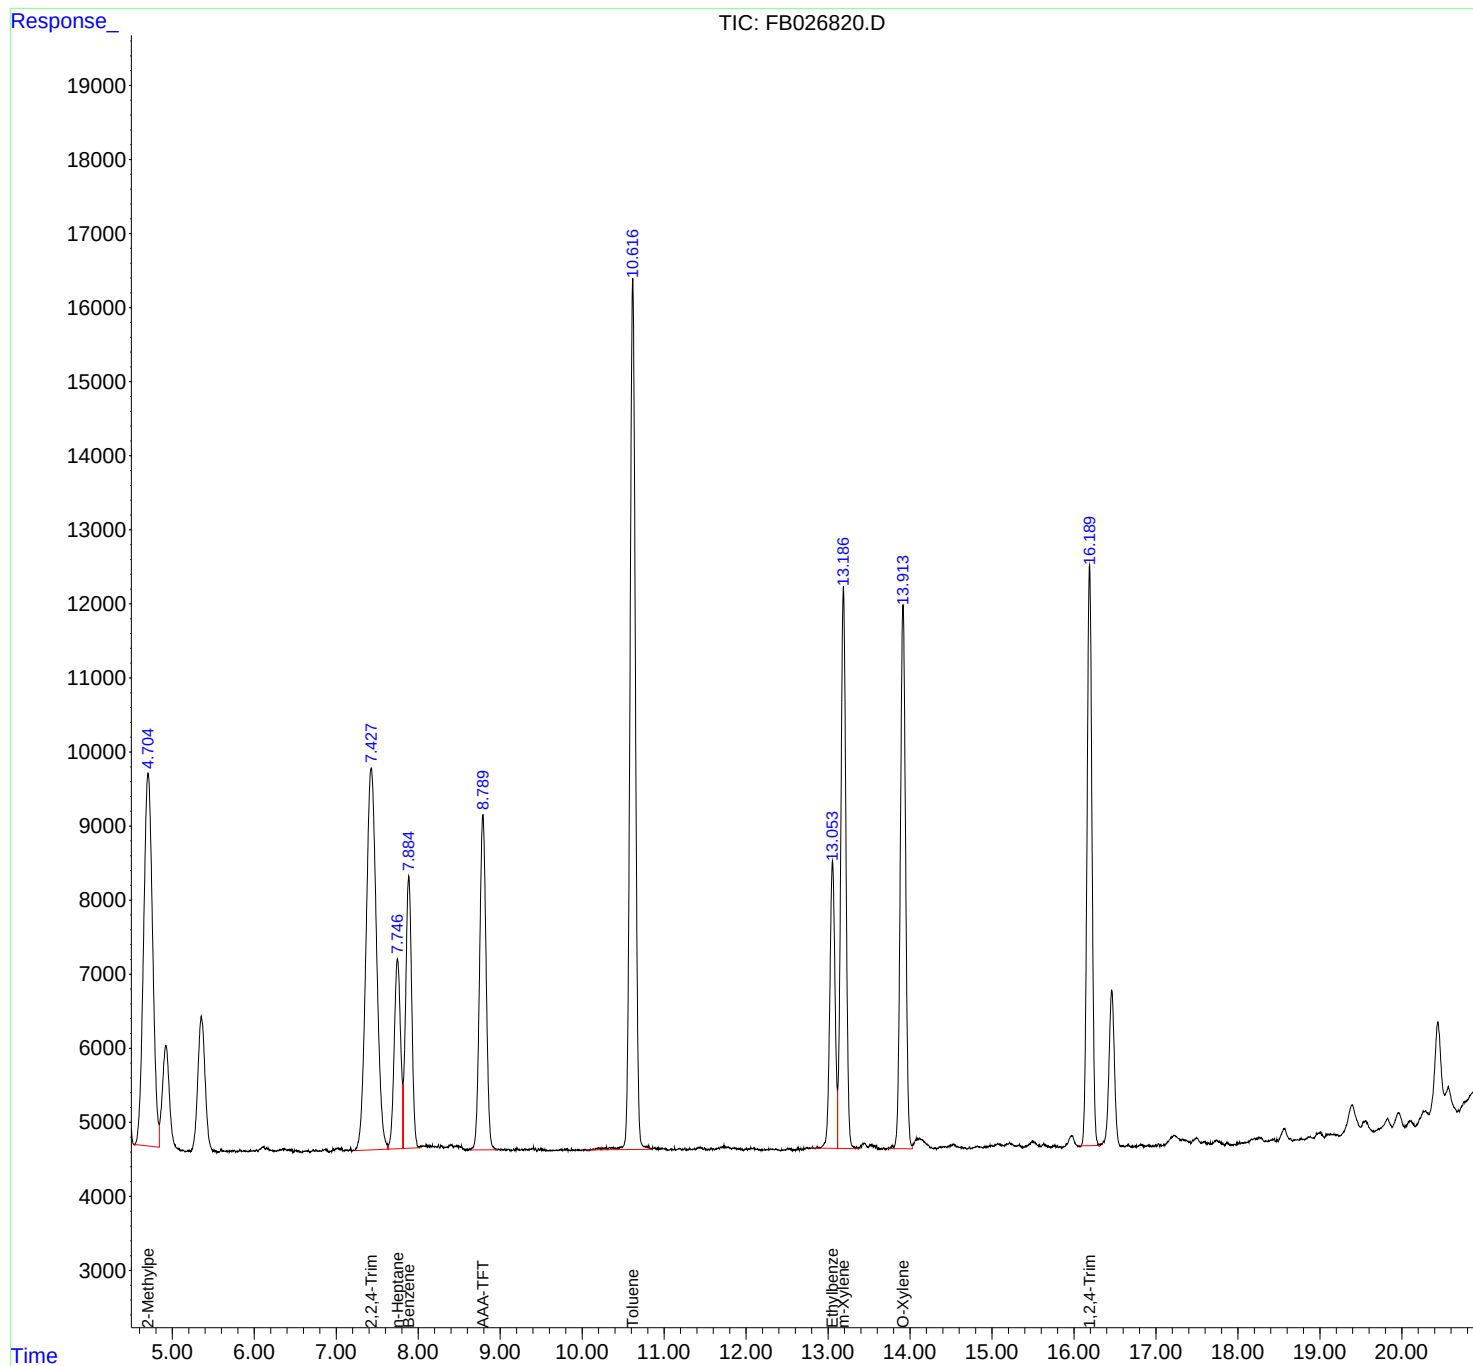


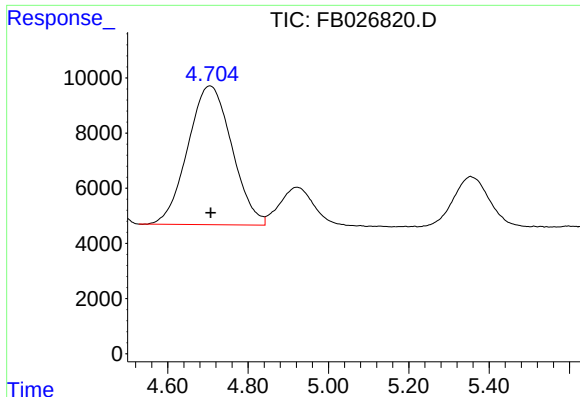

#1 2-Methylpentane


R.T.: 4.706 min
Delta R.T.: -0.001 min
Response: 383599
Conc: 20.26 ng/ml

Instrument :
FID_B
ClientSampleId :
BSDF0404S1

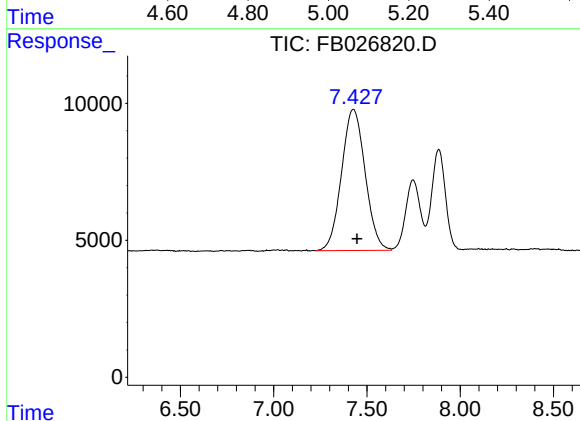


#2 2,2,4-Trimethylpentane

R.T.: 7.428 min
Delta R.T.: -0.019 min
Response: 453958
Conc: 21.90 ng/ml

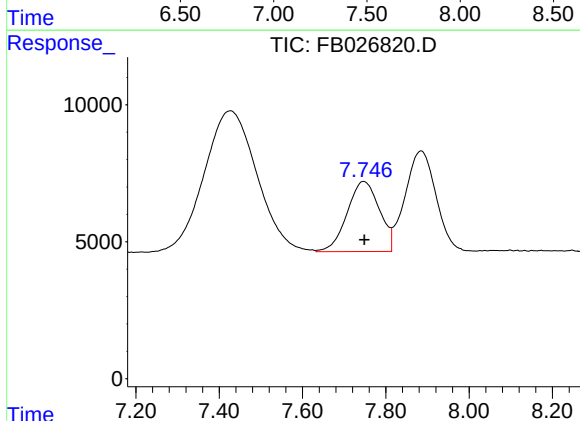


#3 n-Heptane

R.T.: 7.747 min
Delta R.T.: -0.002 min
Response: 138182
Conc: 6.98 ng/ml

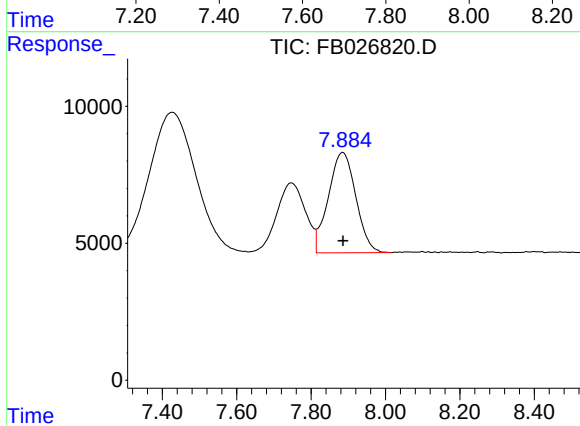

#4 Benzene


R.T.: 7.886 min
Delta R.T.: 0.000 min
Response: 188556
Conc: 8.17 ng/ml

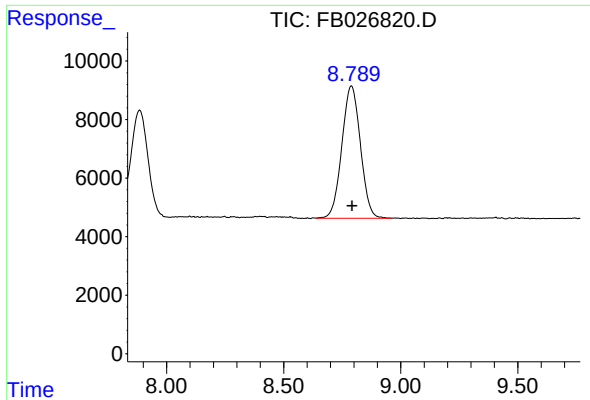

#5 AAA-TFT


R.T.: 8.790 min
Delta R.T.: -0.002 min
Response: 249348
Conc: 23.76 ng/ml

Instrument :
FID_B
ClientSampleId :
BSDF0404S1

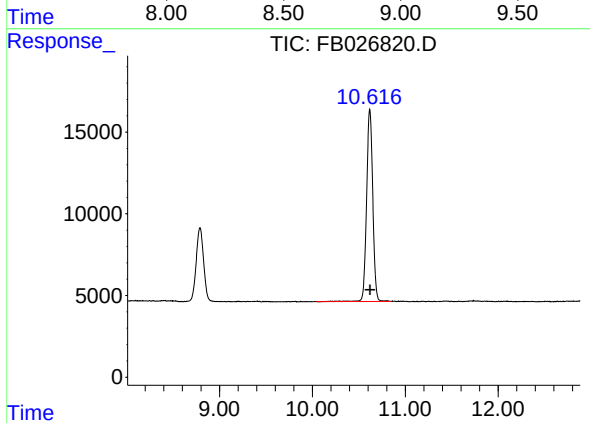


#6 Toluene

R.T.: 10.618 min
Delta R.T.: -0.003 min
Response: 542736
Conc: 24.79 ng/ml

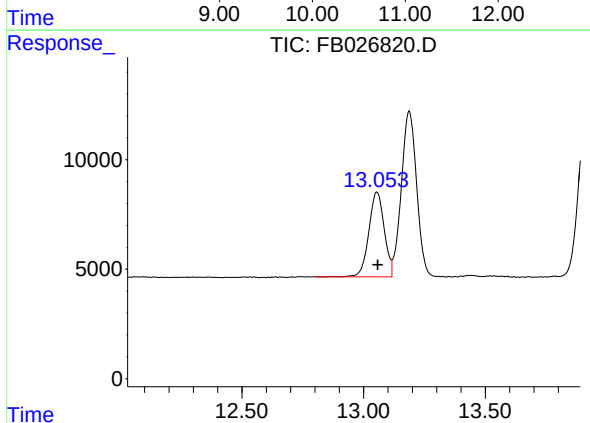


#7 Ethylbenzene

R.T.: 13.055 min
Delta R.T.: -0.004 min
Response: 170257
Conc: 8.47 ng/ml

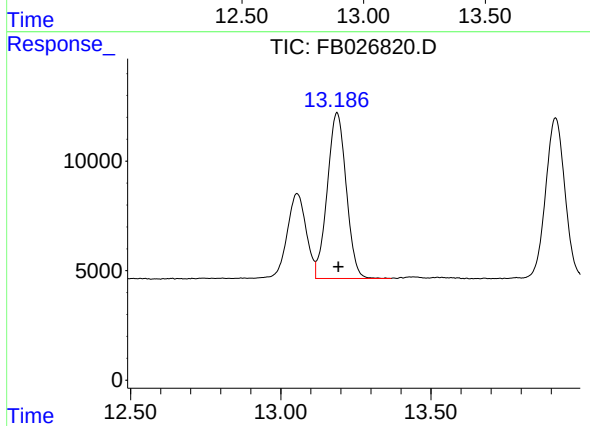

#8 m-Xylene


R.T.: 13.188 min
Delta R.T.: -0.004 min
Response: 331732
Conc: 16.46 ng/ml

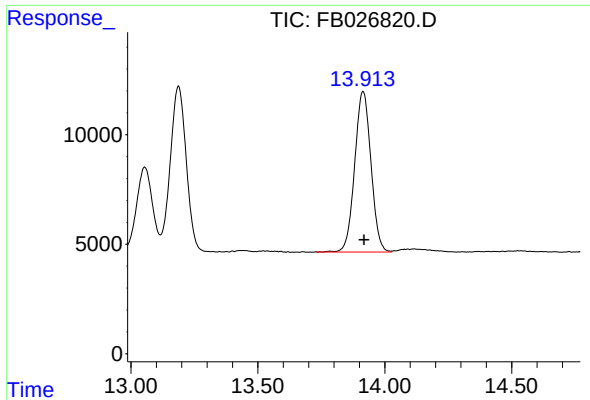

#9 O-Xylene

R.T.: 13.915 min
Delta R.T.: -0.004 min
Response: 326616
Conc: 16.37 ng/ml

Instrument :
FID_B
ClientSampleId :
BSDF0404S1

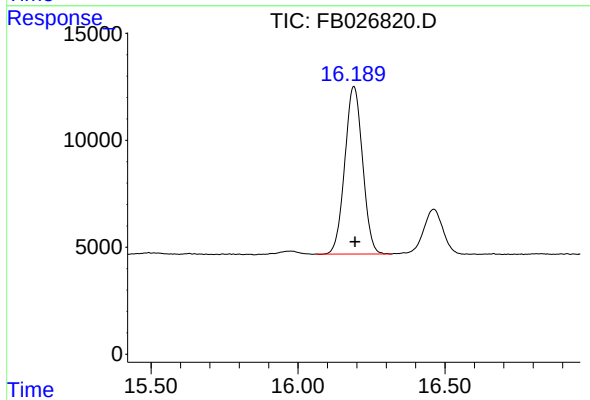

#10 1,2,4-Trimethylbenzene

R.T.: 16.190 min
Delta R.T.: -0.004 min
Response: 328648
Conc: 16.49 ng/ml